

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036005.D
 Acq On : 29 Jul 2022 22:46
 Operator : CG/JU
 Sample : N3790-20
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	37	rVB	85599	103414	2.14%	0.169%
2	3.558	77	80	85	rVB	38079	50687	1.05%	0.083%
3	3.693	100	103	120	rBV	1005535	1411186	29.14%	2.308%
4	4.022	155	159	167	rVB	26155	40224	0.83%	0.066%
5	5.563	415	421	427	rBV4	9493	22062	0.46%	0.036%
6	7.040	666	672	683	rBV	1137179	1715532	35.43%	2.806%
7	7.210	693	701	710	rBV	938402	1442713	29.80%	2.360%
8	7.293	710	715	718	rVB	9194	14248	0.29%	0.023%
9	7.405	727	734	744	rBV	1152881	1794469	37.06%	2.935%
10	7.734	788	790	795	rVB6	3238	4863	0.10%	0.008%
11	7.875	807	814	823	rBV	1073395	1663615	34.36%	2.721%
12	7.946	823	826	829	rVB4	5963	6100	0.13%	0.010%
13	8.587	928	935	949	rBV	1320774	2079500	42.95%	3.401%
14	9.040	1003	1012	1022	rBV	1017100	1666884	34.42%	2.726%
15	9.157	1026	1032	1036	rVV6	13584	23176	0.48%	0.038%
16	9.204	1036	1040	1047	rVB10	11754	21371	0.44%	0.035%
17	9.763	1127	1135	1145	rBV	789352	1304654	26.94%	2.134%
18	10.298	1219	1226	1238	rBV	1223033	2071141	42.77%	3.387%
19	10.475	1253	1256	1261	rVB7	5331	8090	0.17%	0.013%
20	10.681	1283	1291	1301	rVB	1463661	2373454	49.02%	3.882%
21	10.822	1308	1315	1327	rBV	1241246	2091508	43.19%	3.421%
22	11.198	1375	1379	1381	rBV5	3332	5261	0.11%	0.009%
23	11.293	1390	1395	1402	rVV5	2298	6746	0.14%	0.011%
24	11.728	1465	1469	1471	rBV5	3128	5314	0.11%	0.009%
25	11.887	1490	1496	1499	rBV7	3618	6703	0.14%	0.011%
26	11.940	1499	1505	1506	rBV6	7078	9357	0.19%	0.015%
27	12.175	1542	1545	1547	rBV4	3746	5561	0.11%	0.009%
28	12.269	1555	1561	1566	rBV	24800	41342	0.85%	0.068%
29	12.481	1594	1597	1601	rVB5	4189	5324	0.11%	0.009%
30	12.692	1630	1633	1635	rBV4	4066	5477	0.11%	0.009%
31	12.881	1659	1665	1668	rBV5	9169	14928	0.31%	0.024%
32	13.128	1702	1707	1712	rVB7	9013	14885	0.31%	0.024%
33	13.339	1741	1743	1748	rVB6	4838	7451	0.15%	0.012%
34	13.416	1751	1756	1761	rVV2	21833	38724	0.80%	0.063%
35	13.486	1764	1768	1772	rVB6	5546	8893	0.18%	0.015%
36	13.734	1806	1810	1813	rVB5	3985	5693	0.12%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036005.D
 Acq On : 29 Jul 2022 22:46
 Operator : CG/JU
 Sample : N3790-20
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	13.792	1816	1820	1826	rBV7	6019	12113	0.25%	0.020%
38	13.928	1836	1843	1853	rBV	2106188	2784335	57.50%	4.554%
39	14.204	1880	1890	1900	rBV	2491645	3599774	74.34%	5.887%
40	14.416	1923	1926	1929	rVB5	4183	4935	0.10%	0.008%
41	14.510	1936	1942	1949	rBV	2079279	2928660	60.48%	4.790%
42	14.581	1952	1954	1959	rVB5	4532	5608	0.12%	0.009%
43	14.710	1965	1976	1993	rBV	729895	1165381	24.07%	1.906%
44	14.933	2009	2014	2024	rVB10	18114	35703	0.74%	0.058%
45	15.151	2048	2051	2058	rVB9	3210	5909	0.12%	0.010%
46	15.304	2072	2077	2080	rBV6	11583	19571	0.40%	0.032%
47	15.428	2094	2098	2101	rVB6	4398	4939	0.10%	0.008%
48	15.504	2104	2111	2119	rBV	3042030	4336666	89.56%	7.093%
49	15.622	2124	2131	2140	rBV	626215	889772	18.38%	1.455%
50	15.739	2147	2151	2156	rVB2	30703	45766	0.95%	0.075%
51	16.063	2201	2206	2211	rBV7	8369	17996	0.37%	0.029%
52	16.222	2230	2233	2235	rVB4	7578	6886	0.14%	0.011%
53	16.286	2239	2244	2248	rBV6	9503	14030	0.29%	0.023%
54	16.386	2259	2261	2268	rVB8	7706	12826	0.26%	0.021%
55	16.569	2287	2292	2299	rBV8	8592	20554	0.42%	0.034%
56	16.651	2304	2306	2310	rVB4	9948	11494	0.24%	0.019%
57	16.733	2315	2320	2329	rVV2	25917	45460	0.94%	0.074%
58	17.016	2364	2368	2370	rBV3	15253	20209	0.42%	0.033%
59	17.251	2402	2408	2416	rBV	2328004	3192896	65.94%	5.222%
60	17.351	2418	2425	2435	rVV	3121454	4311899	89.05%	7.052%
61	17.445	2437	2441	2446	rVB8	32188	48271	1.00%	0.079%
62	17.639	2470	2474	2483	rVB7	26903	46431	0.96%	0.076%
63	17.757	2489	2494	2496	rBV6	8425	12096	0.25%	0.020%
64	17.804	2498	2502	2506	rVB2	23953	33248	0.69%	0.054%
65	17.927	2519	2523	2532	rVB	78329	101043	2.09%	0.165%
66	18.021	2535	2539	2544	rBV8	13151	24480	0.51%	0.040%
67	18.145	2556	2560	2570	rBV	109829	169086	3.49%	0.277%
68	18.751	2660	2663	2668	rVB3	24681	31725	0.66%	0.052%
69	19.016	2704	2708	2712	rBV3	46092	60151	1.24%	0.098%
70	19.098	2718	2722	2727	rBV	185404	218179	4.51%	0.357%
71	19.204	2736	2740	2742	rBV2	43170	52215	1.08%	0.085%
72	19.233	2742	2745	2749	rVV	67807	76670	1.58%	0.125%
73	19.274	2749	2752	2755	rVV	36917	46817	0.97%	0.077%
74	19.327	2758	2761	2766	rVB2	51200	64938	1.34%	0.106%
75	19.545	2795	2798	2801	rBV	27055	30620	0.63%	0.050%
76	19.639	2808	2814	2820	rBV	3689133	4842092	100.00%	7.919%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036005.D
Acq On : 29 Jul 2022 22:46
Operator : CG/JU
Sample : N3790-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

77	20.239	2914	2916	2920	rBV3	27877	29857	0.62%	0.049%
78	20.639	2981	2984	2988	rBV	142812	155477	3.21%	0.254%
79	21.145	3067	3070	3074	rBV	148000	165304	3.41%	0.270%
80	21.427	3113	3118	3127	rBV	2781575	3420563	70.64%	5.594%
81	23.639	3488	3494	3501	rBV2	2472018	4590082	94.80%	7.507%
82	23.792	3514	3520	3529	rVB2	1714536	3340831	69.00%	5.464%




Sum of corrected areas: 61144108

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036005.D
Acq On : 29 Jul 2022 22:46
Operator : CG/JU
Sample : N3790-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

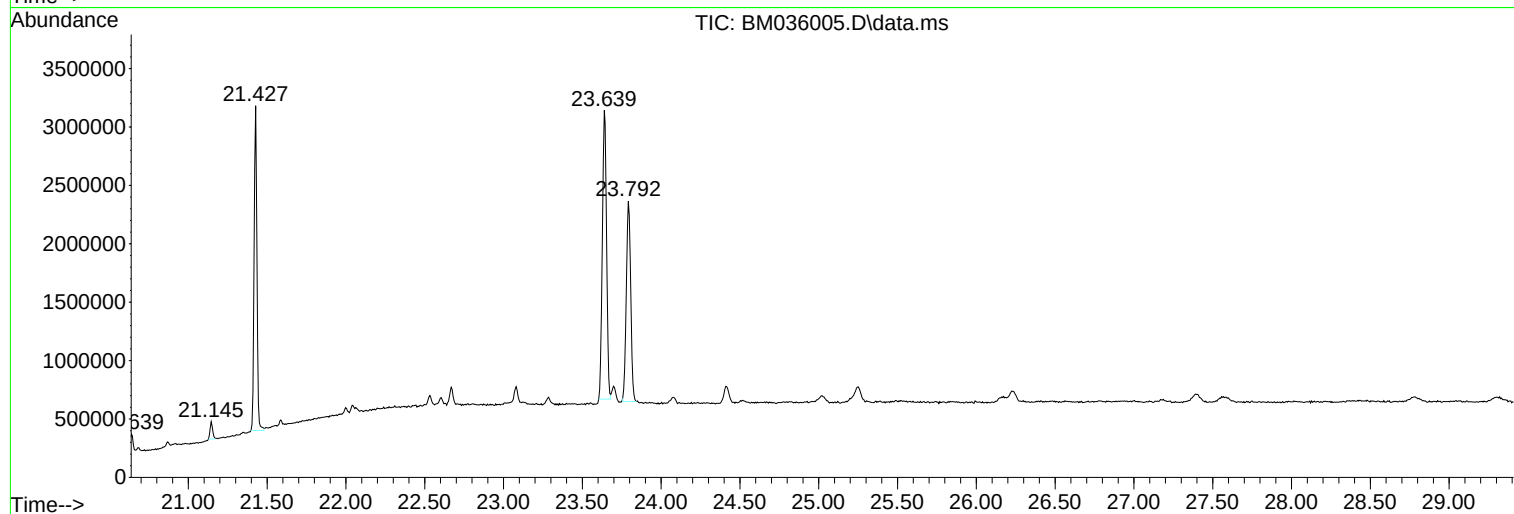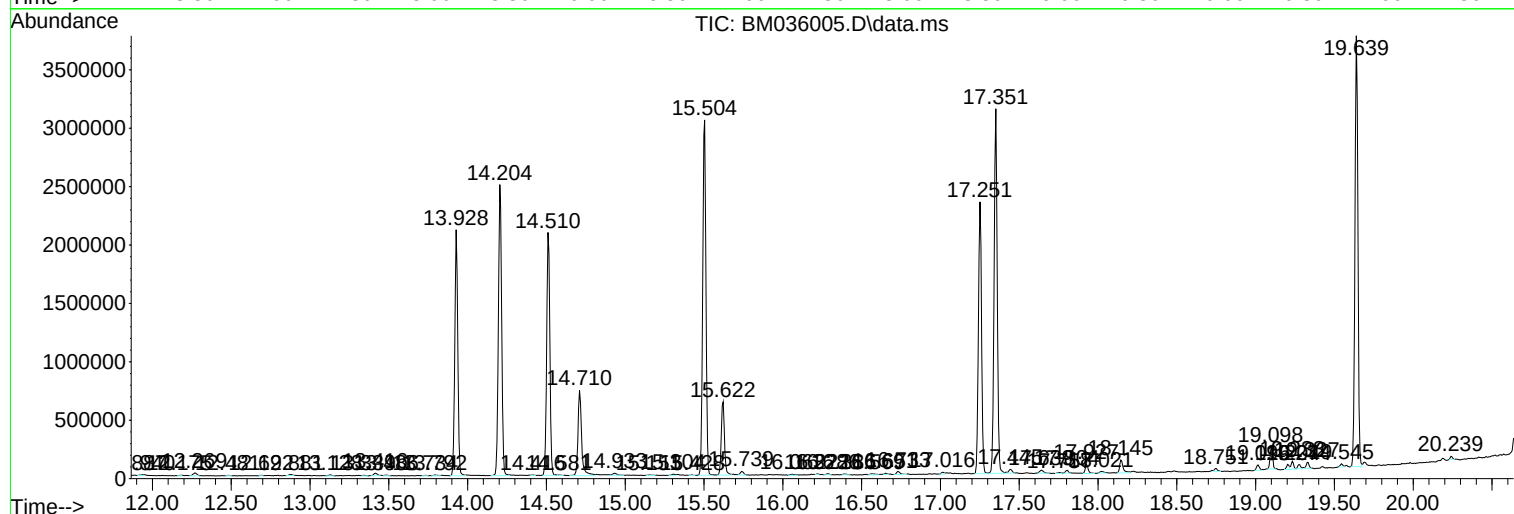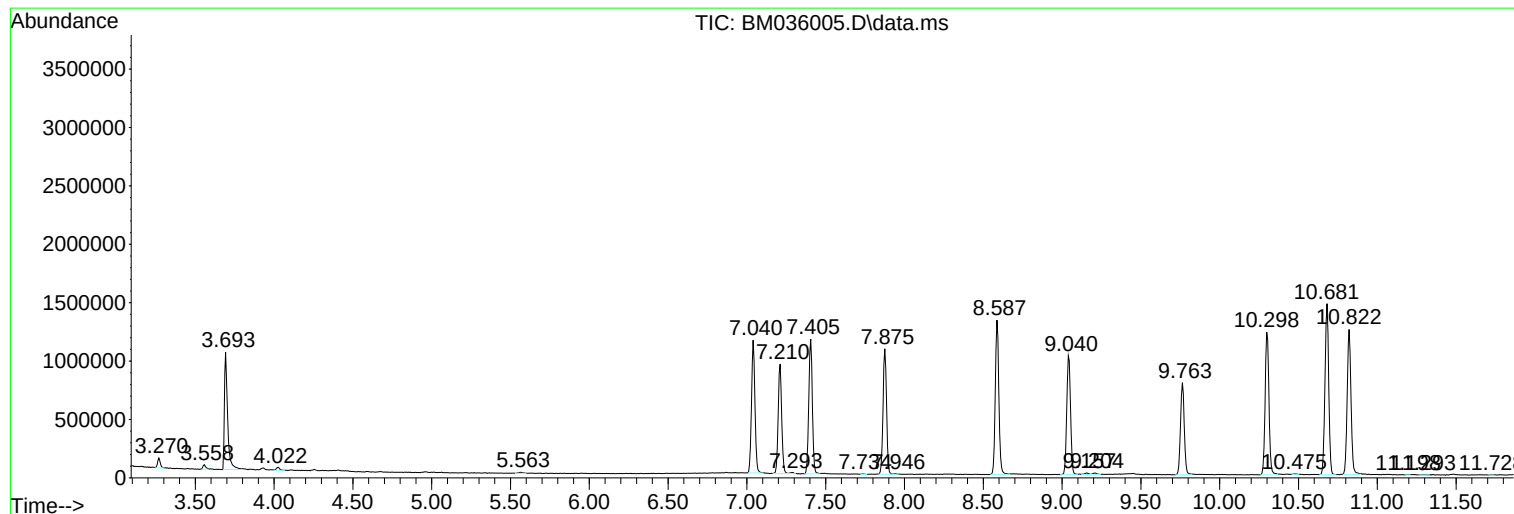

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036005.D
Acq On : 29 Jul 2022 22:46
Operator : CG/JU
Sample : N3790-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036005.D
Acq On : 29 Jul 2022 22:46
Operator : CG/JU
Sample : N3790-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc