

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036008.D
 Acq On : 30 Jul 2022 00:35
 Operator : CG/JU
 Sample : N3890-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBEA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	39	rVB	68322	89052	1.20%	0.117%
2	3.693	100	103	114	rBV	369630	535036	7.20%	0.700%
3	3.928	139	143	148	rVB2	40546	57711	0.78%	0.076%
4	4.022	156	159	166	rVB	31125	46404	0.62%	0.061%
5	4.963	316	319	321	rBV4	7353	7861	0.11%	0.010%
6	7.039	665	672	685	rVB	248478	403021	5.42%	0.527%
7	7.210	694	701	712	rVB	1265674	1939926	26.10%	2.538%
8	7.404	727	734	745	rBV	1099846	1680273	22.61%	2.198%
9	7.875	807	814	823	rBV	1492405	2275389	30.62%	2.977%
10	8.586	928	935	946	rBV	719203	1168789	15.73%	1.529%
11	9.039	1003	1012	1028	rBV	1388621	2290770	30.82%	2.997%
12	9.216	1037	1042	1047	rBV9	4672	8521	0.11%	0.011%
13	9.763	1128	1135	1148	rBV	927465	1522730	20.49%	1.992%
14	10.298	1219	1226	1244	rBV	1405512	2367827	31.86%	3.098%
15	10.680	1283	1291	1298	rBV	2051103	3281690	44.15%	4.293%
16	10.822	1306	1315	1333	rBV	1463422	2481005	33.38%	3.246%
17	11.945	1499	1506	1514	rVB	26362	49764	0.67%	0.065%
18	12.269	1554	1561	1570	rVB2	33003	57941	0.78%	0.076%
19	12.874	1657	1664	1669	rBV7	10786	24643	0.33%	0.032%
20	13.127	1703	1707	1711	rVB6	6212	10514	0.14%	0.014%
21	13.333	1739	1742	1748	rVB8	3861	7581	0.10%	0.010%
22	13.486	1763	1768	1773	rBV6	10008	19701	0.27%	0.026%
23	13.804	1815	1822	1823	rBV7	6389	9412	0.13%	0.012%
24	13.927	1834	1843	1852	rBV	2840635	3826857	51.49%	5.007%
25	14.204	1879	1890	1899	rBV	3300164	4827932	64.96%	6.316%
26	14.410	1921	1925	1929	rVB5	9707	15522	0.21%	0.020%
27	14.510	1935	1942	1955	rBV	2790685	4107734	55.27%	5.374%
28	14.715	1971	1977	1987	rBV	112819	220533	2.97%	0.289%
29	14.933	2009	2014	2018	rBV8	8888	14357	0.19%	0.019%
30	15.015	2026	2028	2034	rVB7	7553	10481	0.14%	0.014%
31	15.304	2071	2077	2080	rBV2	12643	19841	0.27%	0.026%
32	15.362	2084	2087	2090	rVB4	10055	11657	0.16%	0.015%
33	15.504	2102	2111	2121	rBV	4294187	6061254	81.55%	7.930%
34	15.621	2124	2131	2142	rBV	791106	1109665	14.93%	1.452%
35	15.739	2147	2151	2160	rVB	42884	73813	0.99%	0.097%
36	16.062	2203	2206	2210	rBV5	5659	7946	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036008.D
 Acq On : 30 Jul 2022 00:35
 Operator : CG/JU
 Sample : N3890-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YBEA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	16.221	2221	2233	2237	rBV9	18465	52918	0.71%	0.069%
38	16.286	2240	2244	2249	rVB4	16898	26265	0.35%	0.034%
39	16.380	2256	2260	2265	rBV8	5080	10310	0.14%	0.013%
40	16.562	2287	2291	2295	rBV7	9383	15821	0.21%	0.021%
41	16.733	2316	2320	2325	rBV3	27833	44652	0.60%	0.058%
42	16.933	2348	2354	2358	rBV8	11557	22550	0.30%	0.030%
43	17.015	2364	2368	2374	rBV3	24206	46293	0.62%	0.061%
44	17.168	2393	2394	2400	rVB6	6626	9394	0.13%	0.012%
45	17.251	2402	2408	2415	rVV	3254657	4443395	59.79%	5.813%
46	17.351	2418	2425	2436	rVV	4941457	6721047	90.43%	8.793%
47	17.751	2491	2493	2497	rBV4	10629	13135	0.18%	0.017%
48	17.803	2498	2502	2506	rVV	28015	38034	0.51%	0.050%
49	17.927	2520	2523	2526	rVB5	12089	12570	0.17%	0.016%
50	18.145	2556	2560	2564	rBV5	25112	40573	0.55%	0.053%
51	18.227	2571	2574	2577	rVB	13560	14433	0.19%	0.019%
52	18.286	2582	2584	2587	rBV4	7031	7842	0.11%	0.010%
53	18.750	2659	2663	2667	rBV	33600	42613	0.57%	0.056%
54	19.209	2736	2741	2747	rBV	62136	92449	1.24%	0.121%
55	19.274	2748	2752	2756	rBV2	57991	77448	1.04%	0.101%
56	19.545	2795	2798	2801	rBV	44717	48836	0.66%	0.064%
57	19.574	2801	2803	2806	rVB3	21790	19605	0.26%	0.026%
58	19.639	2808	2814	2820	rBV	5706531	7432205	100.00%	9.723%
59	20.239	2913	2916	2922	rVB2	74062	91539	1.23%	0.120%
60	20.639	2981	2984	2990	rVB	285784	309611	4.17%	0.405%
61	20.868	3020	3023	3026	rBV	108614	122808	1.65%	0.161%
62	21.427	3113	3118	3125	rBV	3662653	4582767	61.66%	5.996%
63	23.638	3487	3494	3501	rBV2	3641633	7034060	94.64%	9.203%
64	23.791	3513	3520	3529	rVB2	2250249	4419903	59.47%	5.782%




Sum of corrected areas: 76436229

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036008.D
Acq On : 30 Jul 2022 00:35
Operator : CG/JU
Sample : N3890-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBEA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

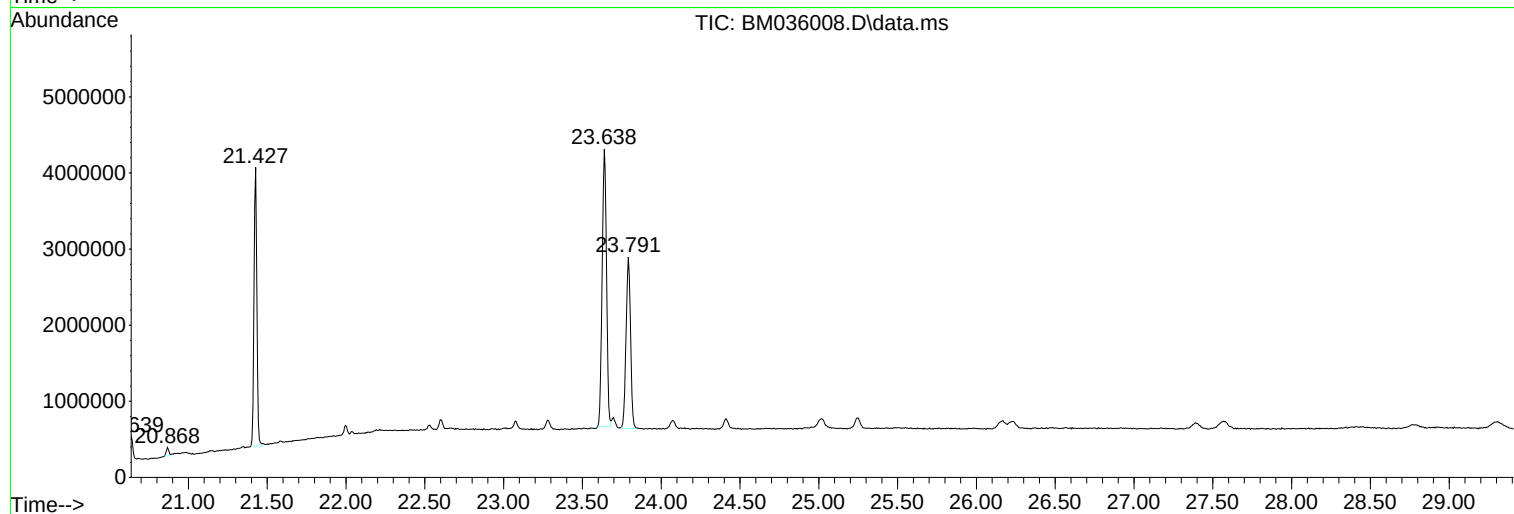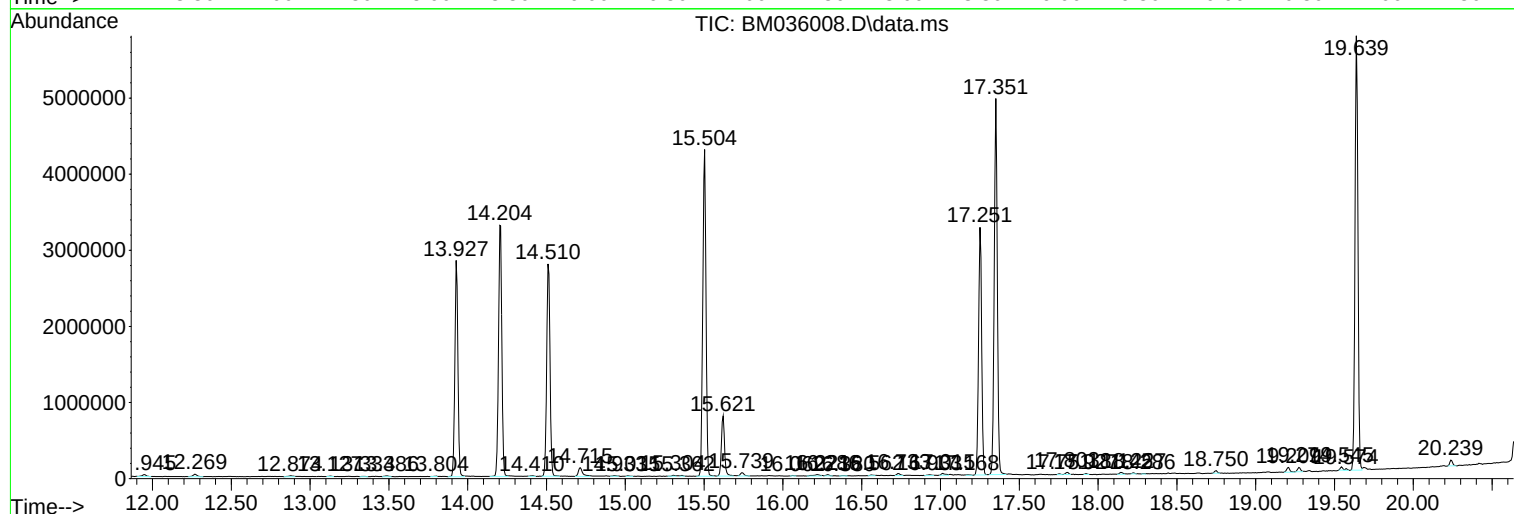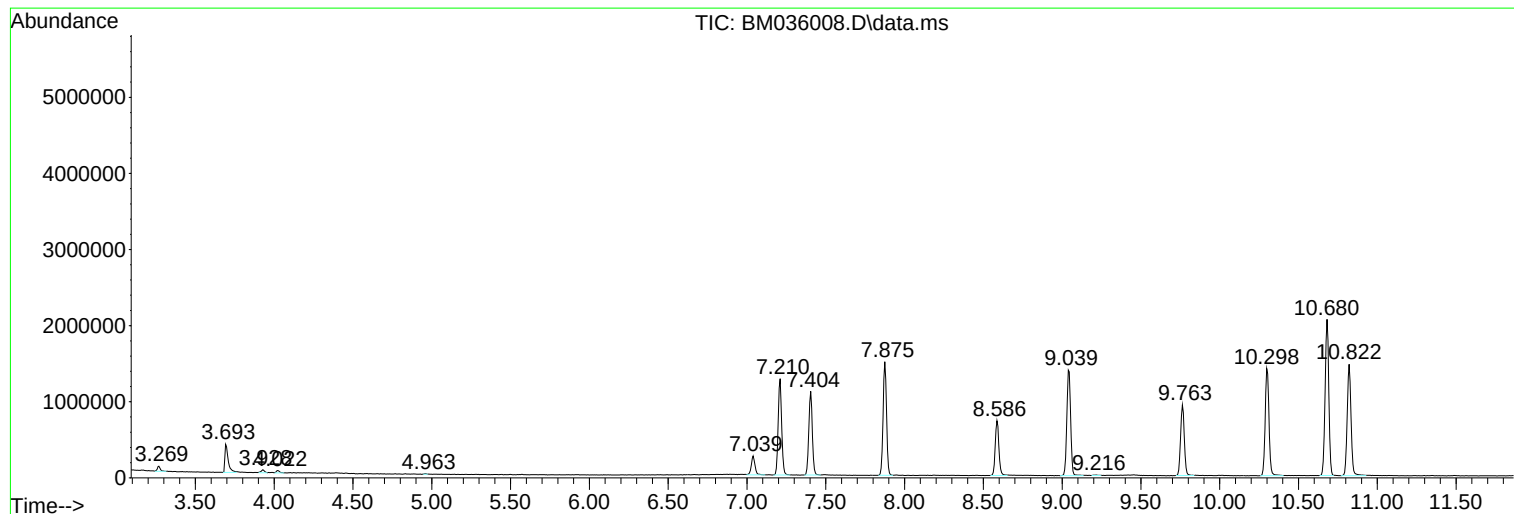

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036008.D
Acq On : 30 Jul 2022 00:35
Operator : CG/JU
Sample : N3890-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBEA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036008.D
Acq On : 30 Jul 2022 00:35
Operator : CG/JU
Sample : N3890-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YBEA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------