

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036014.D
 Acq On : 30 Jul 2022 04:49
 Operator : CG/JU
 Sample : PB146355BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK355

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	41	rVB	158723	211306	2.62%	0.210%
2	3.693	99	103	130	rBV	1802353	2662633	32.99%	2.650%
3	4.022	156	159	167	rVB	30827	44799	0.56%	0.045%
4	7.040	665	672	682	rVB	2052998	3121911	38.68%	3.107%
5	7.210	694	701	713	rVB	1754213	2692424	33.36%	2.679%
6	7.404	725	734	743	rBV	2146770	3341723	41.40%	3.326%
7	7.875	807	814	823	rBV	1633490	2545946	31.54%	2.534%
8	8.587	928	935	948	rBV	2501089	3908814	48.43%	3.890%
9	9.040	1005	1012	1021	rBV	1908652	3078776	38.15%	3.064%
10	9.151	1027	1031	1034	rBV5	8370	11290	0.14%	0.011%
11	9.763	1127	1135	1148	rBV	1512462	2447026	30.32%	2.435%
12	10.298	1217	1226	1242	rBV	2277070	3776745	46.79%	3.759%
13	10.681	1283	1291	1300	rBV	2208920	3661351	45.36%	3.644%
14	10.822	1306	1315	1334	rBV	2332058	3985769	49.38%	3.967%
15	12.263	1554	1560	1569	rBV2	40407	74714	0.93%	0.074%
16	13.416	1750	1756	1761	rVB8	5928	10938	0.14%	0.011%
17	13.480	1764	1767	1772	rVB6	6665	10642	0.13%	0.011%
18	13.798	1817	1821	1825	rBV6	5349	8547	0.11%	0.009%
19	13.927	1837	1843	1857	rBV	3806632	5008502	62.05%	4.984%
20	14.204	1879	1890	1905	rBV	4513056	6390113	79.17%	6.359%
21	14.510	1935	1942	1953	rBV	3097145	4378465	54.25%	4.357%
22	14.710	1968	1976	1993	rBV	1454939	2164967	26.82%	2.155%
23	14.874	2002	2004	2010	rVB6	6397	8887	0.11%	0.009%
24	15.498	2103	2110	2118	rBV	5220214	7555822	93.61%	7.519%
25	15.621	2124	2131	2146	rBV	1237600	1737675	21.53%	1.729%
26	15.739	2146	2151	2161	rVB	68106	103604	1.28%	0.103%
27	16.074	2204	2208	2212	rVB6	5786	9527	0.12%	0.009%
28	16.180	2222	2226	2229	rBV6	6466	10502	0.13%	0.010%
29	16.280	2239	2243	2249	rVB4	18008	26508	0.33%	0.026%
30	16.563	2286	2291	2295	rBV7	7477	15504	0.19%	0.015%
31	16.733	2316	2320	2324	rBV3	24882	33286	0.41%	0.033%
32	16.927	2349	2353	2356	rBV6	9254	12318	0.15%	0.012%
33	17.015	2363	2368	2369	rBV5	10616	12851	0.16%	0.013%
34	17.251	2401	2408	2417	rBV	3225620	4493560	55.67%	4.472%
35	17.351	2418	2425	2439	rVV	5201782	7426453	92.01%	7.391%
36	17.804	2498	2502	2505	rVB2	22557	28367	0.35%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036014.D
 Acq On : 30 Jul 2022 04:49
 Operator : CG/JU
 Sample : PB146355BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK355

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	18.745	2659	2662	2665	rBV3	24030	28194	0.35%	0.028%
38	19.204	2736	2740	2746	rVB2	64741	82704	1.02%	0.082%
39	19.274	2748	2752	2758	rBV	59092	83186	1.03%	0.083%
40	19.545	2795	2798	2801	rBV2	24548	26761	0.33%	0.027%
41	19.639	2808	2814	2821	rBV	6256173	7991047	99.01%	7.952%
42	20.239	2913	2916	2919	rBV2	28716	36790	0.46%	0.037%
43	20.639	2981	2984	2988	rBV	110639	124542	1.54%	0.124%
44	21.427	3113	3118	3124	rBV	3555104	4451375	55.15%	4.430%
45	23.639	3487	3494	3502	rBV2	4316386	8071231	100.00%	8.032%
46	23.792	3513	3520	3533	rVB2	2358277	4576893	56.71%	4.555%




Sum of corrected areas: 100484988

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036014.D
Acq On : 30 Jul 2022 04:49
Operator : CG/JU
Sample : PB146355BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK355

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

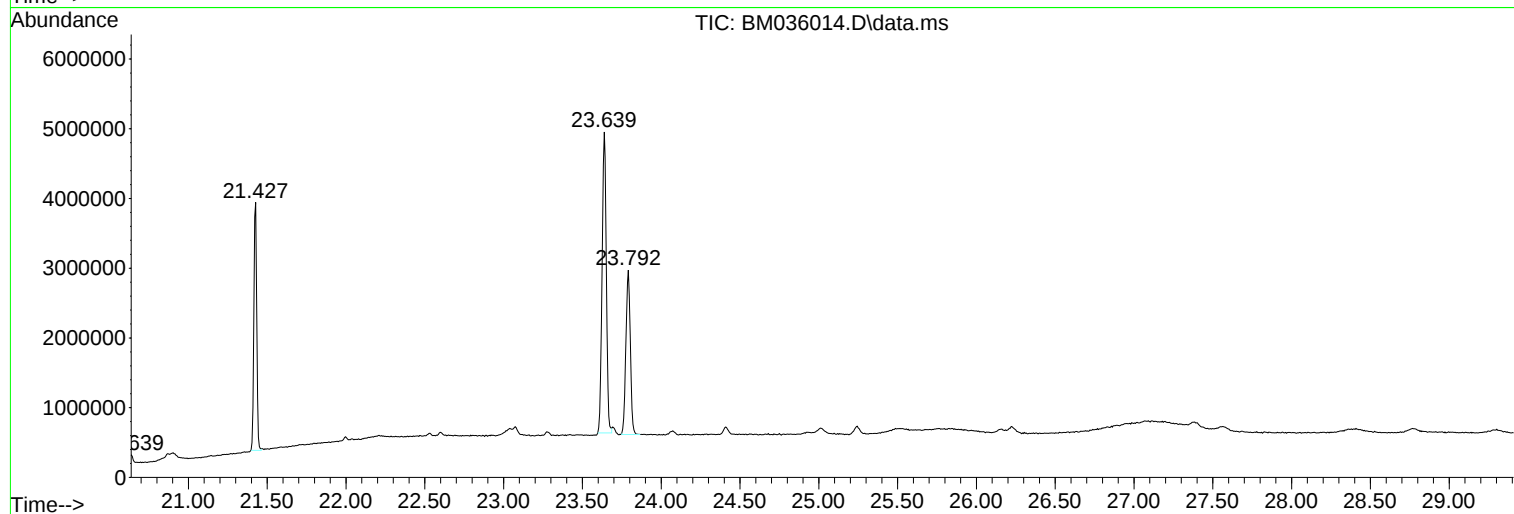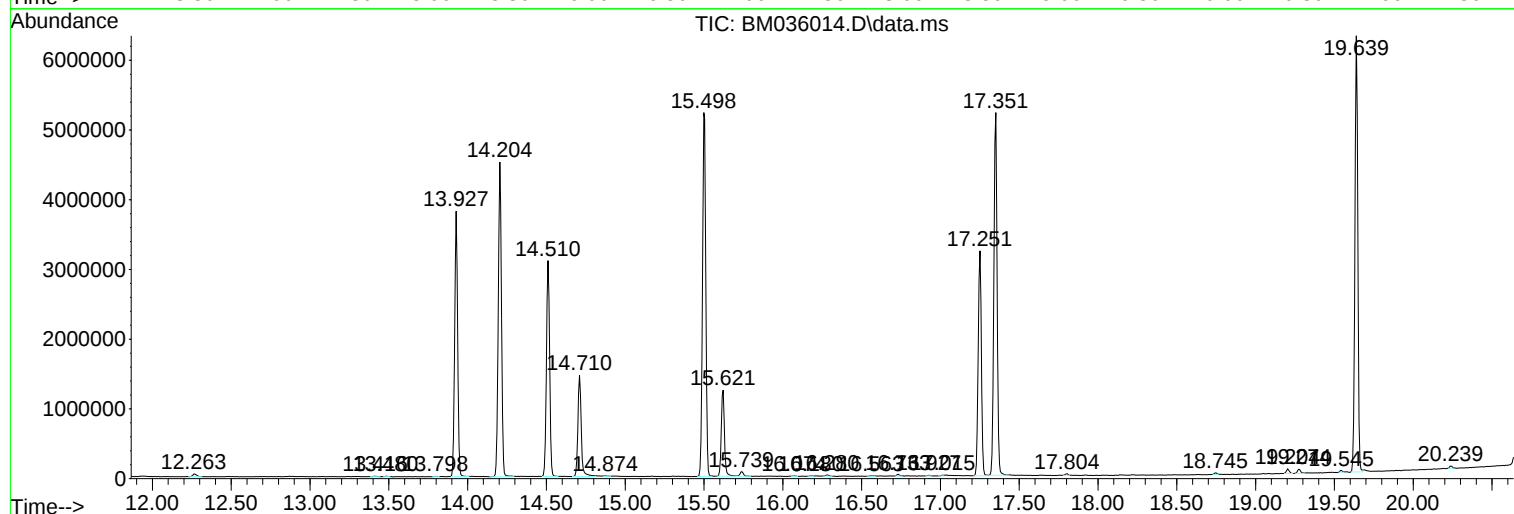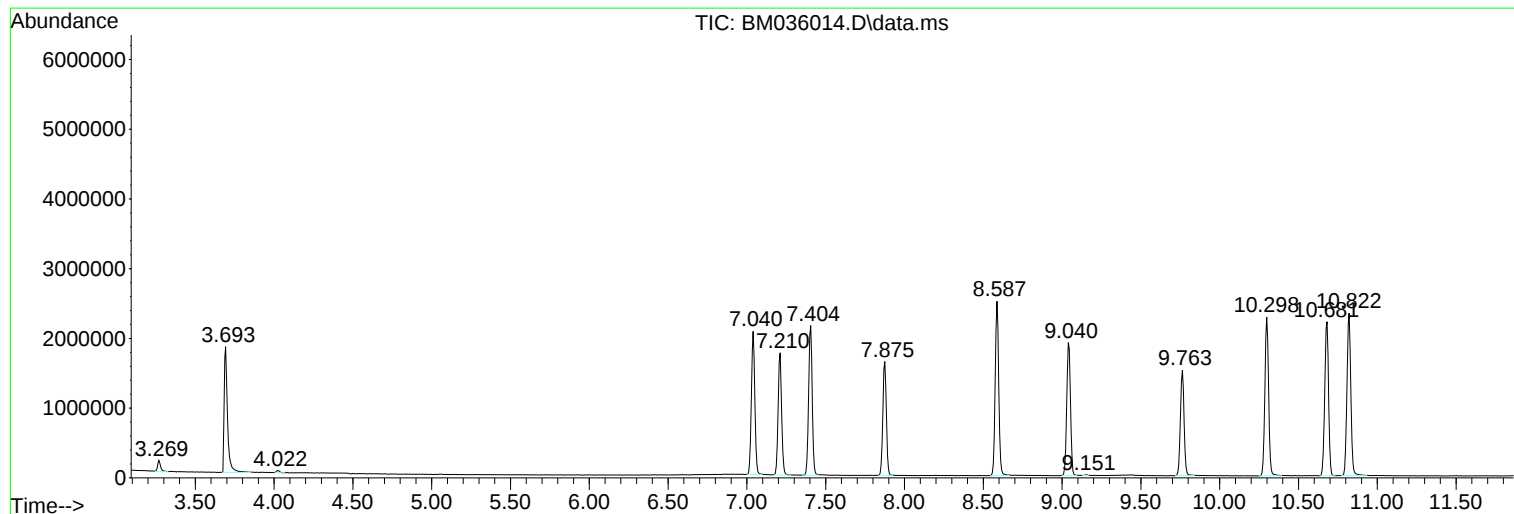

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036014.D
Acq On : 30 Jul 2022 04:49
Operator : CG/JU
Sample : PB146355BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK355

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036014.D
Acq On : 30 Jul 2022 04:49
Operator : CG/JU
Sample : PB146355BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK355

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc