

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036015.D
 Acq On : 30 Jul 2022 05:25
 Operator : CG/JU
 Sample : PB146356BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK356

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	38	rVB	126794	159166	2.21%	0.189%
2	3.687	99	102	119	rBV	1440782	2140230	29.76%	2.535%
3	4.022	155	159	165	rVB	30286	45058	0.63%	0.053%
4	7.040	665	672	690	rVB	1672702	2582482	35.91%	3.059%
5	7.210	695	701	711	rVB	1417152	2197175	30.55%	2.603%
6	7.404	727	734	746	rBV	1739385	2721592	37.84%	3.224%
7	7.875	807	814	821	rBV	1303635	2022241	28.12%	2.395%
8	8.587	928	935	950	rBV	2001286	3182751	44.26%	3.770%
9	9.039	1004	1012	1020	rBV	1578651	2517993	35.01%	2.983%
10	9.763	1127	1135	1147	rBV	1227907	1967057	27.35%	2.330%
11	10.298	1218	1226	1237	rBV	1893780	3081961	42.85%	3.651%
12	10.681	1283	1291	1300	rVB	1777593	2902645	40.36%	3.438%
13	10.822	1307	1315	1333	rBV	1922242	3297769	45.85%	3.906%
14	11.939	1503	1505	1510	rVB6	7450	10012	0.14%	0.012%
15	12.269	1556	1561	1570	rVB2	35465	61128	0.85%	0.072%
16	12.875	1658	1664	1667	rBV7	6776	13065	0.18%	0.015%
17	13.486	1764	1768	1772	rBV7	6860	9060	0.13%	0.011%
18	13.927	1834	1843	1856	rBV	3082184	4173975	58.04%	4.944%
19	14.204	1883	1890	1905	rBV	3781948	5296498	73.65%	6.274%
20	14.510	1935	1942	1949	rBV	2503181	3494423	48.59%	4.139%
21	14.710	1970	1976	1996	rBV	1219250	1860748	25.87%	2.204%
22	15.304	2073	2077	2086	rVB	6833	15911	0.22%	0.019%
23	15.498	2099	2110	2121	rBV	4387181	6396374	88.94%	7.577%
24	15.621	2124	2131	2142	rVV	1005429	1464356	20.36%	1.735%
25	15.739	2146	2151	2157	rVB	54254	82734	1.15%	0.098%
26	16.068	2203	2207	2212	rVB8	6637	10042	0.14%	0.012%
27	16.180	2220	2226	2227	rBV6	5621	7327	0.10%	0.009%
28	16.280	2240	2243	2249	rVB5	18820	24393	0.34%	0.029%
29	16.557	2285	2290	2294	rBV7	8124	17626	0.25%	0.021%
30	16.733	2315	2320	2325	rBV3	21585	32196	0.45%	0.038%
31	16.927	2349	2353	2357	rBV5	9570	13464	0.19%	0.016%
32	17.015	2364	2368	2369	rBV4	10796	13113	0.18%	0.016%
33	17.251	2401	2408	2415	rBV	2714299	3731650	51.89%	4.420%
34	17.351	2418	2425	2438	rVV	4691794	6466971	89.92%	7.660%
35	17.633	2471	2473	2480	rVB7	4671	10137	0.14%	0.012%
36	17.804	2498	2502	2506	rBV2	19916	27401	0.38%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036015.D
Acq On : 30 Jul 2022 05:25
Operator : CG/JU
Sample : PB146356BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK356

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

37	18.745	2659	2662	2668	rBV3	19164	25454	0.35%	0.030%
38	19.204	2736	2740	2747	rVB2	51979	69832	0.97%	0.083%
39	19.274	2748	2752	2756	rBV	55066	70719	0.98%	0.084%
40	19.545	2795	2798	2801	rBV5	18163	19747	0.27%	0.023%
41	19.639	2808	2814	2821	rBV	5557897	7191757	100.00%	8.519%
42	20.639	2981	2984	2988	rVB2	90494	100475	1.40%	0.119%
43	21.421	3112	3117	3126	rBV	3080035	3943554	54.83%	4.671%
44	23.639	3487	3494	3500	rBV2	3779224	7047781	98.00%	8.348%
45	23.791	3513	3520	3528	rVB2	1939590	3900004	54.23%	4.620%




Sum of corrected areas: 84420047

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036015.D
Acq On : 30 Jul 2022 05:25
Operator : CG/JU
Sample : PB146356BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK356

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

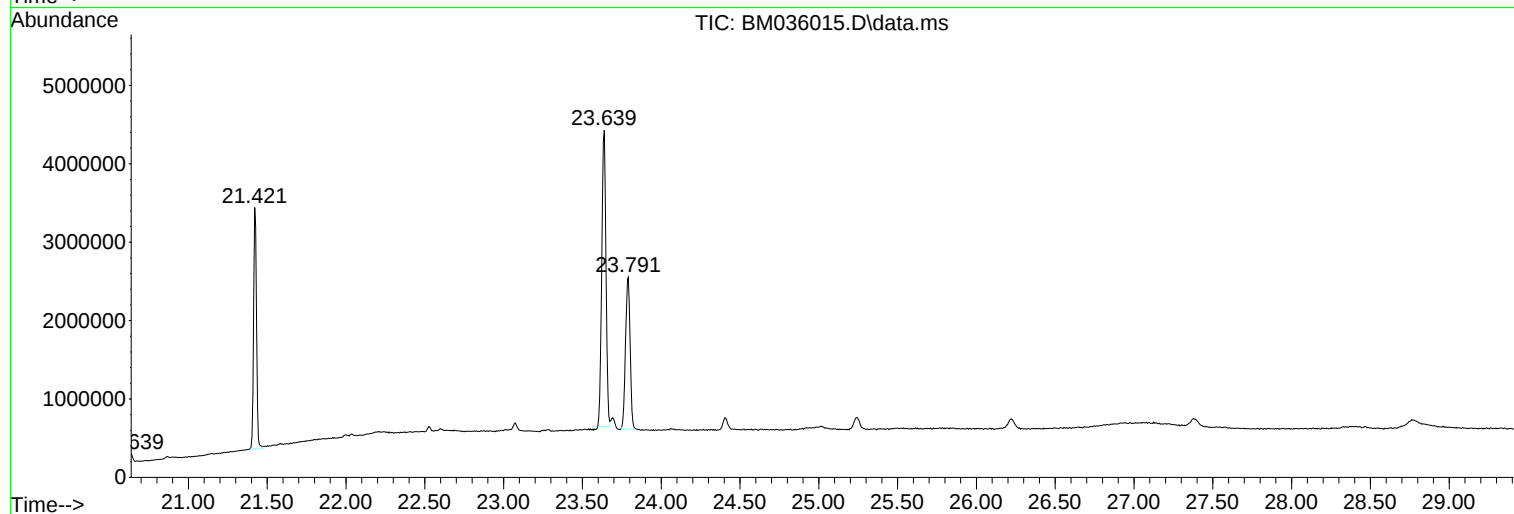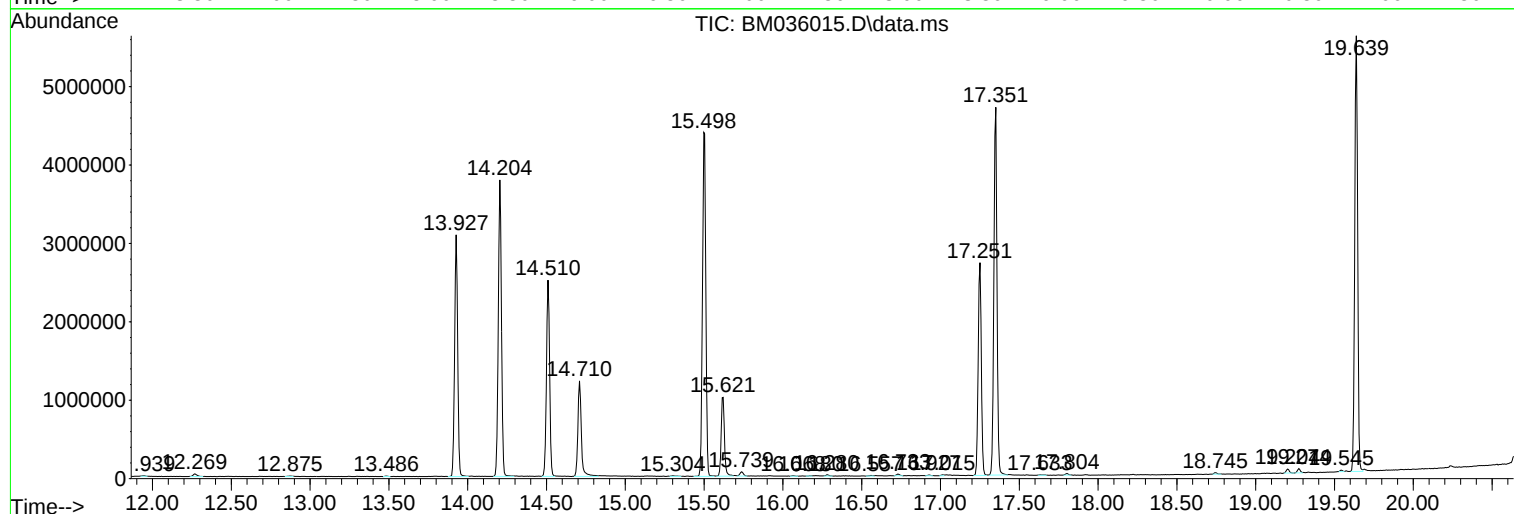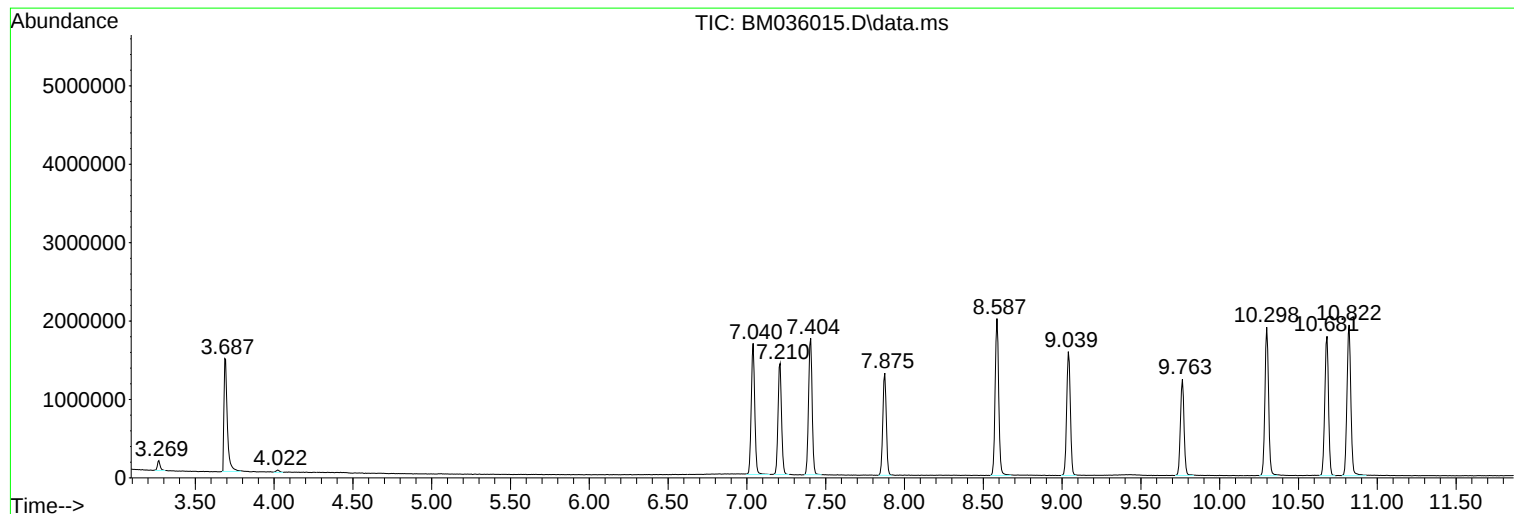

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036015.D
Acq On : 30 Jul 2022 05:25
Operator : CG/JU
Sample : PB146356BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK356

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036015.D
Acq On : 30 Jul 2022 05:25
Operator : CG/JU
Sample : PB146356BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK356

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc