

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036023.D
 Acq On : 30 Jul 2022 10:14
 Operator : CG/JU
 Sample : N3792-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	41	rVB	98114	124355	1.45%	0.158%
2	3.557	78	80	86	rBV	16888	24973	0.29%	0.032%
3	3.699	100	104	119	rBV	268733	407285	4.76%	0.519%
4	3.928	139	143	148	rVB	39987	61012	0.71%	0.078%
5	4.022	156	159	165	rVB	24726	30418	0.36%	0.039%
6	4.963	315	319	322	rVB5	7112	9698	0.11%	0.012%
7	5.563	417	421	427	rVB	9689	13707	0.16%	0.017%
8	7.034	665	671	684	rVB	361410	588503	6.88%	0.750%
9	7.204	693	700	708	rBV	1444104	2198910	25.70%	2.801%
10	7.398	727	733	745	rBV	1333441	2107839	24.63%	2.685%
11	7.492	745	749	751	rVV5	7083	8813	0.10%	0.011%
12	7.869	803	813	822	rBV	1170610	1845645	21.57%	2.351%
13	8.581	926	934	948	rBV	992819	1642093	19.19%	2.092%
14	9.039	1004	1012	1022	rBV	1595481	2553615	29.84%	3.253%
15	9.151	1026	1031	1035	rVV3	13466	24343	0.28%	0.031%
16	9.198	1035	1039	1047	rVB8	13559	26599	0.31%	0.034%
17	9.439	1078	1080	1087	rVB8	10384	18913	0.22%	0.024%
18	9.757	1127	1134	1145	rBV	1132952	1868122	21.83%	2.380%
19	10.298	1218	1226	1238	rBV	1674994	2805297	32.78%	3.574%
20	10.675	1282	1290	1298	rBV	1601723	2599519	30.38%	3.311%
21	10.816	1304	1314	1330	rBV	1027852	1812703	21.18%	2.309%
22	11.474	1422	1426	1430	rBV6	9249	16784	0.20%	0.021%
23	11.939	1500	1505	1507	rBV6	7683	10780	0.13%	0.014%
24	12.263	1555	1560	1567	rBV2	31343	51878	0.61%	0.066%
25	12.880	1659	1665	1672	rVB7	11723	25101	0.29%	0.032%
26	13.127	1702	1707	1710	rVB5	10893	13675	0.16%	0.017%
27	13.416	1751	1756	1760	rBV6	8056	16516	0.19%	0.021%
28	13.486	1764	1768	1771	rBV6	7483	11052	0.13%	0.014%
29	13.927	1836	1843	1853	rBV	3033720	4232048	49.46%	5.391%
30	14.204	1878	1890	1903	rBV	3731147	5275097	61.65%	6.720%
31	14.404	1922	1924	1928	rVB5	9053	10851	0.13%	0.014%
32	14.510	1934	1942	1949	rBV	2197006	3134275	36.63%	3.993%
33	14.710	1969	1976	1989	rBV	223576	406988	4.76%	0.518%
34	14.862	2000	2002	2008	rVB6	9221	14077	0.16%	0.018%
35	14.927	2008	2013	2016	rBV6	9029	11619	0.14%	0.015%
36	15.304	2073	2077	2080	rBV4	12859	23052	0.27%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
 Data File : BM036023.D
 Acq On : 30 Jul 2022 10:14
 Operator : CG/JU
 Sample : N3792-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUM7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.498	2101	2110	2123	rBV	4876048	6617928	77.34%	8.430%
38	15.615	2123	2130	2142	rVV	1268885	1761428	20.59%	2.244%
39	15.739	2146	2151	2156	rVB	54484	85344	1.00%	0.109%
40	15.868	2170	2173	2178	rVB6	8465	11423	0.13%	0.015%
41	16.057	2201	2205	2213	rVB10	7534	16722	0.20%	0.021%
42	16.180	2221	2226	2229	rBV7	10467	21602	0.25%	0.028%
43	16.221	2229	2233	2239	rVV6	14817	28255	0.33%	0.036%
44	16.280	2239	2243	2250	rVB5	23547	36152	0.42%	0.046%
45	16.392	2258	2262	2266	rVB5	5804	8568	0.10%	0.011%
46	16.562	2287	2291	2293	rBV5	8232	9503	0.11%	0.012%
47	16.727	2315	2319	2323	rBV3	26783	33985	0.40%	0.043%
48	16.927	2350	2353	2357	rVB6	12119	16672	0.19%	0.021%
49	17.009	2364	2367	2370	rBV3	14740	17316	0.20%	0.022%
50	17.168	2392	2394	2398	rVB4	9450	10591	0.12%	0.013%
51	17.251	2401	2408	2414	rVV	2263892	3264228	38.15%	4.158%
52	17.345	2418	2424	2435	rVV	5126316	7357899	85.99%	9.373%
53	17.621	2467	2471	2472	rBV4	8854	11306	0.13%	0.014%
54	17.745	2489	2492	2495	rBV5	8726	11569	0.14%	0.015%
55	17.798	2497	2501	2506	rVB	20435	30826	0.36%	0.039%
56	17.921	2519	2522	2527	rVB6	15629	18987	0.22%	0.024%
57	18.145	2555	2560	2566	rBV	112540	157837	1.84%	0.201%
58	18.221	2570	2573	2577	rVB	23062	30254	0.35%	0.039%
59	18.474	2614	2616	2621	rVB5	11669	15579	0.18%	0.020%
60	18.633	2639	2643	2650	rBV9	13790	22530	0.26%	0.029%
61	18.745	2659	2662	2667	rVB	20315	25158	0.29%	0.032%
62	19.203	2736	2740	2745	rVB	64293	85173	1.00%	0.108%
63	19.274	2748	2752	2755	rBV	61804	78271	0.91%	0.100%
64	19.333	2760	2762	2766	rVB4	15092	16313	0.19%	0.021%
65	19.421	2774	2777	2782	rBV7	21647	26633	0.31%	0.034%
66	19.639	2808	2814	2820	rBV	6571233	8440707	98.64%	10.752%
67	19.868	2850	2853	2858	rVB	79287	95866	1.12%	0.122%
68	20.639	2981	2984	2988	rBV	96765	96878	1.13%	0.123%
69	21.144	3066	3070	3078	rBV2	411177	584004	6.83%	0.744%
70	21.427	3113	3118	3127	rBV	2636823	3386133	39.57%	4.313%
71	23.638	3487	3494	3501	rBV2	4505018	8556723	100.00%	10.900%
72	23.791	3513	3520	3531	rVB2	1757994	3486642	40.75%	4.442%



Sum of corrected areas: 78501160

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036023.D
Acq On : 30 Jul 2022 10:14
Operator : CG/JU
Sample : N3792-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUM7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

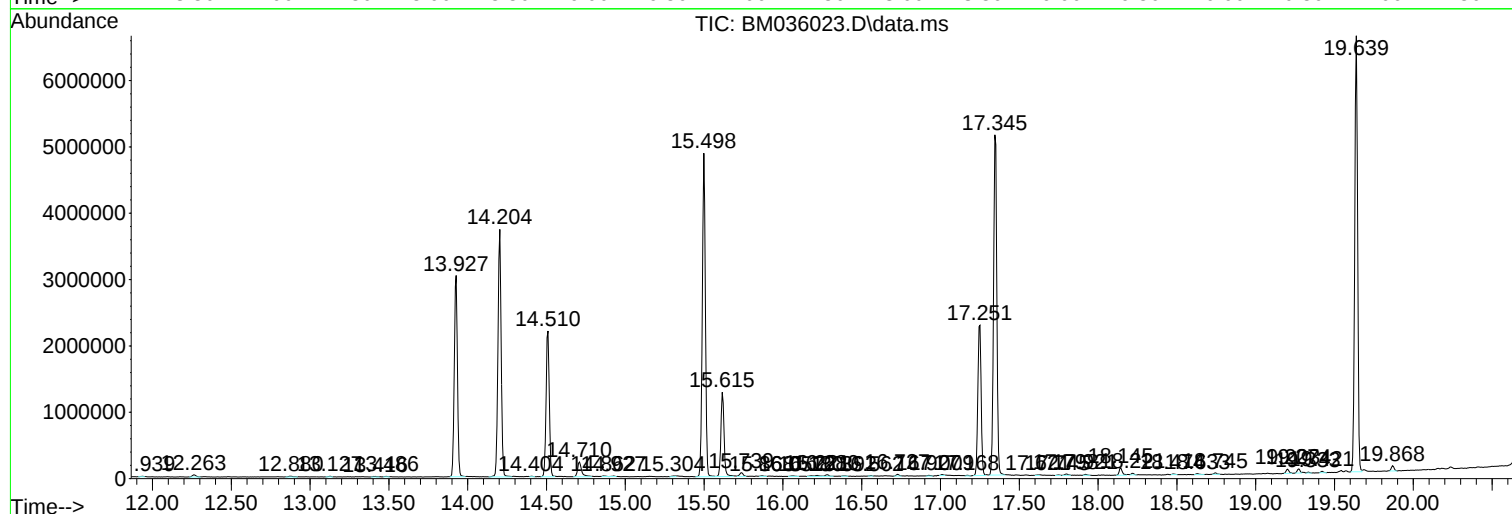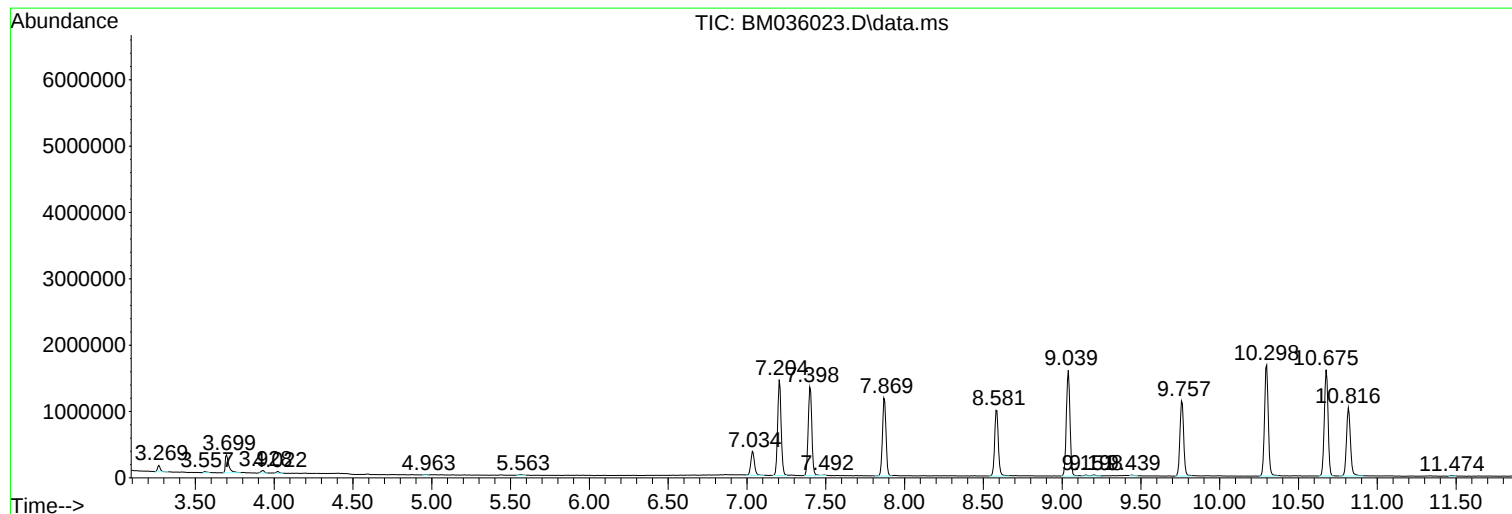

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036023.D
Acq On : 30 Jul 2022 10:14
Operator : CG/JU
Sample : N3792-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUM7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.144	3.45 ng/ul	584004	Chrysene-d12	21.427

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
2			1-Heneicosyl formate	340	C22H44O2	077899-03-7	94
3			Octacosanol	410	C28H58O	000557-61-9	91
4			Cyclotetracosane	336	C24H48	000297-03-0	91
5			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	91

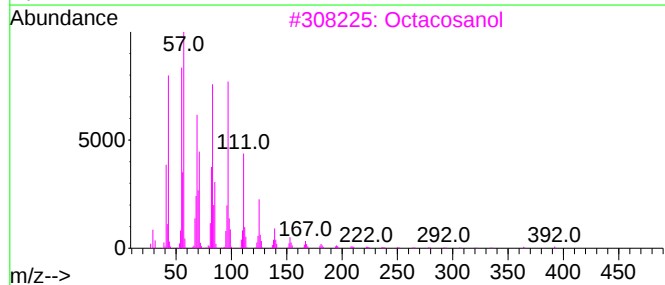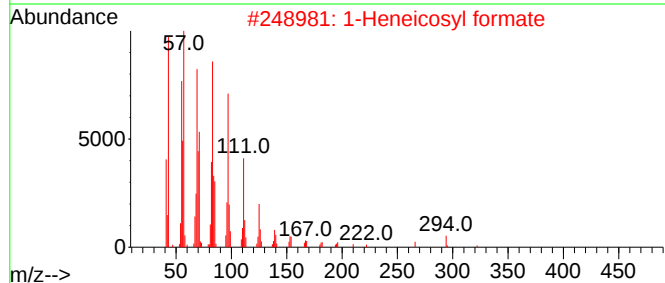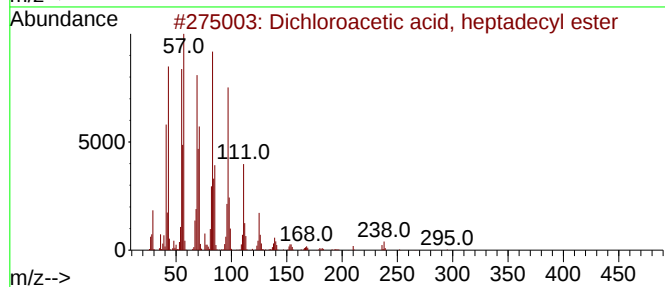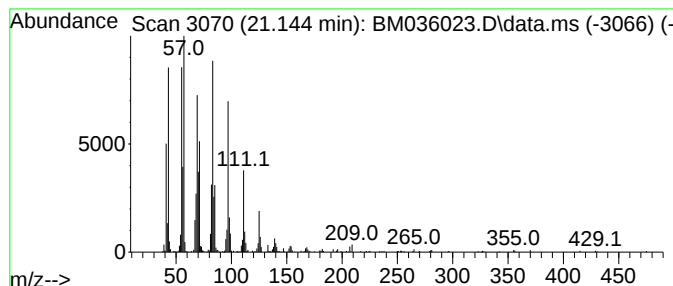

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072922\
Data File : BM036023.D
Acq On : 30 Jul 2022 10:14
Operator : CG/JU
Sample : N3792-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUM7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	21.144	3.5	ng/ul	584004	5	21.427	3386130	20.0