

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
 Data File : BM006772.D
 Acq On : 30 Jul 2016 14:19
 Operator : UM/SJ
 Sample : H4190-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9ZN6

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:04:58 PM

Quant Time: Aug 01 04:25:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

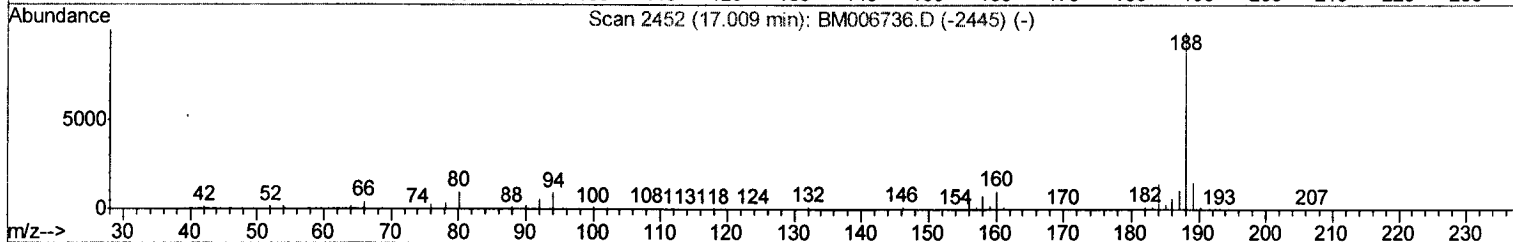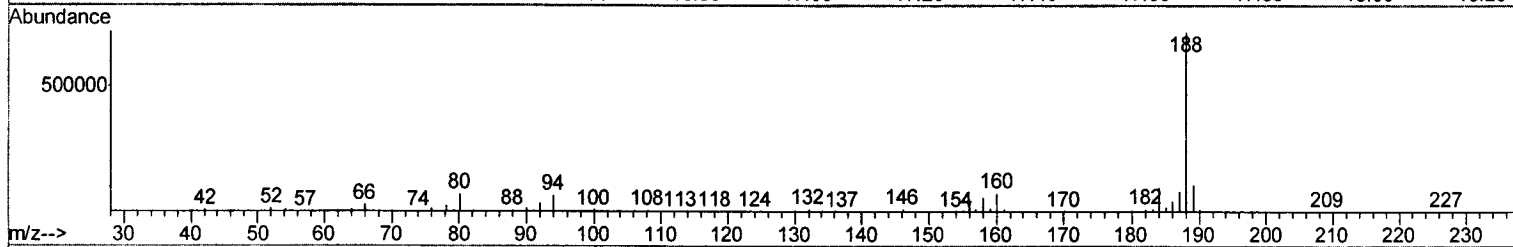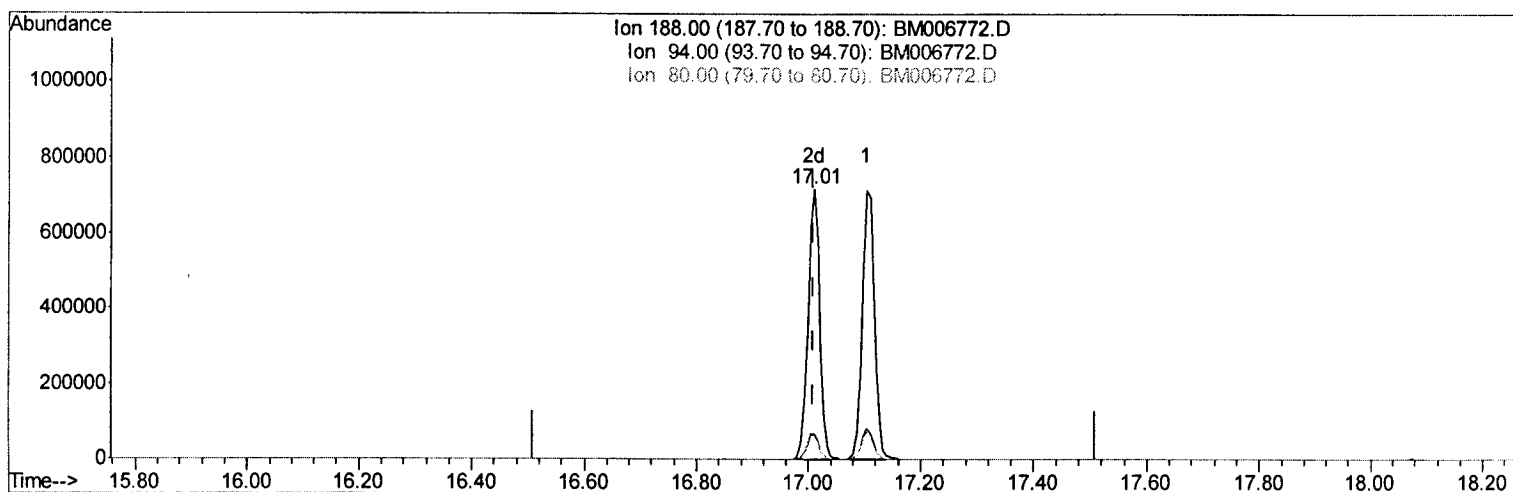

TIC: BM006772.D

(23) Phenanthrene-d10 (I)

17.010min (+0.000) 20.00ng/ul m U, M
 response 1030937 08/02/16

Ion	Exp%	Act%
188.00	100	100
94.00	9.60	9.10
80.00	12.20	9.70#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
 Data File : BM006772.D
 Acq On : 30 Jul 2016 14:19
 Operator : UM/SJ
 Sample : H4190-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampled :
 D9ZN6

Quant Time: Aug 01 04:25:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
 8/1/2016 7:04:58 PM

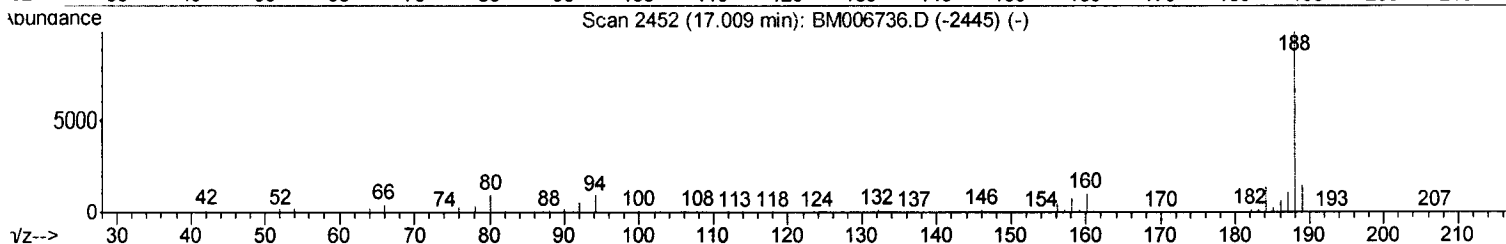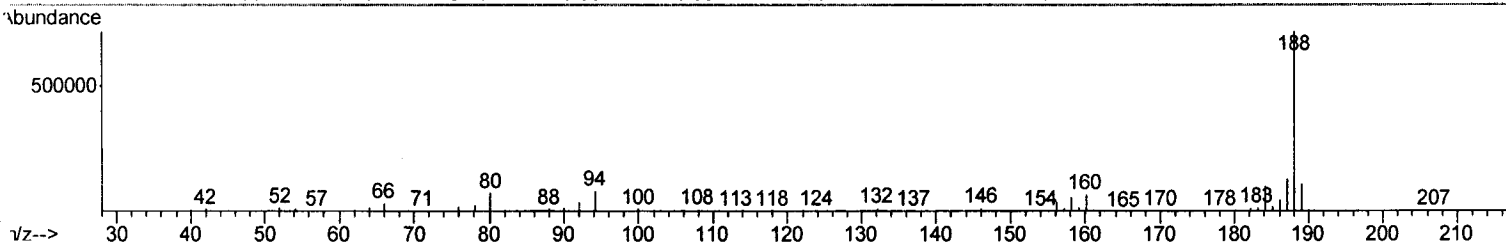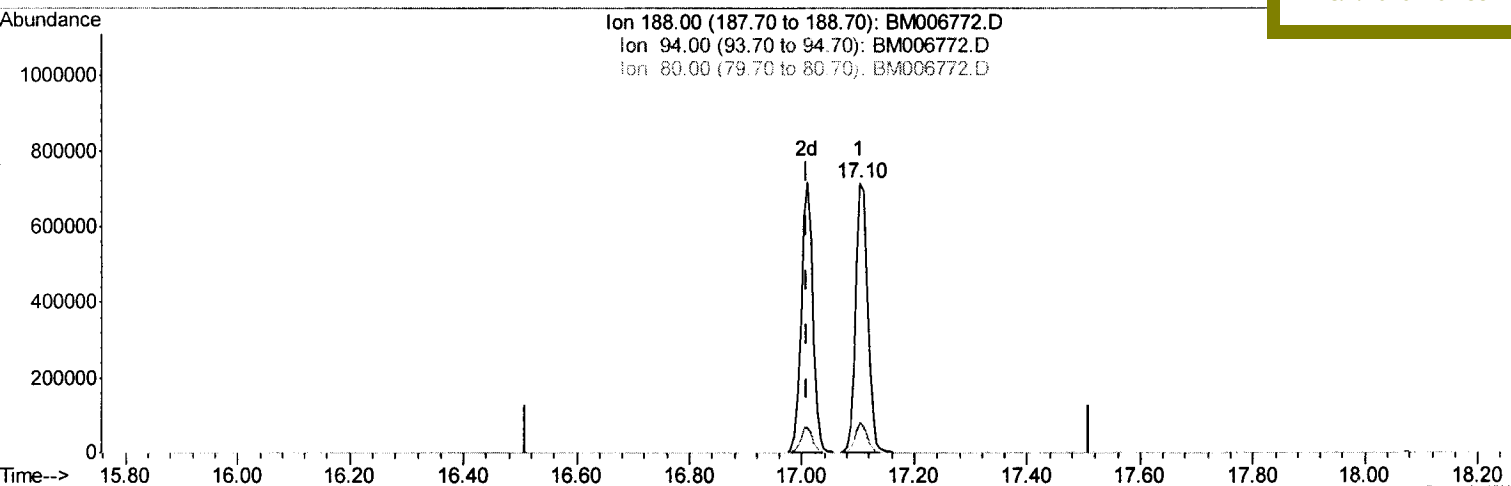

TIC: BM006772.D

(23) Phenanthrene-d10 (I)

17.104min (+0.094) 20.00ng/ul

response 1079010

Ion	Exp%	Act%
188.00	100	100
94.00	9.60	11.21
80.00	12.20	10.06
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
 Data File : BM006772.D
 Acq On : 30 Jul 2016 14:19
 Operator : UM/SJ
 Sample : H4190-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 D9ZN6

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:04:58 PM

Quant Time: Aug 01 05:49:45 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

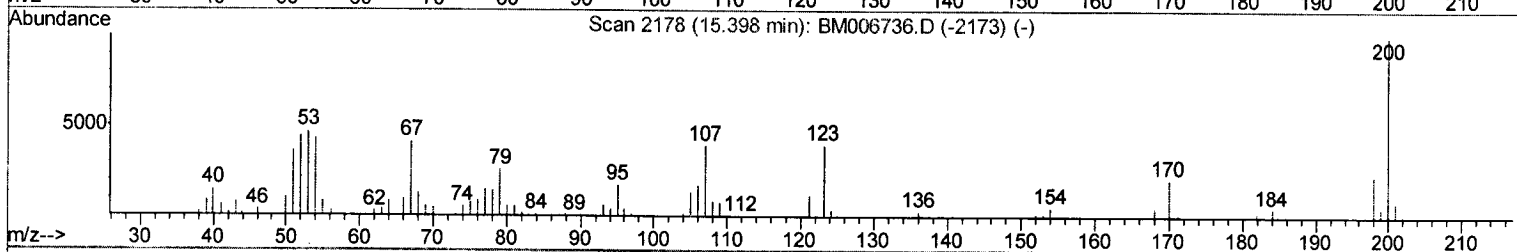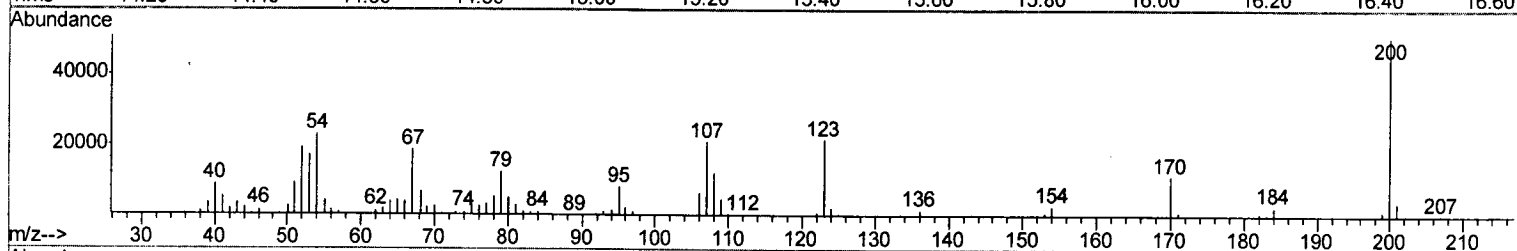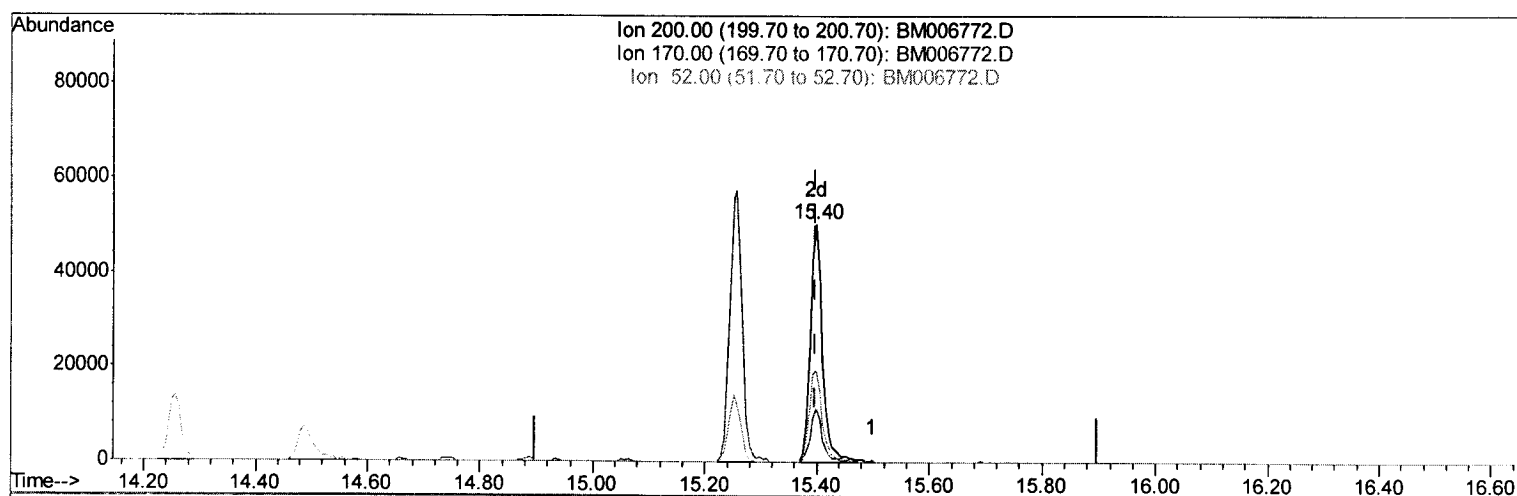

TIC: BM006772.D

(24) 4,6-Dinitro-2-methylphenol-d2 (S)

15.398min (+0.000) 14.22ng/ul m

response 76083

Ion	Exp%	Act%
200.00	100	100
170.00	22.30	22.18
52.00	53.20	38.38#
0.00	0.00	0.00

UM
 08/02/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
 Data File : BM006772.D
 Acq On : 30 Jul 2016 14:19
 Operator : UM/SJ
 Sample : H4190-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 D9ZN6

Quant Time: Aug 01 05:49:45 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
 8/1/2016 7:04:58 PM

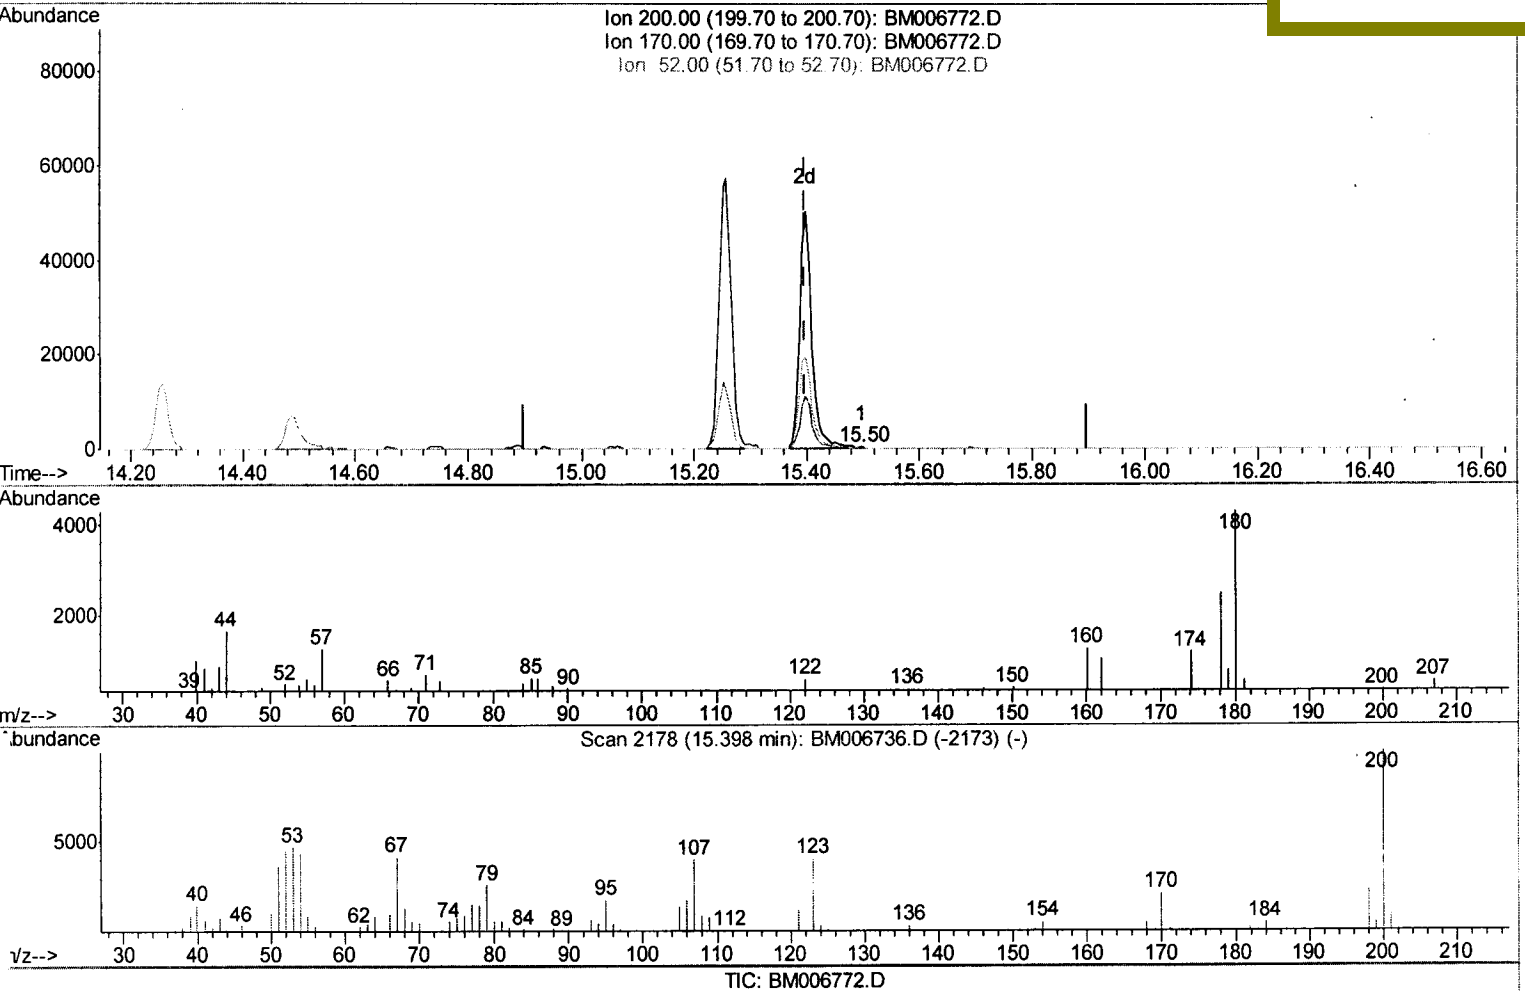

(24) 4,6-Dinitro-2-methylphenol-d2 (S)

15.498min (+0.100) 0.02ng/ul

response 112

Ion	Exp%	Act%
200.00	100	100
170.00	22.30	0.00#
52.00	53.20	143.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
 Data File : BM006772.D
 Acq On : 30 Jul 2016 14:19
 Operator : UM/SJ
 Sample : H4190-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 D9ZN6

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:04:58 PM

Quant Time: Aug 01 05:49:45 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

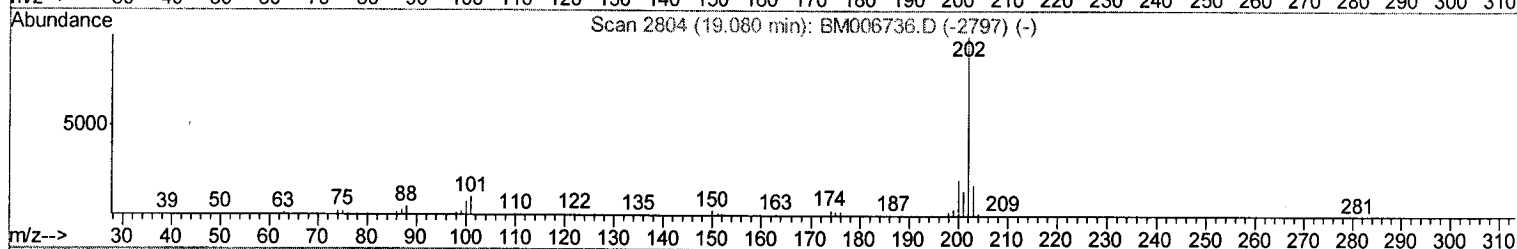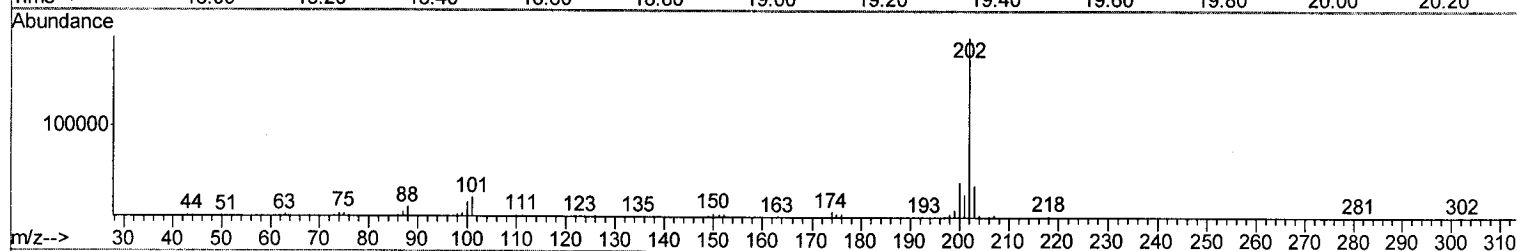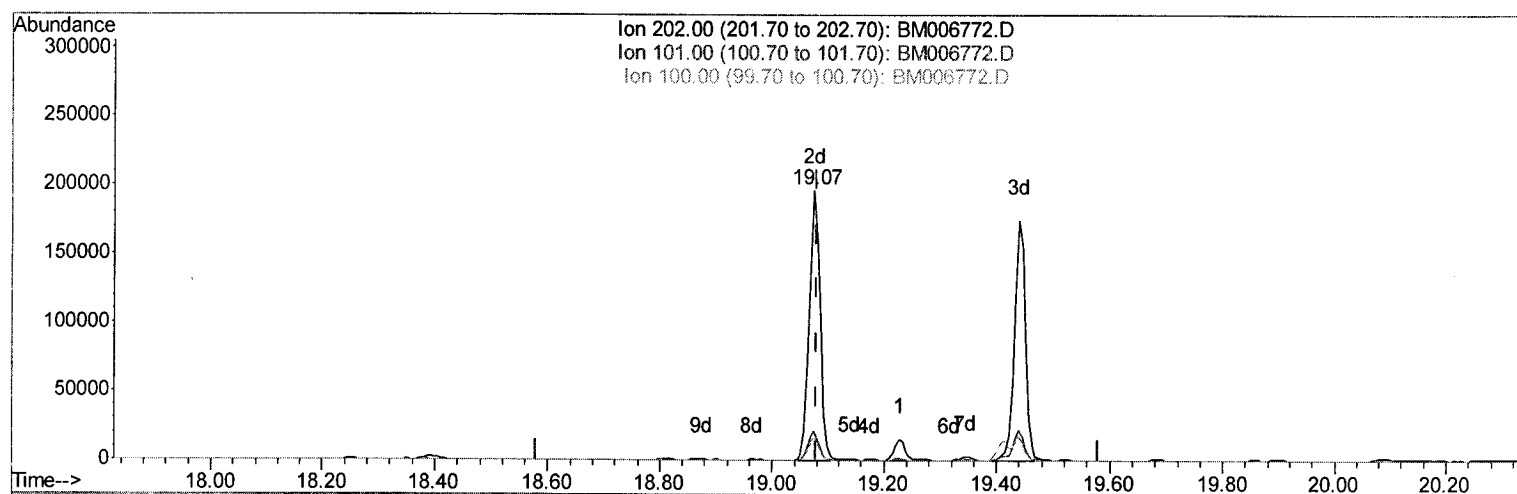

TIC: BM006772.D

(28) Fluoranthene (C)

19.074min (-0.006) 3.89ng/ul m

response 264960

Ion	Exp%	Act%
202.00	100	100
101.00	11.10	10.83
100.00	8.70	8.22
0.00	0.00	0.00

U.M
 08/02/16



Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
Data File : BM006772.D
Acq On : 30 Jul 2016 14:19
Operator : UM/SJ
Sample : H4190-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9ZN6

Quant Time: Aug 01 05:49:45 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 30 01:37:26 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
8/1/2016 7:04:58 PM

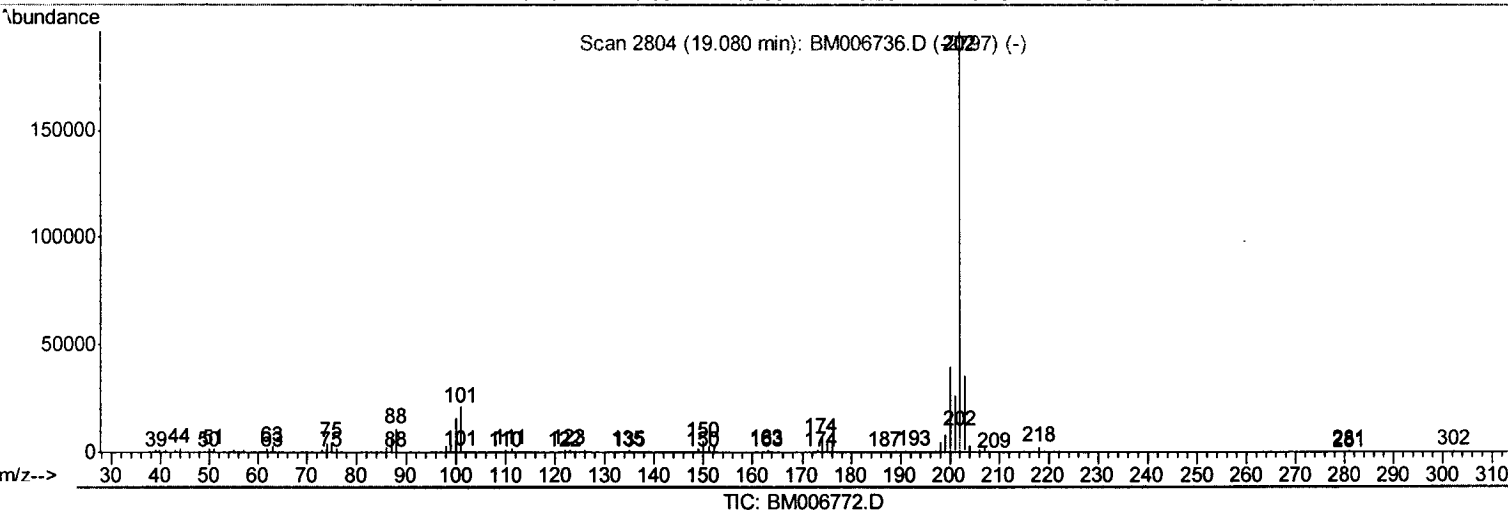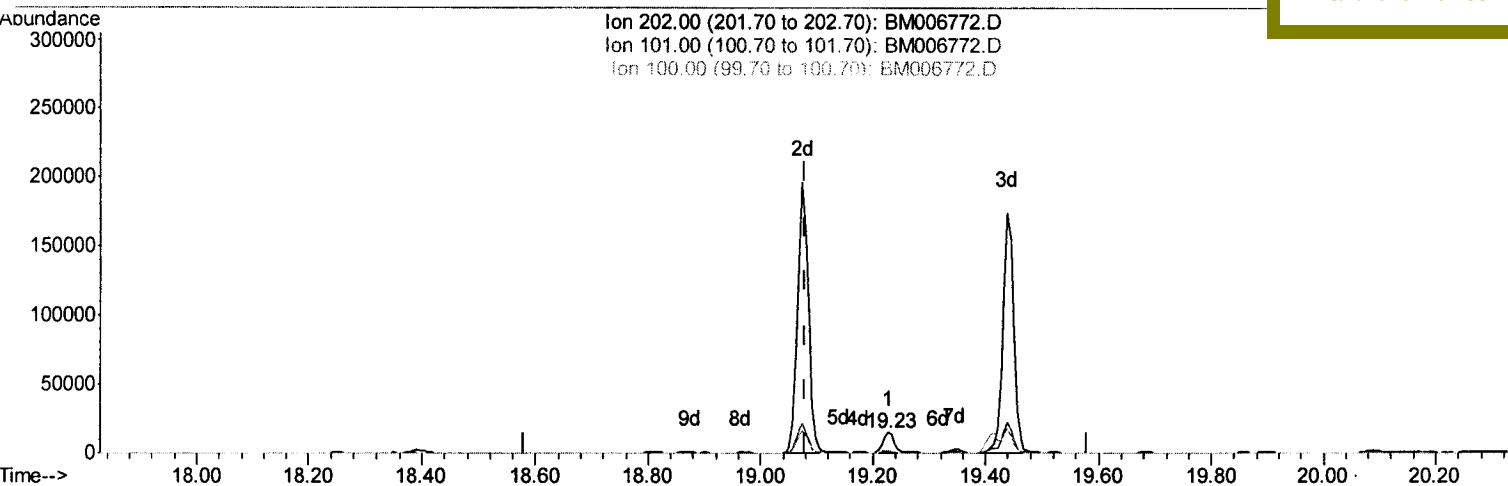

(28) Fluoranthene (C)

19.227min (+0.147) 0.29ng/ul

response 19529

Ion	Exp%	Act%
202.00	100	100
101.00	11.10	10.54
100.00	8.70	9.06
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
 Data File : BM006772.D
 Acq On : 30 Jul 2016 14:19
 Operator : UM/SJ
 Sample : H4190-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 D9ZN6

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:04:58 PM

Quant Time: Aug 01 05:49:45 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

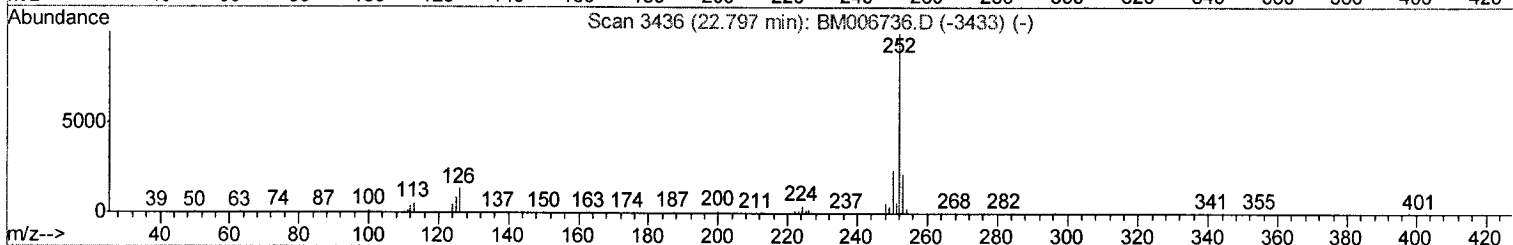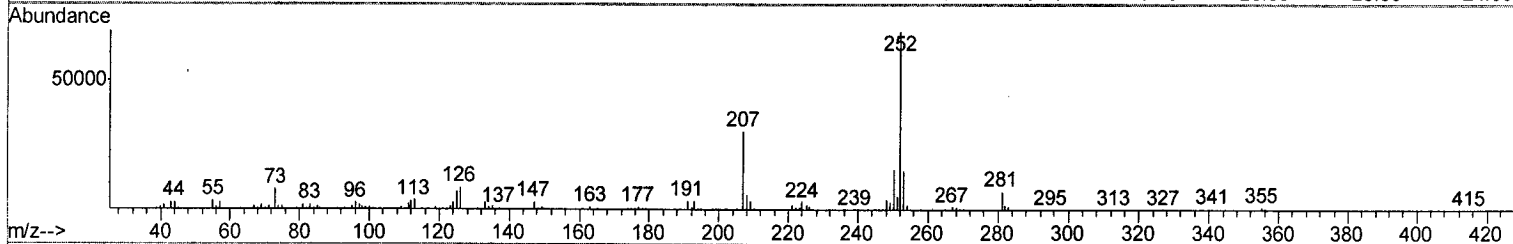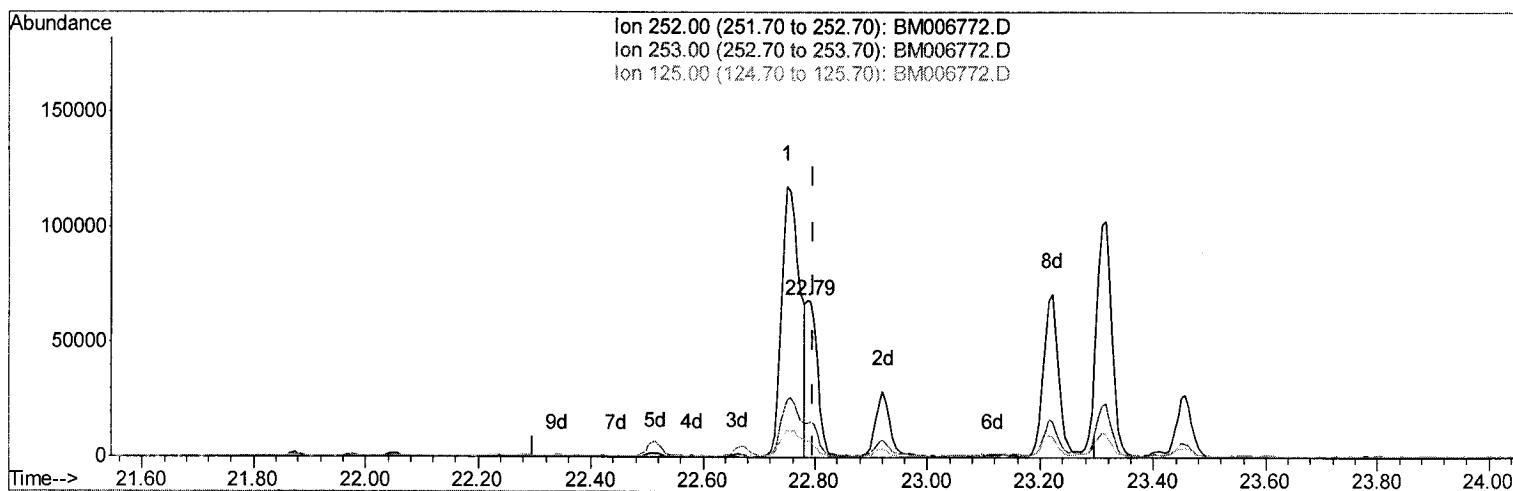

TIC: BM006772.D

(36) Benzo(k)fluoranthene

22.786min (-0.012) 1.38ng/ul m

response 96611

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	22.21
125.00	9.60	10.54
0.00	0.00	0.00

U.M
 08/02/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
 Data File : BM006772.D
 Acq On : 30 Jul 2016 14:19
 Operator : UM/SJ
 Sample : H4190-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 D9ZN6

Quant Time: Aug 01 05:49:45 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
 8/1/2016 7:04:58 PM

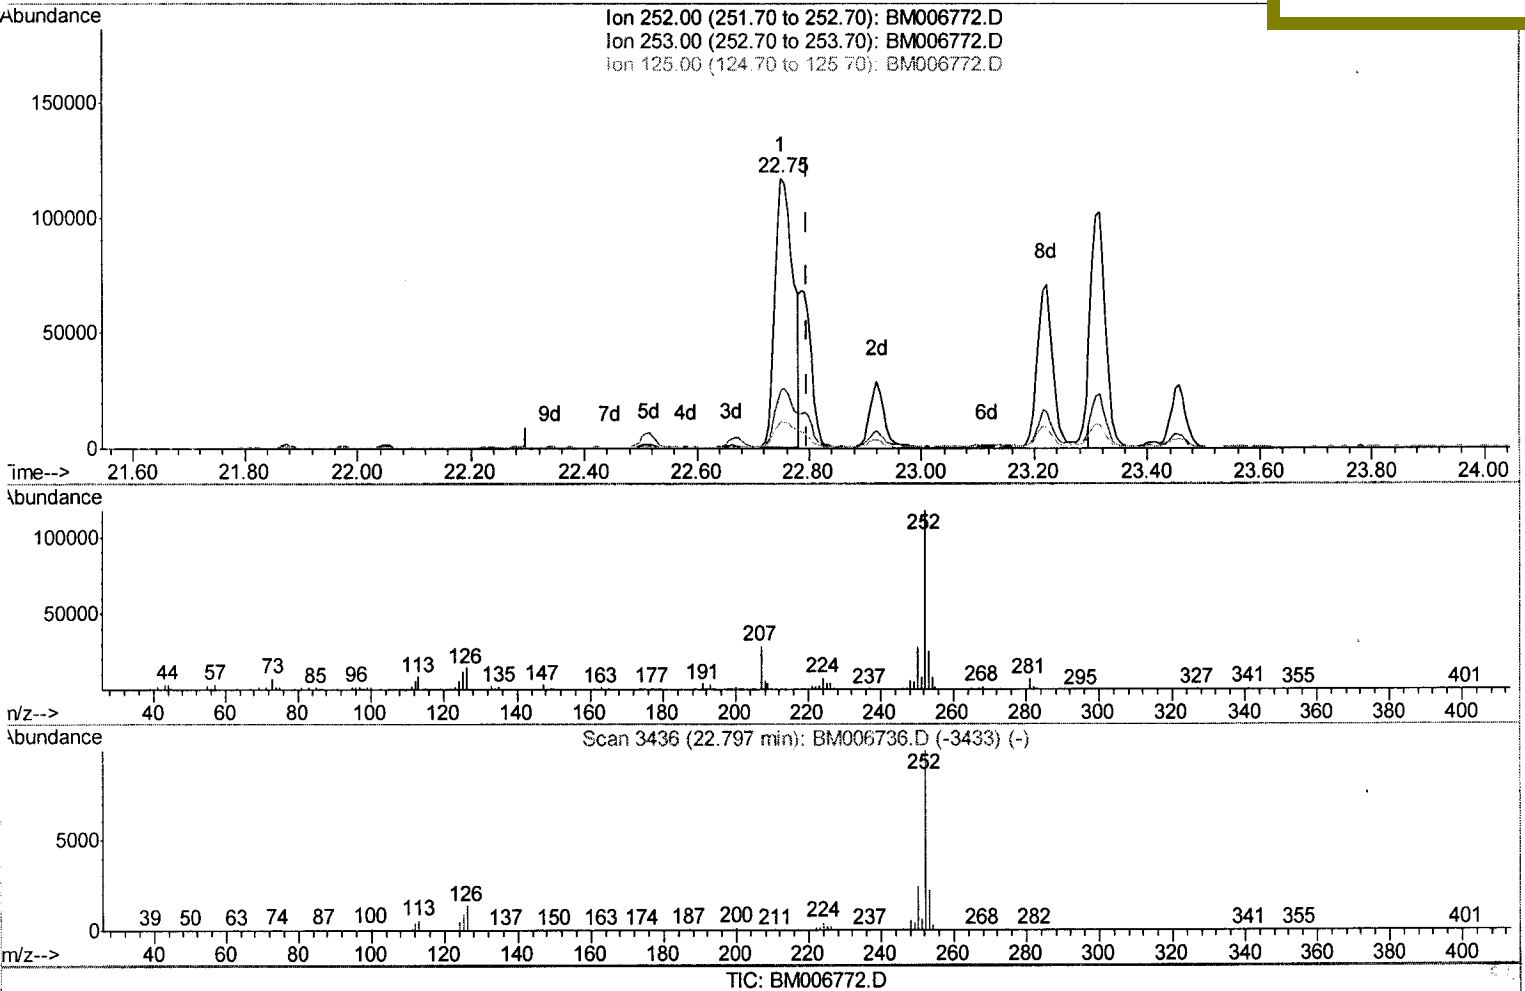

(36) Benzo(k)fluoranthene

22.750min (-0.047) 3.78ng/ul

response 265548

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	21.22
125.00	9.60	10.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
 Data File : BM006772.D
 Acq On : 30 Jul 2016 14:19
 Operator : UM/SJ
 Sample : H4190-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9ZN6

Quant Time: Aug 01 08:31:40 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:04:58 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	181891	20.00	ng/ul	0.00
7) Naphthalene-d8	10.38	136	812498	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.26	164	462819	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.01	188	1030937m	20.00	ng/ul	0.00
29) Chrysene-d12	21.21	240	1176737	20.00	ng/ul	0.00
34) Perylene-d12	23.41	264	1212017	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.13	96	8277	1.84	ng/uL	0.00
3) Phenol-d5	6.79	99	320685	20.72	ng/ul	0.00
4) Bis-(2-Chloroethyl) ether-d	6.95	67	218774	22.82	ng/ul	0.00
5) 2-Chlorophenol-d4	7.14	132	255525	20.67	ng/ul	0.00
6) 4-Methylphenol-d8	8.32	113	212714	17.72	ng/ul	0.00
8) Nitrobenzene-d5	8.76	128	131130	21.32	ng/ul	0.00
9) 2-Nitrophenol-d4	9.47	143	143481	21.94	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.01	165	250980	20.31	ng/ul	0.00
12) 4-Chloroaniline-d4	10.53	131	309824	22.76	ng/ul	0.00
16) Dimethylphthalate-d6	13.67	166	804920	22.18	ng/ul	0.00
17) Acenaphthylene-d8	13.95	160	1026138	22.15	ng/ul	0.00
20) 4-Nitrophenol-d4	14.49	143	92965	14.75	ng/ul	0.00
21) Fluorene-d10	15.26	176	714183	22.01	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.40	200	76083m	14.22	ng/ul	0.00
26) Anthracene-d10	17.10	188	1079010	22.04	ng/ul	0.00
30) Pyrene-d10	19.41	212	1242342	23.17	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.27	264	1238507	22.22	ng/ul	-0.01

Target Compounds

						Qvalue
28) Fluoranthene	19.07	202	264960m	3.89	ng/ul	
31) Pyrene	19.44	202	235592	3.31	ng/ul	97
32) Benzo(a)anthracene	21.19	228	189614	2.66	ng/ul	98
33) Chrysene	21.24	228	171656	2.61	ng/ul	98
35) Benzo(b)fluoranthene	22.75	252	265548	3.65	ng/ul	97
36) Benzo(k)fluoranthene	22.79	252	96611m	1.38	ng/ul	
38) Benzo(a)pyrene	23.32	252	192169	2.72	ng/ul	98
39) Indeno(1,2,3-cd)pyrene	25.60	276	141475	1.73	ng/ul	99
41) Benzo(g,h,i)perylene	26.29	276	130341	1.86	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM073016\
 Data File : BM006772.D
 Acq On : 30 Jul 2016 14:19
 Operator : UM/SJ
 Sample : H4190-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 D9ZN6

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:04:58 PM

Quant Time: Aug 01 08:31:40 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

