

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM073016\
 Data File : BM006760.D
 Acq On : 30 Jul 2016 06:21
 Operator : UM/SJ
 Sample : H4188-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9ZL1

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:04:30 PM

Quant Time: Aug 01 04:53:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	154703	20.00	ng/ul	0.00
7) Naphthalene-d8	10.38	136	664113	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.26	164	380469	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.01	188	871549	20.00	ng/ul	0.00
29) Chrysene-d12	21.21	240	1053203	20.00	ng/ul	0.00
34) Perylene-d12	23.41	264	1098696	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.13	96	4889	1.28	ng/uL	0.00
3) Phenol-d5	6.79	99	173091	13.15	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	6.95	67	120340	14.76	ng/ul	0.00
5) 2-Chlorophenol-d4	7.14	132	141294	13.44	ng/ul	0.00
6) 4-Methylphenol-d8	8.32	113	127540	12.49	ng/ul	0.00
8) Nitrobenzene-d5	8.76	128	68966	13.72	ng/ul	0.00
9) 2-Nitrophenol-d4	9.47	143	77251	14.45	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.02	165	137513	13.61	ng/ul	0.00
12) 4-Chloroaniline-d4	10.53	131	176059	15.82	ng/ul	0.00
16) Dimethylphthalate-d6	13.67	166	463698	15.54	ng/ul	0.00
17) Acenaphthylene-d8	13.95	160	567568	14.91	ng/ul	0.00
20) 4-Nitrophenol-d4	14.49	143	53431	10.31	ng/ul	0.00
21) Fluorene-d10	15.26	176	414217	15.53	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.40	200	48599	10.74	ng/ul	0.00
26) Anthracene-d10	17.11	188	639363m	15.45	ng/ul	0.00
30) Pyrene-d10	19.41	212	751922	15.67	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.27	264	786372	15.56	ng/ul	-0.01

Target Compounds

					Qvalue
25) Phenanthrene	17.05	178	72919	1.49 ng/ul	99
27) Anthracene	17.05	178	72919	1.44 ng/ul	97
28) Fluoranthene	19.07	202	162475	2.82 ng/ul	99
31) Pyrene	19.44	202	147927	2.32 ng/ul	98
32) Benzo(a)anthracene	21.19	228	114323	1.79 ng/ul	98
33) Chrysene	21.24	228	132930	2.26 ng/ul	97
35) Benzo(b)fluoranthene	22.75	252	239152	3.63 ng/ul	98
36) Benzo(k)fluoranthene	22.79	252	83372m	1.31 ng/ul	
38) Benzo(a)pyrene	23.31	252	164128	2.56 ng/ul	98
39) Indeno(1,2,3-cd)pyrene	25.60	276	132884	1.79 ng/ul	99
41) Benzo(g,h,i)perylene	26.28	276	116511	1.83 ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM073016\
Data File : BM006760.D
Acq On : 30 Jul 2016 06:21
Operator : UM/SJ
Sample : H4188-03
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9ZL1

Quant Time: Aug 01 04:53:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 30 01:37:26 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
8/1/2016 7:04:30 PM

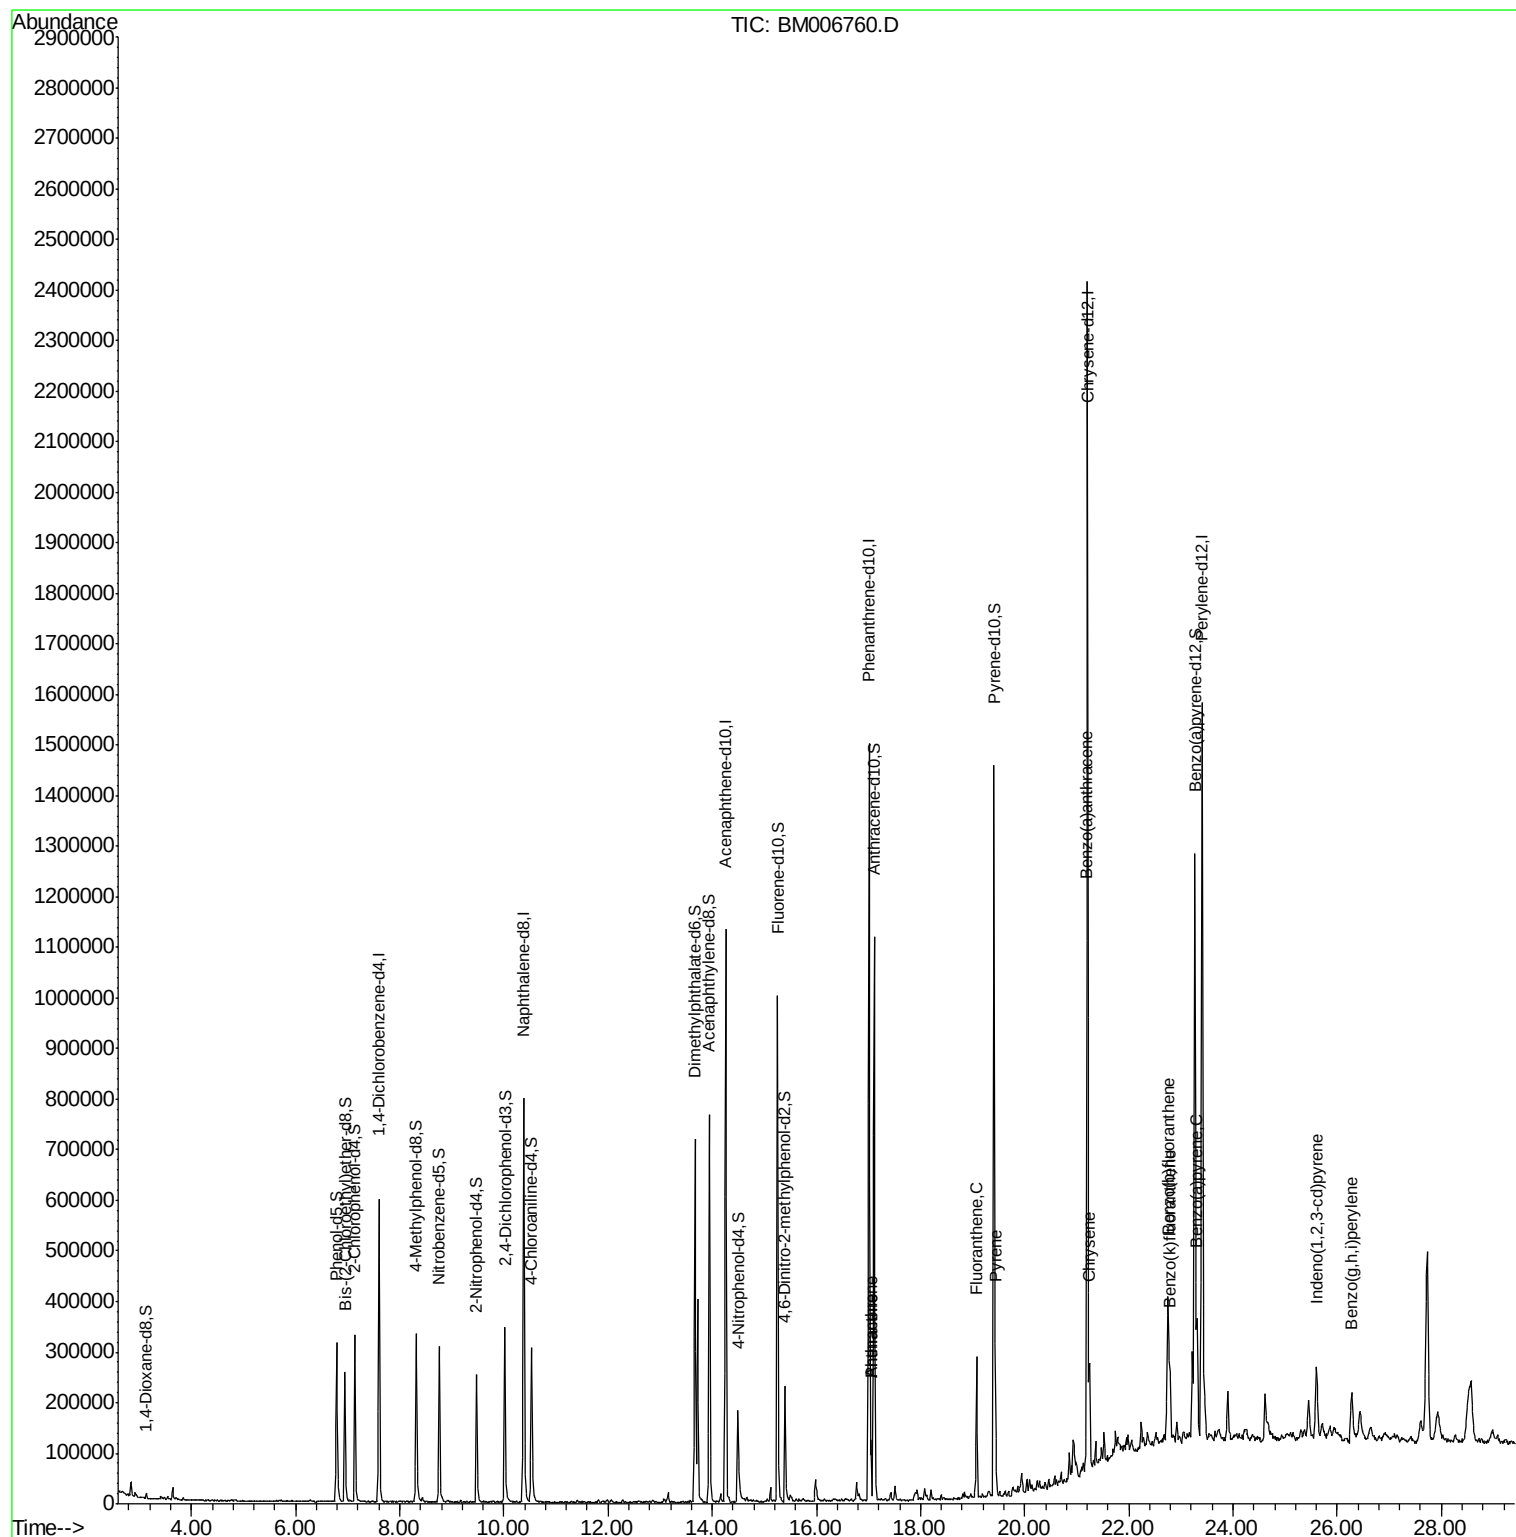

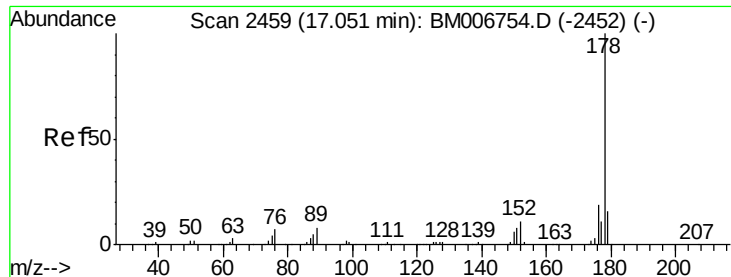

#25

Phenanthrene

Concen: 1.49 ng/ul

RT: 17.05 min Scan# 2459

Delta R.T. 0.00 min

Lab File: BM006760.D

Acq: 30 Jul 2016 06:21

Instrument :

BNA_M

ClientSampleId :

D9ZL1

Tgt Ion:178 Resp: 72919

Ion Ratio Lower Upper


178 100

179 14.2 11.8 17.8




176 19.0 14.8 22.2

Manual Integrations
APPROVED

sohil
8/1/2016 7:04:30 PM

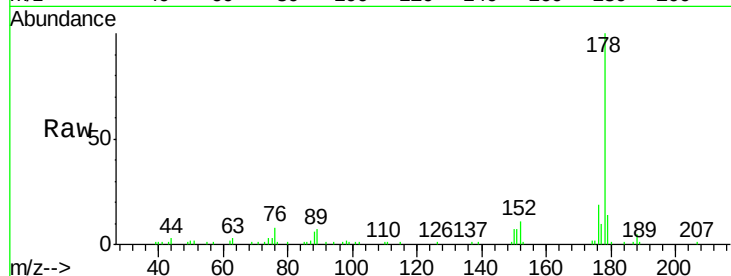

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

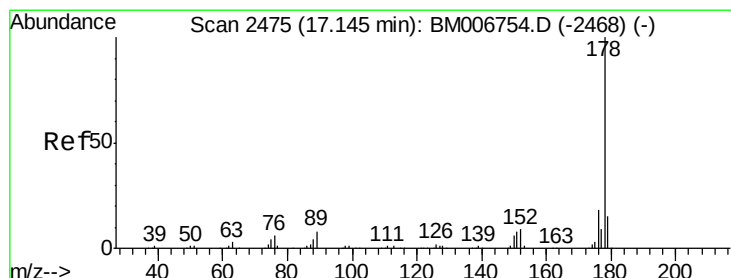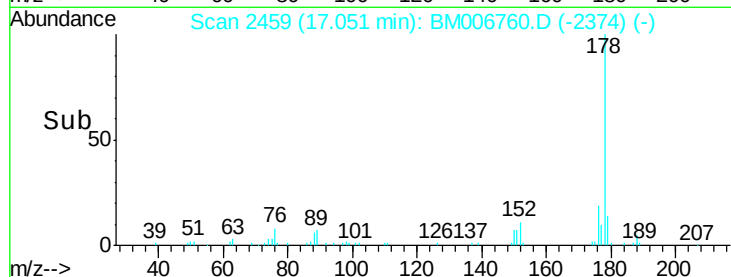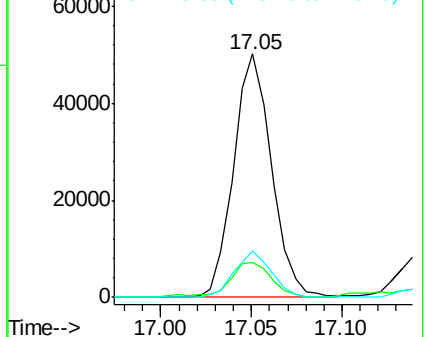

#27

Anthracene

Concen: 1.44 ng/ul

RT: 17.05 min Scan# 2459

Delta R.T. -0.09 min

Lab File: BM006760.D

Acq: 30 Jul 2016 06:21


Tgt Ion:178 Resp: 72919

Ion Ratio Lower Upper



178 100


179 14.2 12.9 19.3

176 19.0 15.6 23.4

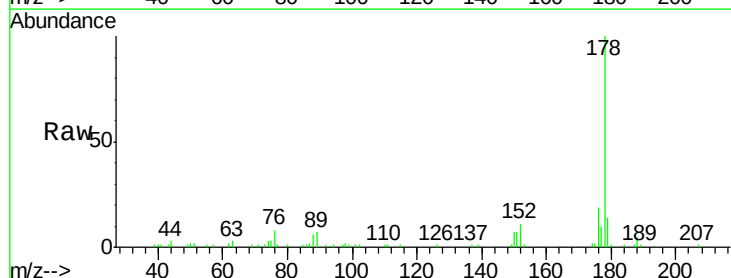

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

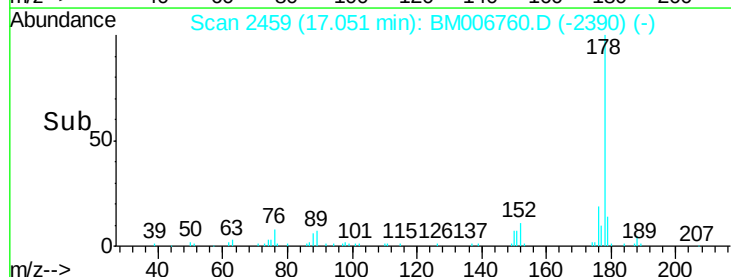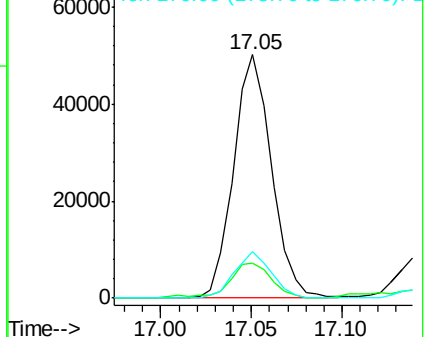

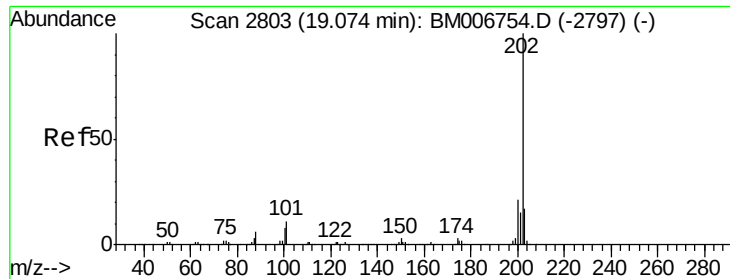





#28
Fluoranthene
Concen: 2.82 ng/ul
RT: 19.07 min Scan# 2803
Delta R.T. -0.01 min
Lab File: BM006760.D
Acq: 30 Jul 2016 06:21

Instrument :
BNA_M
ClientSampleId :
D9ZL1

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	162475		
101	11.3	8.9	13.3	
100	7.8	7.0	10.4	




Manual Integrations
APPROVED


sohil
8/1/2016 7:04:30 PM

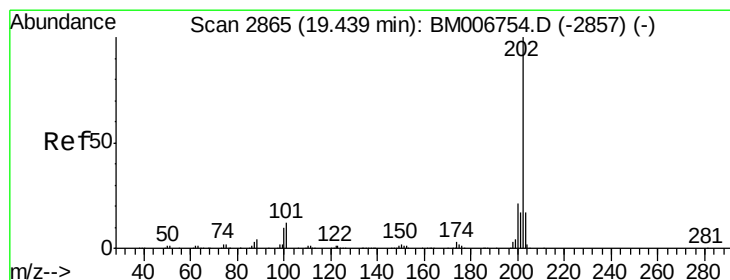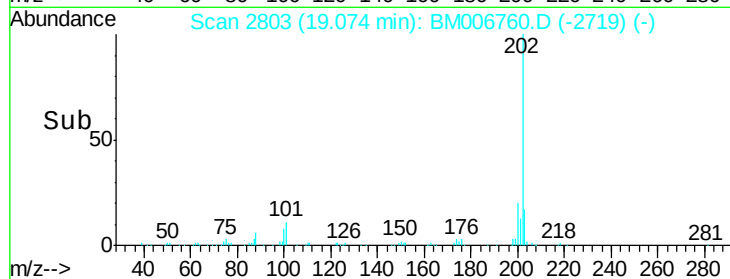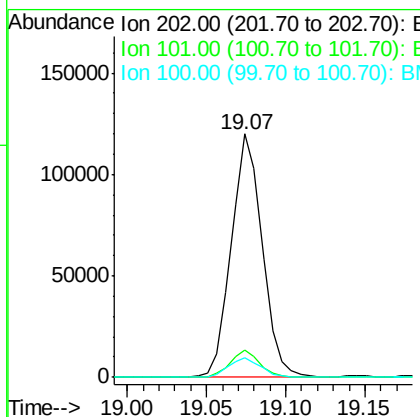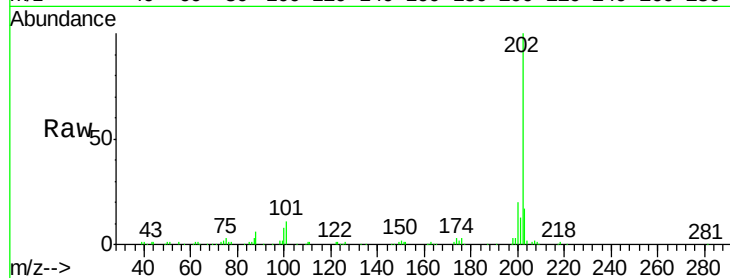

#31
Pyrene
Concen: 2.32 ng/ul
RT: 19.44 min Scan# 2865
Delta R.T. -0.01 min
Lab File: BM006760.D
Acq: 30 Jul 2016 06:21

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	147927		
101	11.6	9.8	14.8	
100	10.8	9.3	13.9	

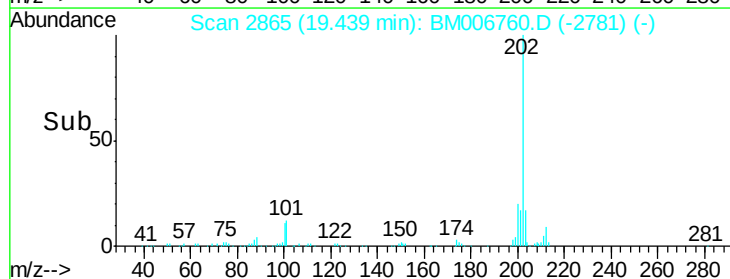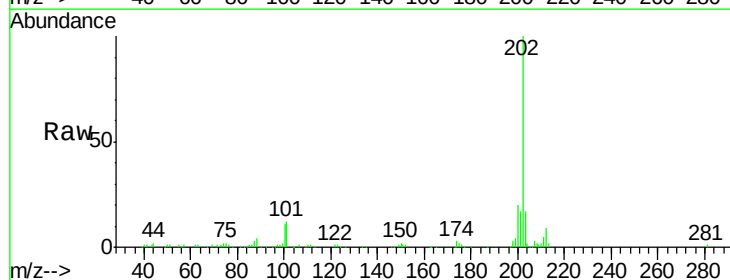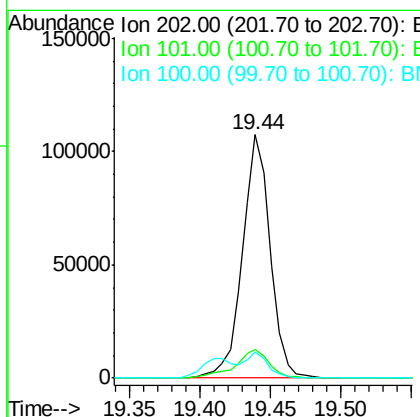

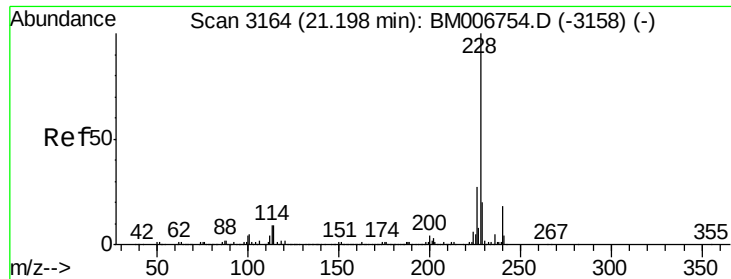





#32
Benzo(a)anthracene
Concen: 1.79 ng/ul
RT: 21.19 min Scan# 3163
Delta R.T. -0.01 min
Lab File: BM006760.D
Acq: 30 Jul 2016 06:21

Instrument :
BNA_M
ClientSampled :
D9ZL1

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	114323		
229	19.9	16.6	25.0	
226	27.1	21.0	31.4	




Manual Integrations
APPROVED


sohil
8/1/2016 7:04:30 PM

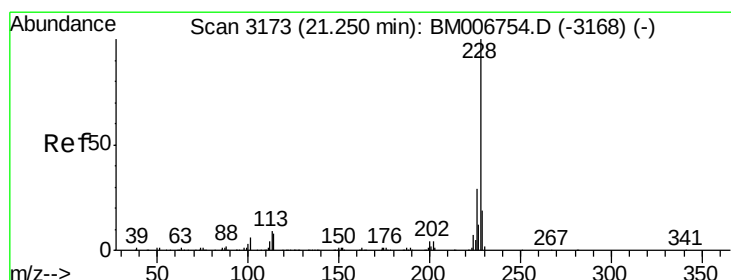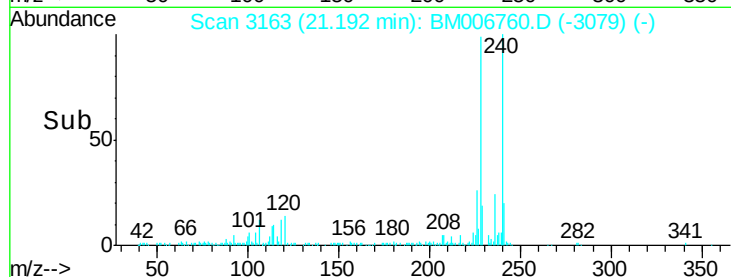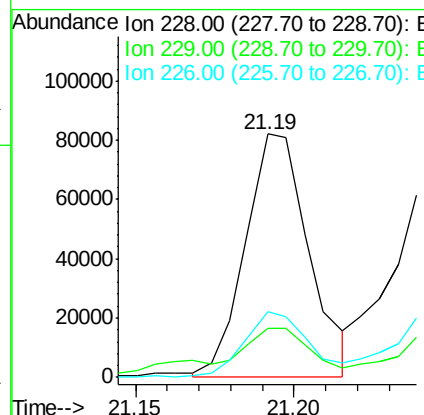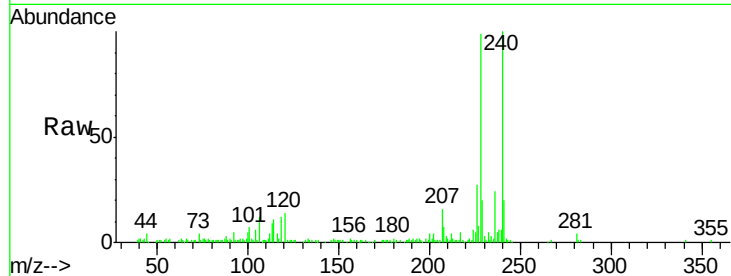

#33
Chrysene
Concen: 2.26 ng/ul
RT: 21.24 min Scan# 3172
Delta R.T. -0.01 min
Lab File: BM006760.D
Acq: 30 Jul 2016 06:21

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	132930		
226	28.6	23.4	35.2	
229	22.3	16.2	24.2	

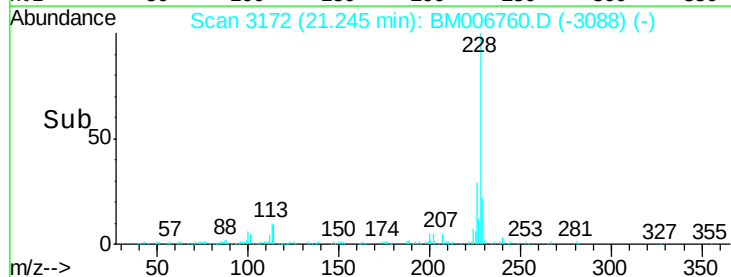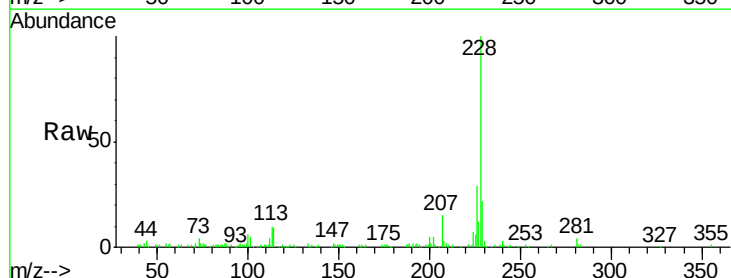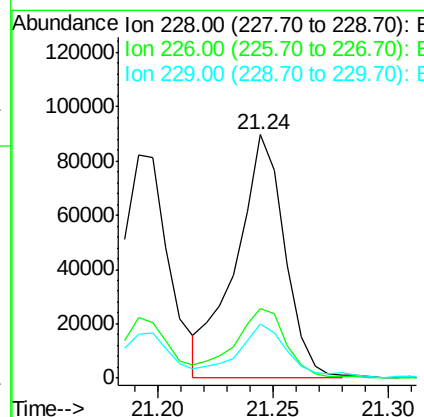

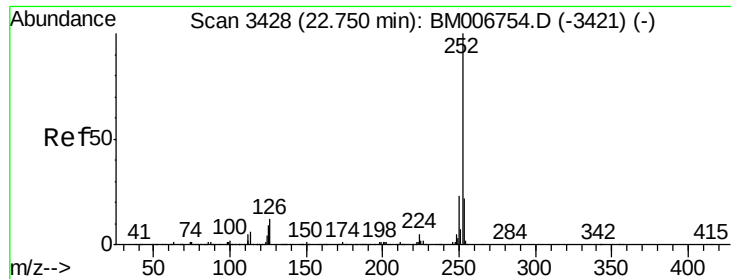





#35
Benzo(b)fluoranthene
Concen: 3.63 ng/ul
RT: 22.75 min Scan# 3428
Delta R.T. -0.01 min
Lab File: BM006760.D
Acq: 30 Jul 2016 06:21

Instrument :
BNA_M
ClientSampled :
D9ZL1

Tgt Ion	Ratio	Resp Lower	Upper
252	100		
253	21.9	18.1	27.1
125	10.5	7.6	11.4




Manual Integrations
APPROVED


sohil
8/1/2016 7:04:30 PM

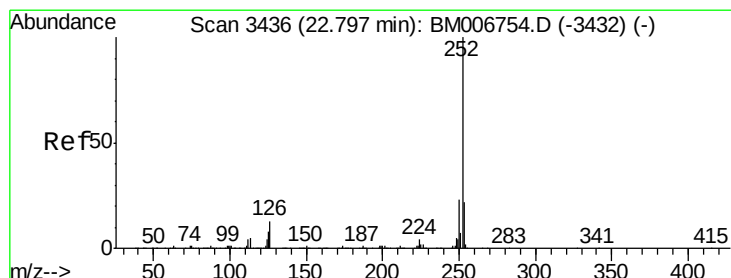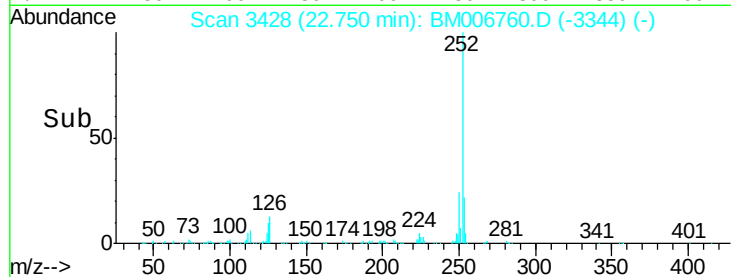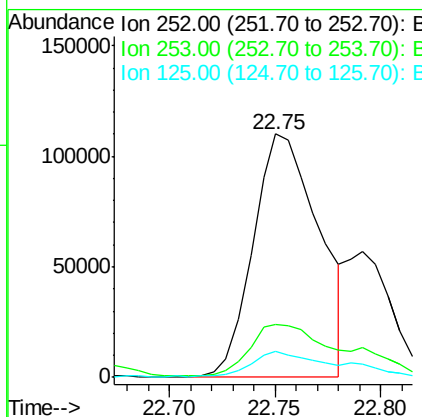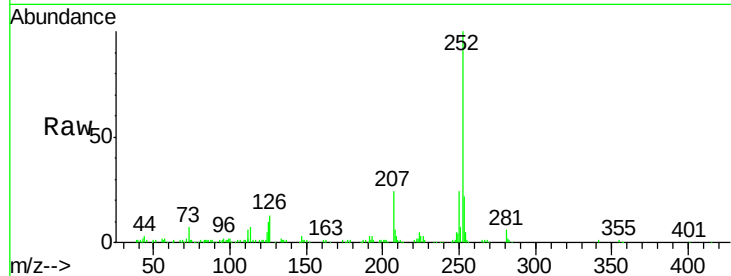

#36
Benzo(k)fluoranthene
Concen: 1.31 ng/ul m
RT: 22.79 min Scan# 3435
Delta R.T. -0.01 min
Lab File: BM006760.D
Acq: 30 Jul 2016 06:21

Tgt Ion	Ratio	Resp Lower	Upper
252	100		
253	23.8	17.8	26.8
125	10.2	7.7	11.5

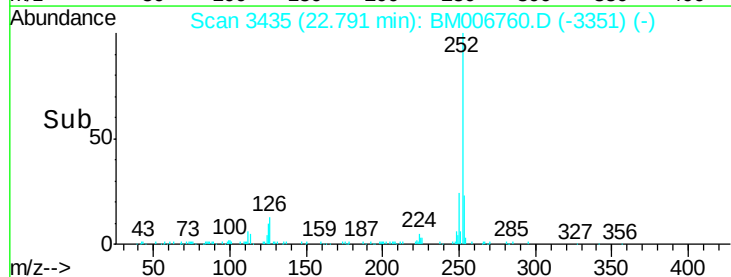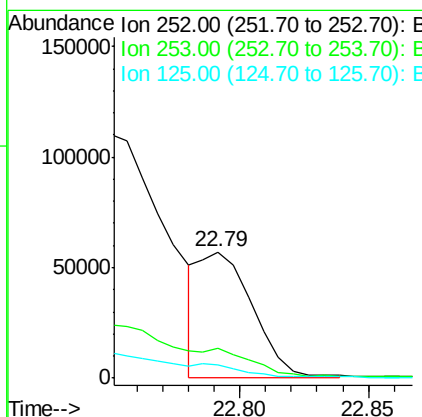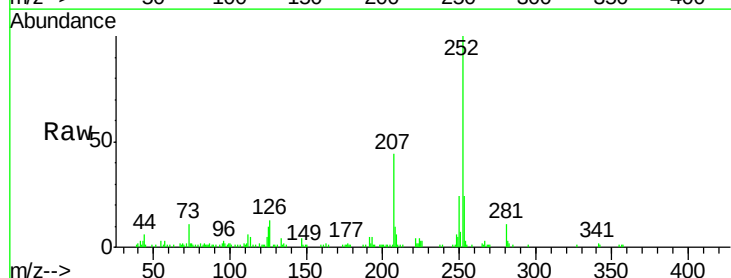

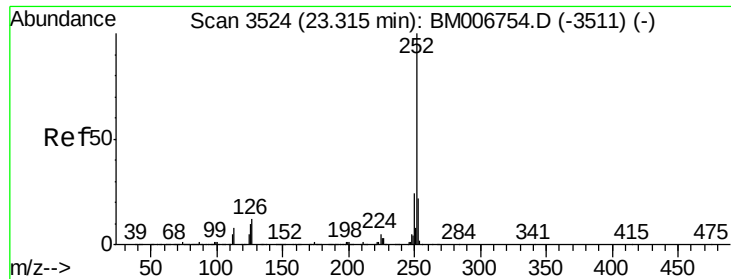





#38
Benzo(a)pyrene
Concen: 2.56 ng/ul
RT: 23.31 min Scan# 3523
Delta R.T. -0.01 min
Lab File: BM006760.D
Acq: 30 Jul 2016 06:21

Instrument :
BNA_M
ClientSampled :
D9ZL1

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	23.2	17.4	26.0
125	10.0	8.2	12.2




Manual Integrations
APPROVED


sohil
8/1/2016 7:04:30 PM

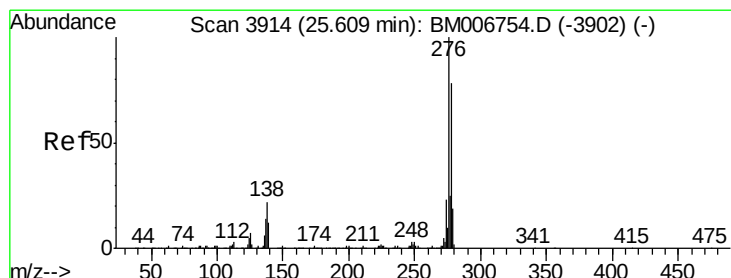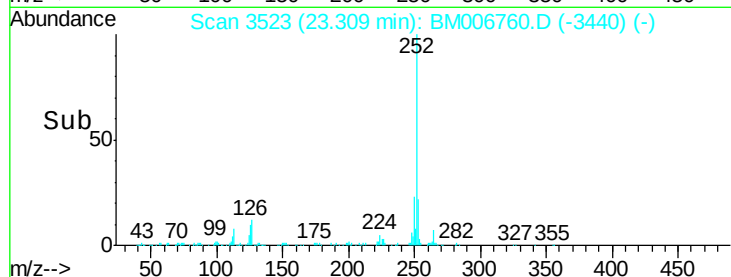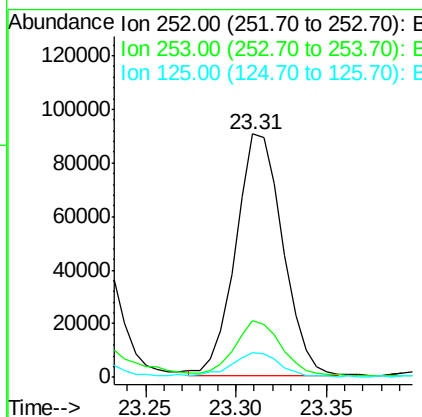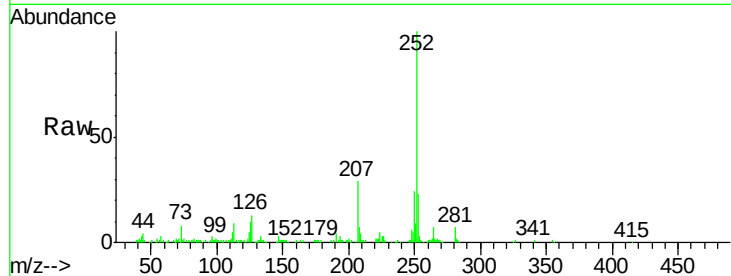

#39
Indeno(1,2,3-cd)pyrene
Concen: 1.79 ng/ul
RT: 25.60 min Scan# 3913
Delta R.T. -0.02 min
Lab File: BM006760.D
Acq: 30 Jul 2016 06:21

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	19.2	15.8	23.6
277	23.8	19.0	28.6

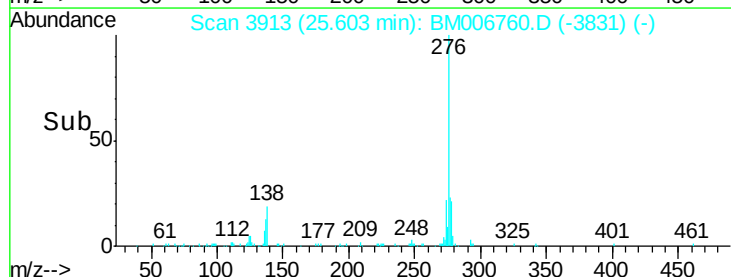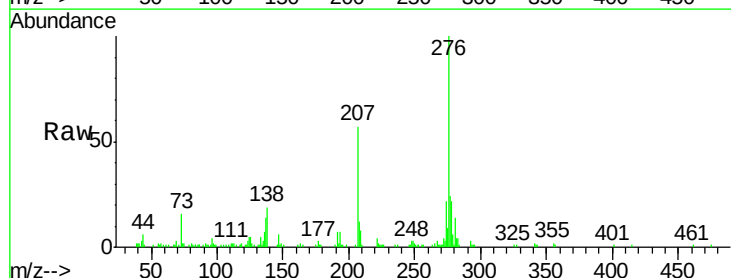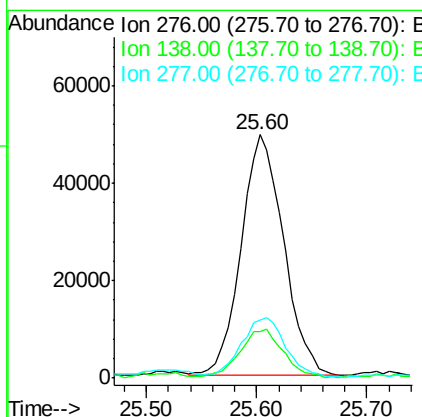

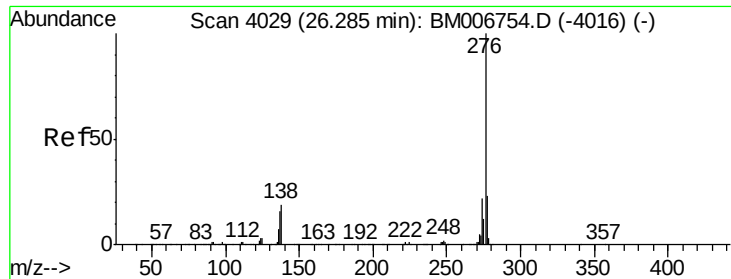

#41
 Benzo(g,h,i)perylene
 Concen: 1.83 ng/ul
 RT: 26.28 min Scan# 4028
 Delta R.T. -0.01 min
 Lab File: BM006760.D
 Acq: 30 Jul 2016 06:21

Instrument :
 BNA_M
 ClientSampleId :
 D9ZL1

Tgt Ion:	276	Resp:	116511
Ion Ratio	Lower	Upper	
276	100		
138	20.4	13.9	20.9
277	22.9	19.8	29.6

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:04:30 PM

