

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073020\
 Data File : BM026949.D
 Acq On : 30 Jul 2020 21:03
 Operator : JU/CG
 Sample : L3487-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4L05

Quant Time: Jul 31 01:17:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 31 01:15:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	72970	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	269804	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	168389	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	362194	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	399208	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	431680	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	8692	5.43	ng/uL	0.00
5) Phenol-d5	6.84	99	33382	5.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	102025	23.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	94465	19.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	61219	12.45	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	54413	25.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	53091	27.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	114390	24.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	1547	0.28	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	390518	29.57	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	447827	26.66	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	12186	5.46	ng/ul	0.00
58) Fluorene-d10	15.29	176	331535	28.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	45309	28.06	ng/ul	0.00
71) Anthracene-d10	17.14	188	555329	30.68	ng/ul	0.00
79) Pyrene-d10	19.43	212	657449	30.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.29	264	756648	31.06	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.75	163	65942	4.759	ng/ul	100
69) Pentachlorophenol	16.69	266	4270	1.781	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073020\
Data File : BM026949.D
Acq On : 30 Jul 2020 21:03
Operator : JU/CG
Sample : L3487-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F4L05

Quant Time: Jul 31 01:17:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 31 01:15:23 2020
Response via : Initial Calibration

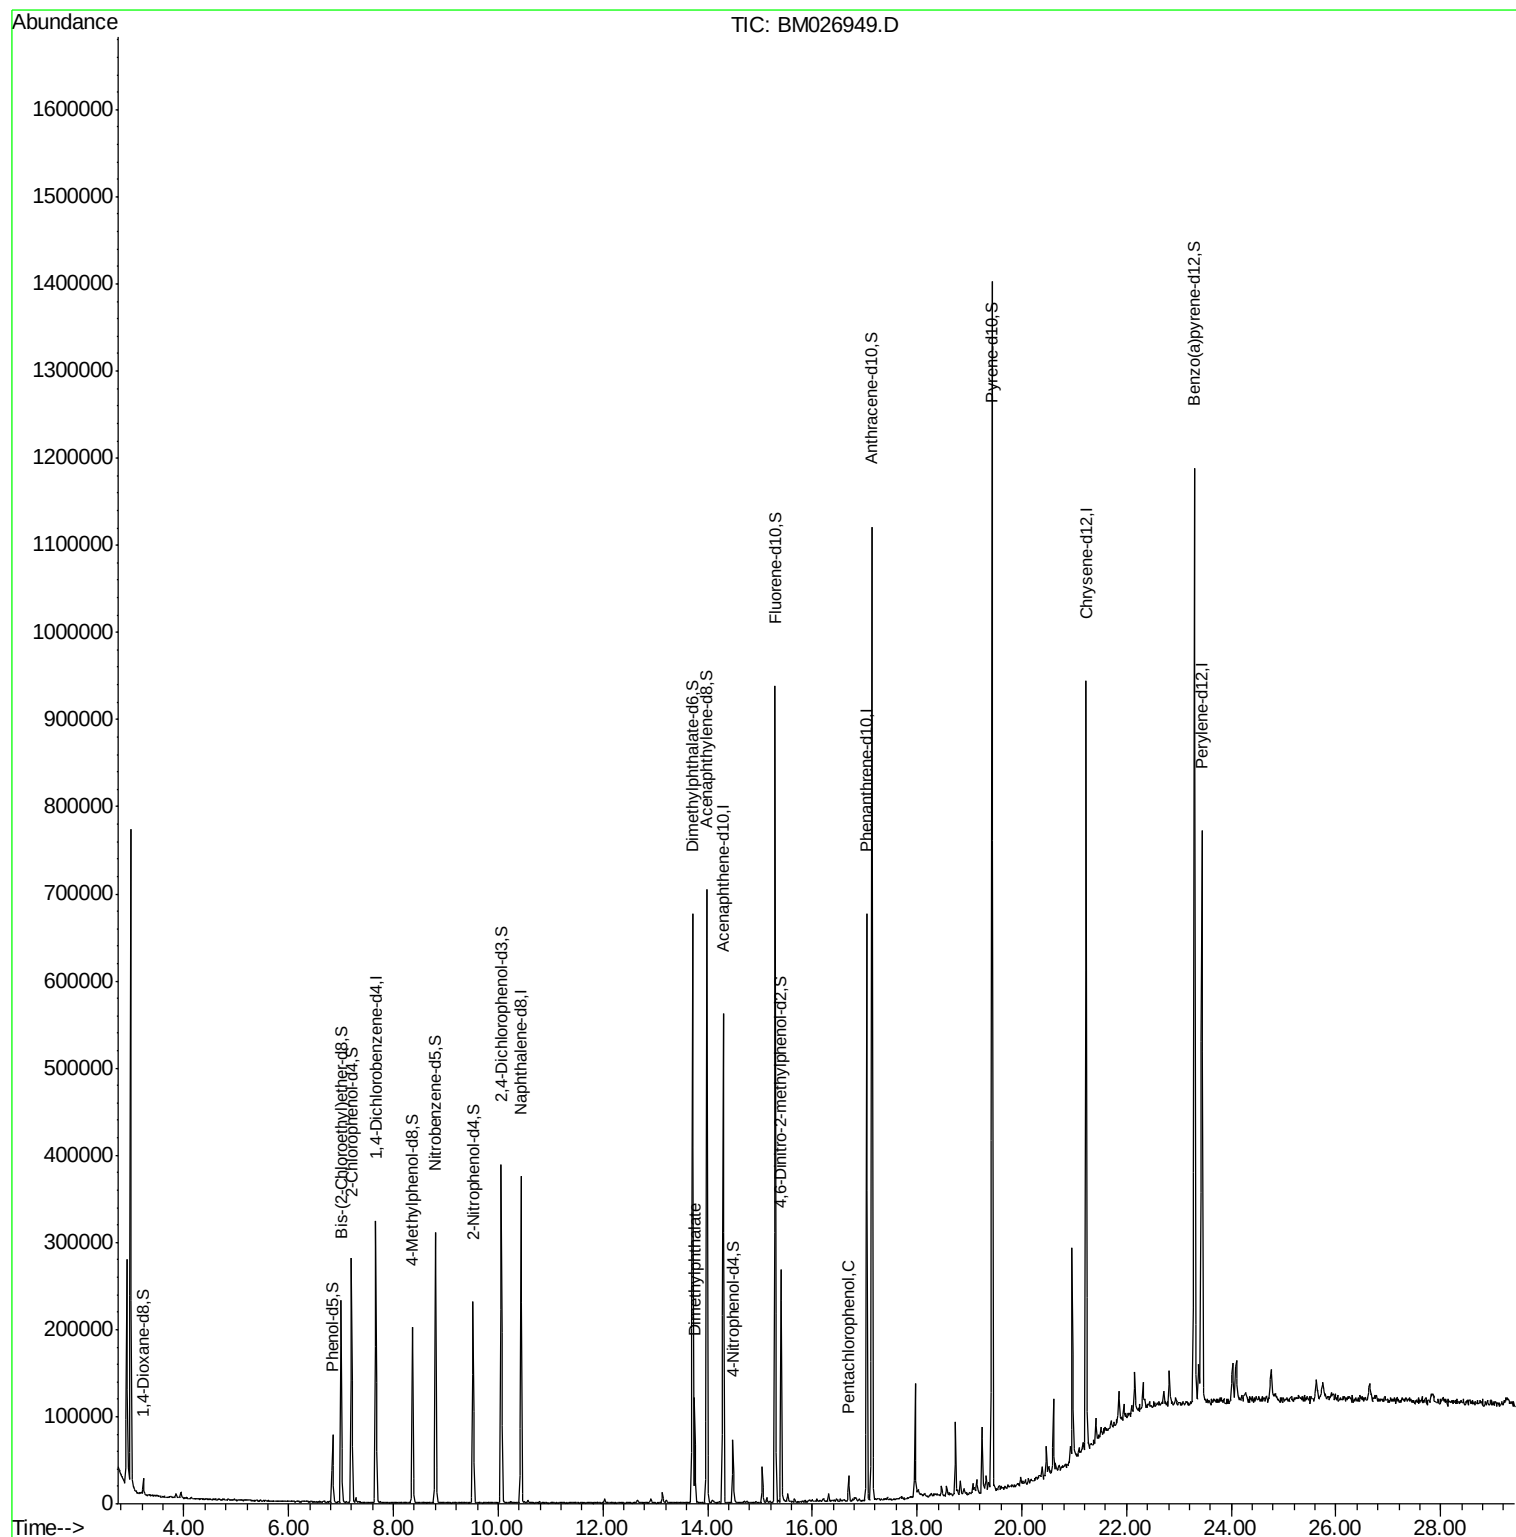

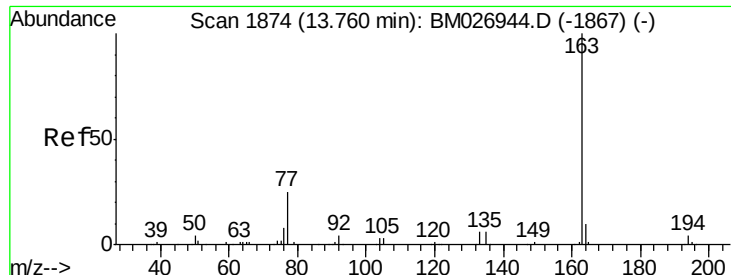

#45

Dimethylphthalate

Concen: 4.759 ng/ul

RT: 13.75 min Scan# 1873

Delta R.T. -0.01 min

Lab File: BM026949.D

Acq: 30 Jul 2020 21:03

Instrument :

BNA_M

ClientSampleId :

F4L05


Tot Ion:163 Resp: 65942

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6




164 10.8 8.6 12.8

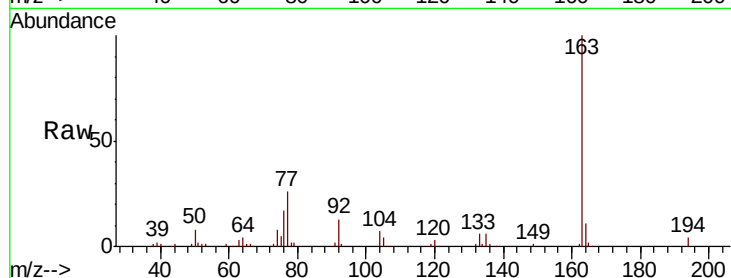

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

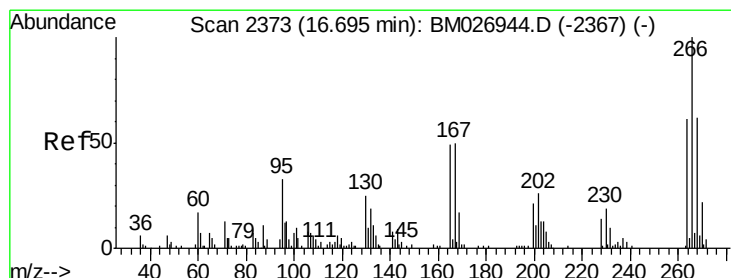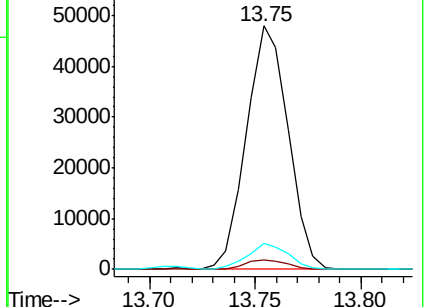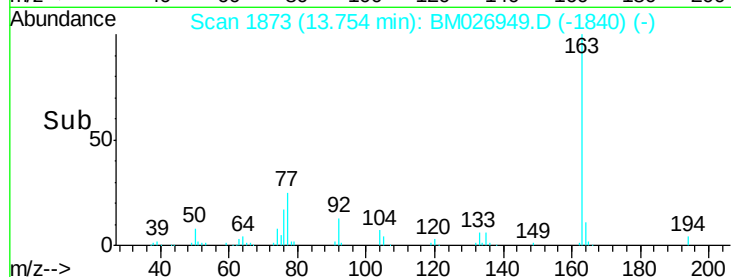

#69

Pentachlorophenol

Concen: 1.781 ng/ul

RT: 16.69 min Scan# 2372

Delta R.T. -0.01 min

Lab File: BM026949.D

Acq: 30 Jul 2020 21:03


Tgt Ion:266 Resp: 4270

Ion Ratio Lower Upper

266 100

264 61.5 49.3 73.9

268 65.8 50.5 75.7

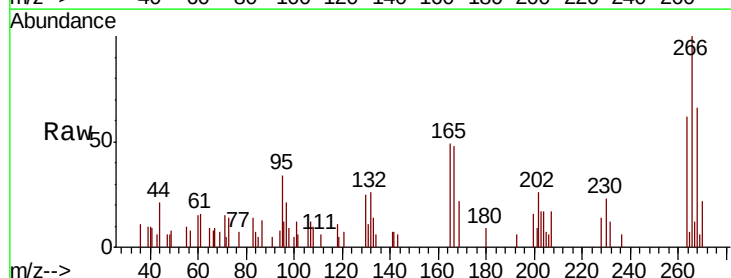

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

