

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073020\
 Data File : BM026948.D
 Acq On : 30 Jul 2020 20:26
 Operator : JU/CG
 Sample : L3487-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4L01

Quant Time: Jul 31 01:17:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 31 01:15:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	74811	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	280557	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	173697	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	361775	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	376613	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	395620	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	9943	6.06	ng/uL	0.00
5) Phenol-d5	6.84	99	34608	5.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	112083	25.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	101069	20.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	64698	12.83	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	59705	27.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	59540	29.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	123211	25.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	16536	2.90	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	419231	30.78	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	509575	29.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	11800	5.12	ng/ul	0.00
58) Fluorene-d10	15.29	176	357085	30.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	46724	28.97	ng/ul	0.00
71) Anthracene-d10	17.14	188	587865	32.51	ng/ul	0.00
79) Pyrene-d10	19.43	212	665972	33.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	753103	33.73	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	46885	3.280	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073020\
Data File : BM026948.D
Acq On : 30 Jul 2020 20:26
Operator : JU/CG
Sample : L3487-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F4L01

Quant Time: Jul 31 01:17:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 31 01:15:23 2020
Response via : Initial Calibration

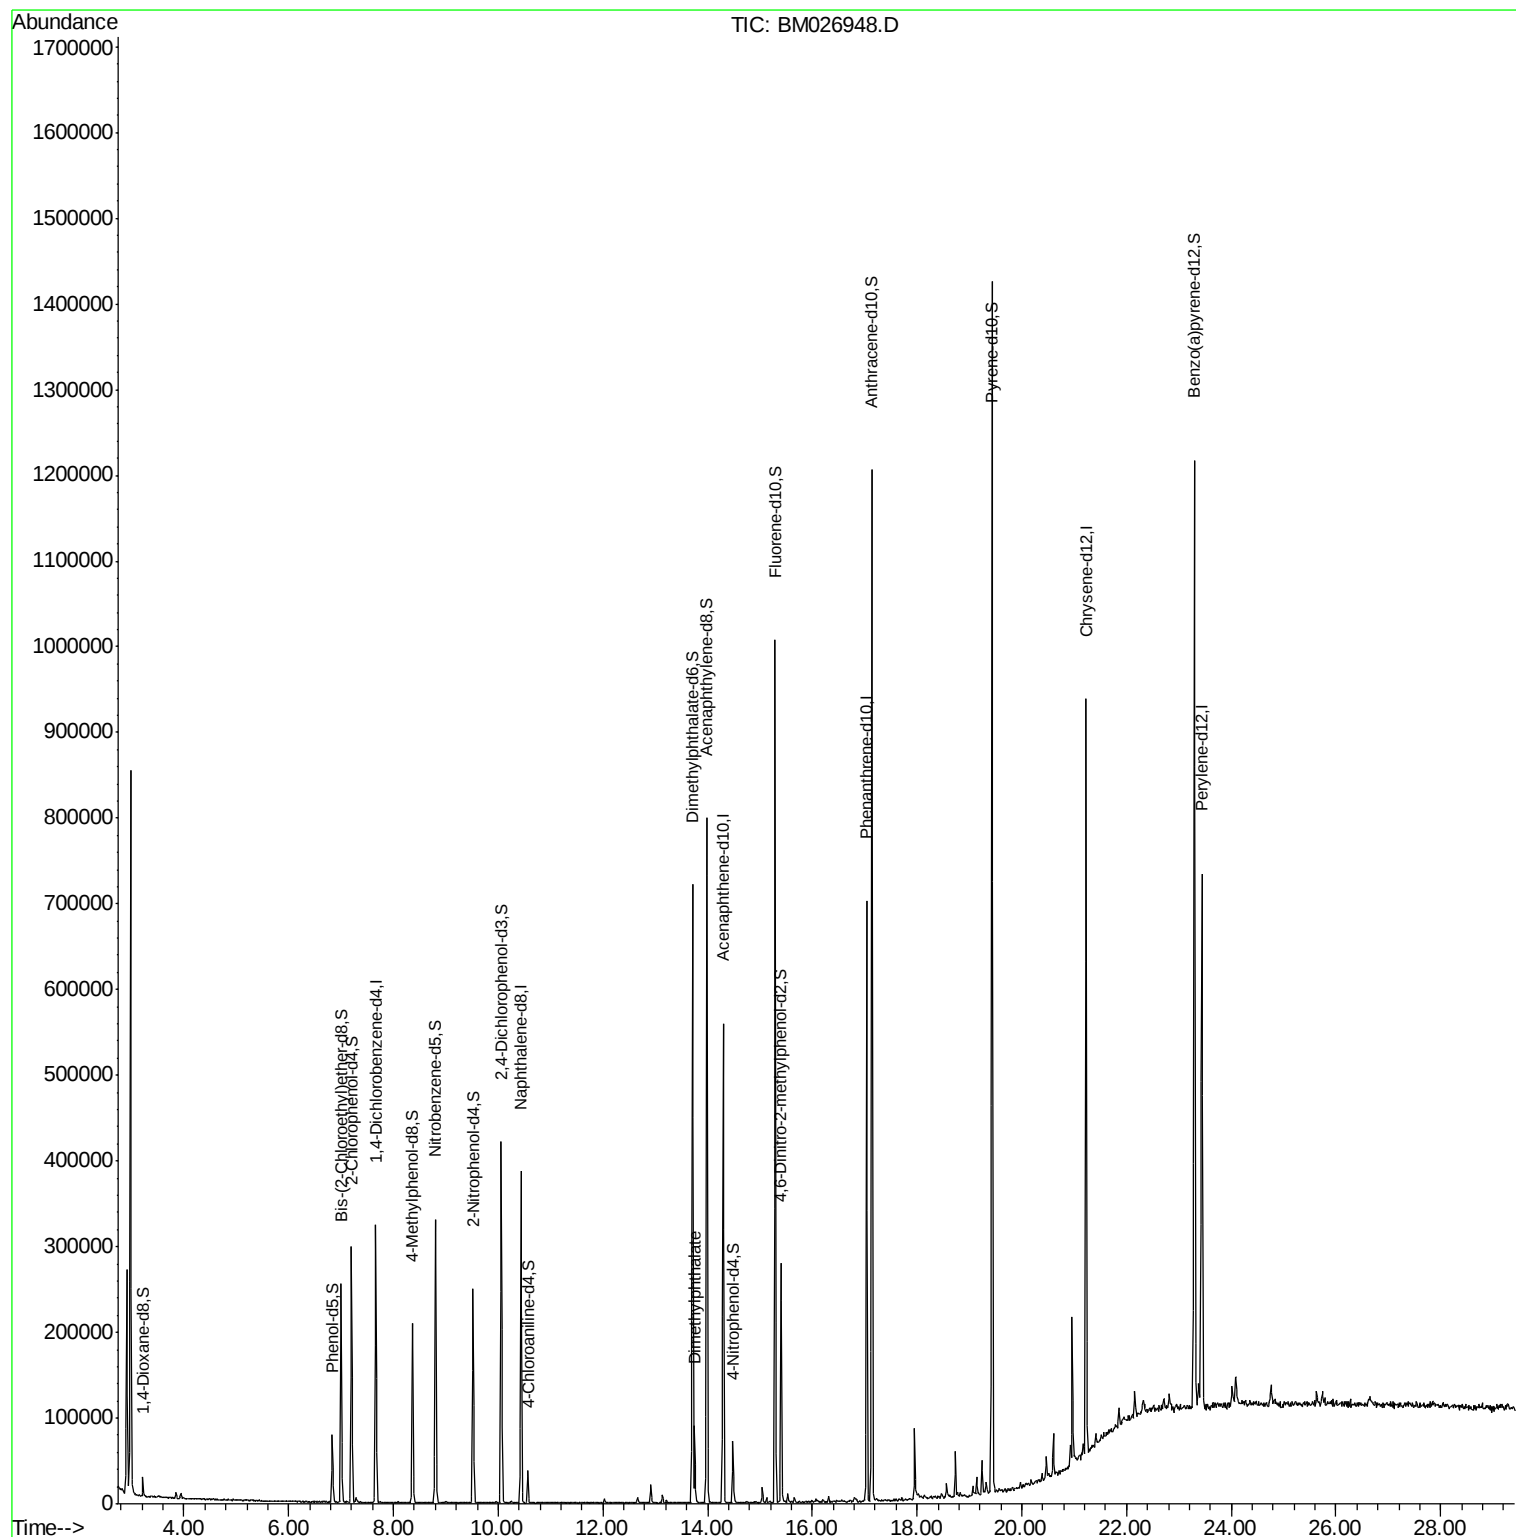

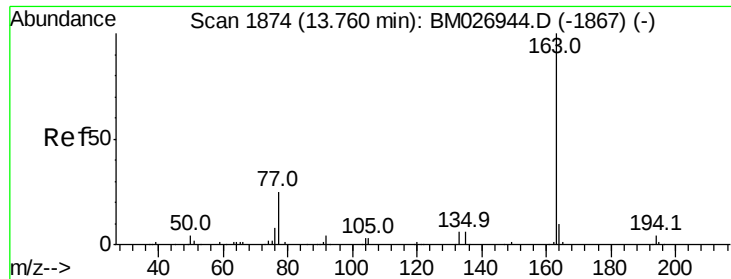

#45

Dimethylphthalate

Concen: 3.280 ng/ul

RT: 13.75 min Scan# 1873

Delta R.T. -0.01 min

Lab File: BM026948.D

Acq: 30 Jul 2020 20:26

Instrument :

BNA_M

ClientSampleId :

F4L01


Tot Ion:163 Resp: 46885

Ion Ratio Lower Upper

163 100

194 4.9 3.0 4.6#

164 12.1 8.6 12.8

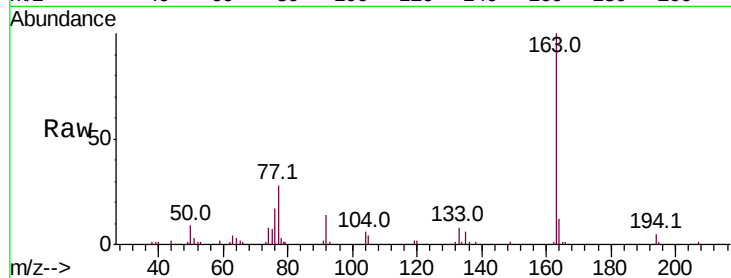

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

