

Data Path : Z:\HPCHEM1\BNA M\DATA\BM073115\
 Data File : BM002160.D
 Acq On : 31 Jul 2015 17:30
 Operator : TP/UM
 Sample : G3065-23
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C02G8

Quant Time: Aug 01 02:22:01 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM072715.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 01 02:15:30 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	65724	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	264548	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	161745	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	373840	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	457670	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	463568	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.03	96	5358	4.22	ng/uL	0.00
5) Phenol-d5	6.76	99	125619	26.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	66020	25.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	108445	27.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	105669	28.29	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	47554	25.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	51896	24.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	113029	28.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	140400	31.75	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	333066	28.11	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	405072	27.34	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	48719	24.64	ng/ul	0.00
58) Fluorene-d10	15.24	176	293241	28.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	20318	8.89	ng/ul	0.00
71) Anthracene-d10	17.09	188	460748	27.61	ng/ul	0.00
79) Pyrene-d10	19.40	212	523166	27.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	581147	25.86	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.70	163	172145	14.55	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM073115\
Data File : BM002160.D
Acq On : 31 Jul 2015 17:30
Operator : TP/UM
Sample : G3065-23
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C02G8

Quant Time: Aug 01 02:22:01 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 01 02:15:30 2015
Response via : Initial Calibration

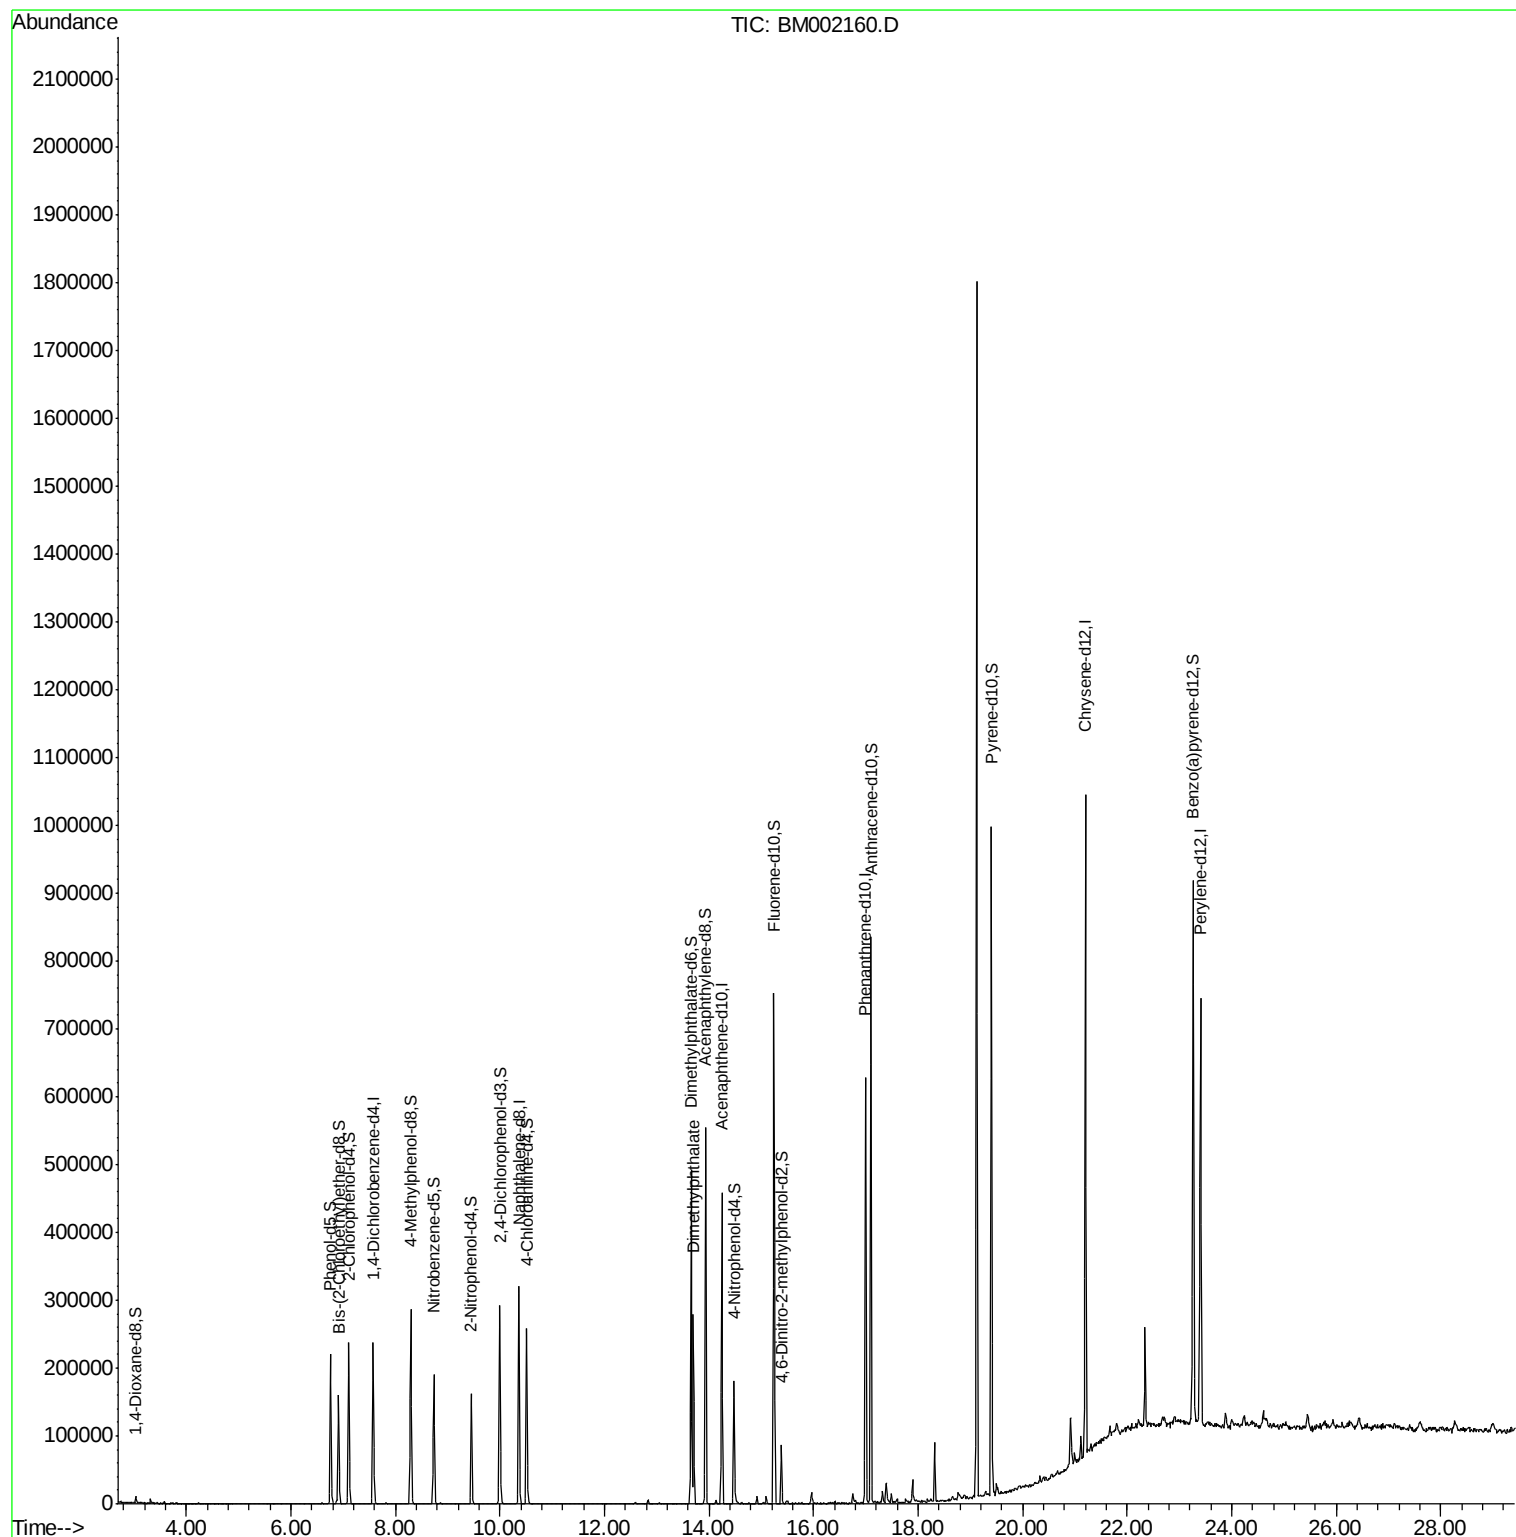

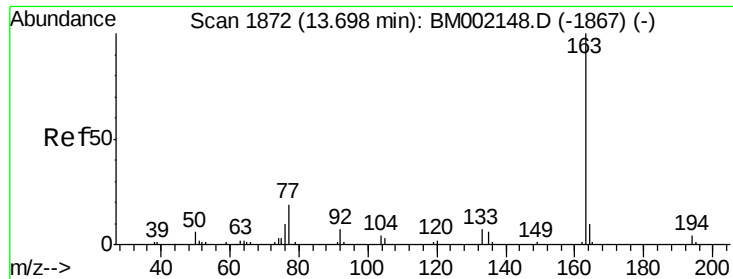

#45

Dimethylphthalate

Concen: 14.55 ng/ul

RT: 13.70 min Scan# 1872

Delta R.T. 0.00 min

Lab File: BM002160.D

Acq: 31 Jul 2015 17:30

Instrument :

BNA_M

ClientSampleId :

C02G8


Tot Ion:163 Resp: 172145

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 10.4 8.0 12.0

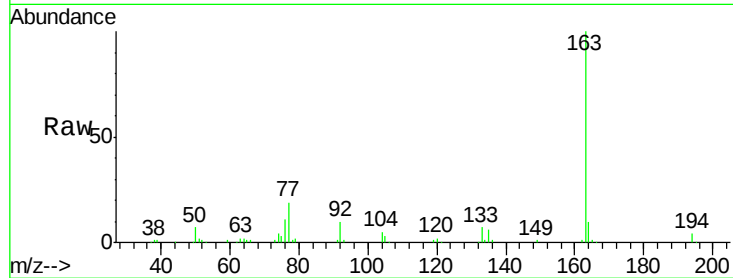

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

