

Data Path : Z:\HPCHEM1\BNA M\DATA\BM073115\
 Data File : BM002158.D
 Acq On : 31 Jul 2015 16:16
 Operator : TP/UM
 Sample : G3065-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C02H6

Quant Time: Aug 01 02:21:44 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM072715.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 01 02:15:30 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	56969	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	245883	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	155821	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	353902	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	410552	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	417672	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.03	96	5825	5.29	ng/uL	0.00
5) Phenol-d5	6.76	99	138119	33.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	70349	31.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	118820	34.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	115814	35.77	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	53197	30.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	57424	29.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	121432	32.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	148934	36.23	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	340678	29.85	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	397584	27.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	51330	26.94	ng/ul	0.00
58) Fluorene-d10	15.24	176	277907	27.67	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	29924	13.82	ng/ul	0.00
71) Anthracene-d10	17.09	188	439742	27.84	ng/ul	0.00
79) Pyrene-d10	19.40	212	464442	26.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	517054	25.54	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.70	163	47461	4.16	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM073115\
Data File : BM002158.D
Acq On : 31 Jul 2015 16:16
Operator : TP/UM
Sample : G3065-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C02H6

Quant Time: Aug 01 02:21:44 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 01 02:15:30 2015
Response via : Initial Calibration

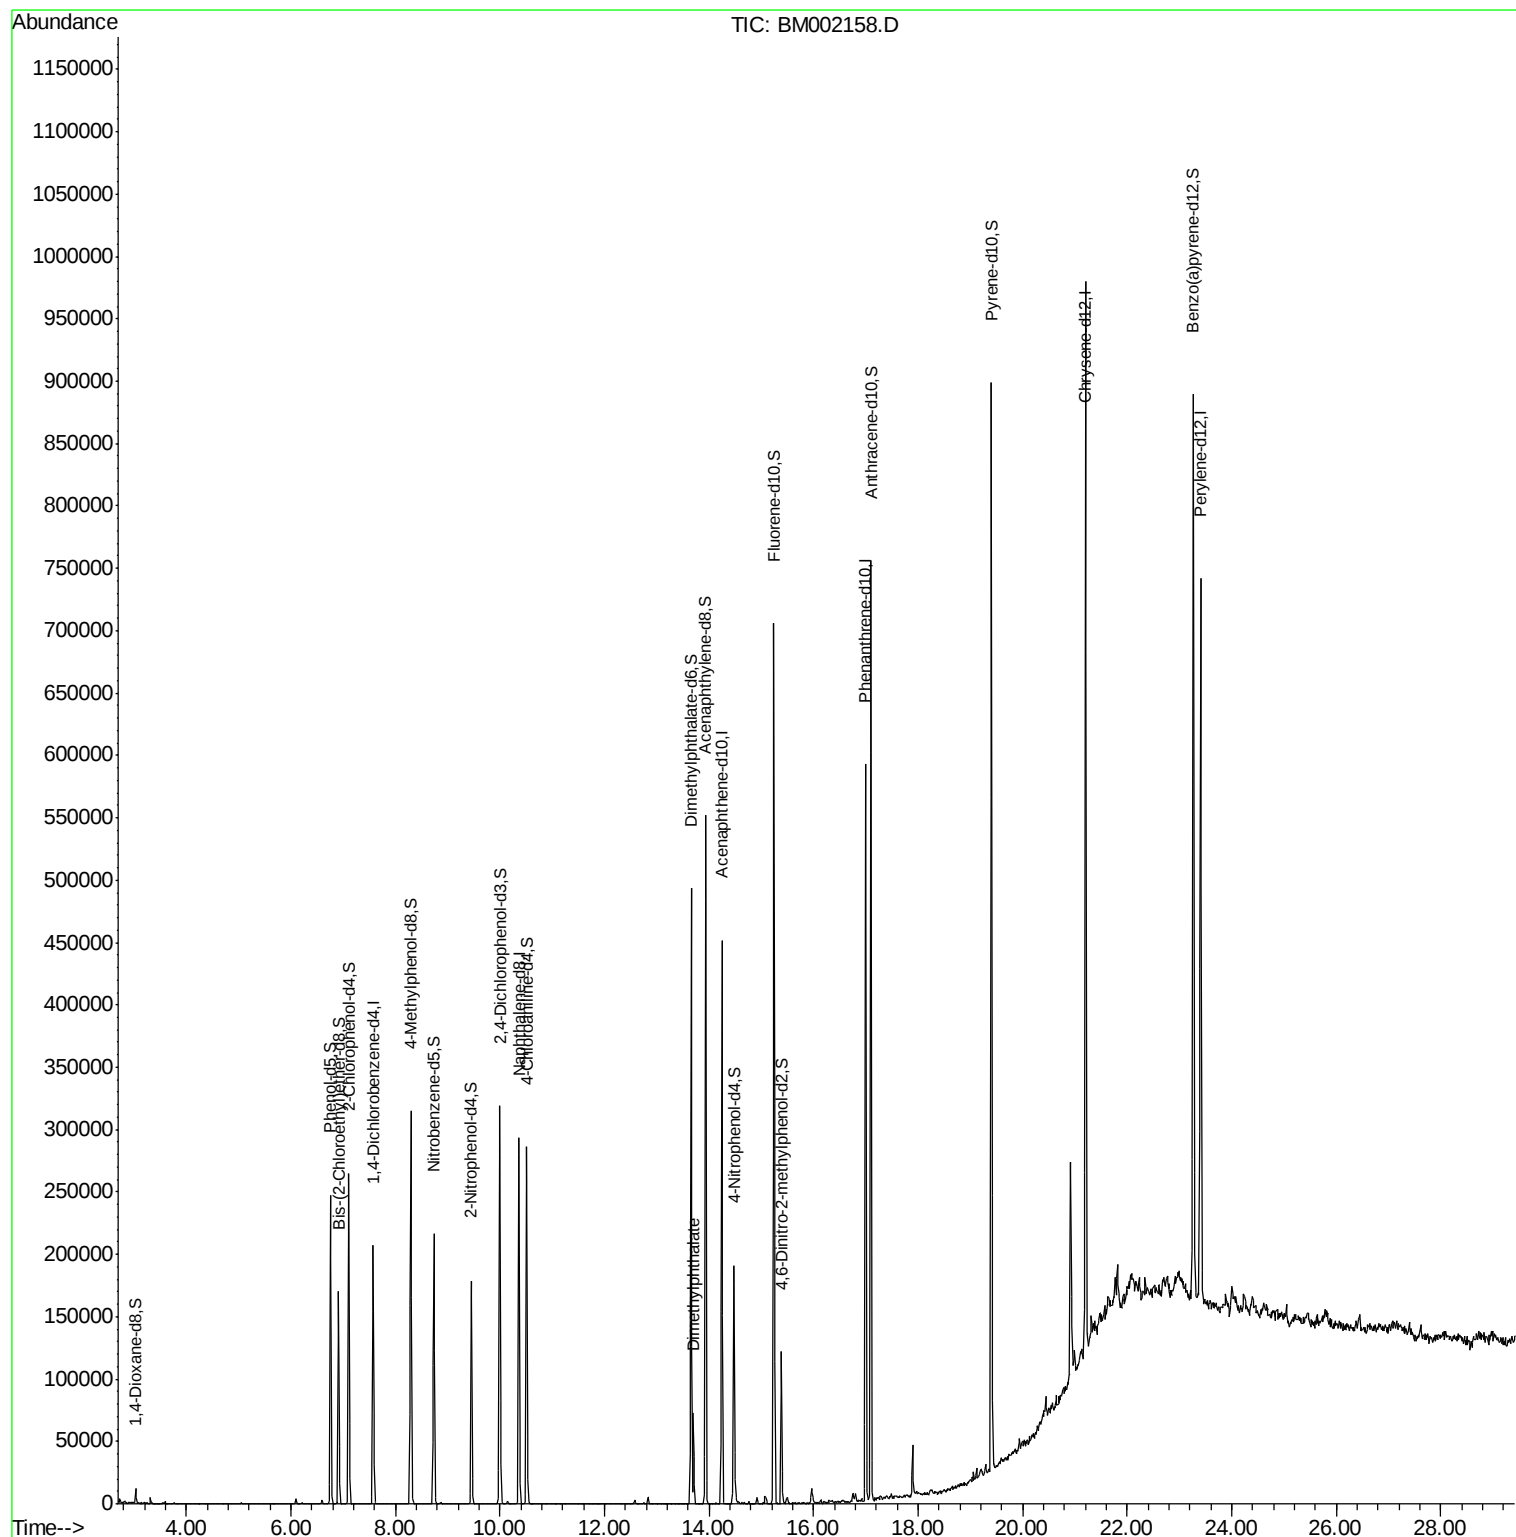

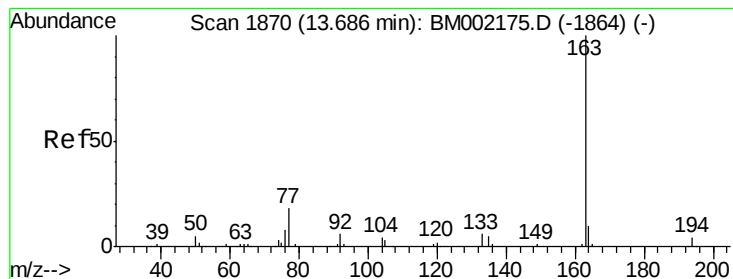

#45

Dimethylphthalate

Concen: 4.16 ng/ul

RT: 13.70 min Scan# 1872

Delta R.T. 0.00 min

Lab File: BM002158.D

Acq: 31 Jul 2015 16:16

Instrument :

BNA_M

ClientSampleId :

C02H6


Tot Ion:163 Resp: 47461

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 11.1 8.0 12.0

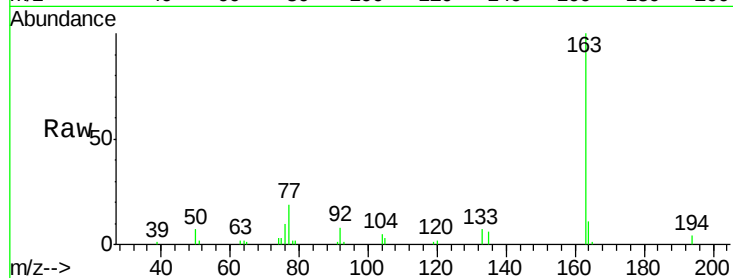

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

