

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM073116\
 Data File : BM006784.D
 Acq On : 31 Jul 2016 11:54
 Operator : UM/SJ
 Sample : H4188-23
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9ZP9

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:06:04 PM

Quant Time: Aug 01 06:59:21 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	134789	20.00	ng/ul	0.00
7) Naphthalene-d8	10.38	136	594160	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.26	164	345793	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.01	188	797233	20.00	ng/ul	0.00
29) Chrysene-d12	21.21	240	923699	20.00	ng/ul	0.00
34) Perylene-d12	23.41	264	958620	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.13	96	4726	1.42	ng/uL	0.00
3) Phenol-d5	6.79	99	174582	15.22	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	6.95	67	124996	17.60	ng/ul	0.00
5) 2-Chlorophenol-d4	7.14	132	150337	16.41	ng/ul	0.00
6) 4-Methylphenol-d8	8.32	113	102101	11.48	ng/ul	0.00
8) Nitrobenzene-d5	8.76	128	74699	16.61	ng/ul	0.00
9) 2-Nitrophenol-d4	9.47	143	82327	17.21	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.01	165	145059	16.05	ng/ul	0.00
12) 4-Chloroaniline-d4	10.53	131	189181	19.01	ng/ul	0.00
16) Dimethylphthalate-d6	13.67	166	483257	17.82	ng/ul	0.00
17) Acenaphthylene-d8	13.94	160	608512	17.58	ng/ul	0.00
20) 4-Nitrophenol-d4	14.49	143	56632	12.03	ng/ul	0.00
21) Fluorene-d10	15.25	176	441394	18.20	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.40	200	50503	12.20	ng/ul	0.00
26) Anthracene-d10	17.10	188	680193	17.97	ng/ul	0.00
30) Pyrene-d10	19.41	212	795443	18.90	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.27	264	807205	18.31	ng/ul	0.00

Target Compounds

						Qvalue
25) Phenanthrene	17.05	178	134986	3.01	ng/ul	99
28) Fluoranthene	19.07	202	361299	6.86	ng/ul	99
31) Pyrene	19.44	202	299771	5.36	ng/ul	98
32) Benzo(a)anthracene	21.20	228	183248	3.27	ng/ul	97
33) Chrysene	21.24	228	188636	3.65	ng/ul	97
35) Benzo(b)fluoranthene	22.76	252	300468	5.23	ng/ul	98
36) Benzo(k)fluoranthene	22.79	252	86183m	1.55	ng/ul	
38) Benzo(a)pyrene	23.31	252	184975	3.31	ng/ul	97
39) Indeno(1,2,3-cd)pyrene	25.61	276	151133	2.33	ng/ul	97
41) Benzo(g,h,i)perylene	26.29	276	126346	2.28	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM073116\
Data File : BM006784.D
Acq On : 31 Jul 2016 11:54
Operator : UM/SJ
Sample : H4188-23
Misc :
ALS Vial : 53 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9ZP9

Manual Integrations
APPROVED

sohil
8/1/2016 7:06:04 PM

Quant Time: Aug 01 06:59:21 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 30 01:37:26 2016
Response via : Initial Calibration

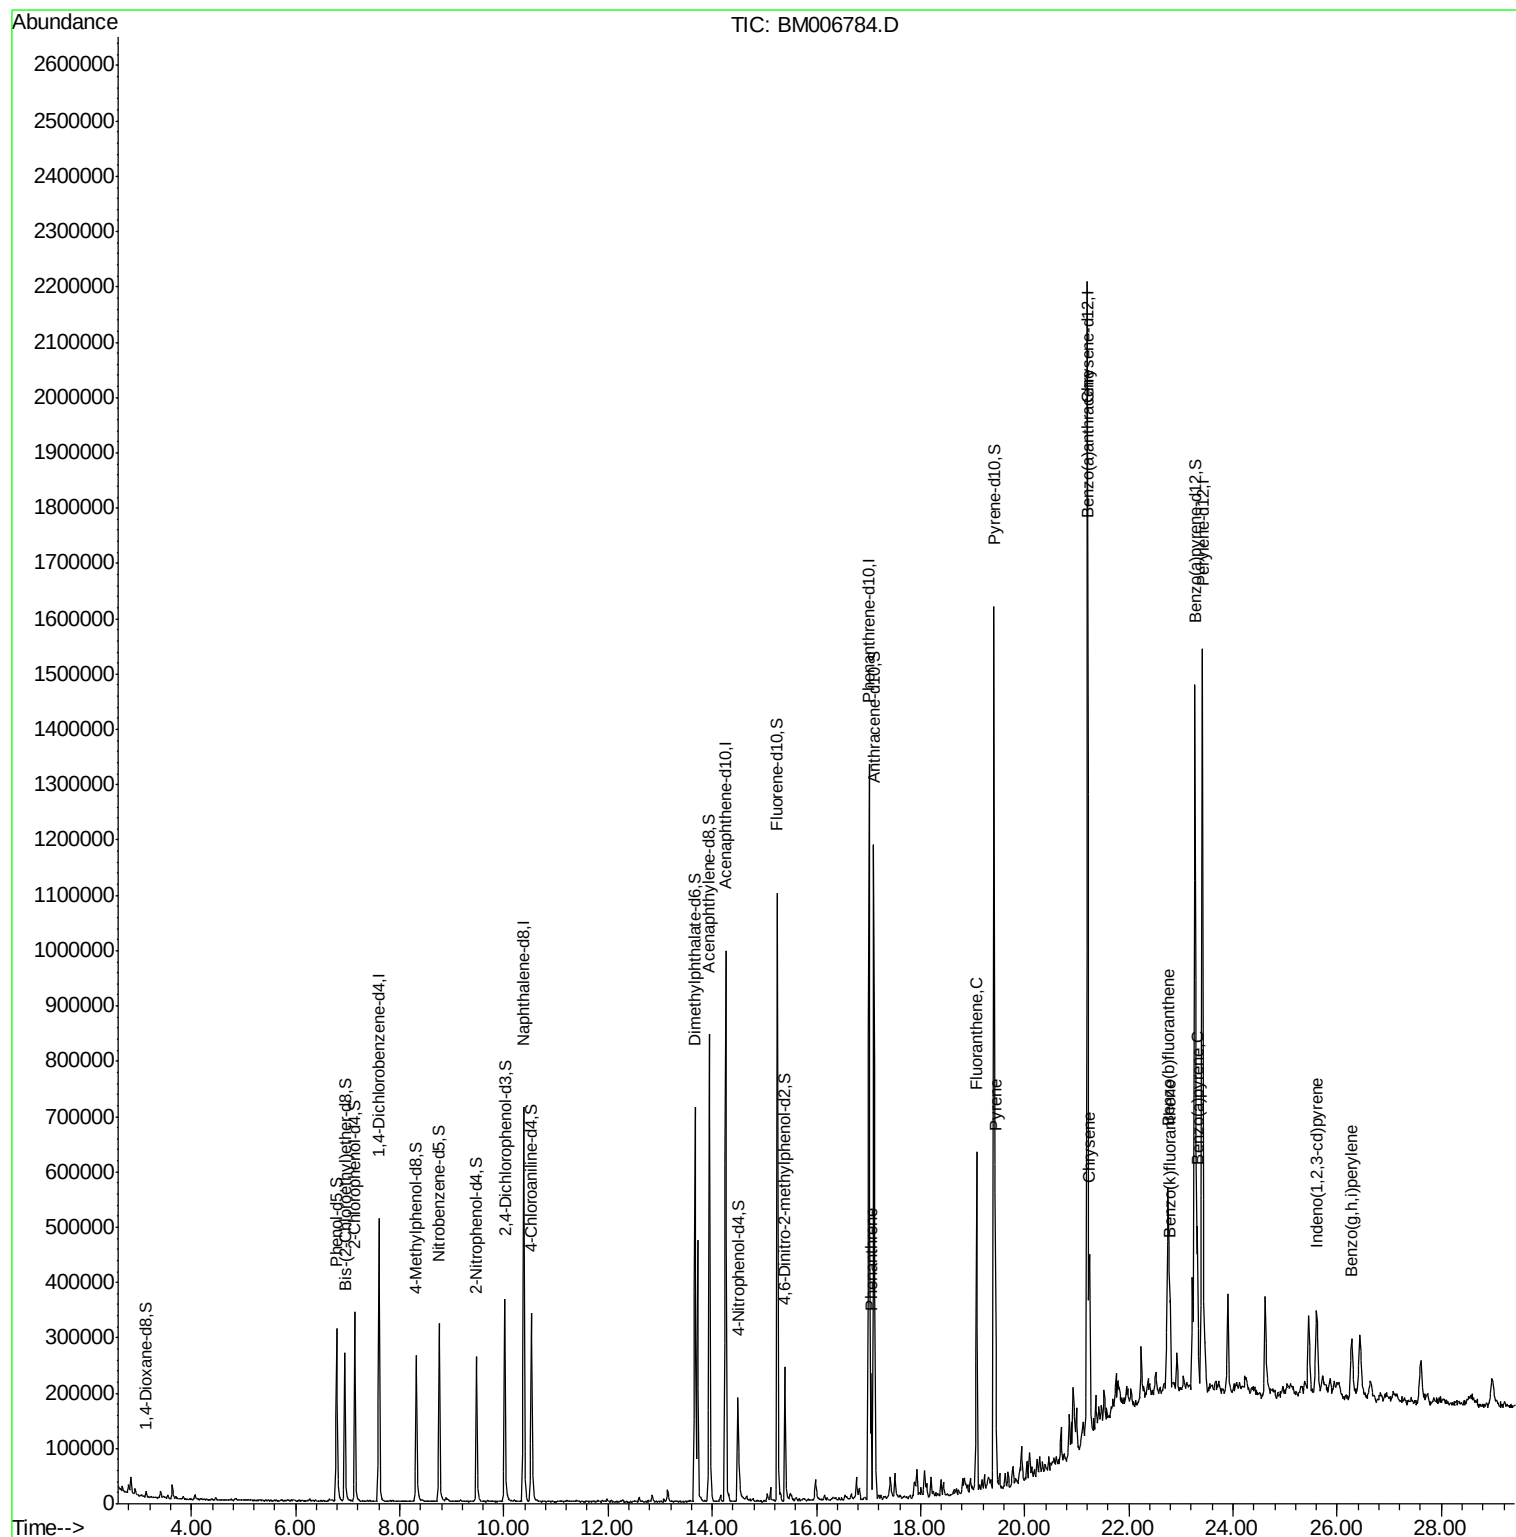

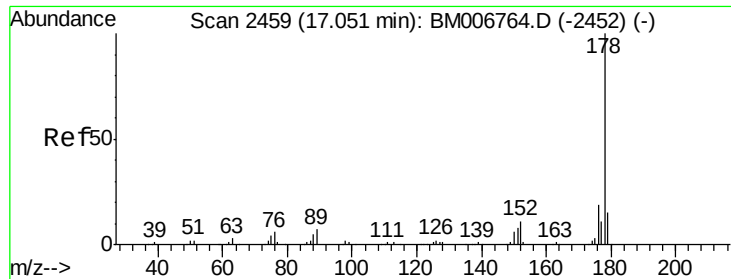

#25

Phenanthrene

Concen: 3.01 ng/ul

RT: 17.05 min Scan# 2459

Delta R.T. -0.00 min

Lab File: BM006784.D

Acq: 31 Jul 2016 11:54

Instrument :

BNA_M


ClientSampleId :

D9ZP9




Tgt Ion:	178	Resp:	134986
Ion Ratio	Lower	Upper	
178	100		
179	14.3	11.8	17.8
176	18.8	14.8	22.2

Manual Integrations
APPROVED

sohil
8/1/2016 7:06:04 PM

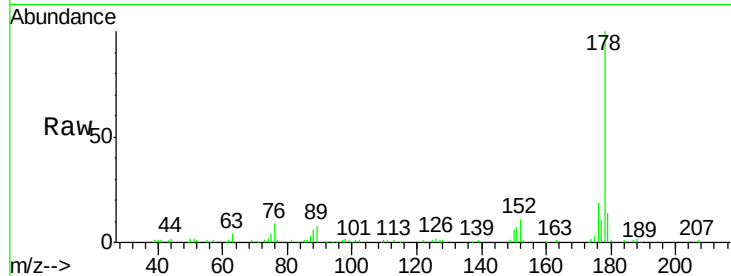

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

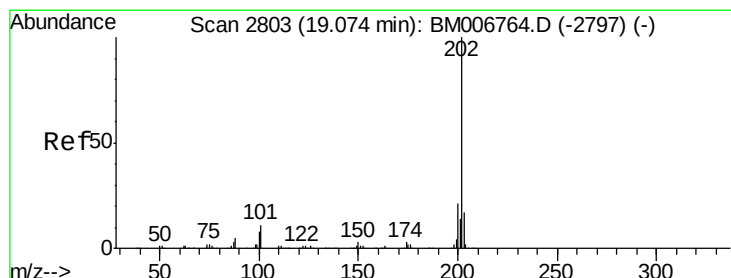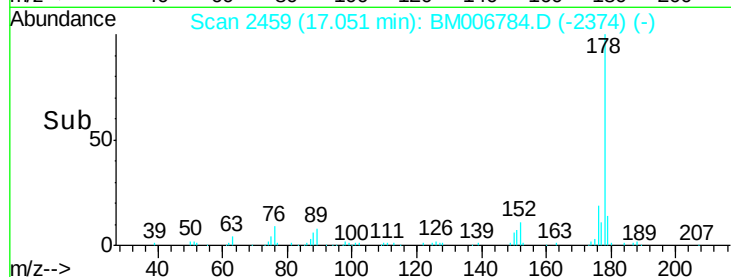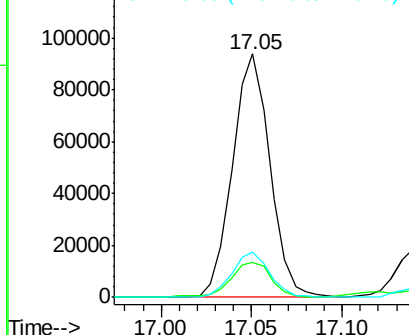

#28

Fluoranthene

Concen: 6.86 ng/ul


RT: 19.07 min Scan# 2803

Delta R.T. -0.01 min



Lab File: BM006784.D


Acq: 31 Jul 2016 11:54

Tgt Ion:	202	Resp:	361299
Ion Ratio	Lower	Upper	
202	100		
101	10.9	8.9	13.3
100	8.3	7.0	10.4

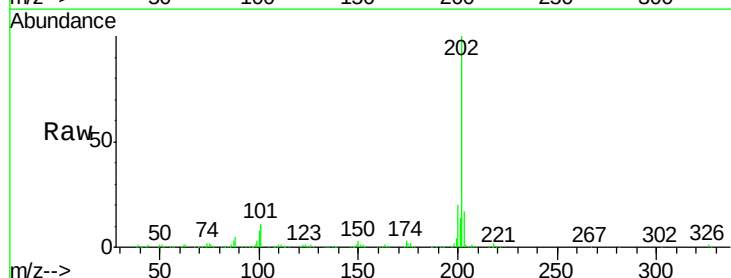

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

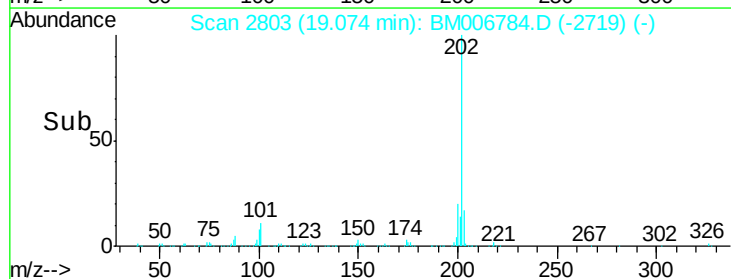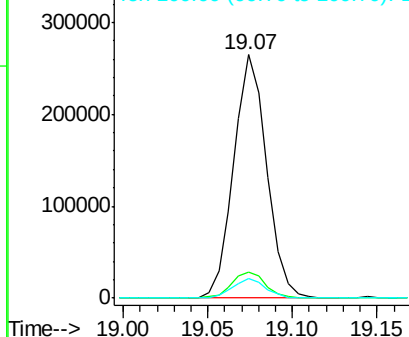

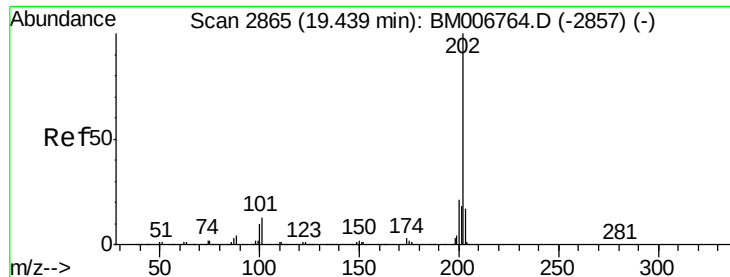





#31
 Pyrene
 Concen: 5.36 ng/ul
 RT: 19.44 min Scan# 2865
 Delta R.T. -0.01 min
 Lab File: BM006784.D
 Acq: 31 Jul 2016 11:54

Instrument :
 BNA_M
 ClientSampleId :
 D9ZP9

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	12.4	9.8	14.8
100	10.0	9.3	13.9




Manual Integrations
 APPROVED


sohil
 8/1/2016 7:06:04 PM

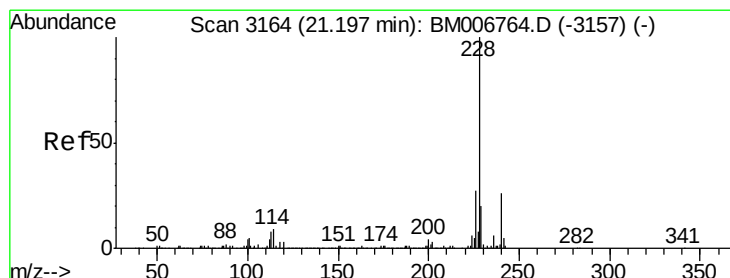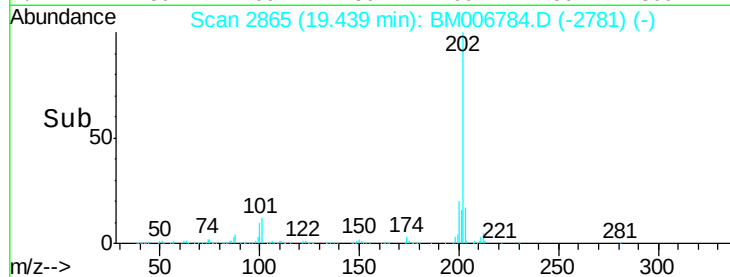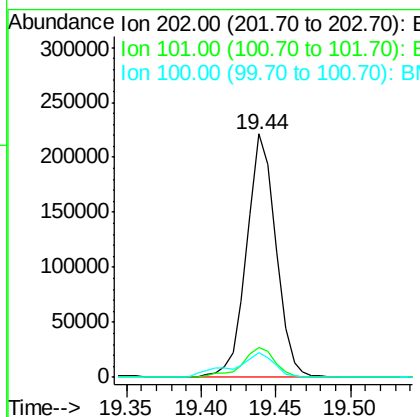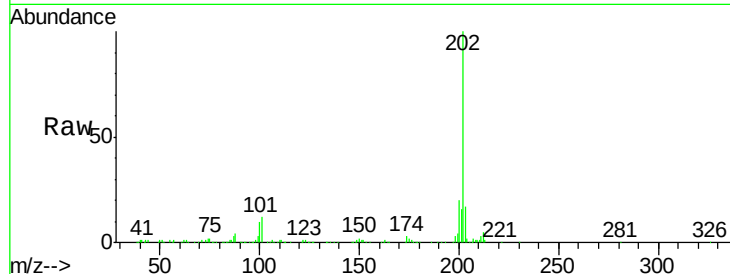

#32
 Benzo(a)anthracene
 Concen: 3.27 ng/ul
 RT: 21.20 min Scan# 3164
 Delta R.T. -0.00 min
 Lab File: BM006784.D
 Acq: 31 Jul 2016 11:54

Tgt Ion	Ratio	Resp Lower	Resp Upper
228	100		
229	21.2	16.6	25.0
226	28.2	21.0	31.4

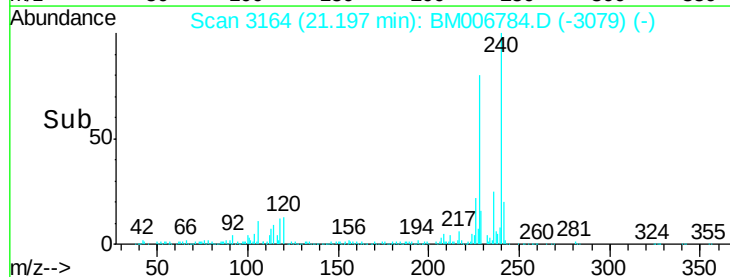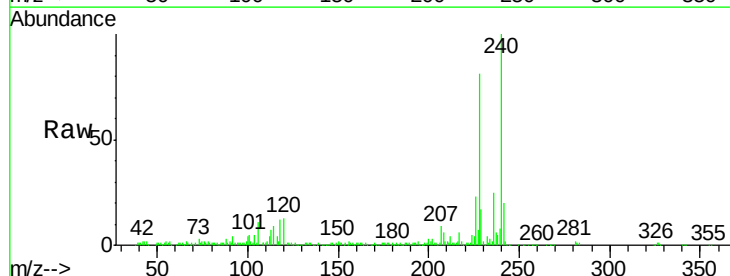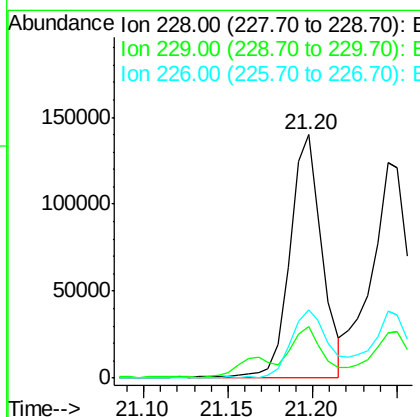

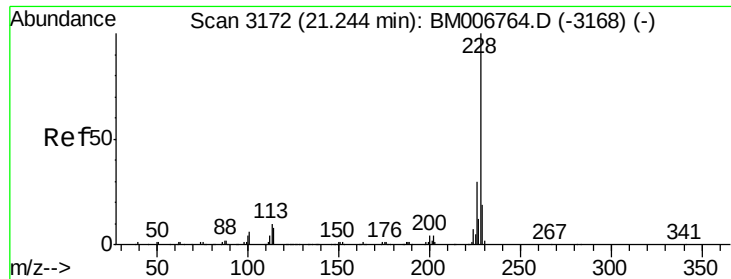





#33
Chrysene
 Concen: 3.65 ng/ul
 RT: 21.24 min Scan# 3172
 Delta R.T. -0.01 min
 Lab File: BM006784.D
 Acq: 31 Jul 2016 11:54

Instrument :
 BNA_M
 ClientSampleId :
 D9ZP9

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	188636		
226	31.0	23.4	35.2	
229	20.9	16.2	24.2	




Manual Integrations
 APPROVED


sohil
 8/1/2016 7:06:04 PM

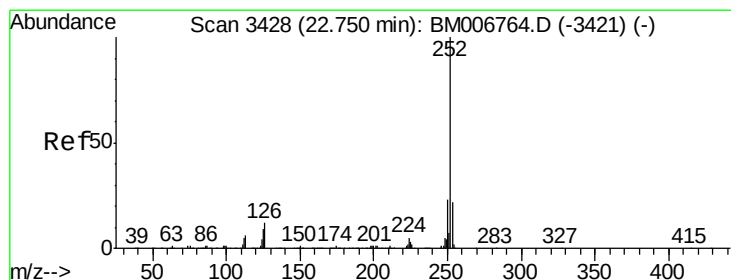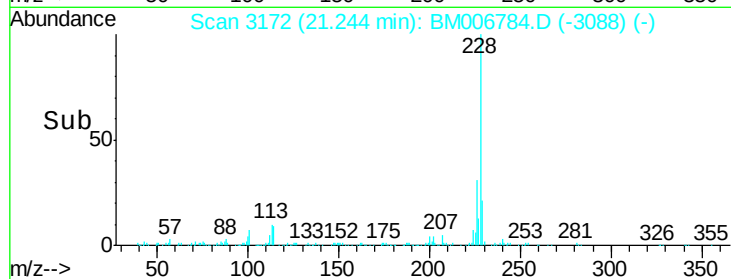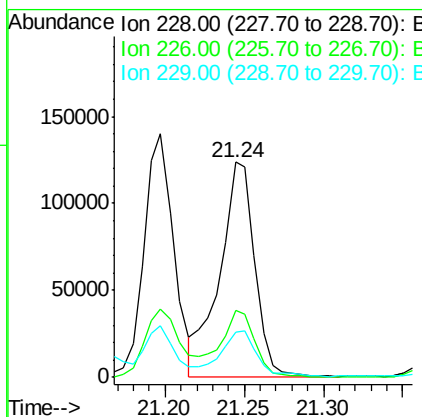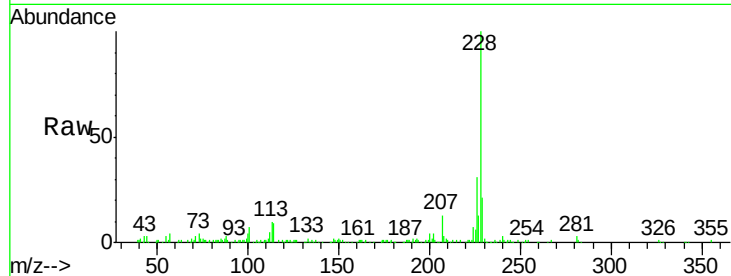

#35
Benzo(b)fluoranthene
 Concen: 5.23 ng/ul
 RT: 22.76 min Scan# 3429
 Delta R.T. -0.00 min
 Lab File: BM006784.D
 Acq: 31 Jul 2016 11:54

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	300468		
253	23.1	18.1	27.1	
125	10.4	7.6	11.4	

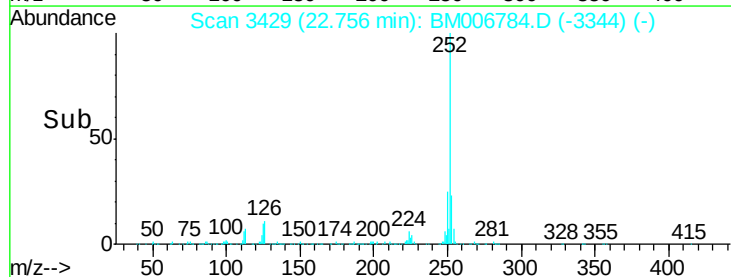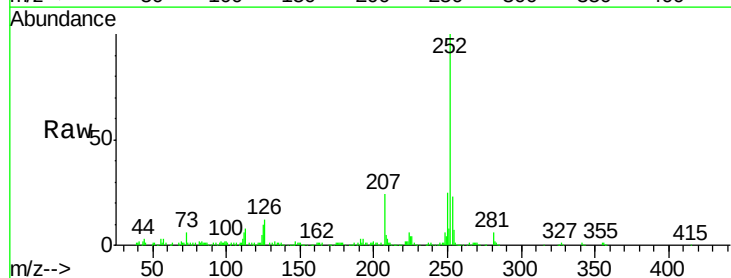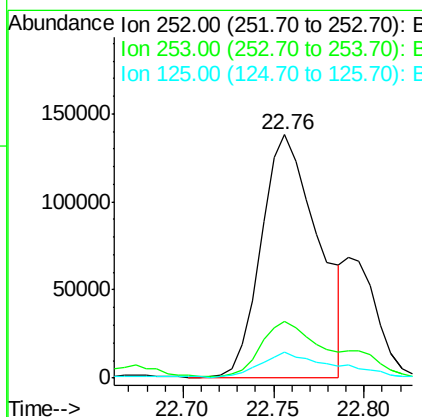

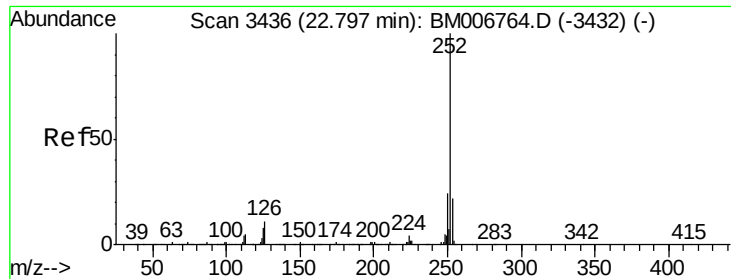





#36
Benzo(k)fluoranthene
Concen: 1.55 ng/ul m
RT: 22.79 min Scan# 3435
Delta R.T. -0.01 min
Lab File: BM006784.D
Acq: 31 Jul 2016 11:54

Instrument :
BNA_M
ClientSampled :
D9ZP9

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.8	26.8
125	10.6	7.7	11.5




Manual Integrations
APPROVED


sohil
8/1/2016 7:06:04 PM

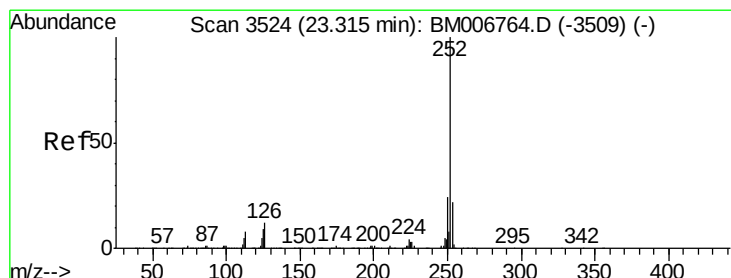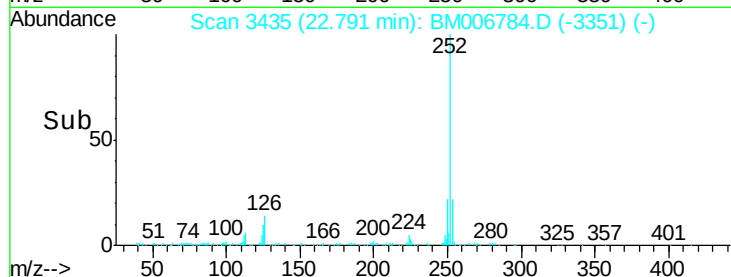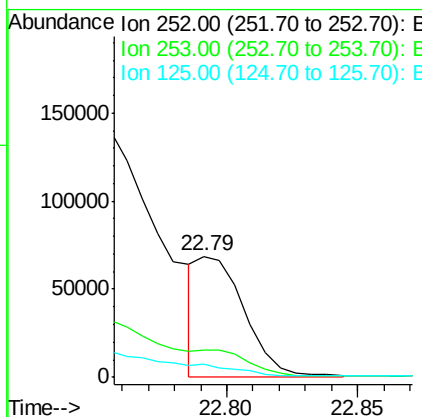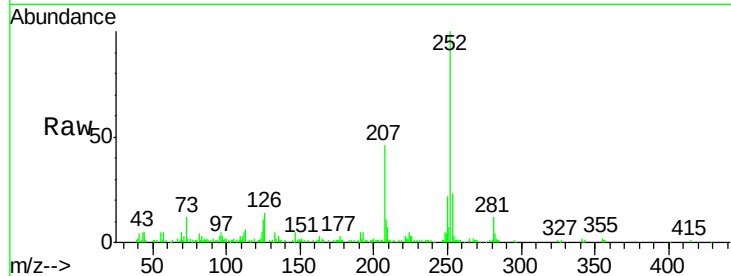

#38
Benzo(a)pyrene
Concen: 3.31 ng/ul
RT: 23.31 min Scan# 3524
Delta R.T. -0.01 min
Lab File: BM006784.D
Acq: 31 Jul 2016 11:54

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.3	17.4	26.0
125	10.7	8.2	12.2

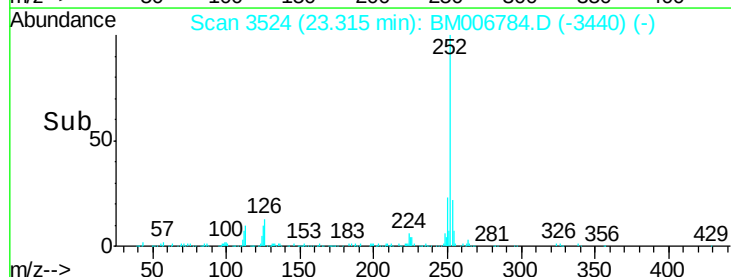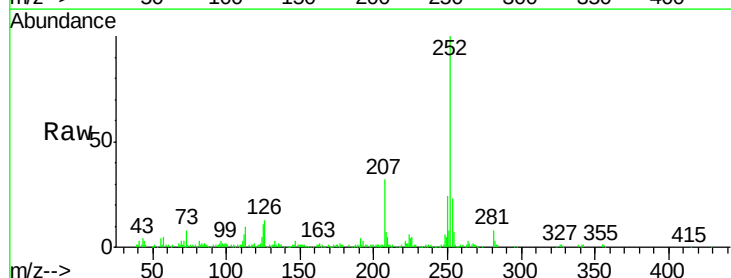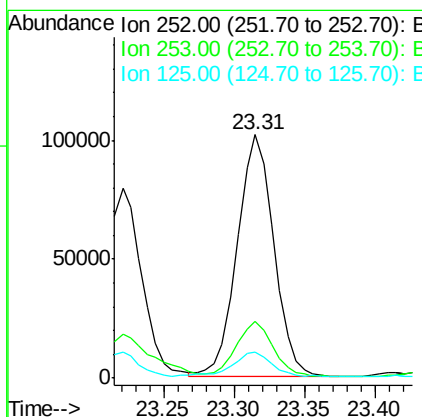

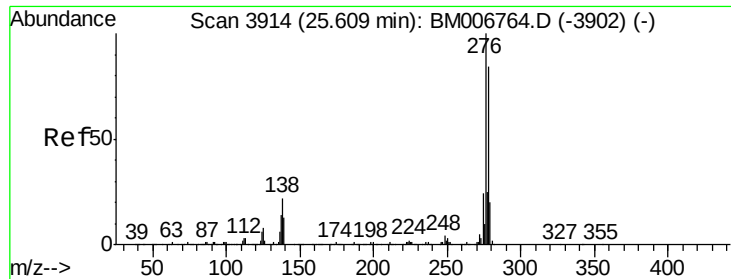





#39
 Indeno(1,2,3-cd)pyrene
 Concen: 2.33 ng/ul
 RT: 25.61 min Scan# 3915
 Delta R.T. -0.01 min
 Lab File: BM006784.D
 Acq: 31 Jul 2016 11:54

Instrument :
 BNA_M
 ClientSampleId :
 D9ZP9

Tgt Ion	Ratio	Lower	Upper
276	100		
138	18.3	15.8	23.6
277	22.2	19.0	28.6

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:06:04 PM

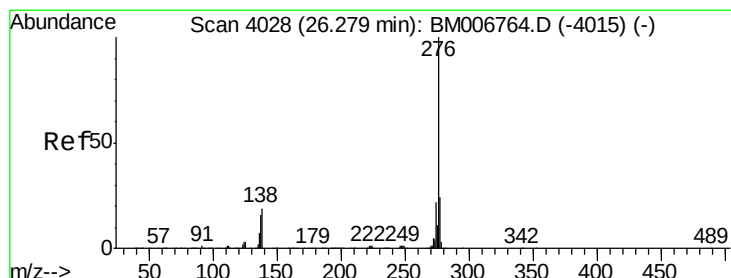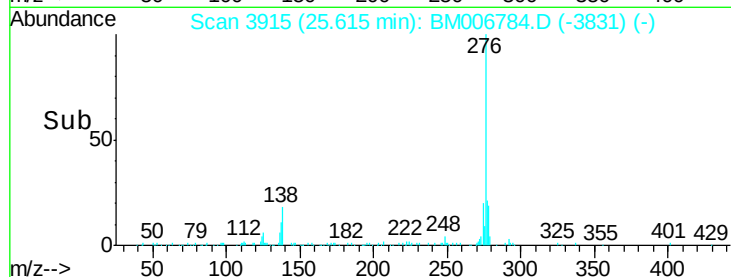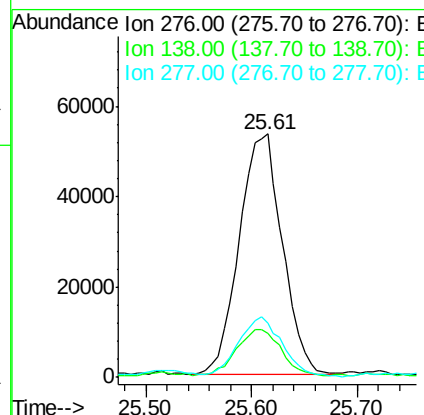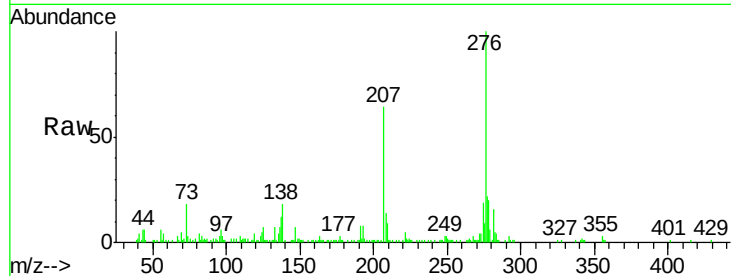

#41
 Benzo(g,h,i)perylene
 Concen: 2.28 ng/ul
 RT: 26.29 min Scan# 4029
 Delta R.T. -0.01 min
 Lab File: BM006784.D
 Acq: 31 Jul 2016 11:54

Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.8	13.9	20.9
277	25.3	19.8	29.6

