

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM073116\
 Data File : BM006804.D
 Acq On : 01 Aug 2016 00:43
 Operator : UM/SJ
 Sample : H4190-04
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9ZN3

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:07:38 PM

Quant Time: Aug 01 07:56:04 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 30 01:37:26 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	232315	20.00	ng/ul	0.00
7) Naphthalene-d8	10.38	136	974012	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.26	164	534449	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.01	188	1185113	20.00	ng/ul	0.00
29) Chrysene-d12	21.21	240	1283075	20.00	ng/ul	0.00
34) Perylene-d12	23.41	264	1380674	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.13	96	4888	0.85	ng/uL	0.00
3) Phenol-d5	6.79	99	206963	10.47	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	6.95	67	144935	11.84	ng/ul	0.00
5) 2-Chlorophenol-d4	7.14	132	174974	11.08	ng/ul	0.00
6) 4-Methylphenol-d8	8.32	113	128713	8.40	ng/ul	0.00
8) Nitrobenzene-d5	8.76	128	87344	11.85	ng/ul	0.00
9) 2-Nitrophenol-d4	9.47	143	94236	12.02	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.02	165	164673	11.11	ng/ul	0.00
12) 4-Chloroaniline-d4	10.53	131	153410	9.40	ng/ul	0.00
16) Dimethylphthalate-d6	13.67	166	505293	12.06	ng/ul	0.00
17) Acenaphthylene-d8	13.94	160	663806	12.41	ng/ul	0.00
20) 4-Nitrophenol-d4	14.50	143	56916	7.82	ng/ul	0.01
21) Fluorene-d10	15.26	176	462816	12.35	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.40	200	38805	6.31	ng/ul	0.00
26) Anthracene-d10	17.11	188	696122	12.37	ng/ul	0.00
30) Pyrene-d10	19.42	212	795263	13.60	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.27	264	804274	12.66	ng/ul	0.00

Target Compounds

						Qvalue
18) Acenaphthylene	13.98	152	69436	1.21	ng/ul	98
25) Phenanthrene	17.05	178	363434	5.45	ng/ul	99
27) Anthracene	17.14	178	99943	1.46	ng/ul	98
28) Fluoranthene	19.08	202	952845	12.17	ng/ul	96
31) Pyrene	19.44	202	822767	10.59	ng/ul	97
32) Benzo(a)anthracene	21.20	228	539212	6.93	ng/ul	97
33) Chrysene	21.25	228	539799	7.53	ng/ul	97
35) Benzo(b)fluoranthene	22.76	252	815865	9.86	ng/ul	98
36) Benzo(k)fluoranthene	22.80	252	258709m	3.23	ng/ul	
38) Benzo(a)pyrene	23.32	252	555931	6.90	ng/ul	97
39) Indeno(1,2,3-cd)pyrene	25.62	276	422759	4.53	ng/ul	98
40) Dibenzo(a,h)anthracene	25.61	278	120856m	1.56	ng/ul	
41) Benzo(g,h,i)perylene	26.30	276	384723	4.81	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM073116\
Data File : BM006804.D
Acq On : 01 Aug 2016 00:43
Operator : UM/SJ
Sample : H4190-04
Misc :
ALS Vial : 72 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9ZN3

Manual Integrations
APPROVED

sohil
8/1/2016 7:07:38 PM

Quant Time: Aug 01 07:56:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 30 01:37:26 2016
Response via : Initial Calibration

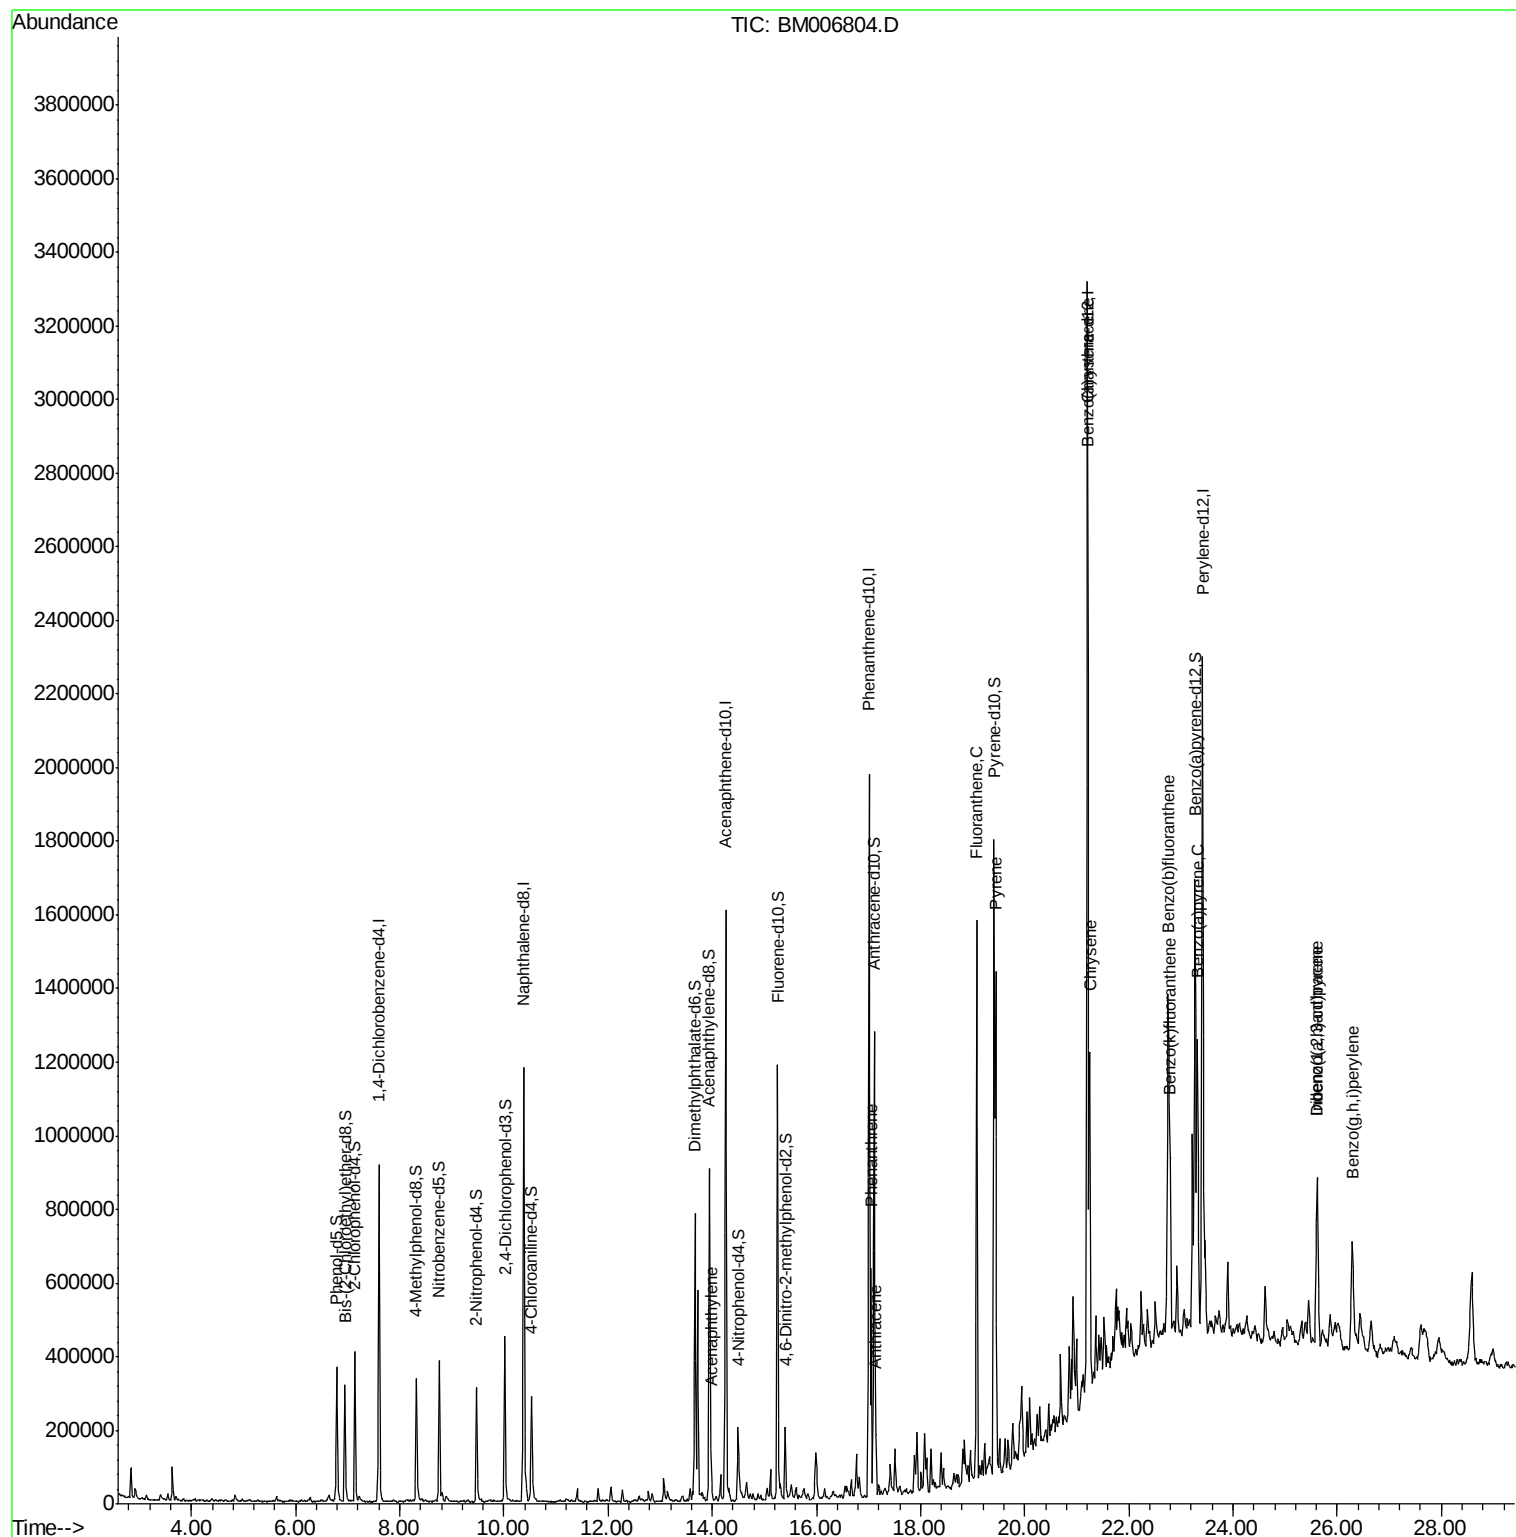

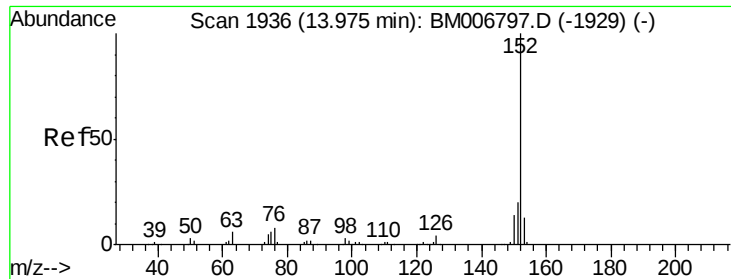





#18
Acenaphthylene
Concen: 1.21 ng/ul
RT: 13.98 min Scan# 1937
Delta R.T. -0.00 min
Lab File: BM006804.D
Acq: 01 Aug 2016 00:43

Instrument :
BNA_M
ClientSampled :
D9ZN3

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.4	17.3	25.9
153	14.8	11.1	16.7




Manual Integrations
APPROVED


sohil
8/1/2016 7:07:38 PM

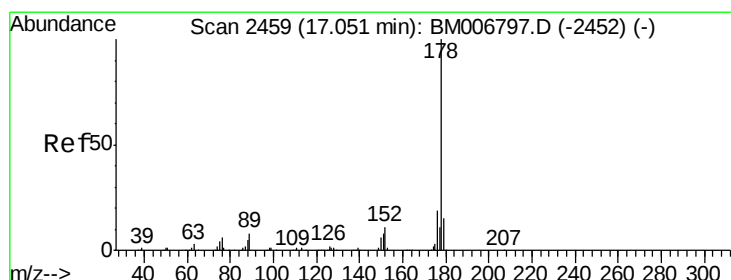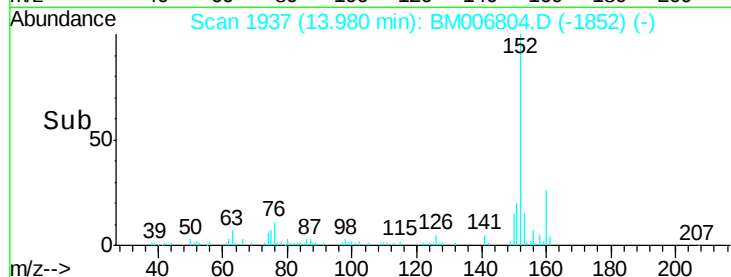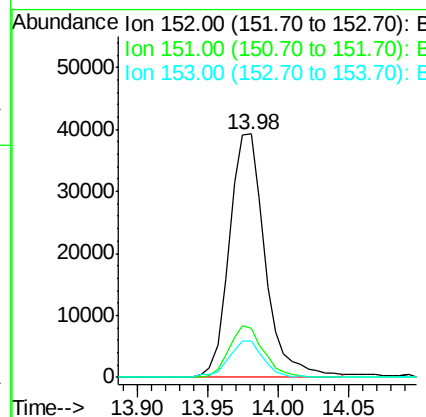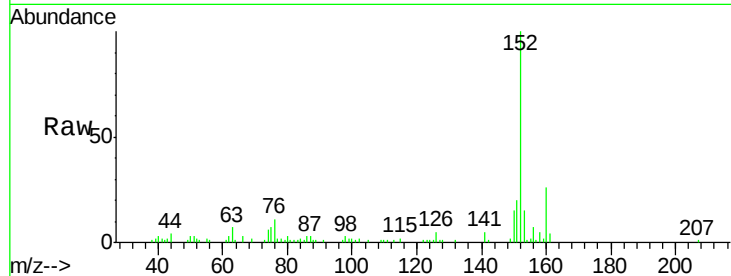

#25
Phenanthrene
Concen: 5.45 ng/ul
RT: 17.05 min Scan# 2459
Delta R.T. -0.00 min
Lab File: BM006804.D
Acq: 01 Aug 2016 00:43

Tgt Ion	Ratio	Lower	Upper
178	100		
179	14.6	11.8	17.8
176	19.2	14.8	22.2

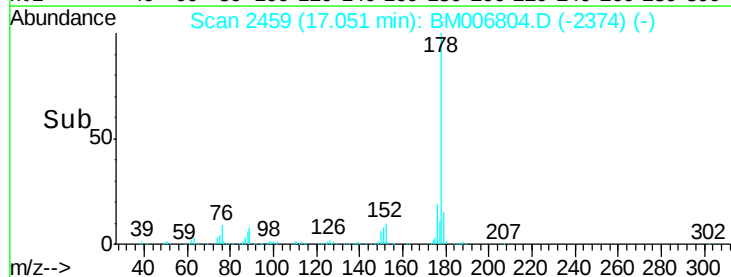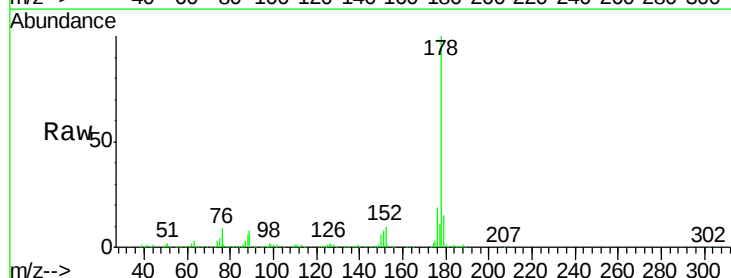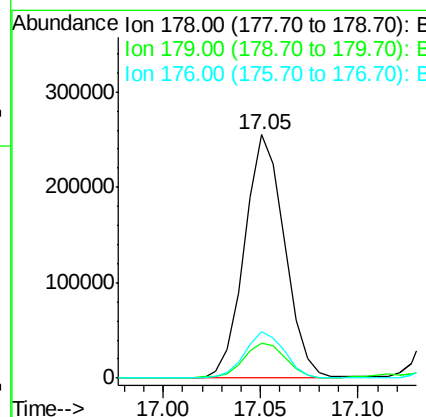

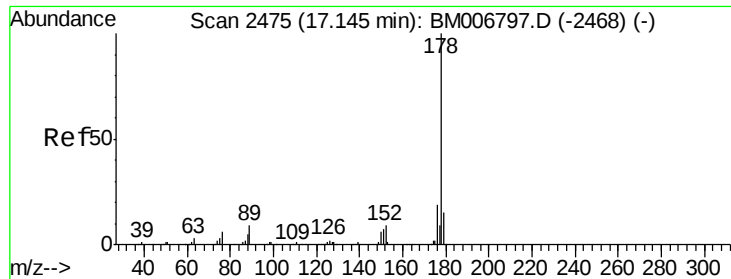





#27
 Anthracene
 Concen: 1.46 ng/ul
 RT: 17.14 min Scan# 2474
 Delta R.T. -0.01 min
 Lab File: BM006804.D
 Acq: 01 Aug 2016 00:43

Instrument :
 BNA_M
 ClientSampleId :
 D9ZN3

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	99943		
179	15.7	12.9	19.3	
176	18.3	15.6	23.4	




Manual Integrations
 APPROVED


sohil
 8/1/2016 7:07:38 PM

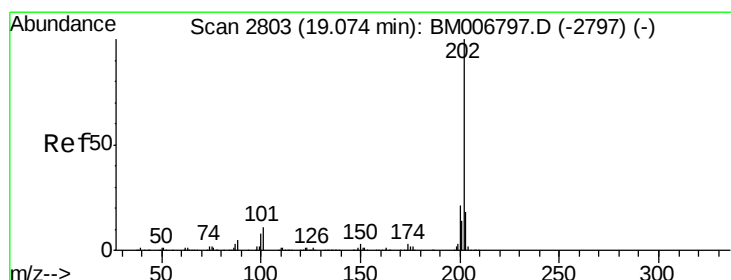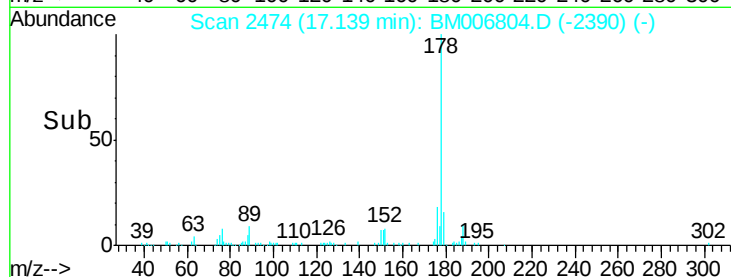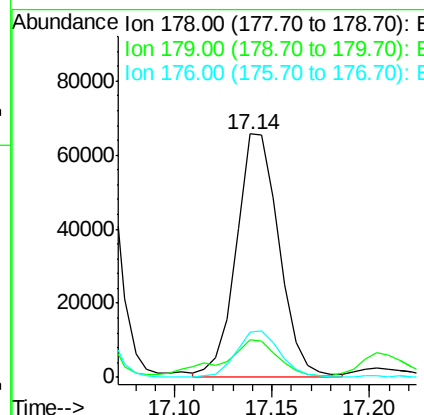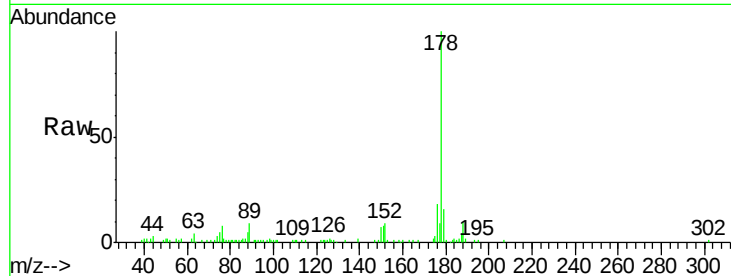

#28
 Fluoranthene
 Concen: 12.17 ng/ul
 RT: 19.08 min Scan# 2804
 Delta R.T. -0.00 min
 Lab File: BM006804.D
 Acq: 01 Aug 2016 00:43

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	952845		
101	9.8	8.9	13.3	
100	7.4	7.0	10.4	

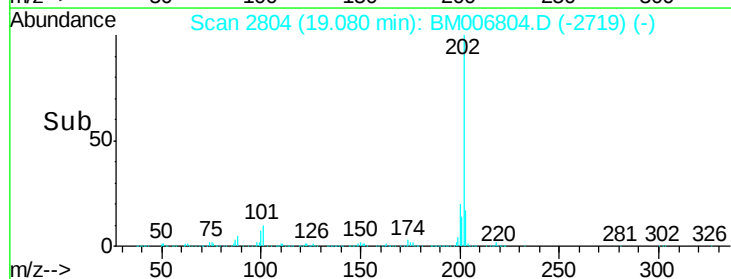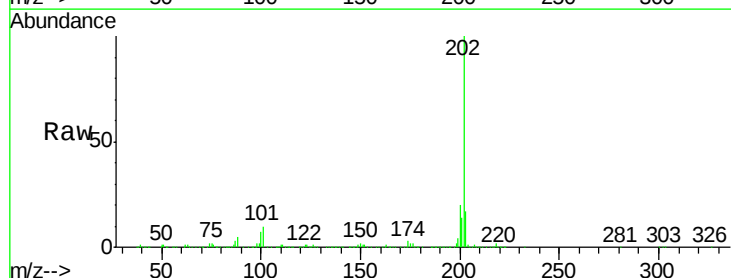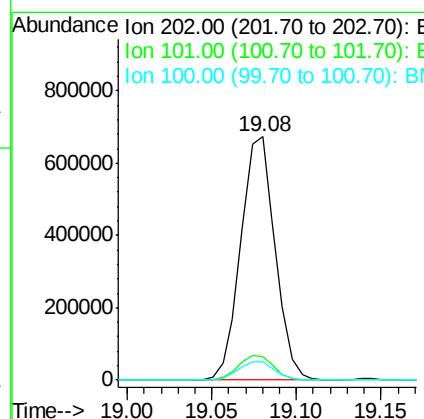

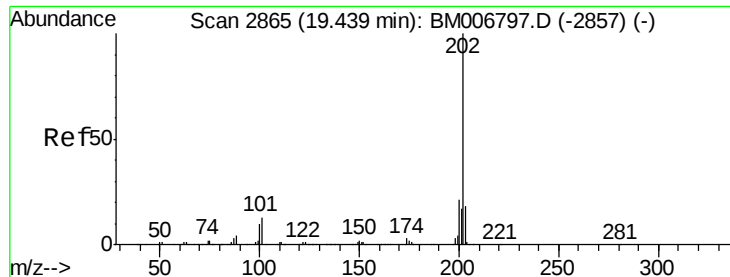





#31
 Pyrene
 Concen: 10.59 ng/ul
 RT: 19.44 min Scan# 2866
 Delta R.T. -0.00 min
 Lab File: BM006804.D
 Acq: 01 Aug 2016 00:43

Instrument :
 BNA_M
 ClientSampleId :
 D9ZN3

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	822767		
101	11.9	9.8	14.8	
100	9.5	9.3	13.9	




Manual Integrations
 APPROVED


sohil
 8/1/2016 7:07:38 PM

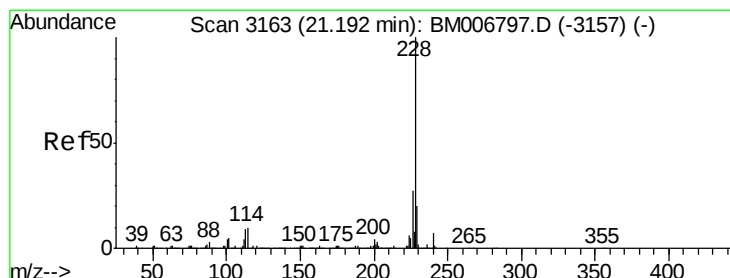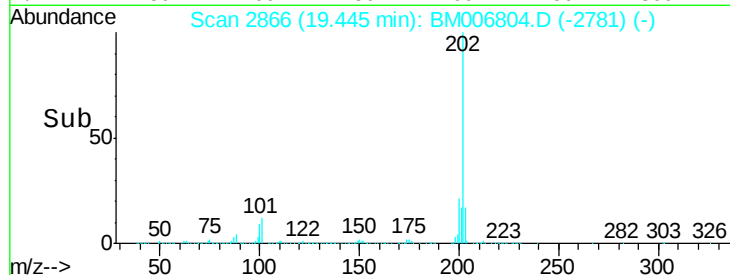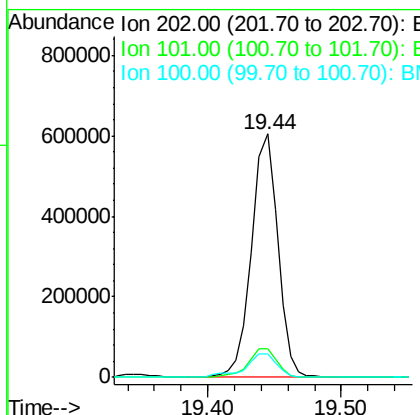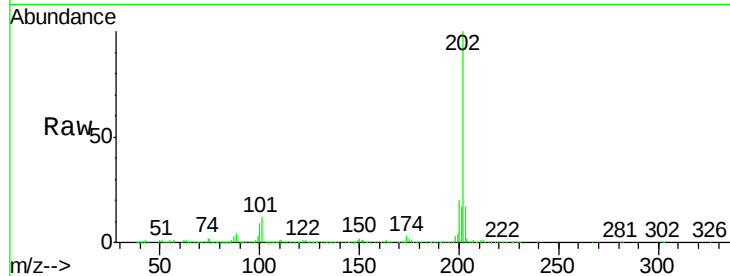

#32
 Benzo(a)anthracene
 Concen: 6.93 ng/ul
 RT: 21.20 min Scan# 3164
 Delta R.T. -0.00 min
 Lab File: BM006804.D
 Acq: 01 Aug 2016 00:43

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	539212		
229	21.0	16.6	25.0	
226	29.1	21.0	31.4	

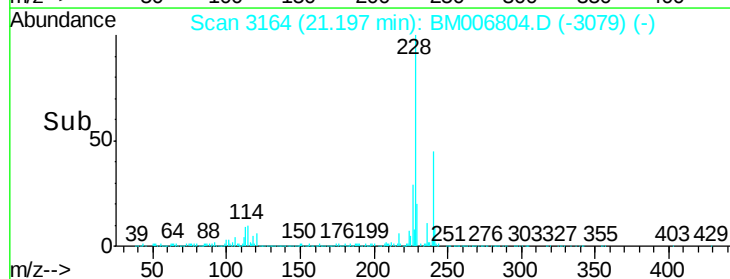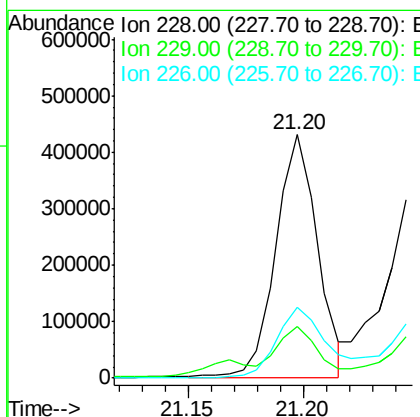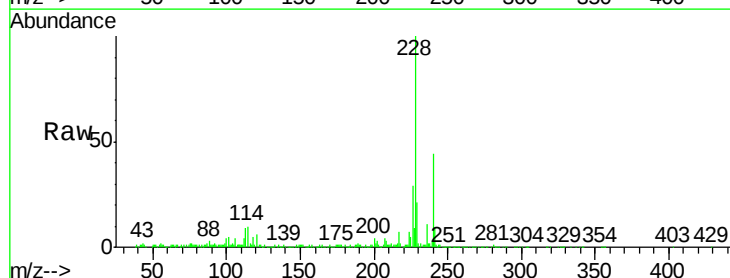

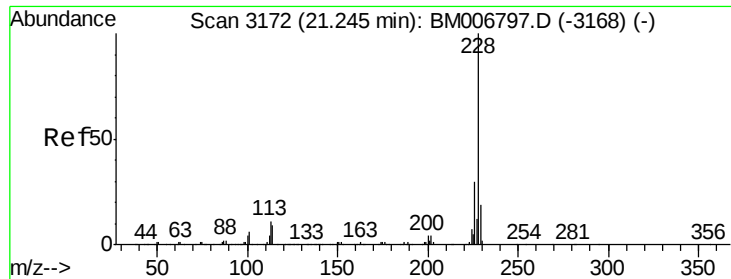





#33
Chrysene
 Concen: 7.53 ng/ul
 RT: 21.25 min Scan# 3173
 Delta R.T. -0.00 min
 Lab File: BM006804.D
 Acq: 01 Aug 2016 00:43

Instrument :
 BNA_M
 ClientSampled :
 D9ZN3

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	539799		
226	30.1	23.4	35.2	
229	22.1	16.2	24.2	




Manual Integrations
 APPROVED


sohil
 8/1/2016 7:07:38 PM

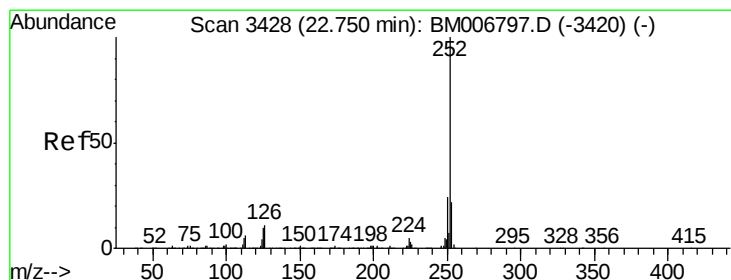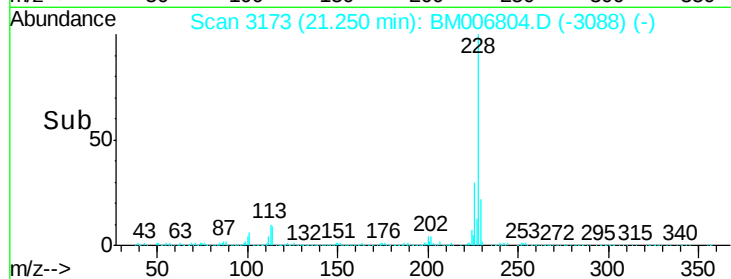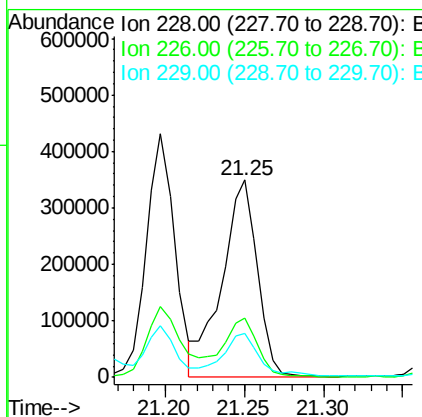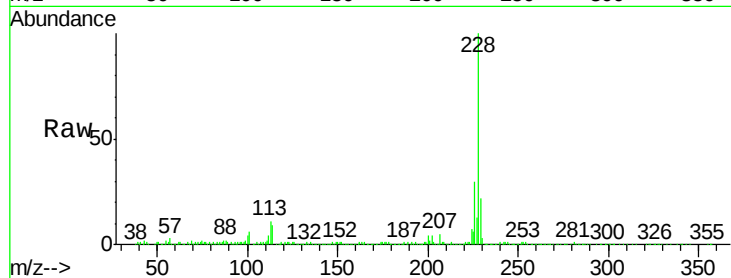

#35
Benzo(b)fluoranthene
 Concen: 9.86 ng/ul
 RT: 22.76 min Scan# 3429
 Delta R.T. -0.00 min
 Lab File: BM006804.D
 Acq: 01 Aug 2016 00:43

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	815865		
253	23.9	18.1	27.1	
125	9.6	7.6	11.4	

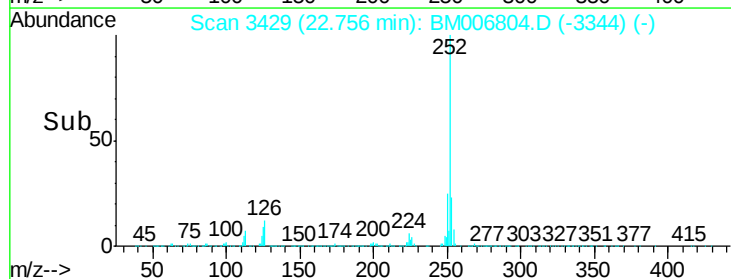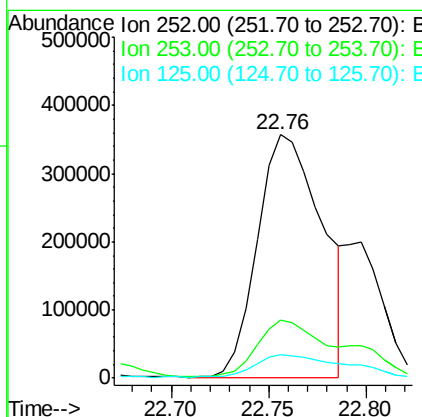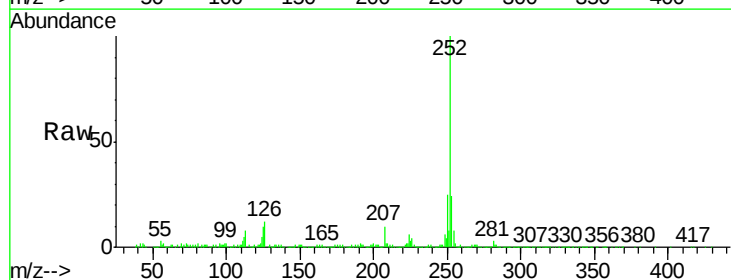

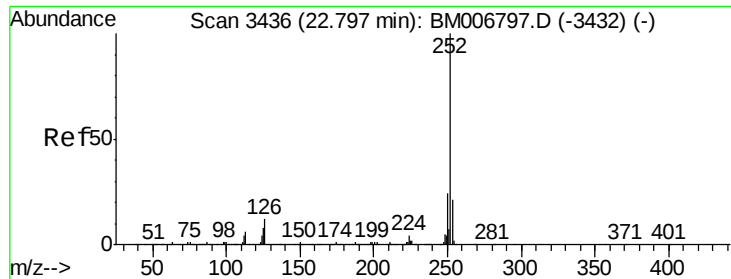


#36
Benzo(k)fluoranthene
Concen: 3.23 ng/ul m
RT: 22.80 min Scan# 3436
Delta R.T. -0.00 min
Lab File: BM006804.D
Acq: 01 Aug 2016 00:43

Instrument :
BNA_M
ClientSampled :
D9ZN3




Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.7	17.8	26.8
125	9.8	7.7	11.5

Manual Integrations
APPROVED

sohil
8/1/2016 7:07:38 PM

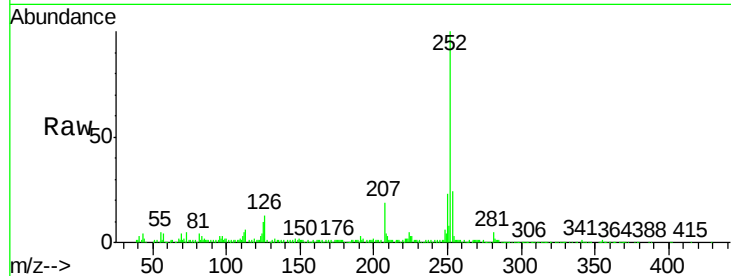




Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

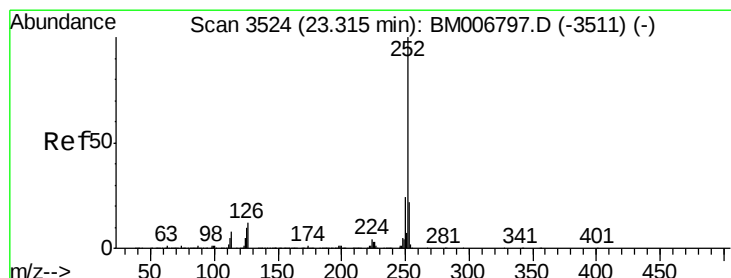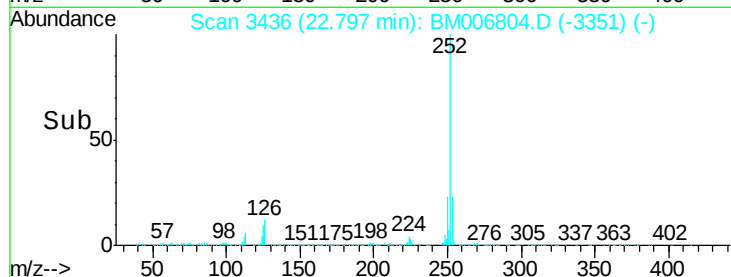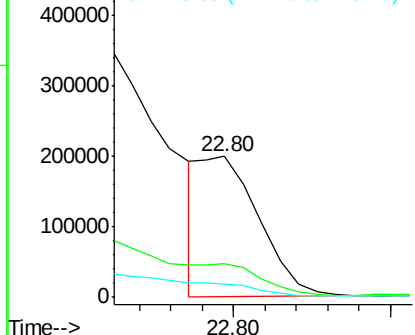


#38
Benzo(a)pyrene
Concen: 6.90 ng/ul
RT: 23.32 min Scan# 3525
Delta R.T. -0.00 min
Lab File: BM006804.D
Acq: 01 Aug 2016 00:43

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	17.4	26.0
125	9.5	8.2	12.2

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

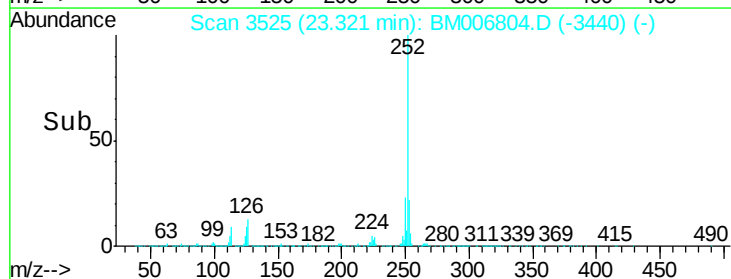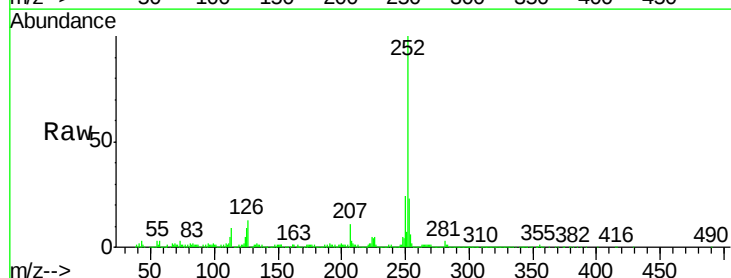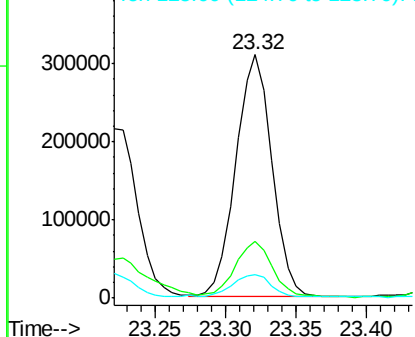

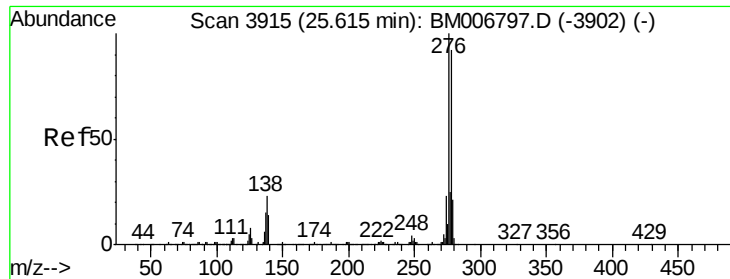





#39
Indeno(1,2,3-cd)pyrene
Concen: 4.53 ng/ul
RT: 25.62 min Scan# 3916
Delta R.T. -0.00 min
Lab File: BM006804.D
Acq: 01 Aug 2016 00:43

Instrument :
BNA_M
ClientSampleId :
D9ZN3

Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.1	15.8	23.6
277	25.2	19.0	28.6




Manual Integrations
APPROVED




sohil
8/1/2016 7:07:38 PM

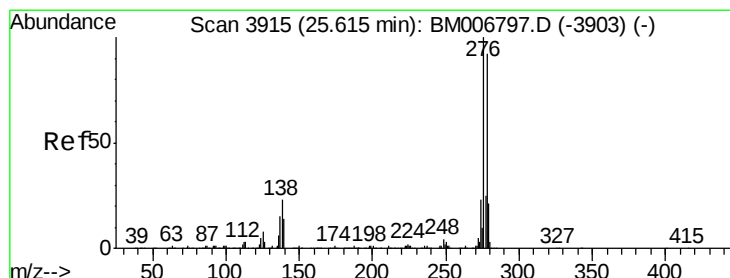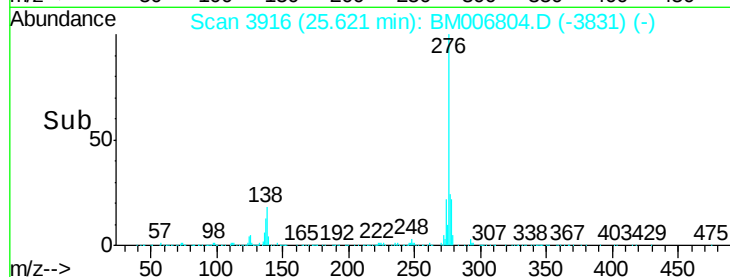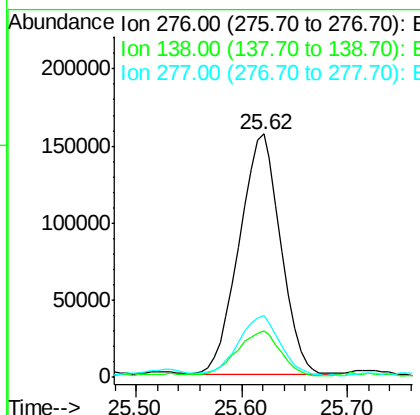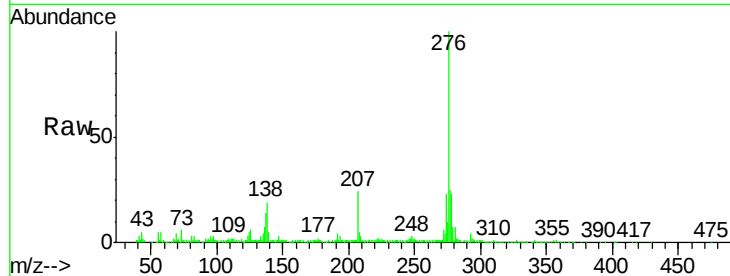

#40
Dibenzo(a,h)anthracene
Concen: 1.56 ng/ul m
RT: 25.61 min Scan# 3915
Delta R.T. -0.01 min
Lab File: BM006804.D
Acq: 01 Aug 2016 00:43

Tgt Ion	Ratio	Lower	Upper
278	100		
139	20.8	12.1	18.1#
279	28.3	19.8	29.8

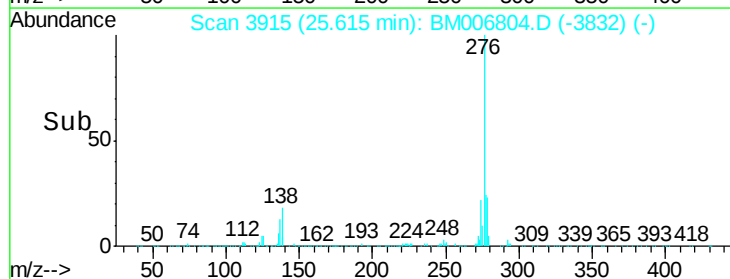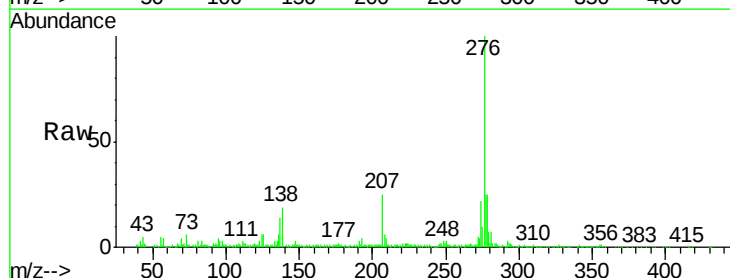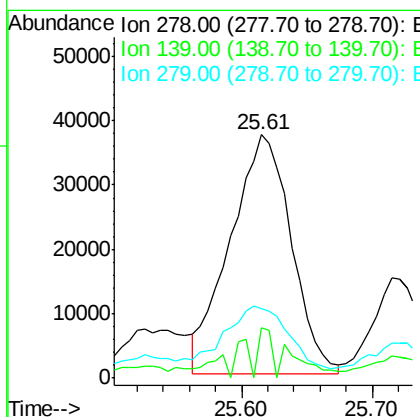

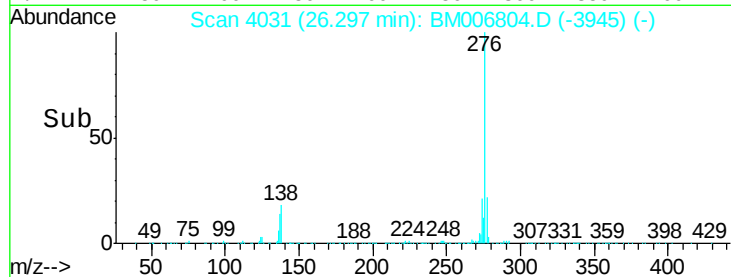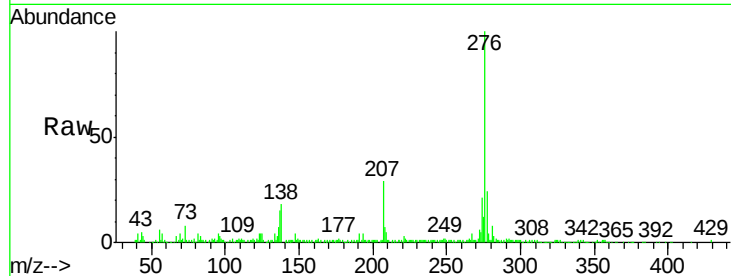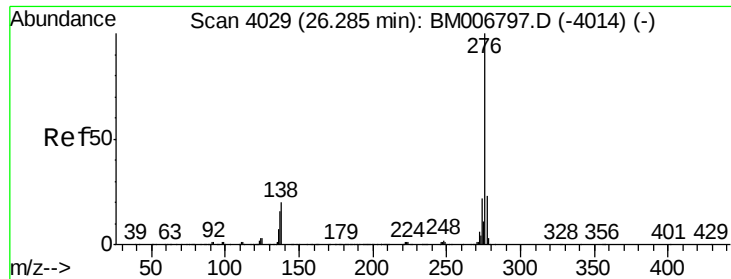

#41
 Benzo(g,h,i)perylene
 Concen: 4.81 ng/ul
 RT: 26.30 min Scan# 4031
 Delta R.T. 0.01 min
 Lab File: BM006804.D
 Acq: 01 Aug 2016 00:43

Tgt Ion:	276	Resp:	384723
Ion Ratio	Lower	Upper	
276	100		
138	18.2	13.9	20.9
277	23.7	19.8	29.6

Instrument :
 BNA_M
 ClientSampleId :
 D9ZN3

Manual Integrations
 APPROVED

sohil
 8/1/2016 7:07:38 PM

