
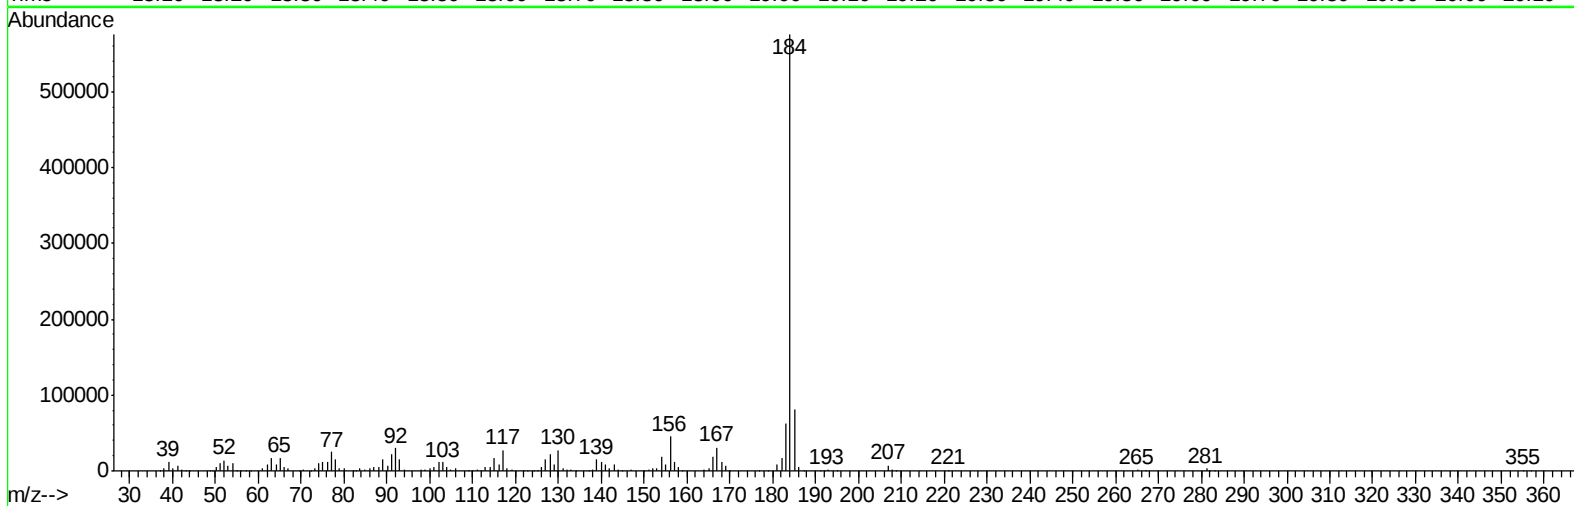


Data Path : Z:\HPCHEM1\BNA M\DATA\BM073117\
Data File : BM011062.D
Acq On : 31 Jul 2017 11:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 02:33:01 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

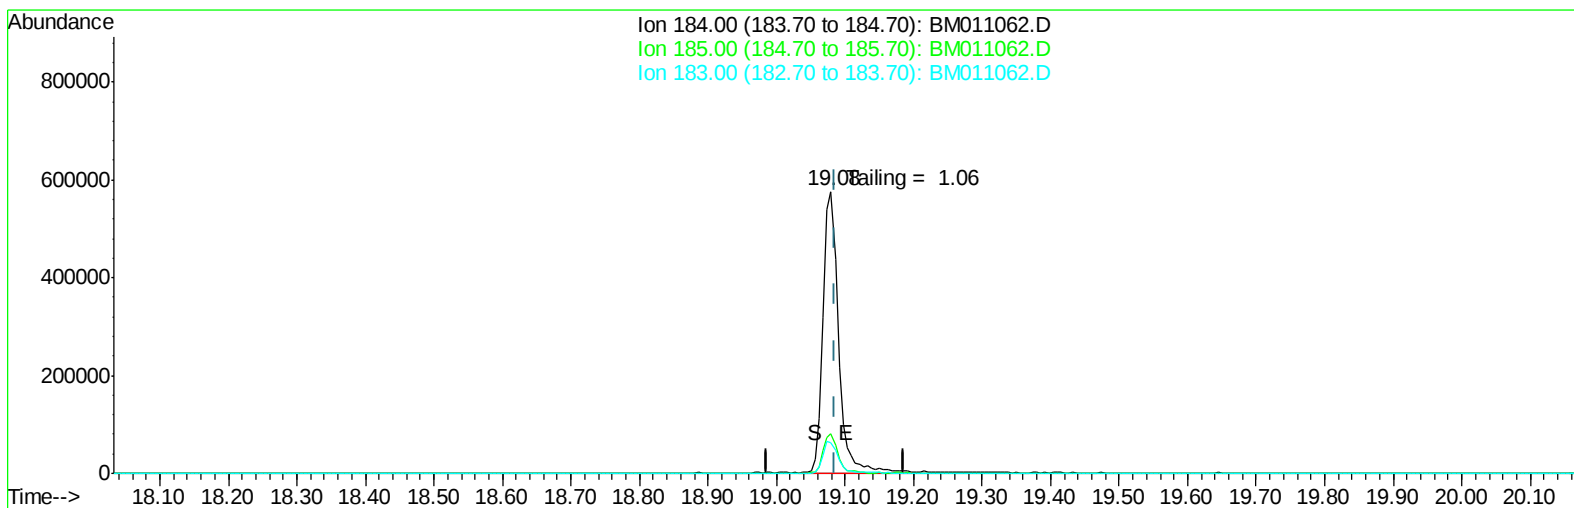

TIC: BM011062.D

(76) Benzidine



19.080min (-0.006) 150534.50ng

response 889497

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.98
183.00	11.10	10.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM073117\
Data File : BM011062.D
Acq On : 31 Jul 2017 11:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 02:33:01 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

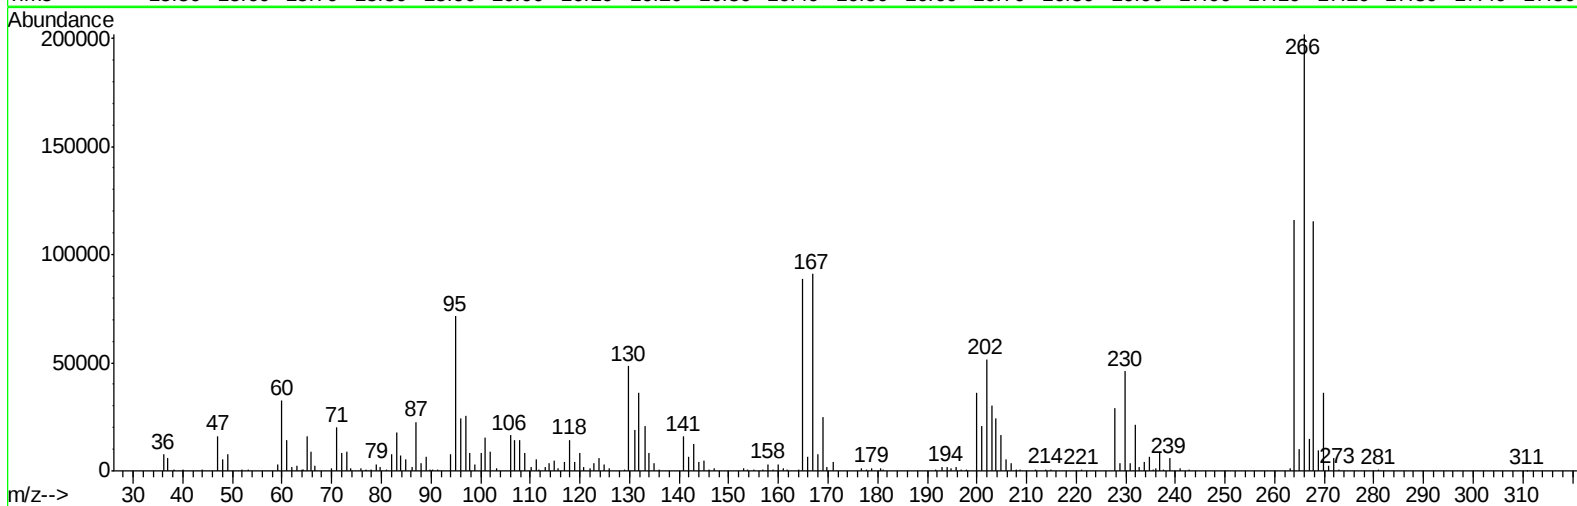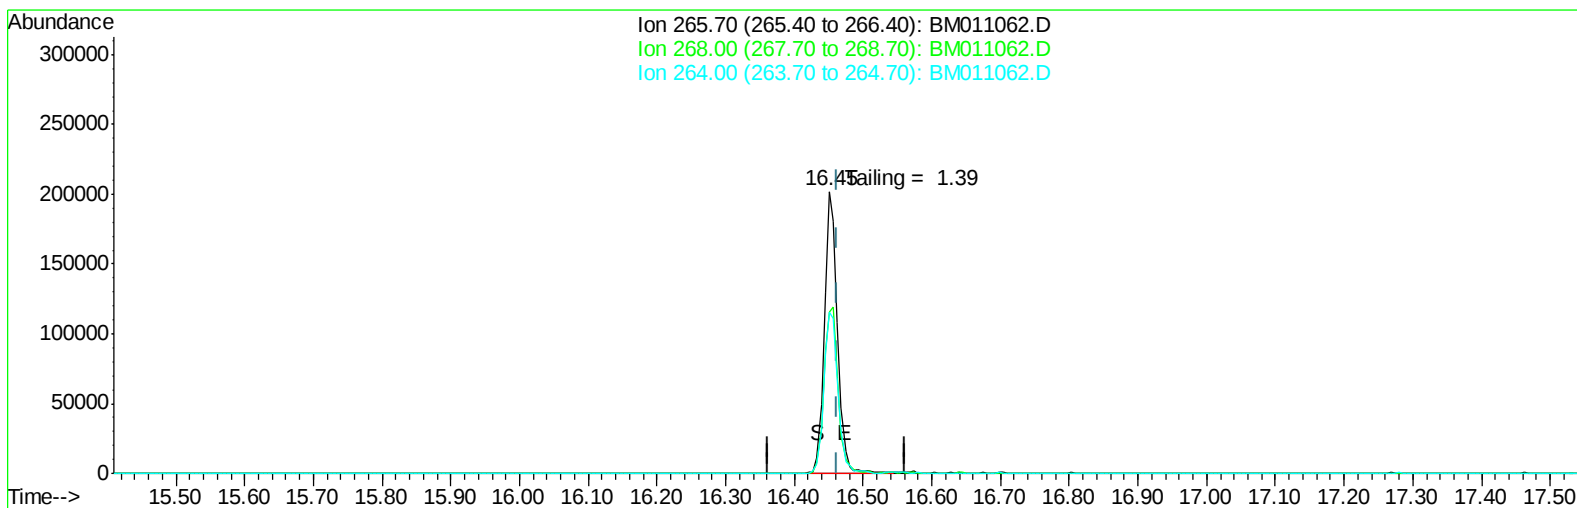

TIC: BM011062.D

(69) Pentachlorophenol (C)

16.451min (-0.012) 0.00ng

response 270340

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	57.09
264.00	61.20	57.36
0.00	0.00	0.00