


Data Path : Z:\HPCHEM1\BNA M\Data\BM073117\
 Data File : BM011062.D
 Acq On : 31 Jul 2017 11:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

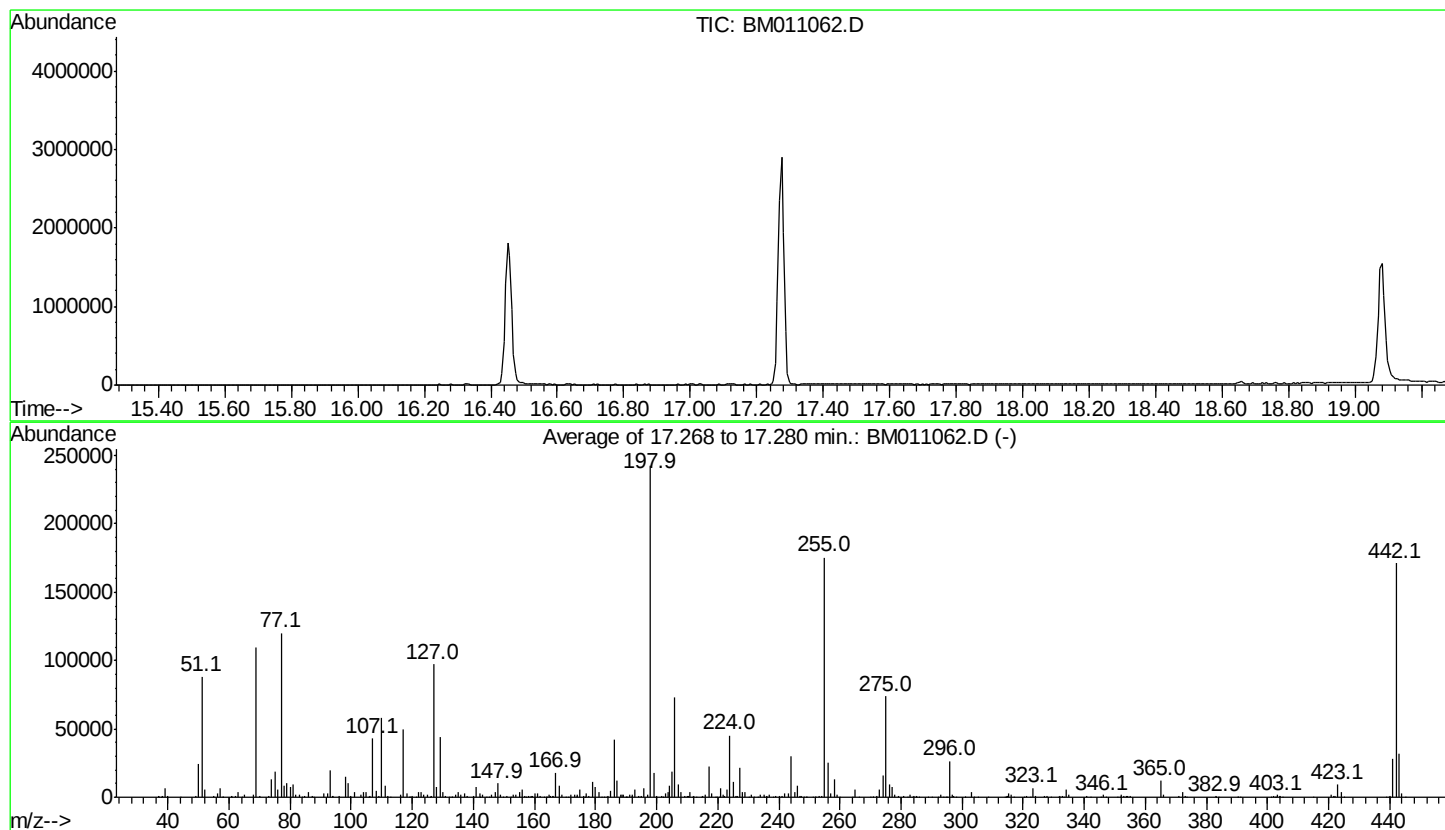

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	88165	PASS
68	69	0.00	2	1.7	1827	PASS
69	198	0.00	100	45.2	109672	PASS
70	69	0.00	2	0.7	730	PASS
127	198	10	80	40.0	97170	PASS
197	198	0.00	2	0.8	2002	PASS
198	198	100	100	100.0	242624	PASS
199	198	5	9	7.3	17782	PASS
275	198	10	60	30.5	73917	PASS
365	198	1	100	4.9	12004	PASS
441	443	0.01	100	87.9	28013	PASS
442	198	50	100	70.6	171346	PASS
443	442	15	24	18.6	31877	PASS