

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073120\
 Data File : BM026955.D
 Acq On : 31 Jul 2020 13:03
 Operator : JU/CG
 Sample : L1955-13
 Misc : MDL-WATER-06
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-06

Manual Integrations
 APPROVED

mohammad
 8/3/2020 12:23:26 PM

Quant Time: Jul 31 13:34:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 31 12:26:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	56226	20.00	ng/ul	0.00
18) Naphthalene-d8	10.44	136	217173	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	141761	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	312283	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	338716	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	338961	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	9843	7.99	ng/uL	0.00
5) Phenol-d5	6.84	99	153033	31.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	110997	33.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	118075	32.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	119116	31.43	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	55249	32.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	56706	36.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	118796	32.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	151420	34.35	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	374249	33.67	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	455230	32.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	62487	33.24	ng/ul	0.00
58) Fluorene-d10	15.29	176	318651	32.95	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	47052	33.80	ng/ul	0.00
71) Anthracene-d10	17.13	188	495595	31.75	ng/ul	0.00
79) Pyrene-d10	19.43	212	562763	31.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.29	264	604106	31.58	ng/ul	0.00

Target Compounds

					Ovalue	
2) 1,4-Dioxane	3.25	88	7436	4.855	ng/uL	91
4) Benzaldehyde	6.81	77	20685	5.155	ng/ul	91
6) Phenol	6.86	94	37317	7.080	ng/ul	92
8) Bis(2-Chloroethyl)ether	7.09	93	30495	7.311	ng/ul	94
10) 2-Chlorophenol	7.23	128	27867	7.282	ng/ul	97
11) 2-Methylphenol	8.10	108	26074	6.914	ng/ul	97
12) 2,2'-oxybis(1-Chloropropan	8.20	45	25516	6.908	ng/ul#	92
14) Acetophenone	8.47	105	46988	7.472	ng/ul	97
15) N-Nitroso-di-n-propylamine	8.46	70	28718	7.561	ng/ul#	93
16) 4-Methylphenol	8.42	108	27927	6.949	ng/ul	95
17) Hexachloroethane	8.74	117	14134	7.749	ng/ul	93
20) Nitrobenzene	8.84	77	43608	7.969	ng/ul	98
21) Isophorone	9.37	82	68602	7.111	ng/ul	96
23) 2-Nitrophenol	9.55	139	14176	8.025	ng/ul#	86
24) 2,4-Dimethylphenol	9.62	107	33969	7.361	ng/ul	95
25) Bis(2-Chloroethoxy)methane	9.85	93	40686	7.569	ng/ul#	94
27) 2,4-Dichlorophenol	10.08	162	27796	7.719	ng/ul	95
28) Naphthalene	10.48	128	91050	7.504	ng/ul	98
30) 4-Chloroaniline	10.58	127	35775	8.047	ng/ul	96
31) Hexachlorobutadiene	10.78	225	20533	8.074	ng/ul	92
32) Caprolactam	11.35	113	7699m	6.846	ng/ul	
33) 4-Chloro-3-methylphenol	11.72	107	28925	7.204	ng/ul	98
34) 2-Methylnaphthalene	12.10	142	64537	7.524	ng/ul	96

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073120\
 Data File : BM026955.D
 Acq On : 31 Jul 2020 13:03
 Operator : JU/CG
 Sample : L1955-13
 Misc : MDL-WATER-06
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 MDL-WATER-06

Manual Integrations
 APPROVED

mohammad
 8/3/2020 12:23:26 PM

Quant Time: Jul 31 13:34:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 31 12:26:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.32	142	62797	7.493	ng/ul	99
37) 1,2,4,5-Tetrachlorobenzene	12.48	216	36082	7.447	ng/ul	97
38) Hexachlorocyclopentadiene	12.47	237	19043	5.796	ng/ul	96
39) 2,4,6-Trichlorophenol	12.71	196	20796	7.490	ng/ul	96
40) 2,4,5-Trichlorophenol	12.78	196	22330	7.527	ng/ul	91
41) 1,1'-Biphenyl	13.12	154	86629	7.313	ng/ul	98
42) 2-Chloronaphthalene	13.16	162	71279	7.478	ng/ul	97
43) 2-Nitroaniline	13.35	65	21726	7.664	ng/ul	87
45) Dimethylphthalate	13.75	163	91167	7.815	ng/ul	98
46) 2,6-Dinitrotoluene	13.86	165	14716	7.155	ng/ul#	80
48) Acenaphthylene	14.01	152	105084	7.312	ng/ul	100
49) 3-Nitroaniline	14.18	138	13038	6.485	ng/ul	97
50) Acenaphthene	14.35	153	72533	7.325	ng/ul	96
51) 2,4-Dinitrophenol	14.39	184	6314	7.667	ng/ul#	78
53) 4-Nitrophenol	14.49	109	18191	9.658	ng/ul	87
54) Dibenzofuran	14.69	168	105874	7.714	ng/ul	92
55) 2,4-Dinitrotoluene	14.65	165	23142	7.831	ng/ul	91
56) 2,3,4,6-Tetrachlorophenol	14.92	232	20070	8.623	ng/ul#	97
57) Diethylphthalate	15.13	149	91672	7.837	ng/ul	97
59) Fluorene	15.34	166	88926	7.694	ng/ul	97
60) 4-Chlorophenyl-phenylether	15.34	204	44708	7.772	ng/ul	92
61) 4-Nitroaniline	15.35	138	14179	5.754	ng/ul	89
64) 4,6-Dinitro-2-methylphenol	15.41	198	12674	8.012	ng/ul#	78
65) N-Nitrosodiphenylamine	15.55	169	72109	7.059	ng/ul	96
66) 4-Bromophenyl-phenylether	16.24	248	26587	7.257	ng/ul	94
67) Hexachlorobenzene	16.35	284	32165	7.742	ng/ul	97
68) Atrazine	16.51	200	27013	7.204	ng/ul	97
69) Pentachlorophenol	16.69	266	15283	7.393	ng/ul	96
70) Phenanthrene	17.07	178	140700	7.422	ng/ul	98
72) Anthracene	17.17	178	142413	7.309	ng/ul	98
73) 1,2,3,4-Tetrachlorobenzene	13.09	216	34852	7.104	ng/uL	97
74) Pentachlorobenzene	14.62	250	35549	7.473	ng/uL	98
75) Carbazole	17.43	167	122665	7.122	ng/ul	98
76) Di-n-butylphthalate	18.02	149	147201	7.265	ng/ul	99
77) Fluoranthene	19.09	202	164748	7.361	ng/ul	96
80) Pvrene	19.46	202	171278	6.950	ng/ul#	95
81) Butylbenzylphthalate	20.38	149	63125	6.889	ng/ul	97
82) 3,3'-Dichlorobenzidine	21.15	252	46872	5.853	ng/ul	100
83) Benzo(a)anthracene	21.21	228	171848	7.361	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.17	149	93554	6.810	ng/ul#	98
85) Chrysene	21.26	228	168659	7.408	ng/ul	99
87) Di-n-octyl phthalate	22.04	149	156474	6.283	ng/ul	100
88) Benzo(b)fluoranthene	22.78	252	172811	7.127	ng/ul	96
89) Benzo(k)fluoranthene	22.82	252	177593	7.633	ng/ul	98
91) Benzo(a)pyrene	23.34	252	160151	7.319	ng/ul	98
92) Indeno(1,2,3-cd)pyrene	25.64	276	205180	7.559	ng/ul	99
93) Dibenzo(a,h)anthracene	25.65	278	174111	7.584	ng/ul	99
94) Benzo(a,h,i)perylene	26.31	276	168781	7.520	ng/ul	98

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM073120\
Data File : BM026955.D
Acq On : 31 Jul 2020 13:03
Operator : JU/CG
Sample : L1955-13
Misc : MDL-WATER-06
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06


Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM

Quant Time: Jul 31 13:34:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 31 12:26:02 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 4.855 ng/uL

RT: 3.25 min Scan# 88

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M


ClientSampleId :

MDL-WATER-06

Tot Ion:	88	Resp:	7436
Ion	Ratio	Lower	Upper
88	100		
43	30.6	24.7	37.1
58	53.6	50.8	76.2

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM




Abundance Ion 88.00 (87.70 to 88.70): BM026955.D (-54) (-)


Ion 43.00 (42.70 to 43.70): BM026955.D (-54) (-)

Ion 58.00 (57.70 to 58.70): BM026955.D (-54) (-)

Time-->

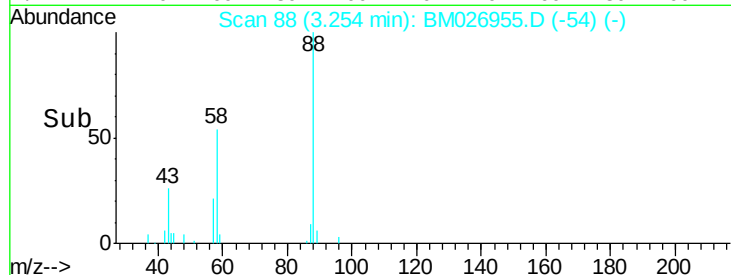

Time-->



#4

Benzaldehyde

Concen: 5.155 ng/uL


RT: 6.81 min Scan# 692

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tgt Ion:	77	Resp:	20685
Ion	Ratio	Lower	Upper
77	100		
105	71.9	64.9	97.3
106	71.5	62.5	93.7




Abundance Ion 77.00 (76.70 to 77.70): BM026955.D (-658) (-)




Ion 105.00 (104.70 to 105.70): BM026955.D (-658) (-)

Ion 106.00 (105.70 to 106.70): BM026955.D (-658) (-)

Time-->



Time-->

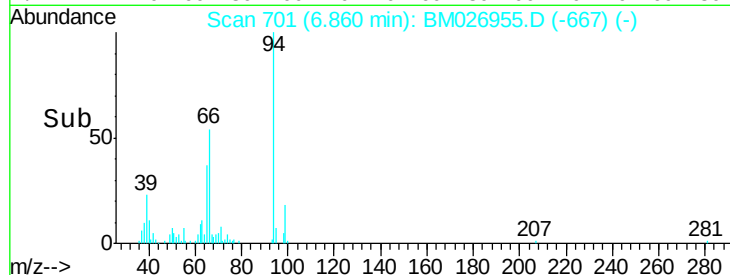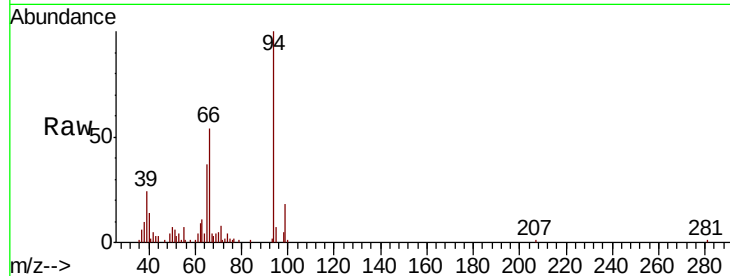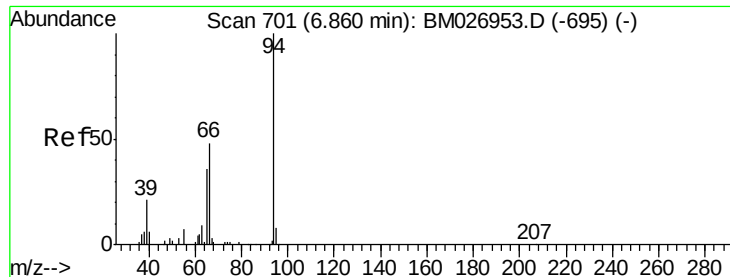

#6

Phenol

Concen: 7.080 ng/ul

RT: 6.86 min Scan# 701

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tot Ion:	94	Resp:	37317
Ion	Ratio	Lower	Upper
94	100		
65	36.9	26.2	39.4
66	53.8	38.2	57.2

Instrument :





BNA_M

ClientSampleId :

MDL-WATER-06

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM

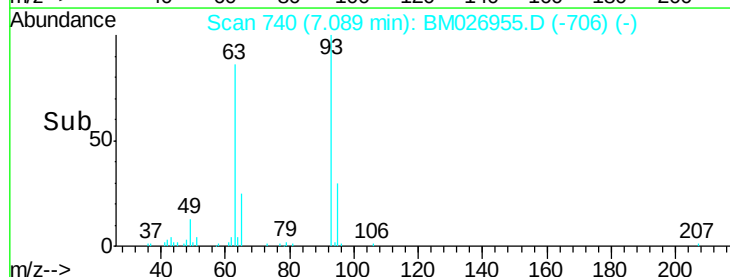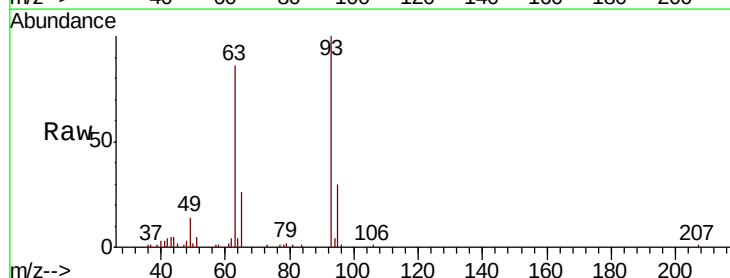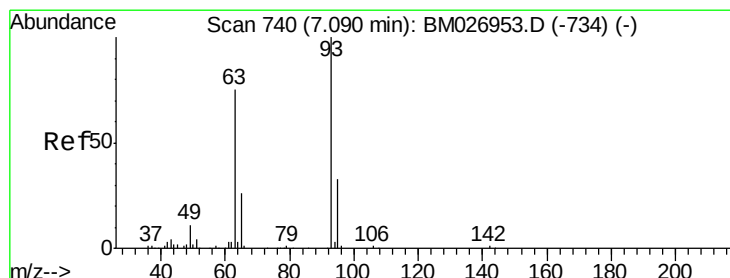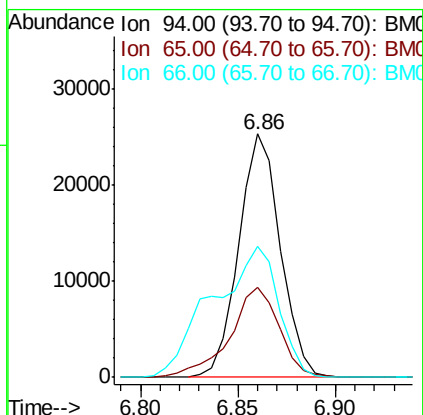

#8

Bis(2-Chloroethyl)ether

Concen: 7.311 ng/ul


RT: 7.09 min Scan# 740


Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tgt Ion:	93	Resp:	30495
Ion	Ratio	Lower	Upper
93	100		
63	85.8	62.9	94.3
95	30.1	24.6	37.0

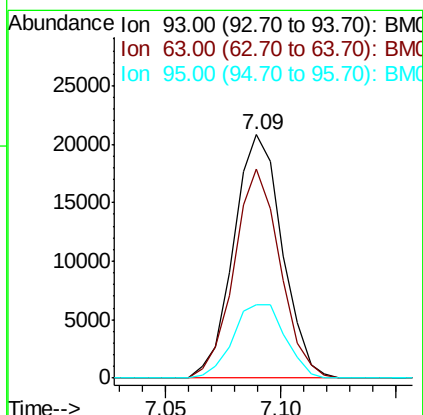







#10
2-Chlorophenol
Concen: 7.282 ng/ul
RT: 7.23 min Scan# 764
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
128	100		
64	51.6	43.4	65.2
130	32.1	26.3	39.5




Manual Integrations
APPROVED




mohammad
8/3/2020 12:23:26 PM

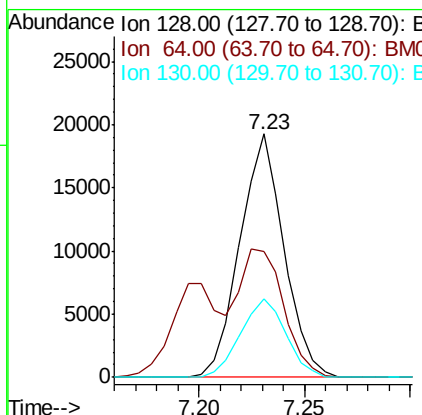

#11
2-Methylphenol
Concen: 6.914 ng/ul
RT: 8.10 min Scan# 912
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
108	100		
107	93.3	72.5	108.7









#12
2,2'-oxvbis(1-Chloropropane)
Concen: 6.908 ng/ul
RT: 8.20 min Scan# 928
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
45	100		
77	28.1	19.7	29.5
79	22.5	14.9	22.3#


Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM



#14
Acetophenone
Concen: 7.472 ng/ul
RT: 8.47 min Scan# 975
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
105	100		
77	94.2	74.0	111.0
51	25.4	17.3	25.9

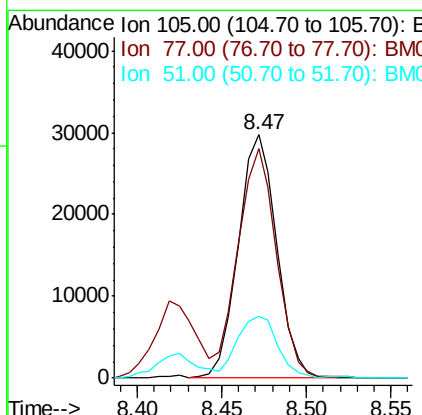



#15

N-Nitroso-di-n-propylamine

Concen: 7.561 ng/ul

RT: 8.46 min Scan# 973

Delta R.T. -0.01 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-06

Tot Ion	Ion	Ratio	Lower	Upper
70	100			
42	47.6	34.2	51.4	
101	8.8	6.4	9.6	
130	12.6	13.2	19.8	

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM

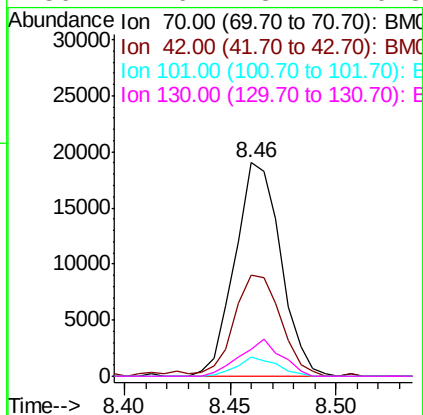

#16

4-Methylphenol

Concen: 6.949 ng/ul




RT: 8.42 min Scan# 967


Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tgt Ion	Ion	Ratio	Lower	Upper
108	100			
107	116.8	88.8	133.2	

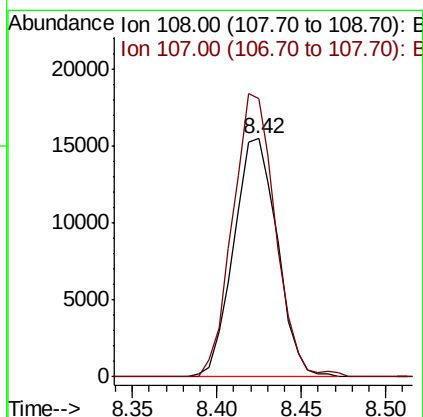



#17

Hexachloroethane

Concen: 7.749 ng/ul

RT: 8.74 min Scan# 1020

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-06

Tot Ion:	117	Resp:	14134
Ion Ratio	Lower	Upper	
117	100		
201	92.5	80.8	121.2
199	58.7	50.3	75.5

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM



#20

Nitrobenzene

Concen: 7.969 ng/ul




RT: 8.84 min Scan# 1038


Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tgt Ion:	77	Resp:	43608
Ion Ratio	Lower	Upper	
77	100		
123	36.2	28.3	42.5
65	12.5	11.0	16.6



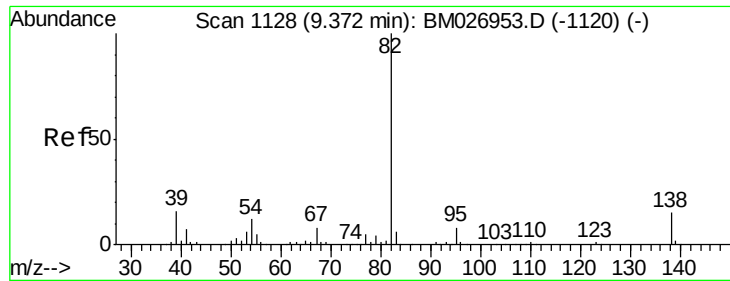

#21

Isophorone

Concen: 7.111 ng/ul

RT: 9.37 min Scan# 1128

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-06

Tot Ion:	82	Resp:	68602
Ion Ratio	Lower	Upper	
82	100		
95	8.0	6.0	9.0
138	16.7	11.5	17.3

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM

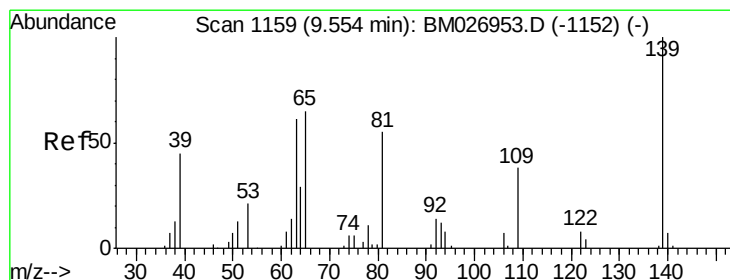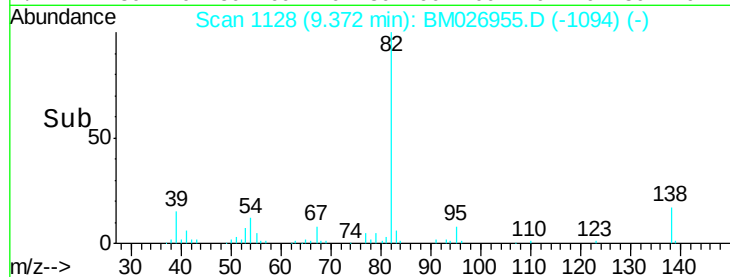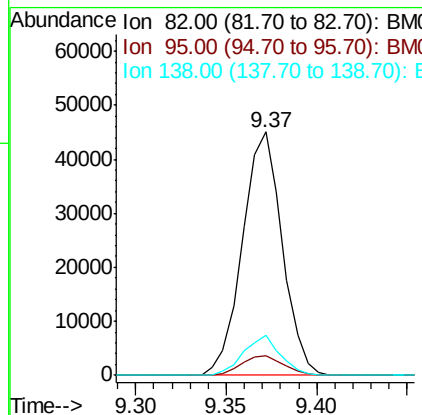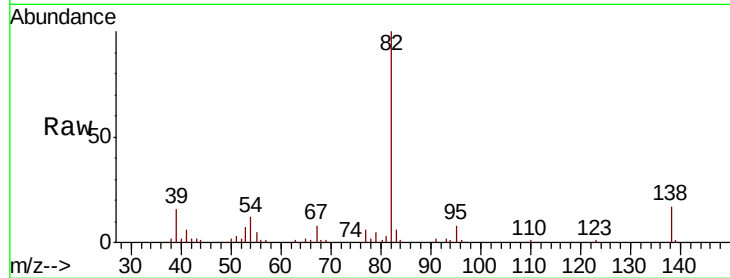

#23

2-Nitrophenol

Concen: 8.025 ng/ul




RT: 9.55 min Scan# 1158


Delta R.T. -0.01 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tgt Ion:	139	Resp:	14176
Ion Ratio	Lower	Upper	
139	100		
65	81.4	53.3	79.9#
109	45.5	32.6	49.0

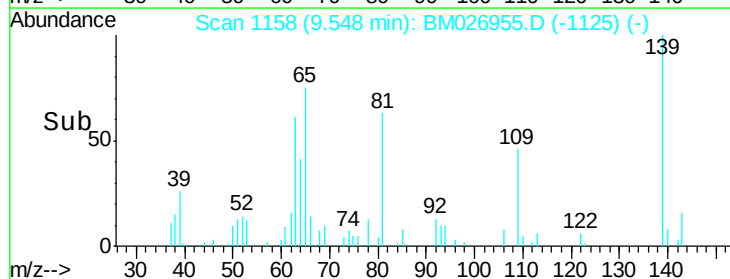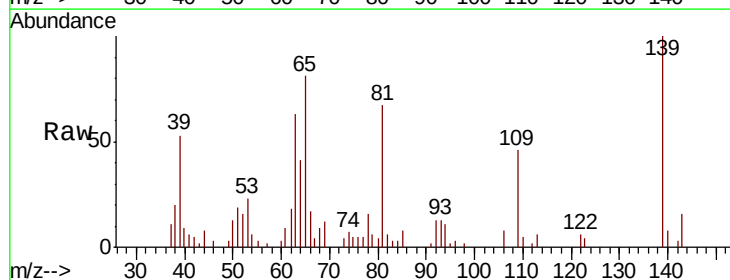







#24
 2,4-Dimethylphenol
 Concen: 7.361 ng/ul
 RT: 9.62 min Scan# 1170
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
107	100		
121	42.0	35.5	53.3
122	71.4	61.0	91.4




Manual Integrations
 APPROVED


mohammad
 8/3/2020 12:23:26 PM

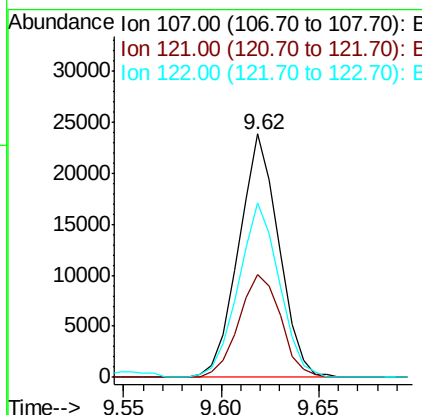

#25
 Bis(2-Chloroethoxy)methane
 Concen: 7.569 ng/ul
 RT: 9.85 min Scan# 1210
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
93	100		
95	28.8	25.7	38.5
123	12.4	7.8	11.8#









#27
 2,4-Dichlorophenol
 Concen: 7.719 ng/ul
 RT: 10.08 min Scan# 1249
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-06

Tot Ion:	162	Resp:	27796
Ion Ratio	Lower	Upper	
162	100		
164	71.7	52.4	78.6
98	40.1	32.2	48.2




Manual Integrations
 APPROVED


mohammad
 8/3/2020 12:23:26 PM



#28
 Naphthalene
 Concen: 7.504 ng/ul
 RT: 10.48 min Scan# 1317
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Tgt Ion:	128	Resp:	91050
Ion Ratio	Lower	Upper	
128	100		
129	11.6	8.3	12.5
127	14.1	11.0	16.6






#30
4-Chloroaniline
Concen: 8.047 ng/ul
RT: 10.58 min Scan# 1334
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06




Tot Ion:127 Resp: 35775
Ion Ratio Lower Upper
127 100
129 32.7 24.3 36.5

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM




Abundance Ion 127.00 (126.70 to 127.70): E
Ion 129.00 (128.70 to 129.70): E


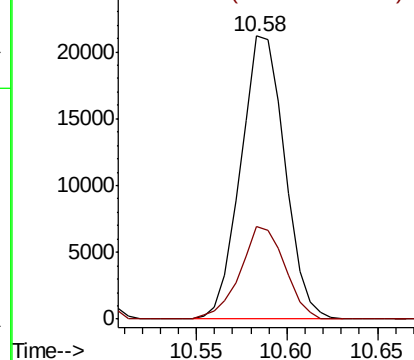



#31
Hexachlorobutadiene
Concen: 8.074 ng/ul
RT: 10.78 min Scan# 1368
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion:225 Resp: 20533
Ion Ratio Lower Upper
225 100
223 58.1 51.4 77.0
227 60.4 53.1 79.7



Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E

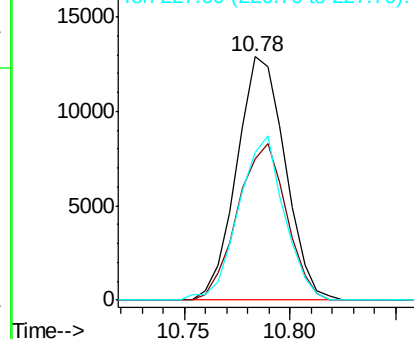







#32
Caprolactam
Concen: 6.846 ng/ul m
RT: 11.35 min Scan# 1465
Delta R.T. 0.02 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
113	100		
55	125.8	119.7	179.5
56	118.4	90.2	135.2




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

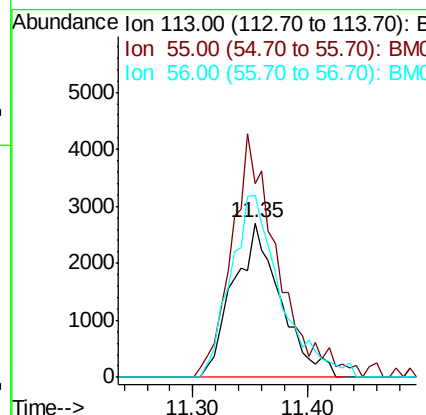

#33
4-Chloro-3-methylphenol
Concen: 7.204 ng/ul
RT: 11.72 min Scan# 1527
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
107	100		
144	27.4	20.6	30.8
142	75.8	59.9	89.9

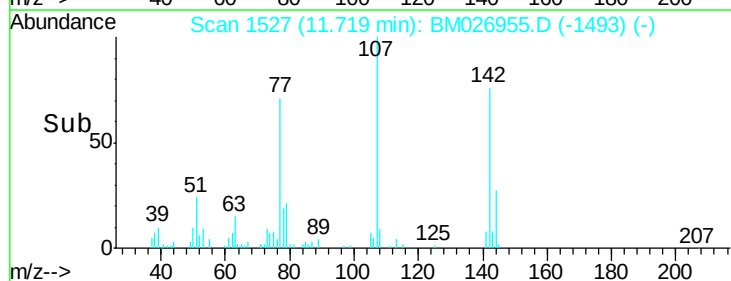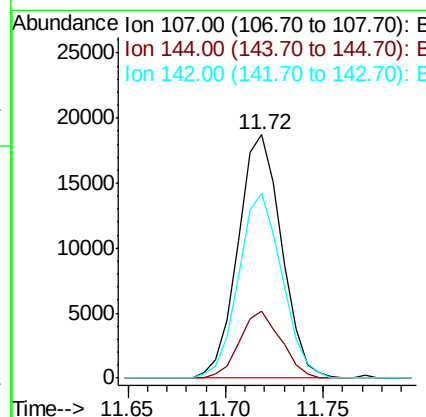

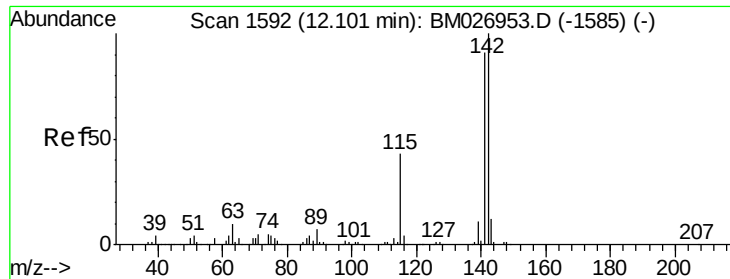





#34
2-Methylnaphthalene
Concen: 7.524 ng/ul
RT: 12.10 min Scan# 1592
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
142	100		
141	92.3	71.1	106.7




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

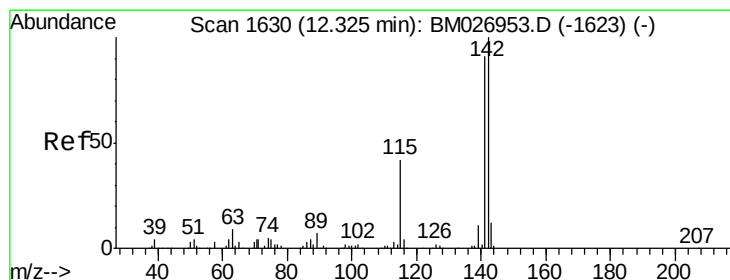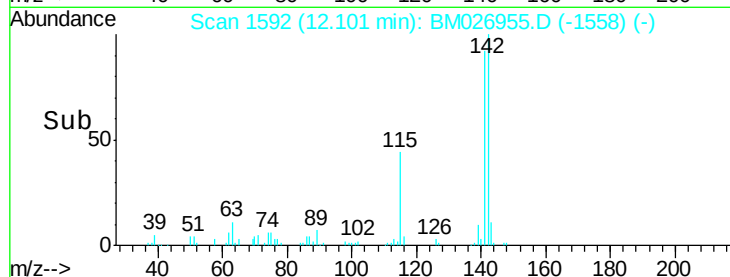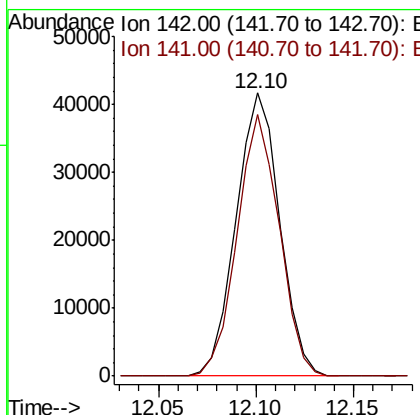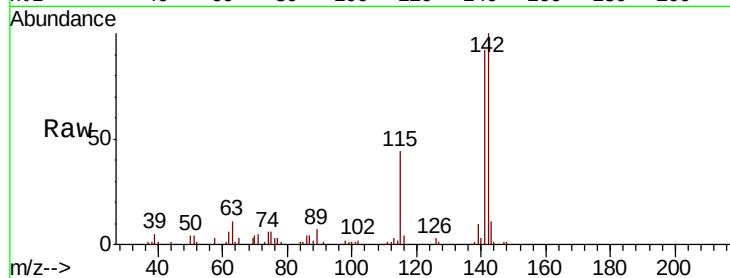

#35
1-Methylnaphthalene
Concen: 7.493 ng/ul
RT: 12.32 min Scan# 1630
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
142	100		
141	90.4	73.3	109.9
116	4.4	3.4	5.0

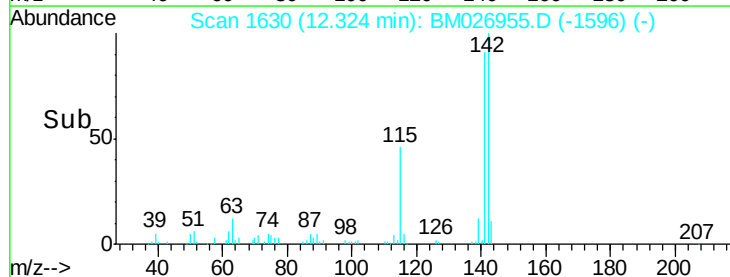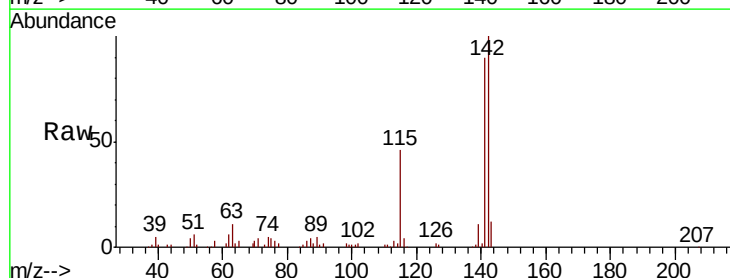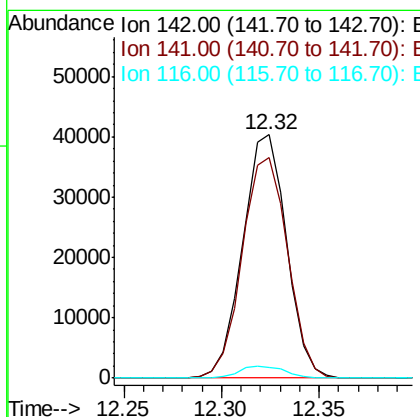







#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 7.447 ng/ul
 RT: 12.48 min Scan# 1656
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
216	100		
214	78.3	64.2	96.4
179	24.2	16.2	24.4
108	21.7	16.7	25.1




Manual Integrations
 APPROVED


mohammad
 8/3/2020 12:23:26 PM

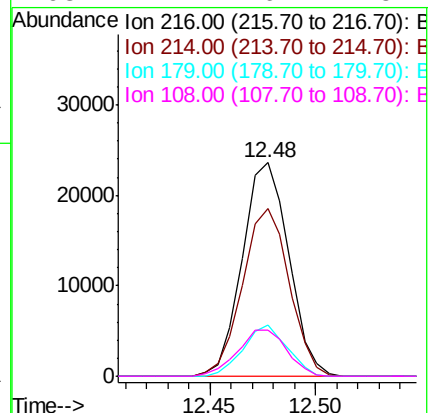

#38
 Hexachlorocyclopentadiene
 Concen: 5.796 ng/ul
 RT: 12.47 min Scan# 1654
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
237	100		
235	65.3	49.8	74.8
272	10.9	10.1	15.1

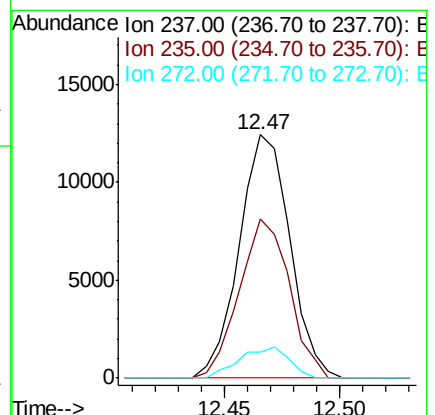







#39
 2,4,6-Trichlorophenol
 Concen: 7.490 ng/ul
 RT: 12.71 min Scan# 1696
 Delta R.T. -0.01 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
196	100		
198	93.7	79.0	118.6
200	28.3	23.3	34.9




Manual Integrations
 APPROVED


mohammad
 8/3/2020 12:23:26 PM

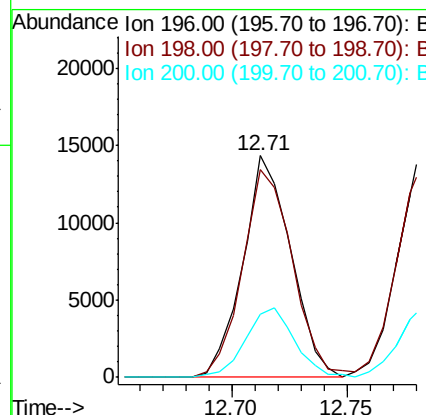

#40
 2,4,5-Trichlorophenol
 Concen: 7.527 ng/ul
 RT: 12.78 min Scan# 1708
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
196	100		
198	88.6	79.0	118.6
200	29.2	25.4	38.2

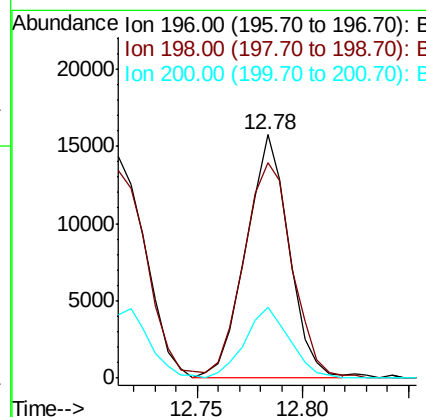







#41
 1,1'-Biphenyl
 Concen: 7.313 ng/ul
 RT: 13.12 min Scan# 1766
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-06

Tot Ion:	154	Resp:	86629
Ion Ratio	Lower	Upper	
154	100		
153	38.5	31.4	47.2
76	12.5	10.8	16.2




Manual Integrations
 APPROVED


mohammad
 8/3/2020 12:23:26 PM

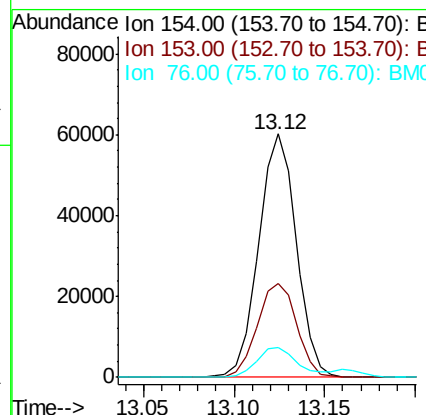

#42
 2-Chloronaphthalene
 Concen: 7.478 ng/ul
 RT: 13.16 min Scan# 1772
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Tgt Ion:	162	Resp:	71279
Ion Ratio	Lower	Upper	
162	100		
164	34.1	26.4	39.6
127	40.7	30.6	45.8

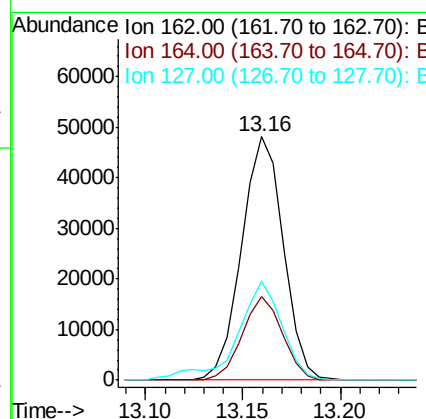







#43
2-Nitroaniline
Concen: 7.664 ng/ul
RT: 13.35 min Scan# 1805
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
65	100		
92	54.8	51.0	76.6
138	71.8	67.3	100.9




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

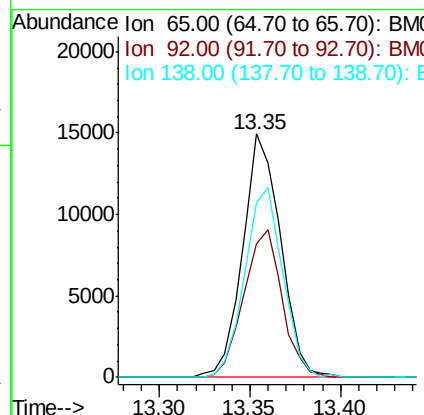

#45
Dimethylphthalate
Concen: 7.815 ng/ul
RT: 13.75 min Scan# 1873
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.6	3.0	4.6
164	9.8	8.6	12.8

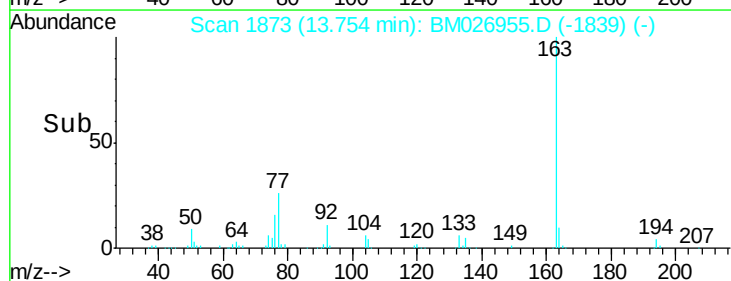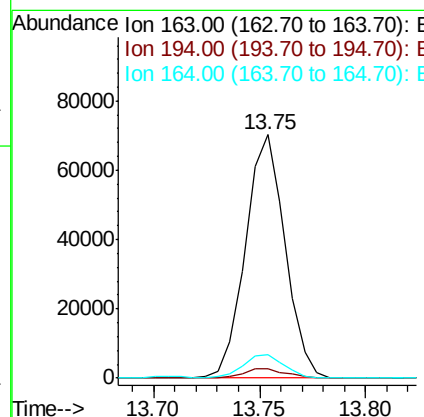







#46
2,6-Dinitrotoluene
Concen: 7.155 ng/ul
RT: 13.86 min Scan# 1891
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
165	100		
89	90.1	55.0	82.4#
121	25.0	19.0	28.6




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

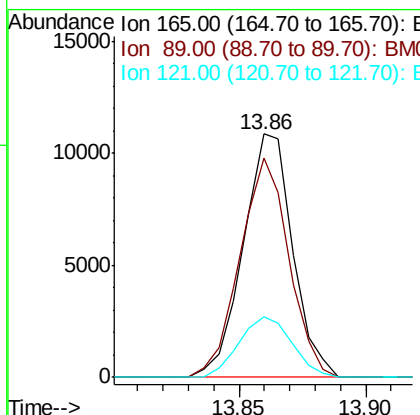

#48
Acenaphthylene
Concen: 7.312 ng/ul
RT: 14.01 min Scan# 1917
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.5	15.8	23.6
153	13.4	10.7	16.1

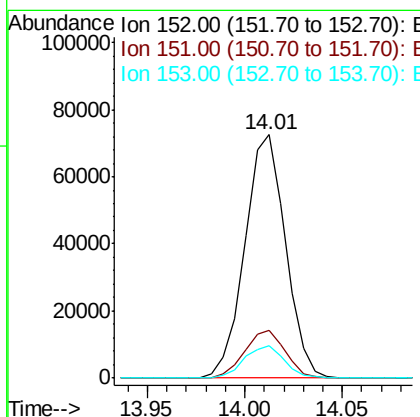







#49
3-Nitroaniline
Concen: 6.485 ng/ul
RT: 14.18 min Scan# 1946
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
138	100		
108	11.7	11.4	17.2
92	132.5	108.7	163.1




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

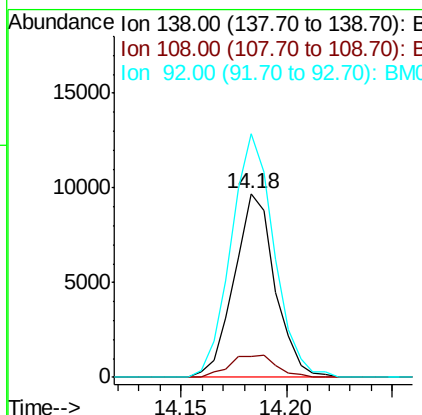

#50
Acenaphthene
Concen: 7.325 ng/ul
RT: 14.35 min Scan# 1975
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
153	100		
152	49.6	37.8	56.6
154	84.0	70.5	105.7





#51

2,4-Dinitrophenol

Concen: 7.667 ng/ul

RT: 14.39 min Scan# 1981

Delta R.T. -0.01 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-06

Tot Ion:	184	Resp:	6314
Ion Ratio	Lower	Upper	
184	100		
63	93.1	57.8	86.8#
154	83.2	55.0	82.4#

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM

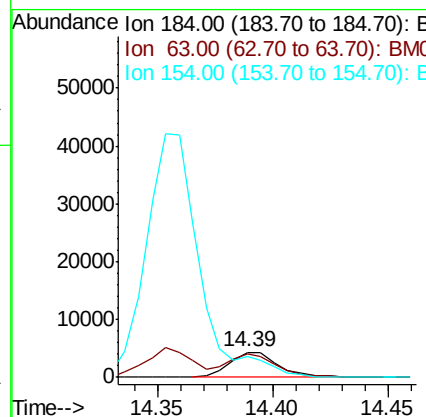

#53

4-Nitrophenol

Concen: 9.658 ng/ul




RT: 14.49 min Scan# 1999


Delta R.T. -0.01 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tgt Ion:	109	Resp:	18191
Ion Ratio	Lower	Upper	
109	100		
139	93.0	92.3	138.5
65	136.4	116.6	174.8

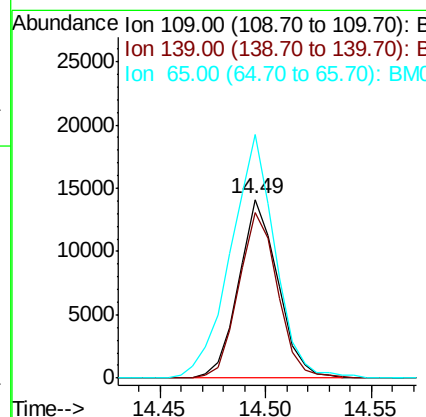



#54

Dibenzofuran

Concen: 7.714 ng/ul

RT: 14.69 min Scan# 2032

Delta R.T. -0.01 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-06

Tot Ion:168 Resp: 105874

Ion Ratio Lower Upper

168 100





139 43.1 30.8 46.2

Manual Integrations

APPROVED

mohammad

8/3/2020 12:23:26 PM

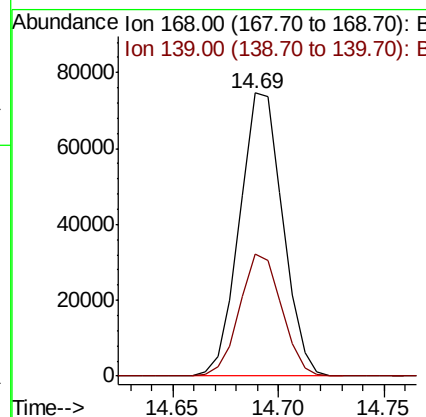

#55

2,4-Dinitrotoluene

Concen: 7.831 ng/ul

RT: 14.65 min Scan# 2025

Delta R.T. -0.01 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03




Tgt Ion:165 Resp: 23142


Ion Ratio Lower Upper

165 100

63 64.8 46.2 69.4

182 2.6 2.4 3.6

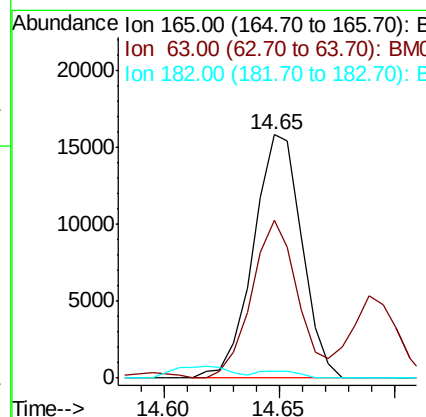

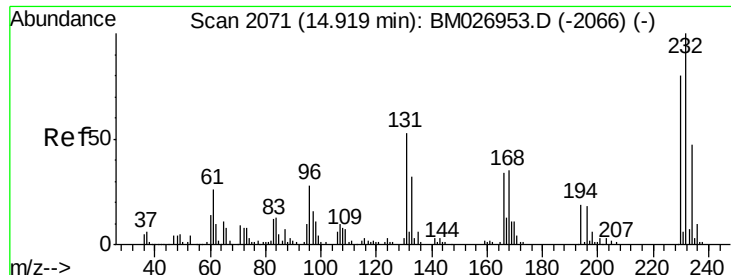


#56
2,3,4,6-Tetrachlorophenol
Concen: 8.623 ng/ul
RT: 14.92 min Scan# 2071
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
232	100		
131	51.8	39.4	59.2
130	2.4	2.6	4.0
166	32.9	26.7	40.1

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM






Abundance

Ion 232.00 (231.70 to 232.70): E

Ion 131.00 (130.70 to 131.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 166.00 (165.70 to 166.70): E

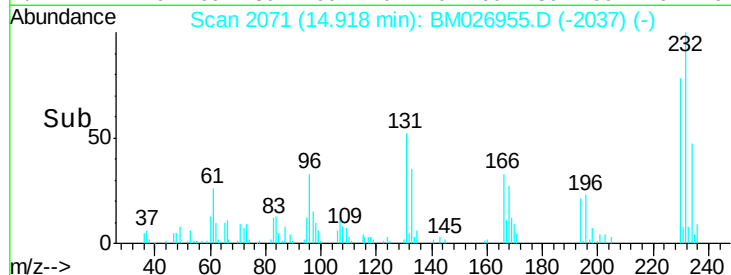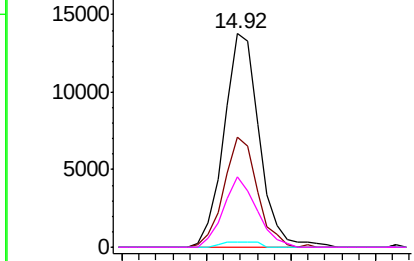

#57
Diethylphthalate
Concen: 7.837 ng/ul
RT: 15.13 min Scan# 2107
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03




Tgt Ion	Ratio	Lower	Upper
149	100		
177	19.9	17.0	25.4
150	12.8	9.2	13.8


Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 177.00 (176.70 to 177.70): E

Ion 150.00 (149.70 to 150.70): E

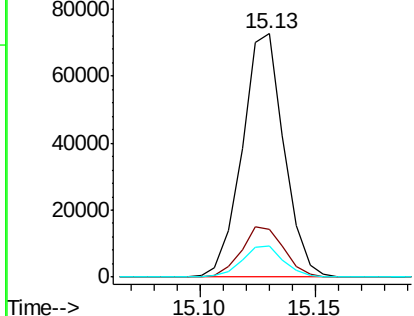

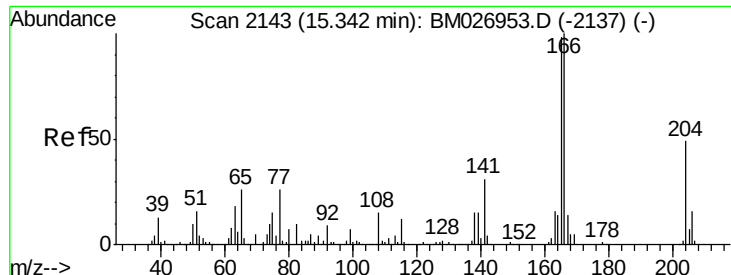

#59

Fluorene

Concen: 7.694 ng/ul

RT: 15.34 min Scan# 2143

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M

ClientSampleId :

MDL-WATER-06

Tot Ion:166 Resp: 88926

Ion Ratio Lower Upper

166 100

165 94.9 78.2 117.2


167 13.6 10.3 15.5

Manual Integrations

APPROVED

mohammad




8/3/2020 12:23:26 PM



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

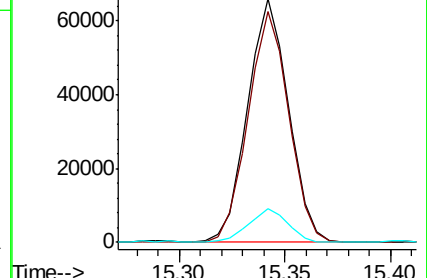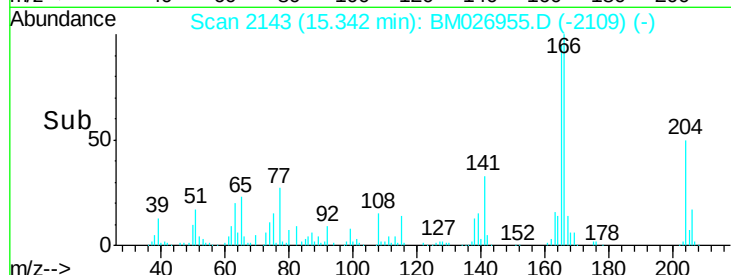

#60

4-Chlorophenyl-phenylether

Concen: 7.772 ng/ul

RT: 15.34 min Scan# 2143

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03


Tgt Ion:204 Resp: 44708

Ion Ratio Lower Upper

204 100

206 35.1 26.0 39.0



141 67.4 48.3 72.5




Abundance Ion 204.00 (203.70 to 204.70): E

Ion 206.00 (205.70 to 206.70): E

Ion 141.00 (140.70 to 141.70): E

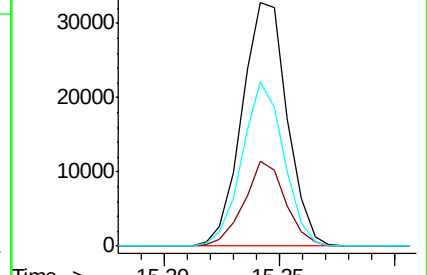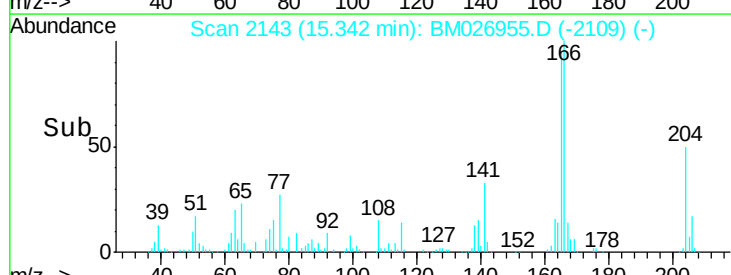

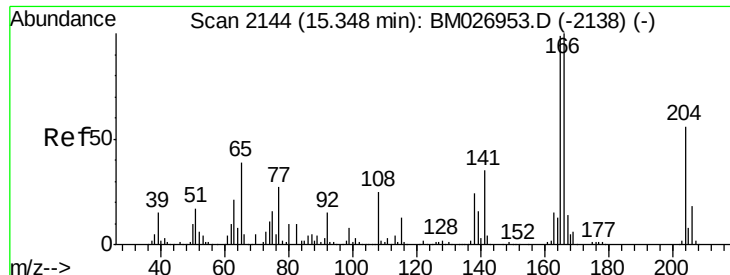





#61
4-Nitroaniline
Concen: 5.754 ng/ul
RT: 15.35 min Scan# 2144
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
138	100		
92	66.4	49.9	74.9
108	113.1	78.9	118.3




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

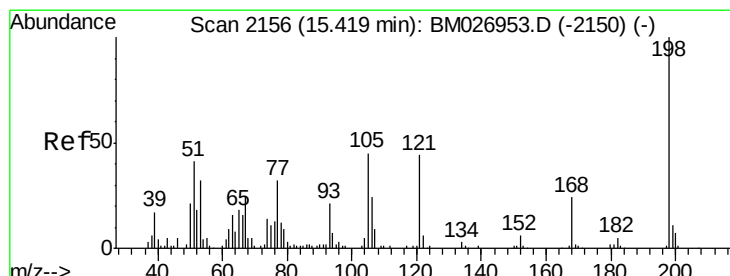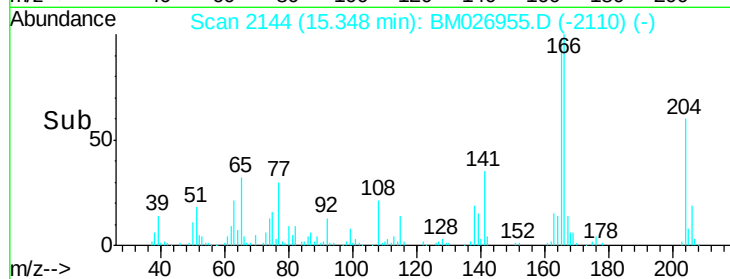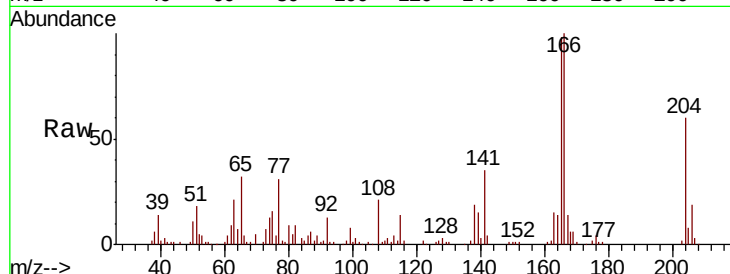

#64
4,6-Dinitro-2-methylphenol
Concen: 8.012 ng/ul
RT: 15.41 min Scan# 2155
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
198	100		
182	7.5	4.2	6.4#
77	51.2	29.3	43.9#

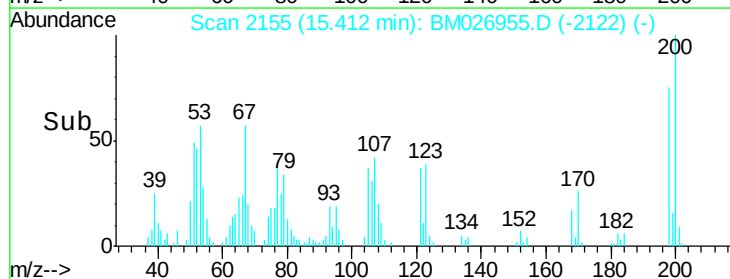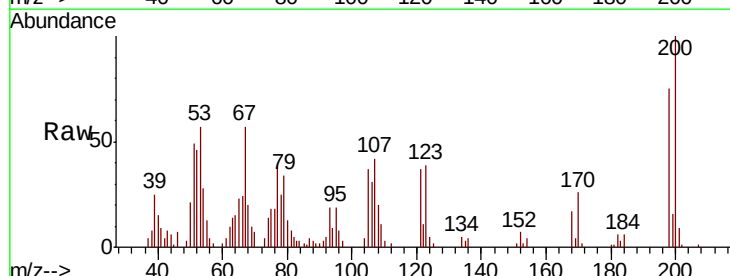



#65


N-Nitrosodiphenylamine
Concen: 7.059 ng/ul
RT: 15.55 min Scan# 2179
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
169	100		
168	65.1	54.6	82.0
167	34.0	29.1	43.7

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM



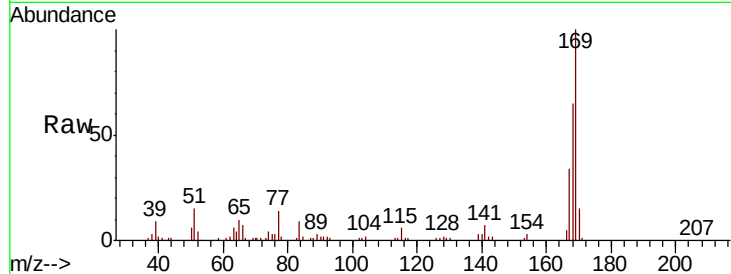


Abundance

Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E


Ion 167.00 (166.70 to 167.70): E

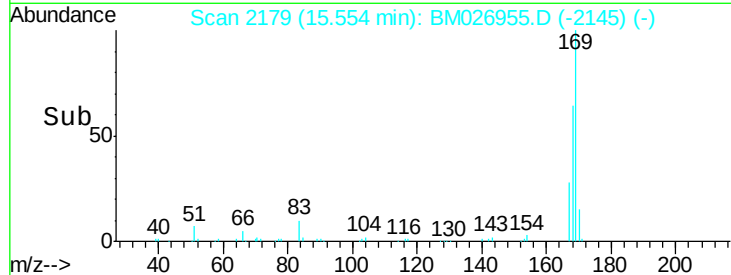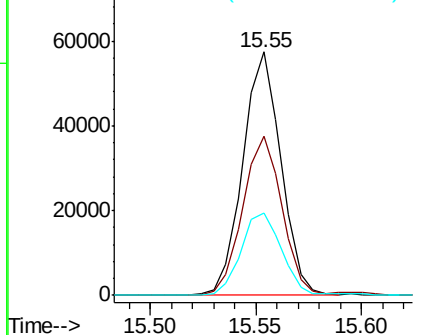

#66

4-Bromophenyl-phenylether
Concen: 7.257 ng/ul
RT: 16.24 min Scan# 2295
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
248	100		
250	100.7	78.2	117.4
141	80.7	57.5	86.3






Abundance

Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

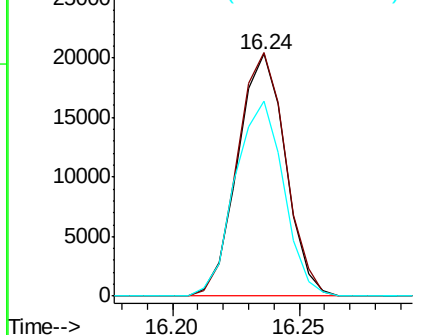



#67

Hexachlorobenzene

Concen: 7.742 ng/ul

RT: 16.35 min Scan# 2314

Delta R.T. -0.01 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-06

Tot Ion:	284	Resp:	32165
Ion Ratio	Lower	Upper	
284	100		
142	42.3	31.7	47.5
249	33.0	25.7	38.5

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM

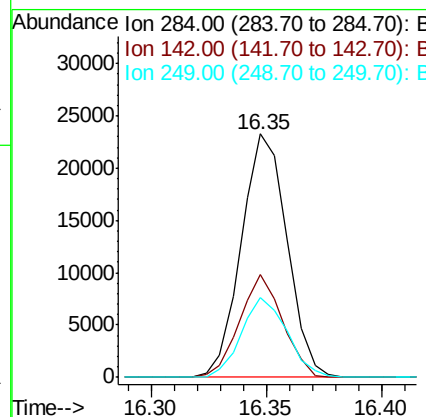

#68

Atrazine

Concen: 7.204 ng/ul




RT: 16.51 min Scan# 2341


Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tgt Ion:	200	Resp:	27013
Ion Ratio	Lower	Upper	
200	100		
173	27.4	22.4	33.6
215	46.0	38.6	58.0

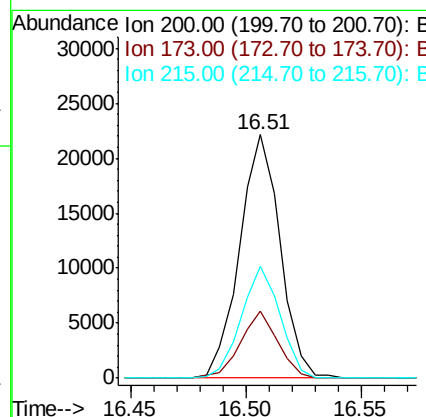




#69
 Pentachlorophenol
 Concen: 7.393 ng/ul
 RT: 16.69 min Scan# 2372
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
266	100		
264	57.8	49.3	73.9
268	65.9	50.5	75.7

Manual Integrations
 APPROVED

mohammad
 8/3/2020 12:23:26 PM






Abundance

Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

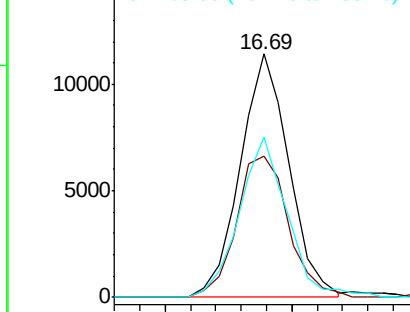

#70
 Phenanthrene
 Concen: 7.422 ng/ul
 RT: 17.07 min Scan# 2437
 Delta R.T. -0.01 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03




Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.0	12.0	18.0
176	19.7	14.7	22.1


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

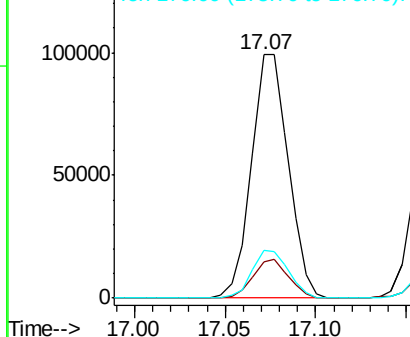

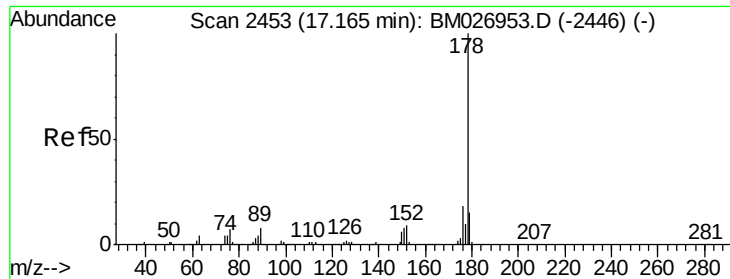

#72

Anthracene

Concen: 7.309 ng/ul

RT: 17.17 min Scan# 2453

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M


ClientSampleId :

MDL-WATER-06


Tot Ion:	178	Resp:	142413
Ion Ratio	Lower	Upper	
178	100		
179	14.5	11.8	17.6
176	17.5	15.0	22.6

Manual Integrations
APPROVED



mohammad
8/3/2020 12:23:26 PM

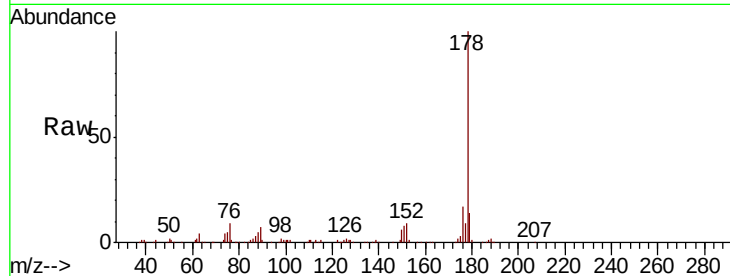

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

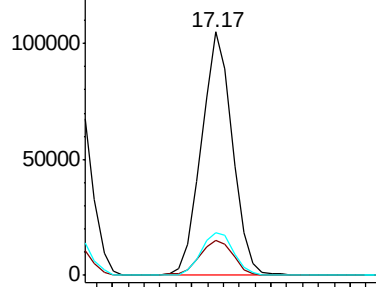

Time-->

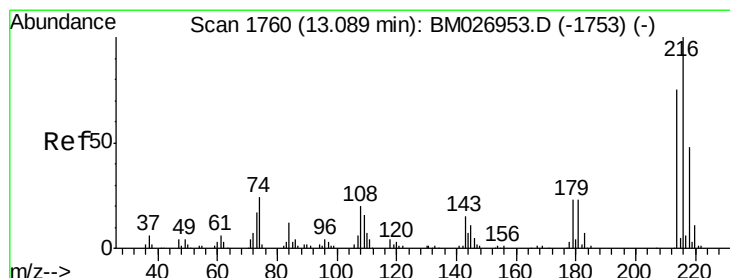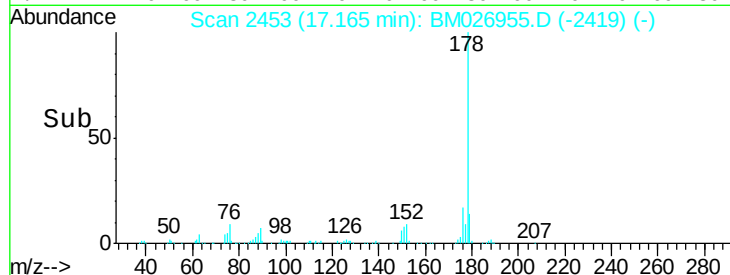

#73

1,2,3,4-Tetrachlorobenzene

Concen: 7.104 ng/uL


RT: 13.09 min Scan# 1760

Delta R.T. -0.00 min


Lab File: BM026955.D

Acq: 31 Jul 2020 13:03


Tgt Ion:	216	Resp:	34852
Ion Ratio	Lower	Upper	
216	100		
214	80.0	62.6	94.0
218	51.1	38.1	57.1

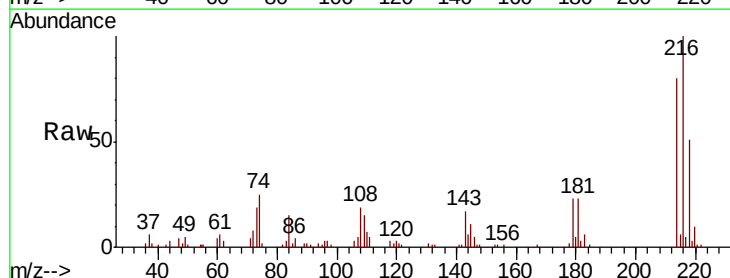


Abundance Ion 216.00 (215.70 to 216.70): E
Ion 214.00 (213.70 to 214.70): E
Ion 218.00 (217.70 to 218.70): E

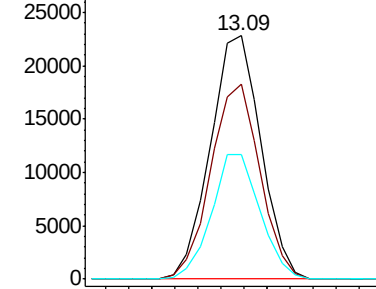

Time-->

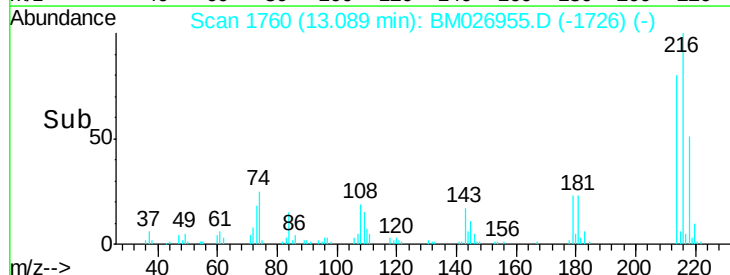







#74
 Pentachlorobenzene
 Concen: 7.473 ng/uL
 RT: 14.62 min Scan# 2020
 Delta R.T. -0.00 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
250	100		
248	63.6	49.6	74.4
252	65.8	51.7	77.5




Manual Integrations
 APPROVED


mohammad
 8/3/2020 12:23:26 PM

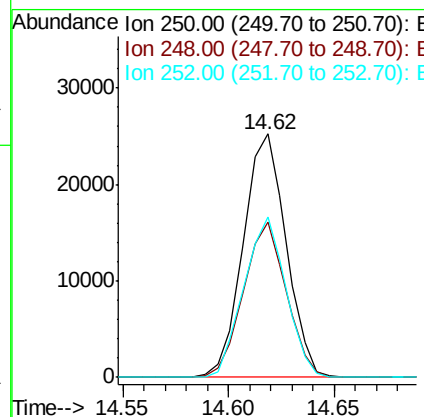

#75
 Carbazole
 Concen: 7.122 ng/uL
 RT: 17.43 min Scan# 2498
 Delta R.T. -0.01 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
167	100		
166	20.4	17.1	25.7
139	13.4	10.1	15.1

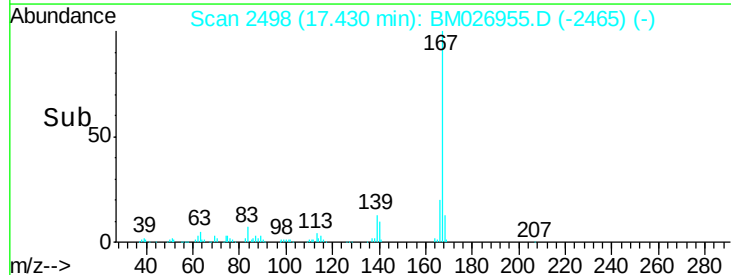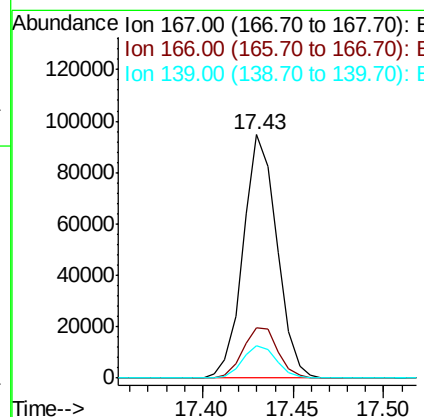

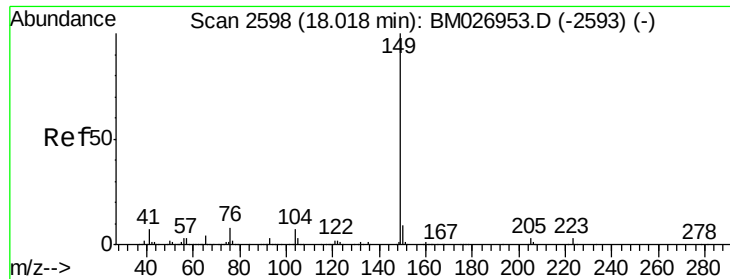





#76
Di-n-butylphthalate
Concen: 7.265 ng/ul
RT: 18.02 min Scan# 2598
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
149	100		
150	9.4	7.6	11.4
104	6.7	4.7	7.1




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

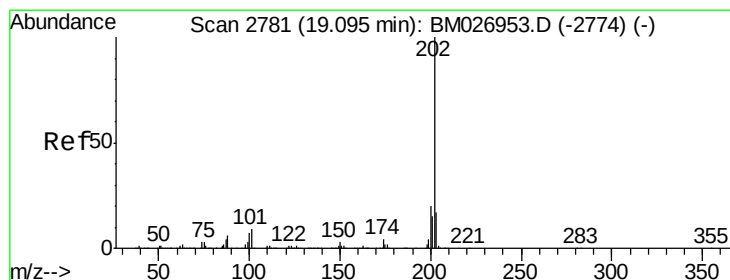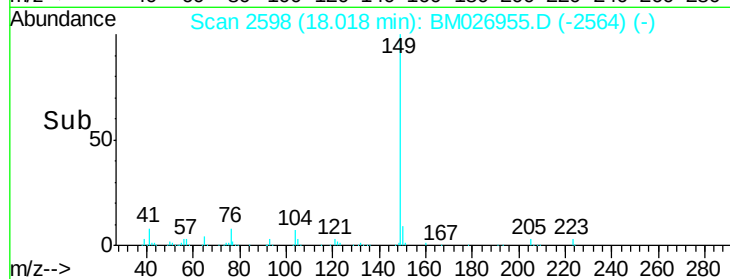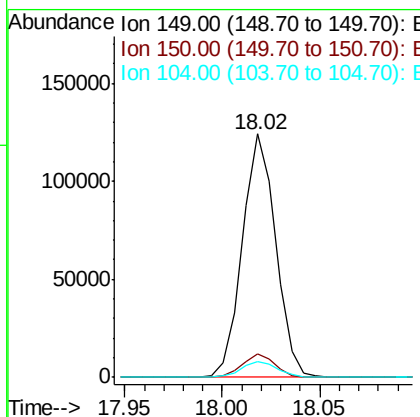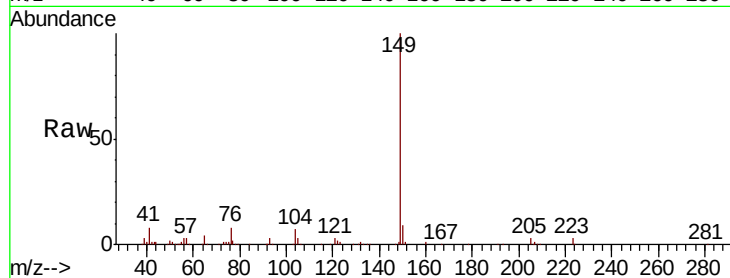

#77
Fluoranthene
Concen: 7.361 ng/ul
RT: 19.09 min Scan# 2781
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.4	7.7	11.5
100	6.4	6.2	9.4

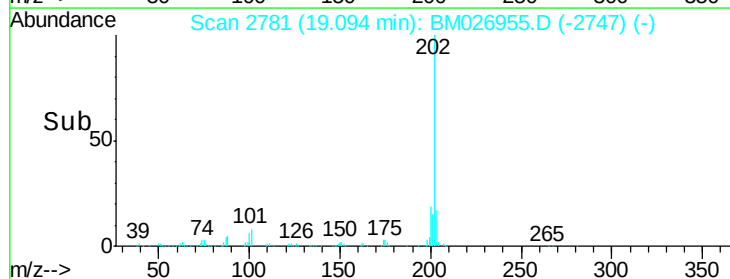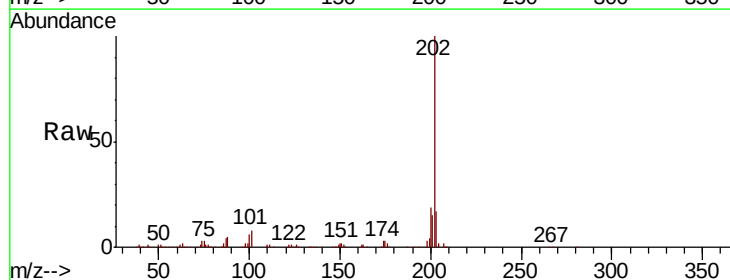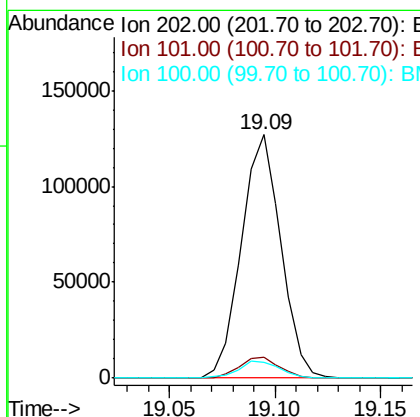







#80
Pvrene
Concen: 6.950 ng/ul
RT: 19.46 min Scan# 2843
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	10.2	9.4	14.2
100	8.0	8.2	12.4




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

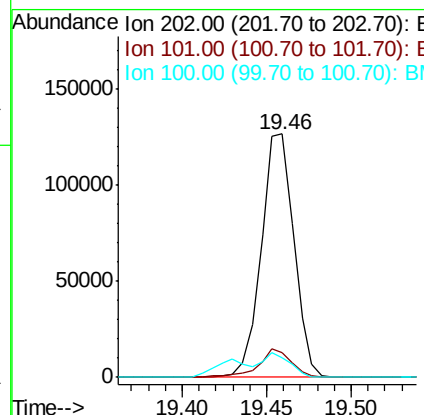

#81
Butylbenzylphthalate
Concen: 6.889 ng/ul
RT: 20.38 min Scan# 2999
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Resp Lower	Upper
149	100		
91	77.3	64.2	96.2
206	20.9	15.8	23.6

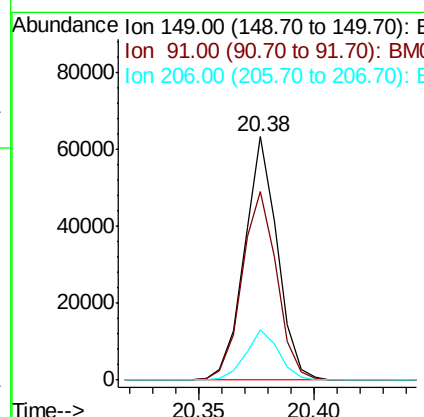



#82

3,3'-Dichlorobenzidine

Concen: 5.853 ng/ul

RT: 21.15 min Scan# 3130

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-06

Tot Ion:	252	Resp:	46872
Ion Ratio	Lower	Upper	
252	100		
254	64.4	51.4	77.2
126	11.0	8.7	13.1

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM

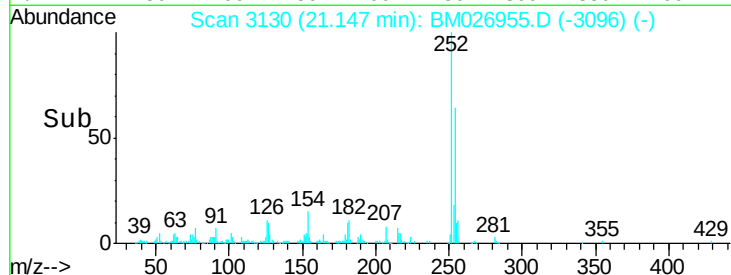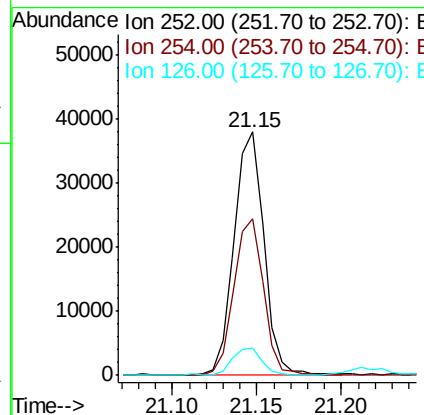

#83

Benzo(a)anthracene

Concen: 7.361 ng/ul




RT: 21.21 min Scan# 3141


Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tgt Ion:	228	Resp:	171848
Ion Ratio	Lower	Upper	
228	100		
229	18.6	15.4	23.2
226	26.6	20.9	31.3

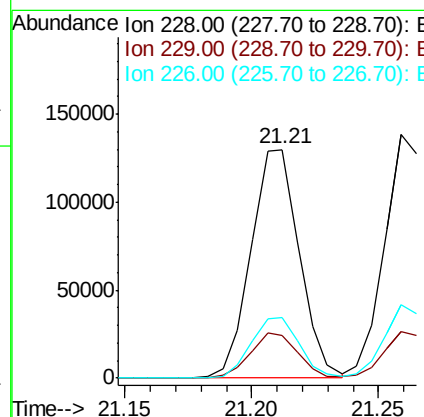



#84

Bis(2-ethylhexyl)phthalate

Concen: 6.810 ng/ul

RT: 21.17 min Scan# 3134

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M


ClientSampleId :

MDL-WATER-06




Tot Ion:	149	Resp:	93554
Ion Ratio	Lower	Upper	
149	100		
167	26.7	20.6	31.0
279	4.9	3.0	4.6#

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

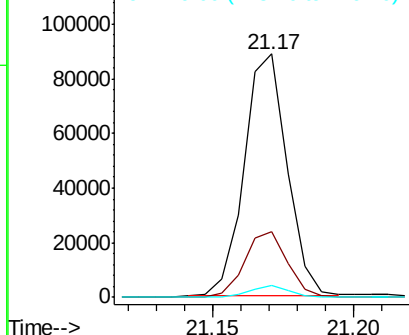

#85

Chrysene

Concen: 7.408 ng/ul


RT: 21.26 min Scan# 3149

Delta R.T. -0.01 min



Lab File: BM026955.D


Acq: 31 Jul 2020 13:03

Tgt Ion:	228	Resp:	168659
Ion Ratio	Lower	Upper	
228	100		
226	30.0	23.2	34.8
229	19.3	15.5	23.3



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

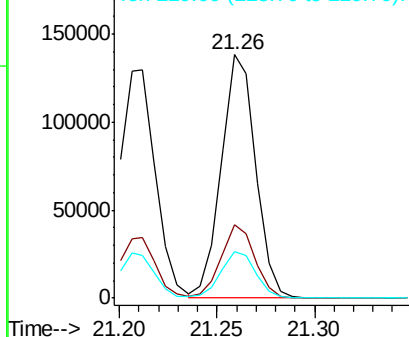



#87

Di-n-octyl phthalate

Concen: 6.283 ng/ul

RT: 22.04 min Scan# 3282

Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Instrument :

BNA_M


ClientSampleId :

MDL-WATER-06




Tgt Ion:149 Resp: 156474

Manual Integrations
APPROVED

mohammad
8/3/2020 12:23:26 PM



Abundance Ion 149.00 (148.70 to 149.70): E

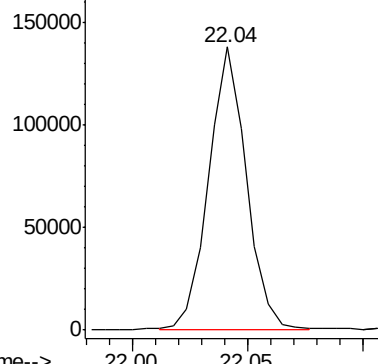

#88

Benzo(b)fluoranthene

Concen: 7.127 ng/ul

RT: 22.78 min Scan# 3407


Delta R.T. -0.00 min

Lab File: BM026955.D

Acq: 31 Jul 2020 13:03

Tgt Ion:252 Resp: 172811



Ion	Ratio	Lower	Upper
252	100		
253	20.0	17.6	26.4
125	7.6	6.6	10.0




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

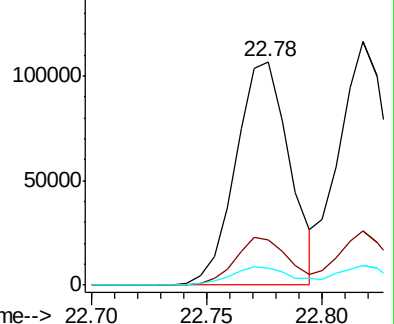







#89
Benzo(k)fluoranthene
Concen: 7.633 ng/ul
RT: 22.82 min Scan# 3414
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.4	26.2
125	8.0	7.3	10.9




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

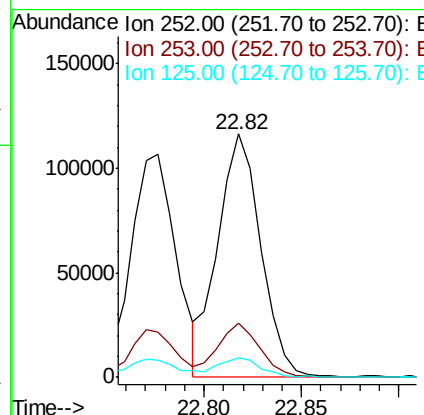

#91
Benzo(a)pyrene
Concen: 7.319 ng/ul
RT: 23.34 min Scan# 3502
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.7	17.7	26.5
125	8.6	8.2	12.2

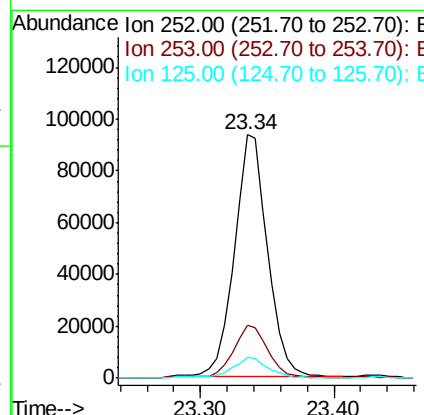







#92
Indeno(1,2,3-cd)pyrene
Concen: 7.559 ng/ul
RT: 25.64 min Scan# 3894
Delta R.T. -0.00 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-06

Tot Ion	Ratio	Lower	Upper
276	100		
138	20.6	17.0	25.4
277	25.1	20.6	30.8




Manual Integrations
APPROVED


mohammad
8/3/2020 12:23:26 PM

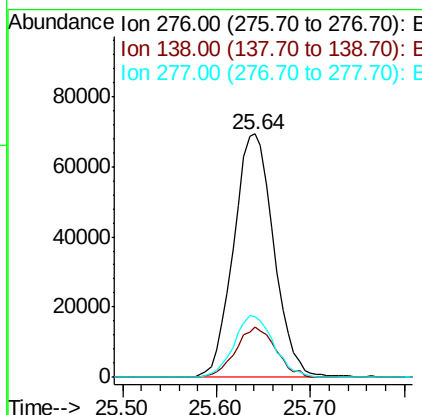

#93
Dibenzo(a,h)anthracene
Concen: 7.584 ng/ul
RT: 25.65 min Scan# 3896
Delta R.T. -0.01 min
Lab File: BM026955.D
Acq: 31 Jul 2020 13:03

Tgt Ion	Ratio	Lower	Upper
278	100		
139	13.3	10.9	16.3
279	23.3	19.4	29.2





#94
 Benzo(a,h,i)perylene
 Concen: 7.520 ng/ul
 RT: 26.31 min Scan# 4007
 Delta R.T. -0.01 min
 Lab File: BM026955.D
 Acq: 31 Jul 2020 13:03

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-06

Tot Ion:	276	Resp:	168781
Ion Ratio	Lower	Upper	
276	100		
138	16.5	14.9	22.3
277	23.8	19.1	28.7

Manual Integrations
 APPROVED

mohammad
 8/3/2020 12:23:26 PM

