
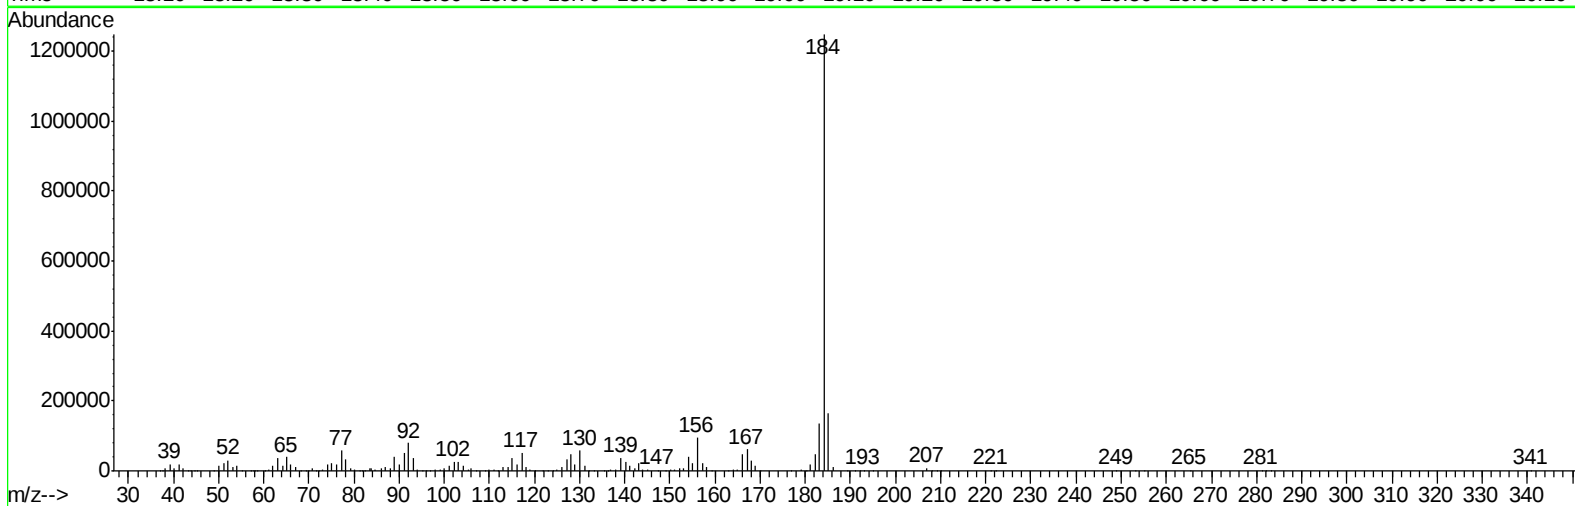


Data Path : Z:\HPCHEM1\BNA M\DATA\BM080117\
Data File : BM011075.D
Acq On : 01 Aug 2017 10:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 02:33:47 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

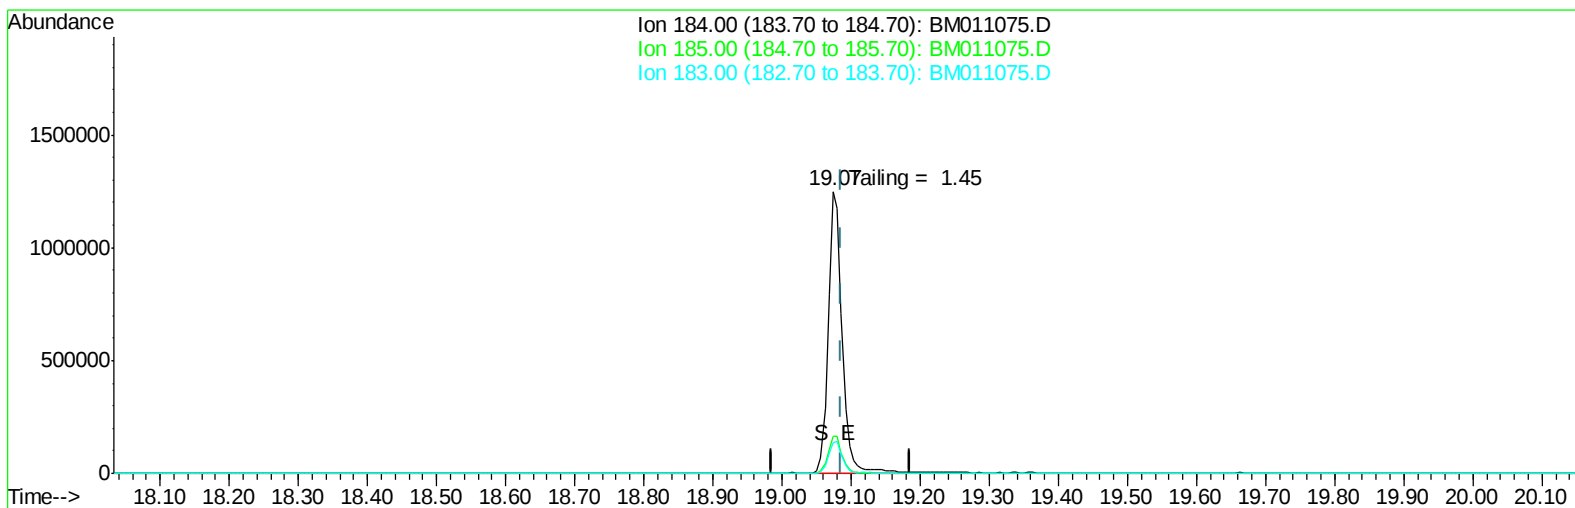

TIC: BM011075.D

(76) Benzidine



19.074min (-0.012) 87851.24ng

response 1723349

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.20
183.00	11.10	10.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080117\
Data File : BM011075.D
Acq On : 01 Aug 2017 10:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 02:33:47 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

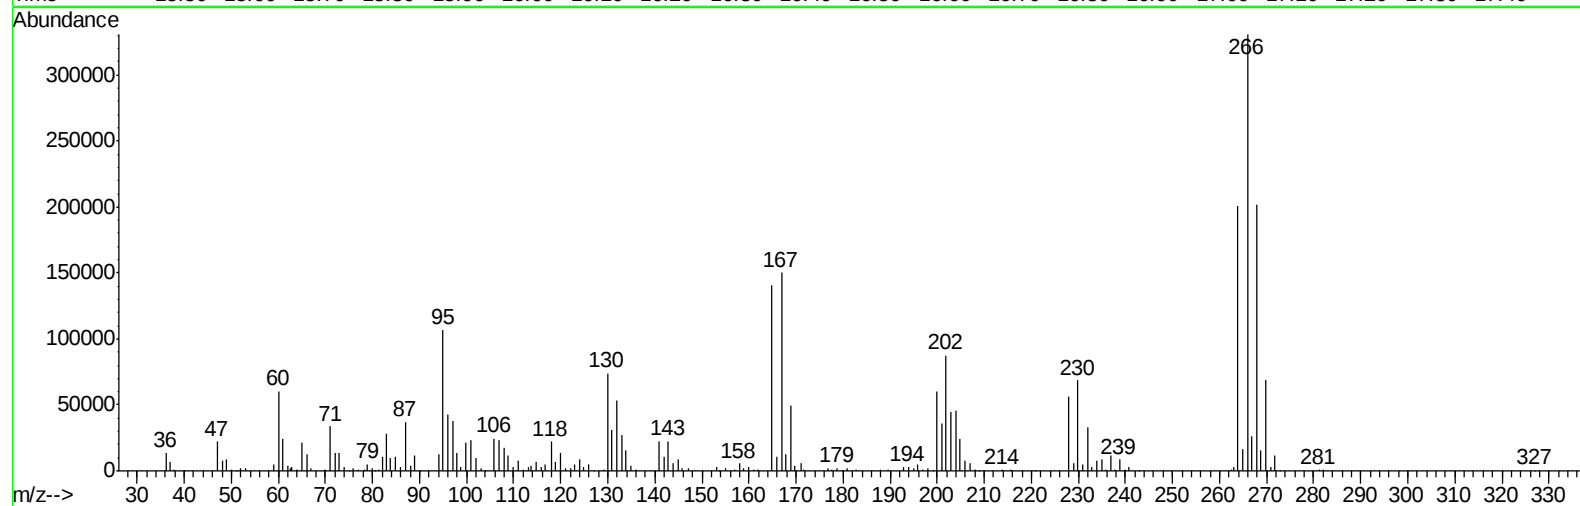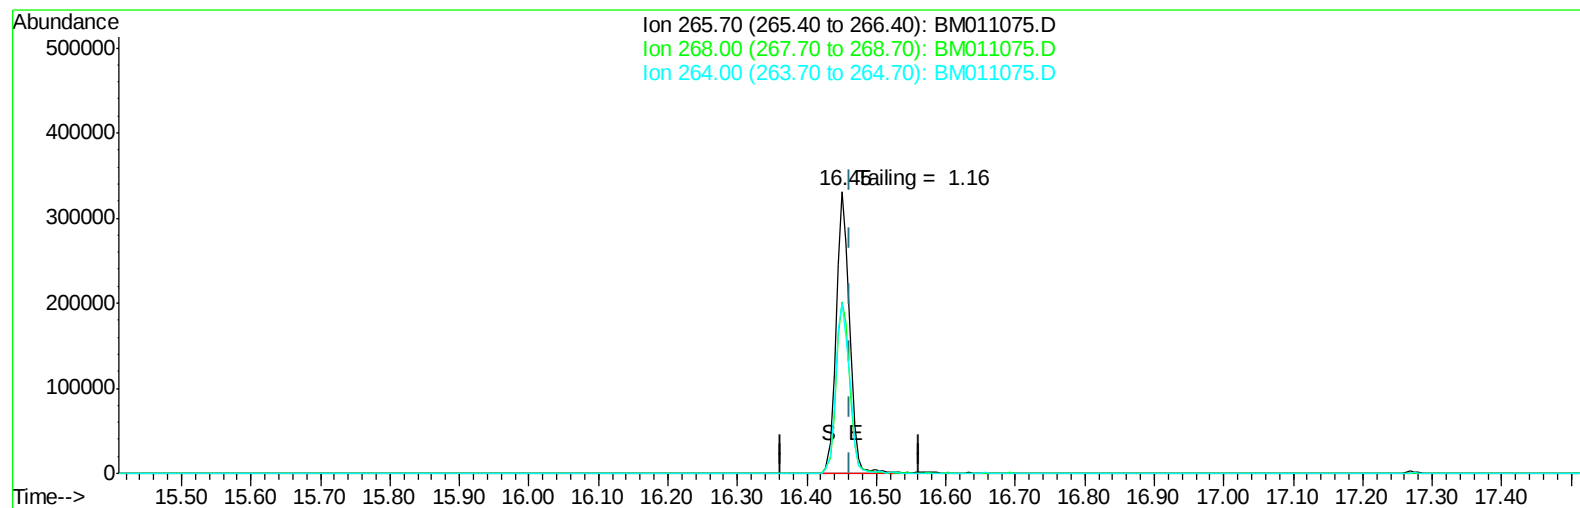

TIC: BM011075.D

(69) Pentachlorophenol (C)

16.451min (-0.012) 0.00ng

response 439568

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.08
264.00	61.20	60.57
0.00	0.00	0.00