


Data Path : Z:\HPCHEM1\BNA M\Data\BM080117\
 Data File : BM011075.D
 Acq On : 01 Aug 2017 10:28
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

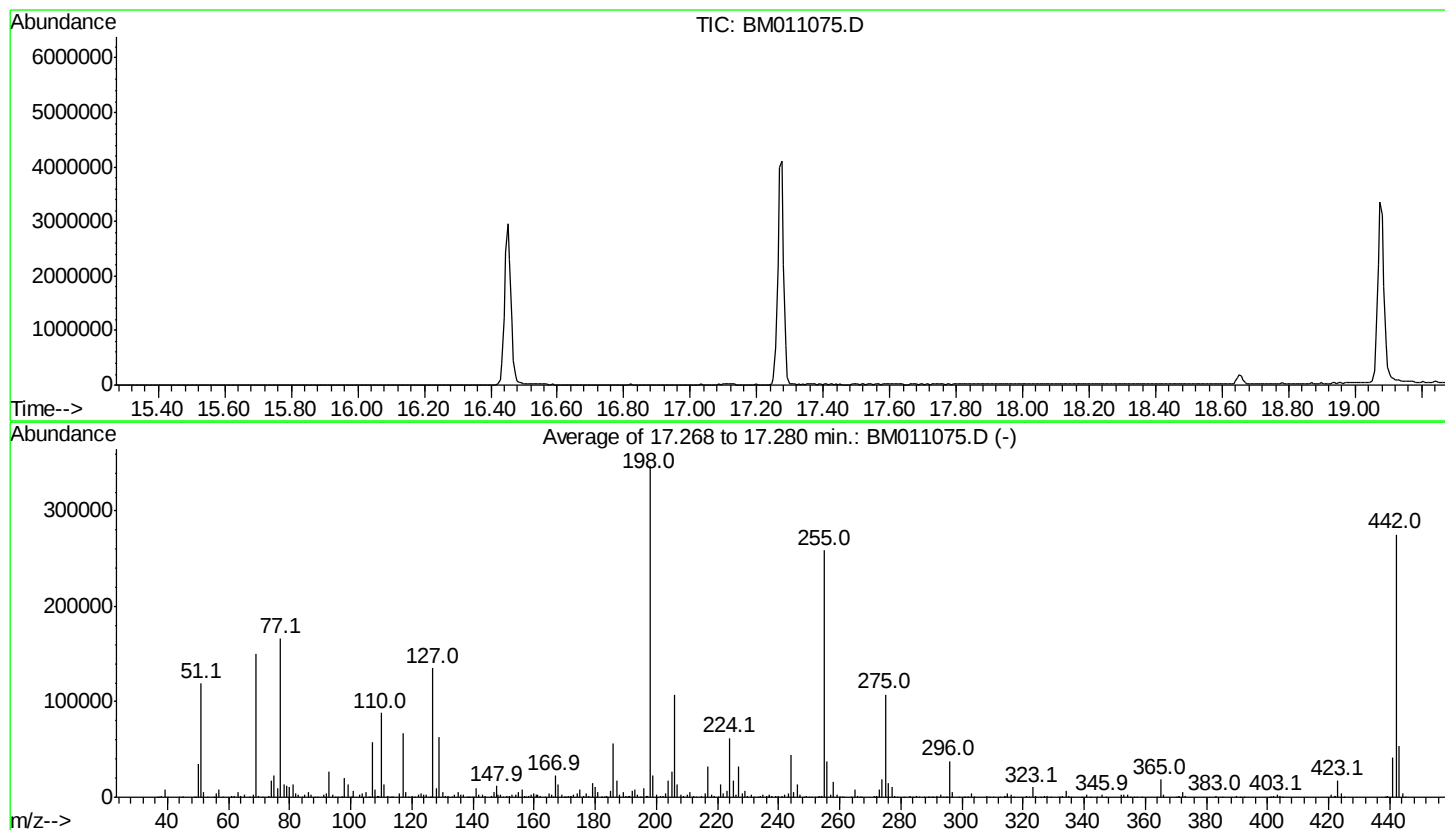

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	119208	PASS
68	69	0.00	2	2.0	3039	PASS
69	198	0.00	100	43.2	150138	PASS
70	69	0.00	2	0.6	906	PASS
127	198	10	80	39.0	135450	PASS
197	198	0.00	2	0.5	1771	PASS
198	198	100	100	100.0	347562	PASS
199	198	5	9	6.5	22557	PASS
275	198	10	60	30.9	107501	PASS
365	198	1	100	5.3	18445	PASS
441	443	0.01	100	78.5	41648	PASS
442	198	50	100	79.1	275050	PASS
443	442	15	24	19.3	53056	PASS