

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080118\
 Data File : BM016146.D
 Acq On : 01 Aug 2018 19:24
 Operator : SJ/JU
 Sample : J4171-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JJ1J2

Quant Time: Aug 02 03:40:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 02 02:25:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.19	152	44332	20.00	ng/ul	0.00
18) Naphthalene-d8	11.02	136	198683	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.82	164	117013	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	261708	20.00	ng/ul	0.00
77) Chrysene-d12	21.67	240	290145	20.00	ng/ul	0.00
85) Perylene-d12	24.03	264	262696	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	6526	6.48	ng/uL	0.00
5) Phenol-d5	7.35	99	117472	28.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.52	67	82015	32.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.72	132	106648	32.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.91	113	105338	30.36	ng/ul	0.00
19) Nitrobenzene-d5	9.38	128	53400	37.43	ng/ul	0.00
22) 2-Nitrophenol-d4	10.10	143	57500	35.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.64	165	100265	31.92	ng/ul	0.00
29) 4-Chloroaniline-d4	11.16	131	126564	33.12	ng/ul	0.00
43) Dimethylphthalate-d6	14.23	166	373101	34.98	ng/ul	0.00
46) Acenaphthylene-d8	14.52	160	426847	35.09	ng/ul	0.00
51) 4-Nitrophenol-d4	15.04	143	35191	19.04	ng/ul	0.00
57) Fluorene-d10	15.81	176	309474	34.20	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.95	200	42391	24.27	ng/ul	0.00
70) Anthracene-d10	17.65	188	472384	35.26	ng/ul	0.00
78) Pyrene-d10	19.92	212	537058	39.94	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.88	264	509656	35.27	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	14.27	163	38324	3.628	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080118\
Data File : BM016146.D
Acq On : 01 Aug 2018 19:24
Operator : SJ/JU
Sample : J4171-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JJ1J2

Quant Time: Aug 02 03:40:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 02 02:25:21 2018
Response via : Initial Calibration

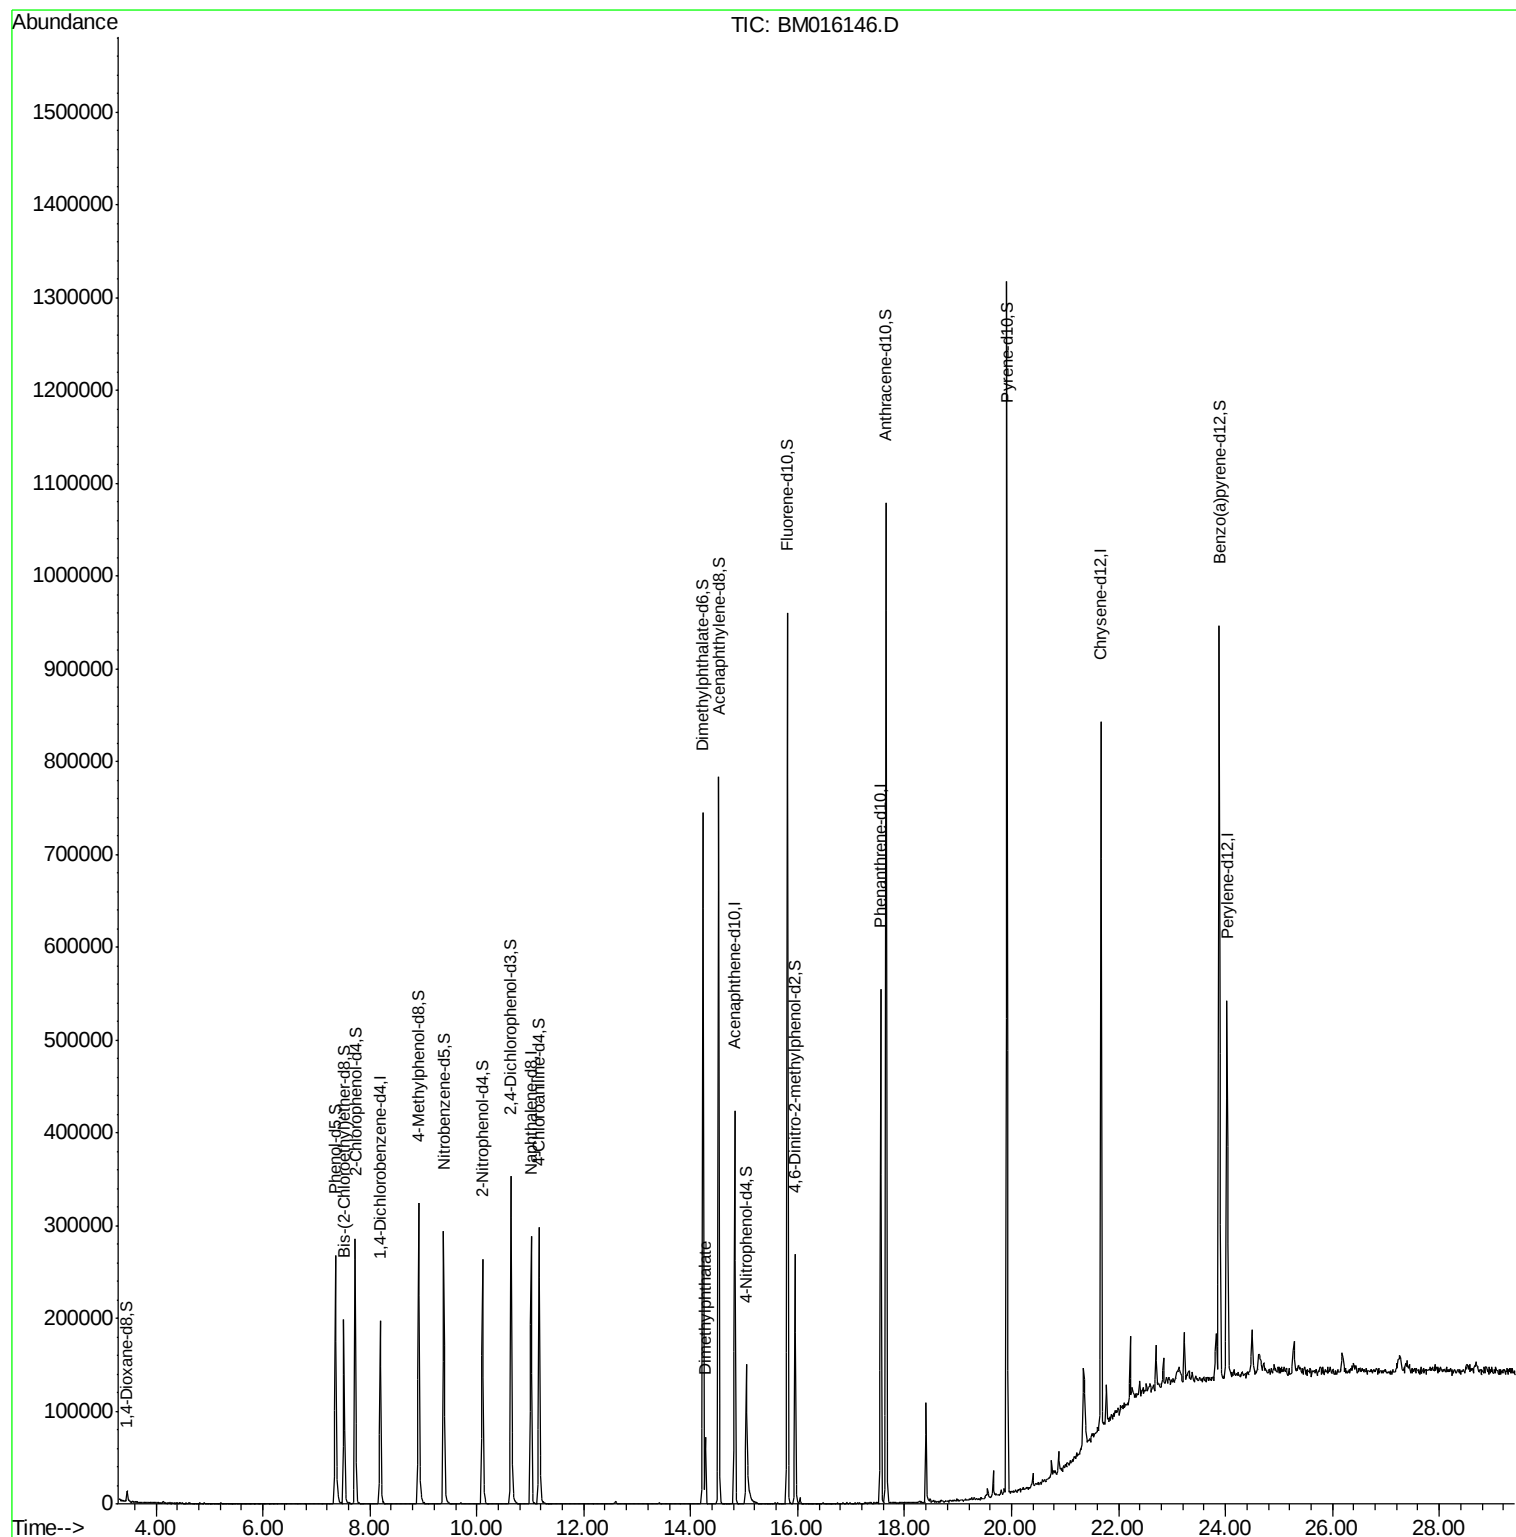

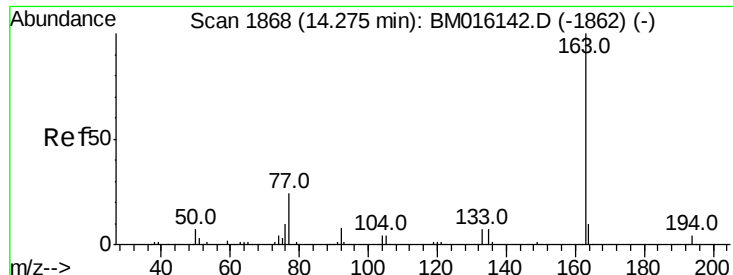

#44

Dimethylphthalate

Concen: 3.628 ng/ul

RT: 14.27 min Scan# 1868

Delta R.T. -0.00 min

Lab File: BM016146.D

Acq: 01 Aug 2018 19:24

Instrument :

BNA_M

ClientSampleId :

JJ1J2


Tot Ion:163 Resp: 38324

Ion Ratio Lower Upper

163 100

194 4.7 3.2 4.8

164 9.6 7.8 11.8

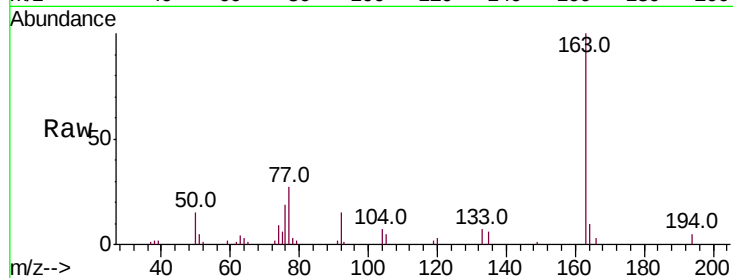

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

