

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080118\
 Data File : BM016156.D
 Acq On : 02 Aug 2018 01:30
 Operator : SJ/JU
 Sample : J4175-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC0

Manual Integrations
 APPROVED

Sohil
 8/2/2018 2:19:42 PM

Quant Time: Aug 02 08:05:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 02 02:25:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.19	152	50183	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	233443	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.82	164	138472	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	304247	20.00	ng/ul	0.00
77) Chrysene-d12	21.67	240	312652	20.00	ng/ul	0.00
85) Perylene-d12	24.03	264	276623	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	6569	5.76	ng/uL	0.00
5) Phenol-d5	7.35	99	114640	24.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.52	67	76938	26.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.72	132	107241	28.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.91	113	109499	27.88	ng/ul	0.00
19) Nitrobenzene-d5	9.38	128	49913	29.78	ng/ul	0.00
22) 2-Nitrophenol-d4	10.10	143	57045	29.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.63	165	101658	27.54	ng/ul	0.00
29) 4-Chloroaniline-d4	11.16	131	138027	30.74	ng/ul	0.00
43) Dimethylphthalate-d6	14.23	166	367240	29.10	ng/ul	0.00
46) Acenaphthylene-d8	14.52	160	427222	29.68	ng/ul	0.00
51) 4-Nitrophenol-d4	15.03	143	50826m	23.24	ng/ul	0.00
57) Fluorene-d10	15.81	176	292154	27.29	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.95	200	47234	23.26	ng/ul	0.00
70) Anthracene-d10	17.65	188	446559	28.67	ng/ul	0.00
78) Pyrene-d10	19.92	212	497188	34.31	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.88	264	402179	26.43	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	7.38	94	6508	1.413 ng/ul#	42
44) Dimethylphthalate	14.27	163	28974	2.318 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080118\
Data File : BM016156.D
Acq On : 02 Aug 2018 01:30
Operator : SJ/JU
Sample : J4175-02
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AC0

Manual Integrations
APPROVED

Sohil
8/2/2018 2:19:42 PM

Quant Time: Aug 02 08:05:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 02 02:25:21 2018
Response via : Initial Calibration

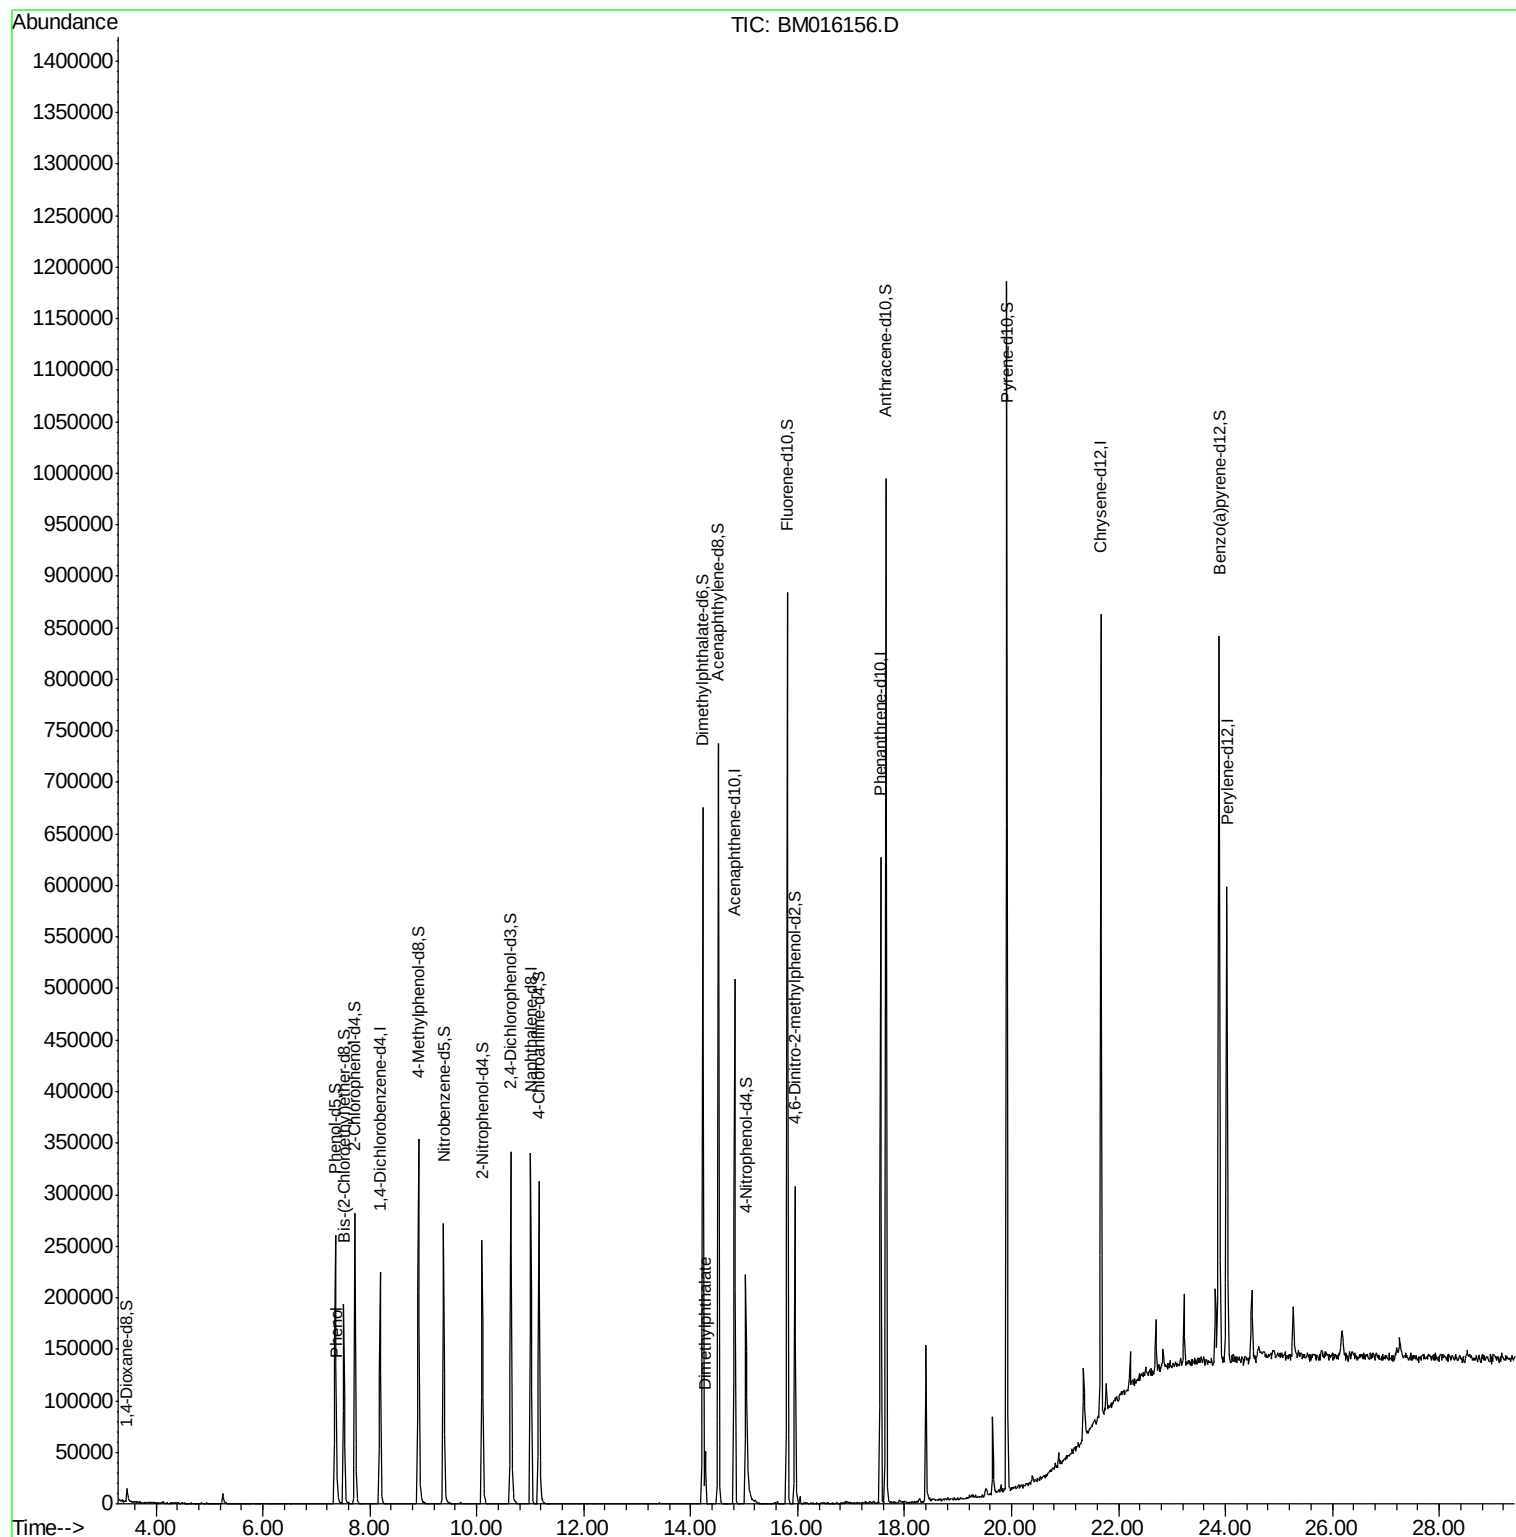

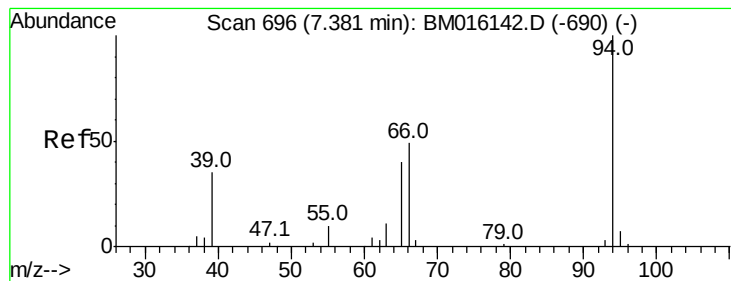

#6

Phenol

Concen: 1.413 ng/ul

RT: 7.38 min Scan# 695

Delta R.T. -0.01 min

Lab File: BM016156.D

Acq: 02 Aug 2018 01:30

Instrument :

BNA_M

ClientSampled :

C0AC0

Tot Ion: 94 Resp: 6508

Ion Ratio Lower Upper

94 100

65 52.8 21.0 31.6#


66 73.9 29.3 43.9#

Manual Integrations

APPROVED

Sohil

8/2/2018 2:19:42 PM

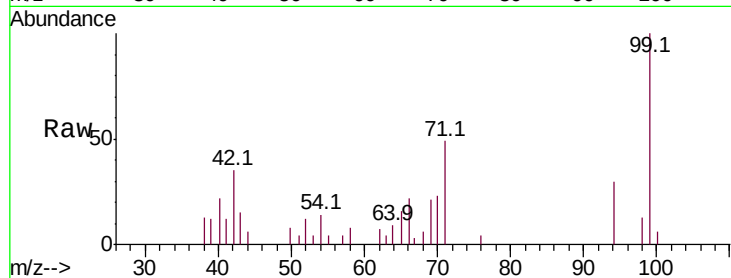


Abundance Ion 94.00 (93.70 to 94.70): BM016142.D (-690) (-)

Ion 65.00 (64.70 to 65.70): BM016142.D (-690) (-)

Ion 66.00 (65.70 to 66.70): BM016142.D (-690) (-)

Time-->

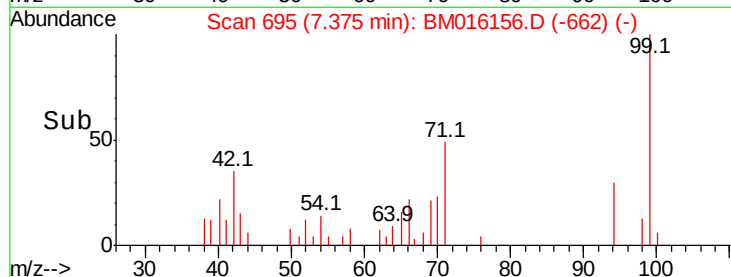


Abundance Ion 94.00 (93.70 to 94.70): BM016156.D (-662) (-)

Ion 65.00 (64.70 to 65.70): BM016156.D (-662) (-)

Ion 66.00 (65.70 to 66.70): BM016156.D (-662) (-)

Time-->

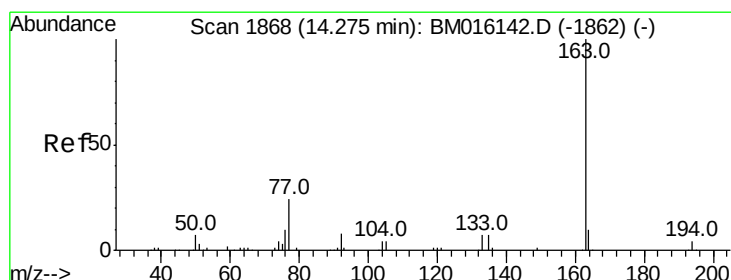

#44

Dimethylphthalate

Concen: 2.318 ng/ul

RT: 14.27 min Scan# 1868

Delta R.T. -0.00 min

Lab File: BM016156.D

Acq: 02 Aug 2018 01:30


Tgt Ion:163 Resp: 28974

Ion Ratio Lower Upper

163 100

194 3.5 3.2 4.8

164 10.2 7.8 11.8

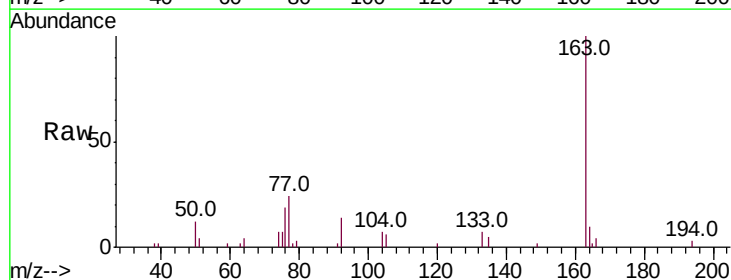


Abundance Ion 163.00 (162.70 to 163.70): BM016142.D (-1862) (-)

Ion 194.00 (193.70 to 194.70): BM016142.D (-1862) (-)

Ion 164.00 (163.70 to 164.70): BM016142.D (-1862) (-)

Time-->

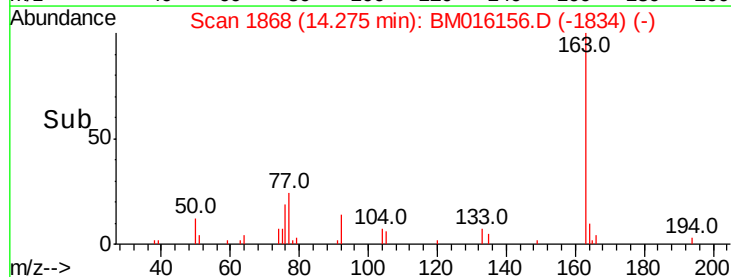

Abundance Ion 163.00 (162.70 to 163.70): BM016156.D (-1834) (-)

Ion 194.00 (193.70 to 194.70): BM016156.D (-1834) (-)

Ion 164.00 (163.70 to 164.70): BM016156.D (-1834) (-)

Time-->