

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
 Data File : BM002169.D
 Acq On : 02 Aug 2015 15:12
 Operator : TP
 Sample : G3095-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01R5

Quant Time: Aug 03 01:36:38 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 03 01:33:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	65307	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	291529	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	195804	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	469266	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	588374	20.00	ng/ul	0.00
86) Perylene-d12	23.37	264	609637	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.00	96	1787	1.42	ng/uL	0.00
5) Phenol-d5	6.74	99	43725	9.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	23945	9.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	37256	9.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	36236	9.76	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	18300	8.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	21694	9.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	40291	9.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	41229	8.46	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	141187	9.84	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	147960	8.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.46	143	14886	6.22	ng/ul	0.00
58) Fluorene-d10	15.22	176	106951	8.48	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	15306	5.33	ng/ul	0.00
71) Anthracene-d10	17.07	188	165090	7.88	ng/ul	0.00
79) Pyrene-d10	19.38	212	192131	7.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	220515	7.46	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	54111	3.78	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002169.D
Acq On : 02 Aug 2015 15:12
Operator : TP
Sample : G3095-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01R5

Quant Time: Aug 03 01:36:38 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 03 01:33:08 2015
Response via : Initial Calibration

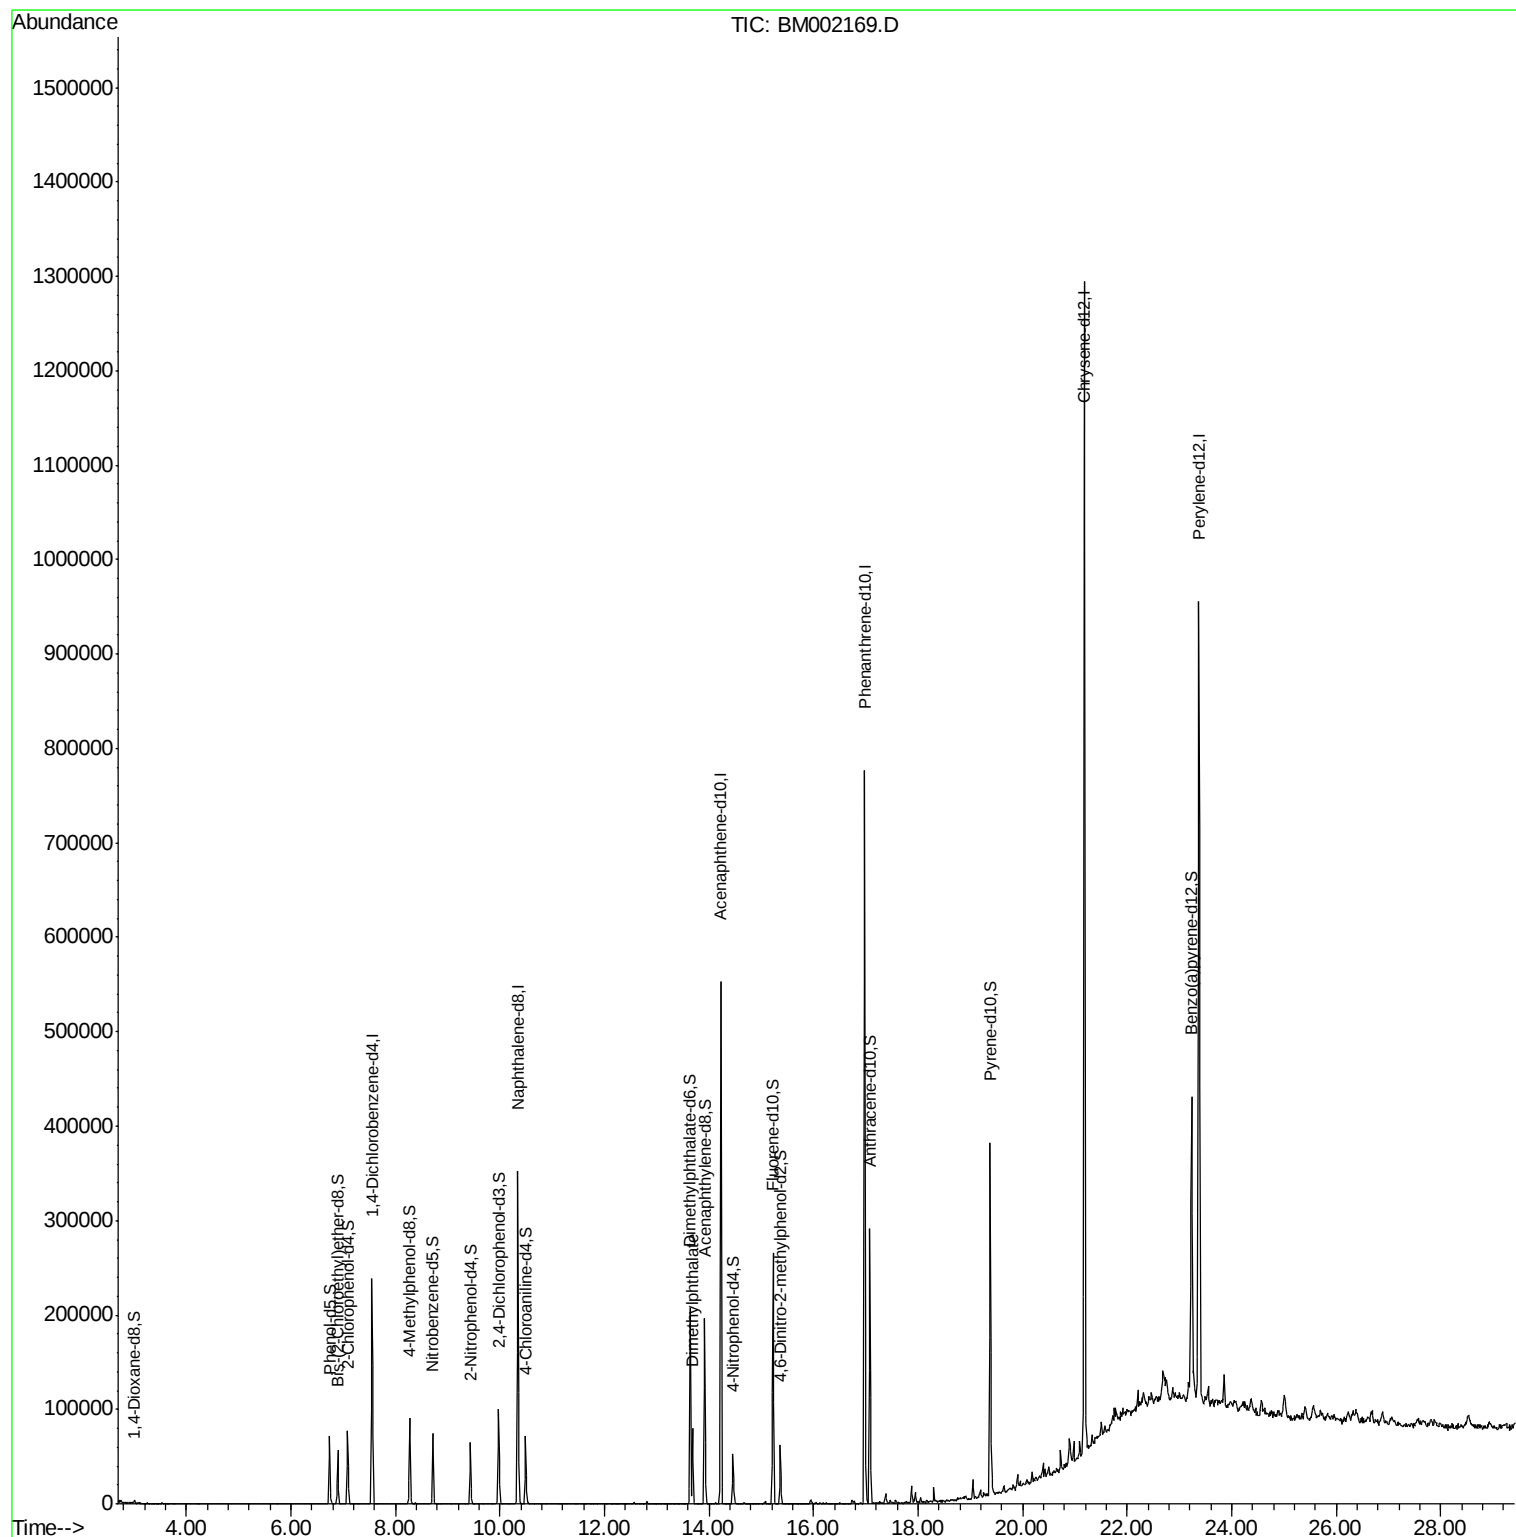

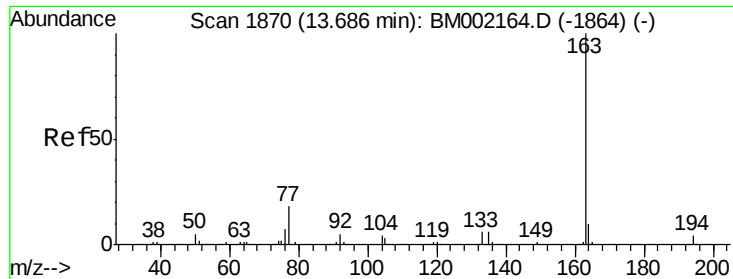

#45

Dimethylphthalate

Concen: 3.78 ng/ul

RT: 13.69 min Scan# 1870

Delta R.T. -0.00 min

Lab File: BM002169.D

Acq: 02 Aug 2015 15:12

Instrument :

BNA_M

ClientSampleId :

C01R5


Tgt Ion:163 Resp: 54111

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 9.7 8.0 12.0

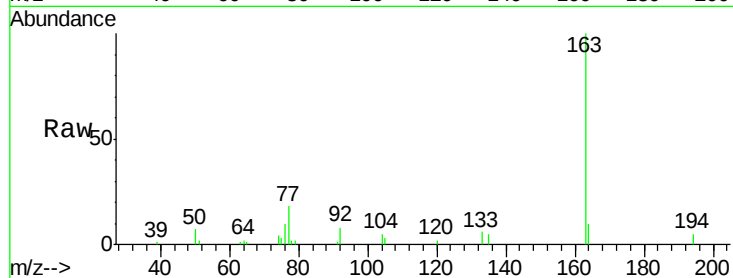

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

