

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
 Data File : BM002174.D
 Acq On : 02 Aug 2015 18:14
 Operator : TP
 Sample : G3095-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01S0

Quant Time: Aug 03 01:37:16 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 03 01:33:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	68226	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	304524	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	203455	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	490095	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	630753	20.00	ng/ul	0.00
86) Perylene-d12	23.37	264	648513	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.00	96	1368	1.04	ng/uL	0.00
5) Phenol-d5	6.74	99	37573	7.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	19102	7.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	30865	7.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	31620	8.15	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	14213	6.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	16460	6.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	33764	7.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	33427	6.57	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	116729	7.83	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	119420	6.41	ng/ul	0.00
52) 4-Nitrophenol-d4	14.46	143	11239	4.52	ng/ul	0.00
58) Fluorene-d10	15.22	176	89961	6.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	8397	2.80	ng/ul	0.00
71) Anthracene-d10	17.07	188	147824	6.76	ng/ul	0.00
79) Pyrene-d10	19.38	212	159847	6.02	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	191519	6.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.68	163	34287	2.30	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002174.D
Acq On : 02 Aug 2015 18:14
Operator : TP
Sample : G3095-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01S0

Quant Time: Aug 03 01:37:16 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 03 01:33:08 2015
Response via : Initial Calibration

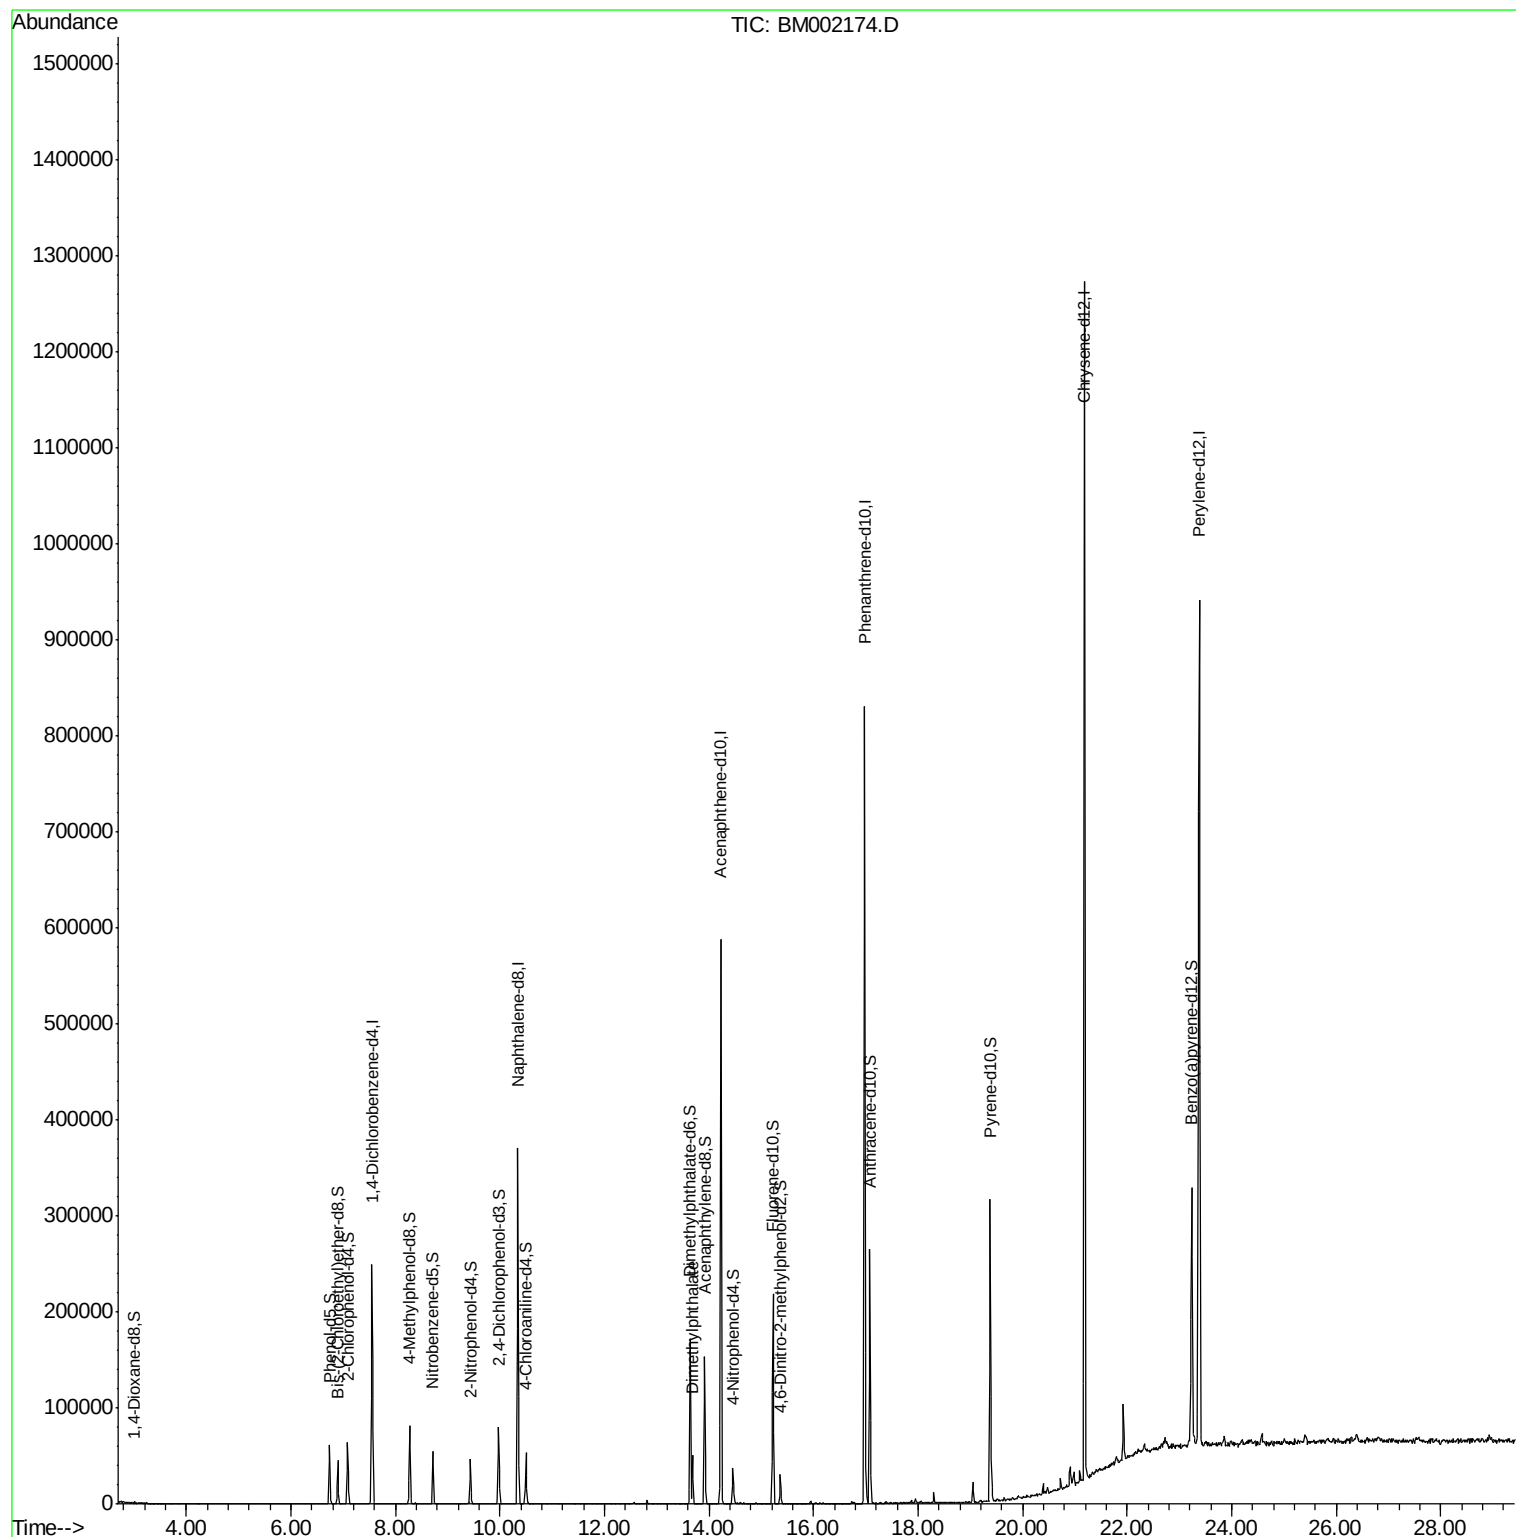

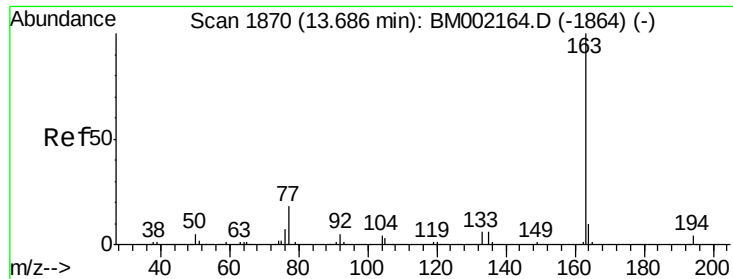

#45

Dimethylphthalate

Concen: 2.30 ng/ul

RT: 13.68 min Scan# 1869

Delta R.T. -0.01 min

Lab File: BM002174.D

Acq: 02 Aug 2015 18:14

Instrument :

BNA_M

ClientSampleId :

C01S0


Tgt Ion:163 Resp: 34287

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 9.0 8.0 12.0

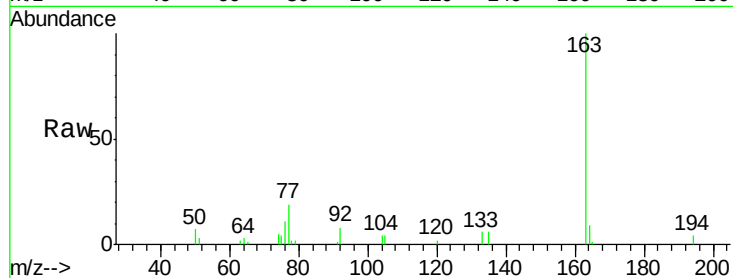

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

