

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
 Data File : BM002168.D
 Acq On : 02 Aug 2015 14:35
 Operator : TP
 Sample : G3095-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01R6

Quant Time: Aug 03 01:36:30 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 03 01:33:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	70413	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	318691	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	211995	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	513274	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	648168	20.00	ng/ul	0.00
86) Perylene-d12	23.37	264	659842	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.00	96	4922	3.62	ng/uL	0.00
5) Phenol-d5	6.74	99	118039	23.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	62653	22.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	98968	23.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	105878	26.46	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	45772	20.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	51824	20.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	112386	23.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	147536	27.69	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	398227	25.65	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	446011	22.97	ng/ul	0.00
52) 4-Nitrophenol-d4	14.46	143	60078	23.18	ng/ul	0.00
58) Fluorene-d10	15.22	176	329032	24.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	47943	15.27	ng/ul	0.00
71) Anthracene-d10	17.07	188	539302	23.54	ng/ul	0.00
79) Pyrene-d10	19.38	212	606386	22.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	703732	22.00	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.68	163	101979	6.58	ng/ul	100
57) Diethylphthalate	15.06	149	18231	1.19	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002168.D
Acq On : 02 Aug 2015 14:35
Operator : TP
Sample : G3095-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01R6

Quant Time: Aug 03 01:36:30 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 03 01:33:08 2015
Response via : Initial Calibration




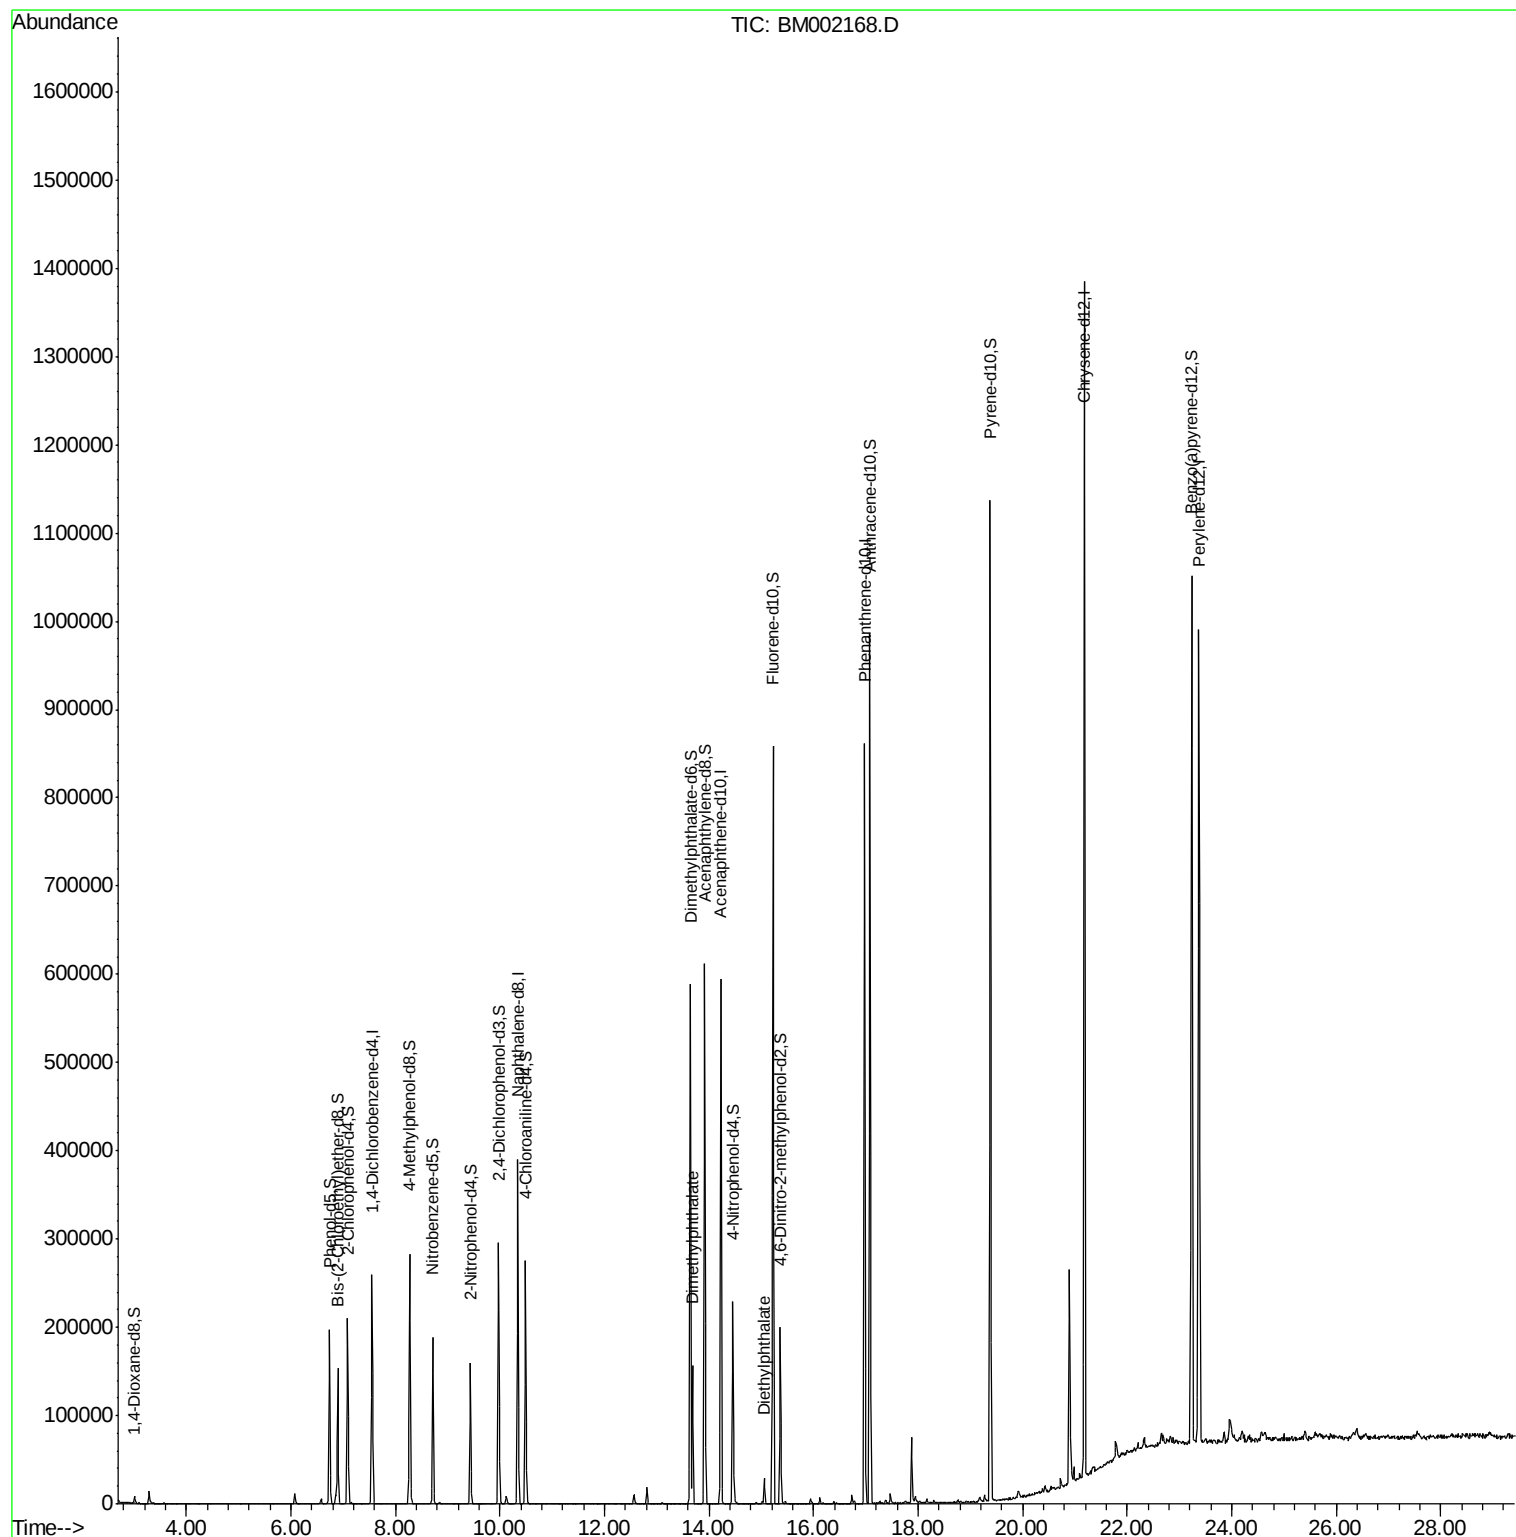


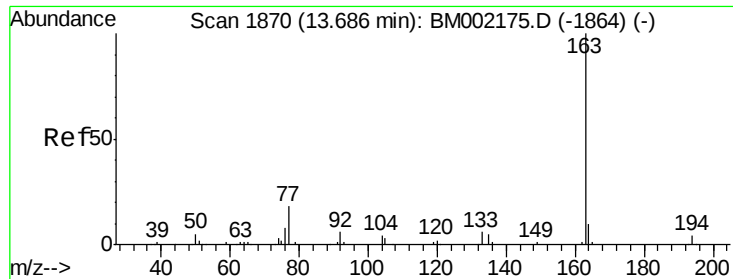

#45
Dimethylphthalate
Concen: 6.58 ng/ul
RT: 13.68 min Scan# 1869
Delta R.T. -0.01 min
Lab File: BM002168.D
Acq: 02 Aug 2015 14:35

Instrument :
BNA_M
ClientSampleId :
C01R6

Tgt Ion:163 Resp: 101979
Ion Ratio Lower Upper
163 100
194 4.4 3.5 5.3
164 10.0 8.0 12.0

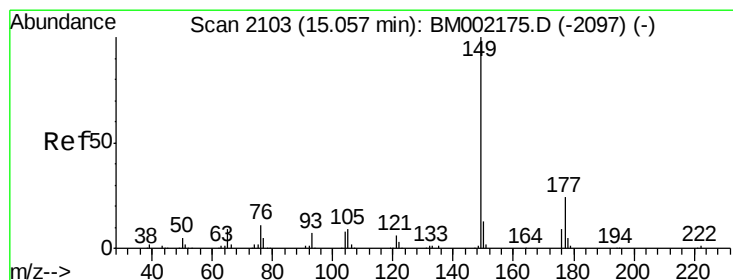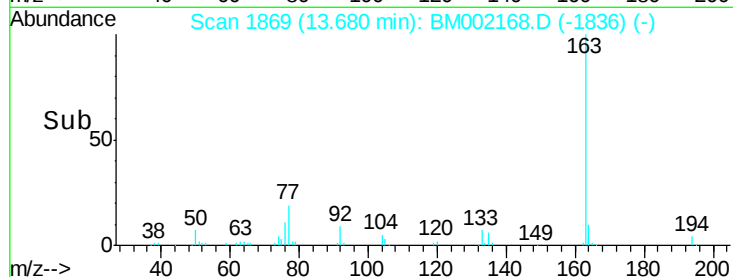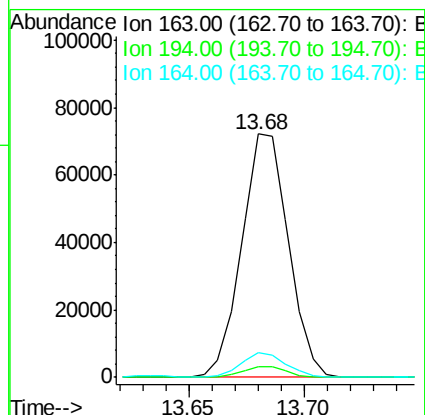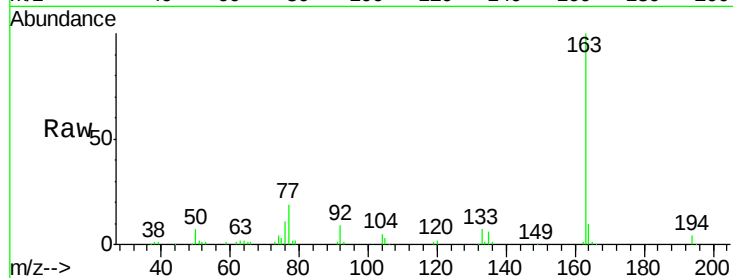

#57
Diethylphthalate
Concen: 1.19 ng/ul
RT: 15.06 min Scan# 2103
Delta R.T. -0.00 min
Lab File: BM002168.D
Acq: 02 Aug 2015 14:35

Tgt Ion:149 Resp: 18231
Ion Ratio Lower Upper
149 100
177 21.1 18.4 27.6
150 12.1 10.1 15.1

