

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
 Data File : BM002172.D
 Acq On : 02 Aug 2015 17:01
 Operator : TP
 Sample : G3095-19
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01J0

Quant Time: Aug 03 01:37:01 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 03 01:33:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	68664	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	315456	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.22	164	218998	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	521762	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	655961	20.00	ng/ul	0.00
86) Perylene-d12	23.37	264	665768	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.00	96	4933	3.72	ng/uL	0.00
5) Phenol-d5	6.74	99	121168	24.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	65843	24.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	102488	24.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	106677	27.34	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	52981	23.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	61208	24.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	113979	23.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	147233	27.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.64	166	386612	24.10	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	440505	21.96	ng/ul	0.00
52) 4-Nitrophenol-d4	14.46	143	62671	23.41	ng/ul	0.00
58) Fluorene-d10	15.22	176	320597	22.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	59366	18.60	ng/ul	0.00
71) Anthracene-d10	17.07	188	511553	21.96	ng/ul	0.00
79) Pyrene-d10	19.38	212	572773	20.74	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	645577	20.00	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.69	163	196430	12.26	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002172.D
Acq On : 02 Aug 2015 17:01
Operator : TP
Sample : G3095-19
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01J0

Quant Time: Aug 03 01:37:01 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 03 01:33:08 2015
Response via : Initial Calibration

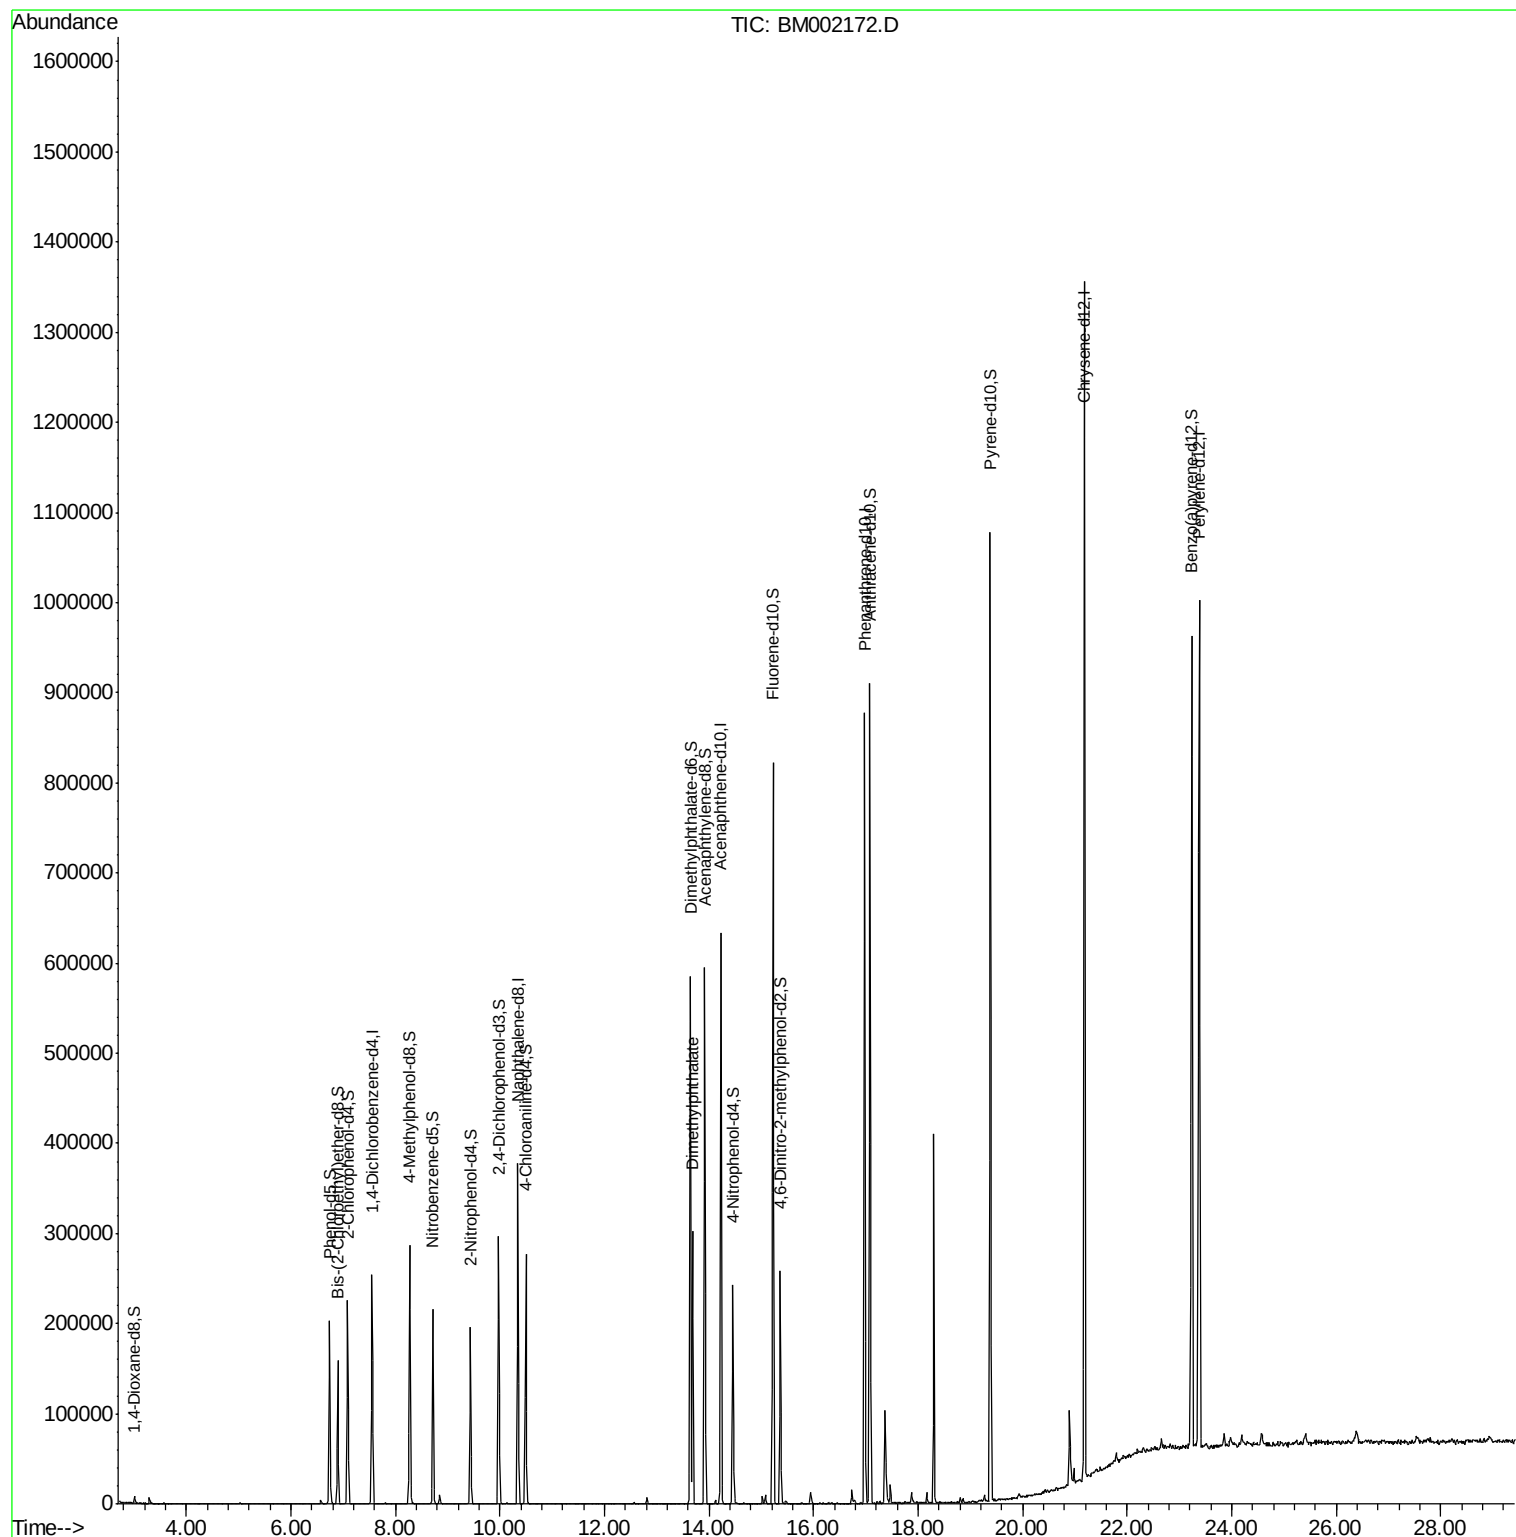


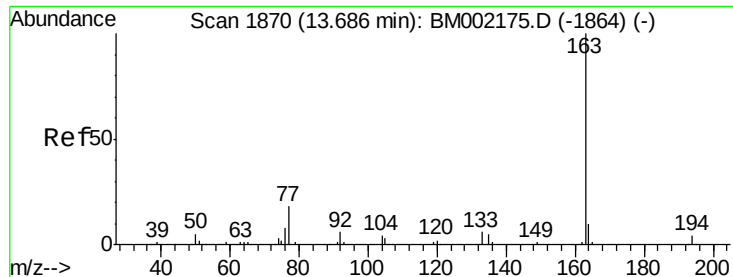

#45
 Dimethylphthalate
 Concen: 12.26 ng/ul
 RT: 13.69 min Scan# 1870
 Delta R.T. -0.00 min
 Lab File: BM002172.D
 Acq: 02 Aug 2015 17:01

Instrument :
 BNA_M
 ClientSampleId :
 C01J0

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.5	5.3
164	10.1	8.0	12.0

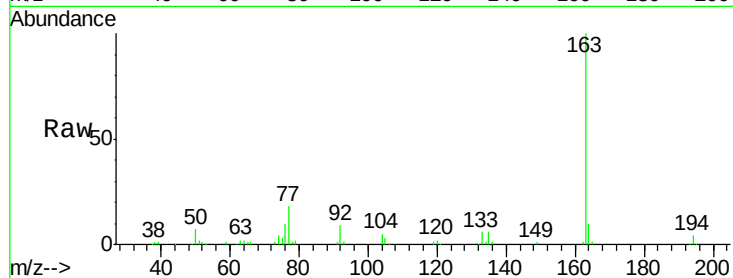

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

