

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
 Data File : BM002166.D
 Acq On : 02 Aug 2015 12:28
 Operator : TP
 Sample : PB84595BL
 Misc : SBLK95
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.005	48	54	64	rVB	21244	28994	0.66%	0.083%
2	3.563	146	149	152	rBB	4623	5812	0.13%	0.017%
3	6.740	682	689	701	rBB	477959	726457	16.47%	2.090%
4	6.899	709	716	725	rVB	371987	551911	12.51%	1.588%
5	7.087	742	748	759	rBB	497981	767286	17.39%	2.207%
6	7.551	821	827	835	rBB	308791	495937	11.24%	1.427%
7	8.275	943	950	963	rBB	642525	1019428	23.11%	2.933%
8	8.722	1018	1026	1034	rBB	484948	786402	17.82%	2.262%
9	9.434	1141	1147	1156	rBB	449115	725518	16.44%	2.087%
10	9.975	1232	1239	1253	rBB	659474	1092091	24.75%	3.142%
11	10.345	1294	1302	1311	rBB	482441	789130	17.89%	2.270%
12	10.492	1320	1327	1336	rBV	662193	1108958	25.14%	3.190%
13	13.639	1855	1862	1868	rBV	1328025	1814937	41.14%	5.221%
14	13.916	1902	1909	1917	rBV	1436710	2075577	47.05%	5.971%
15	14.228	1955	1962	1969	rBB2	761755	1158346	26.26%	3.332%
16	14.457	1995	2001	2018	rBV	574258	859933	19.49%	2.474%
17	15.227	2125	2132	2138	rBV	1853889	2613317	59.23%	7.518%
18	15.369	2150	2156	2168	rBV	665342	905805	20.53%	2.606%
19	15.463	2168	2172	2176	rVB	7513	9587	0.22%	0.028%
20	16.980	2423	2430	2436	rBV	1073854	1473466	33.40%	4.239%
21	17.080	2440	2447	2454	rVB	2245839	3072590	69.64%	8.839%
22	19.268	2814	2819	2824	rBV	19834	24275	0.55%	0.070%
23	19.386	2832	2839	2845	rBV	2806197	3736512	84.69%	10.749%
24	19.639	2877	2882	2885	rBV3	3738	6733	0.15%	0.019%
25	20.727	3065	3067	3070	rVB2	5711	4467	0.10%	0.013%
26	20.974	3106	3109	3114	rVB3	17888	21078	0.48%	0.061%
27	21.186	3139	3145	3150	rBV	1573796	2017961	45.74%	5.805%
28	22.198	3315	3317	3322	rBV6	22268	22069	0.50%	0.063%
29	22.651	3391	3394	3397	rBV	25977	30419	0.69%	0.088%
30	22.686	3398	3400	3405	rVB2	31488	38863	0.88%	0.112%
31	23.245	3486	3495	3506	rBV	2265456	4411794	100.00%	12.691%
32	23.374	3510	3517	3525	rVB2	1148670	2109615	47.82%	6.069%
33	23.850	3594	3598	3606	rVB	60843	107730	2.44%	0.310%
34	24.568	3715	3720	3729	rVB	68104	149180	3.38%	0.429%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002166.D
Acq On : 02 Aug 2015 12:28
Operator : TP
Sample : PB84595BL
Misc : SBLK95
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK95

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Title : SVOA CALIBRATION


Sum of corrected areas: 34762178

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002166.D
Acq On : 02 Aug 2015 12:28
Operator : TP
Sample : PB84595BL
Misc : SBLK95
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK95

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

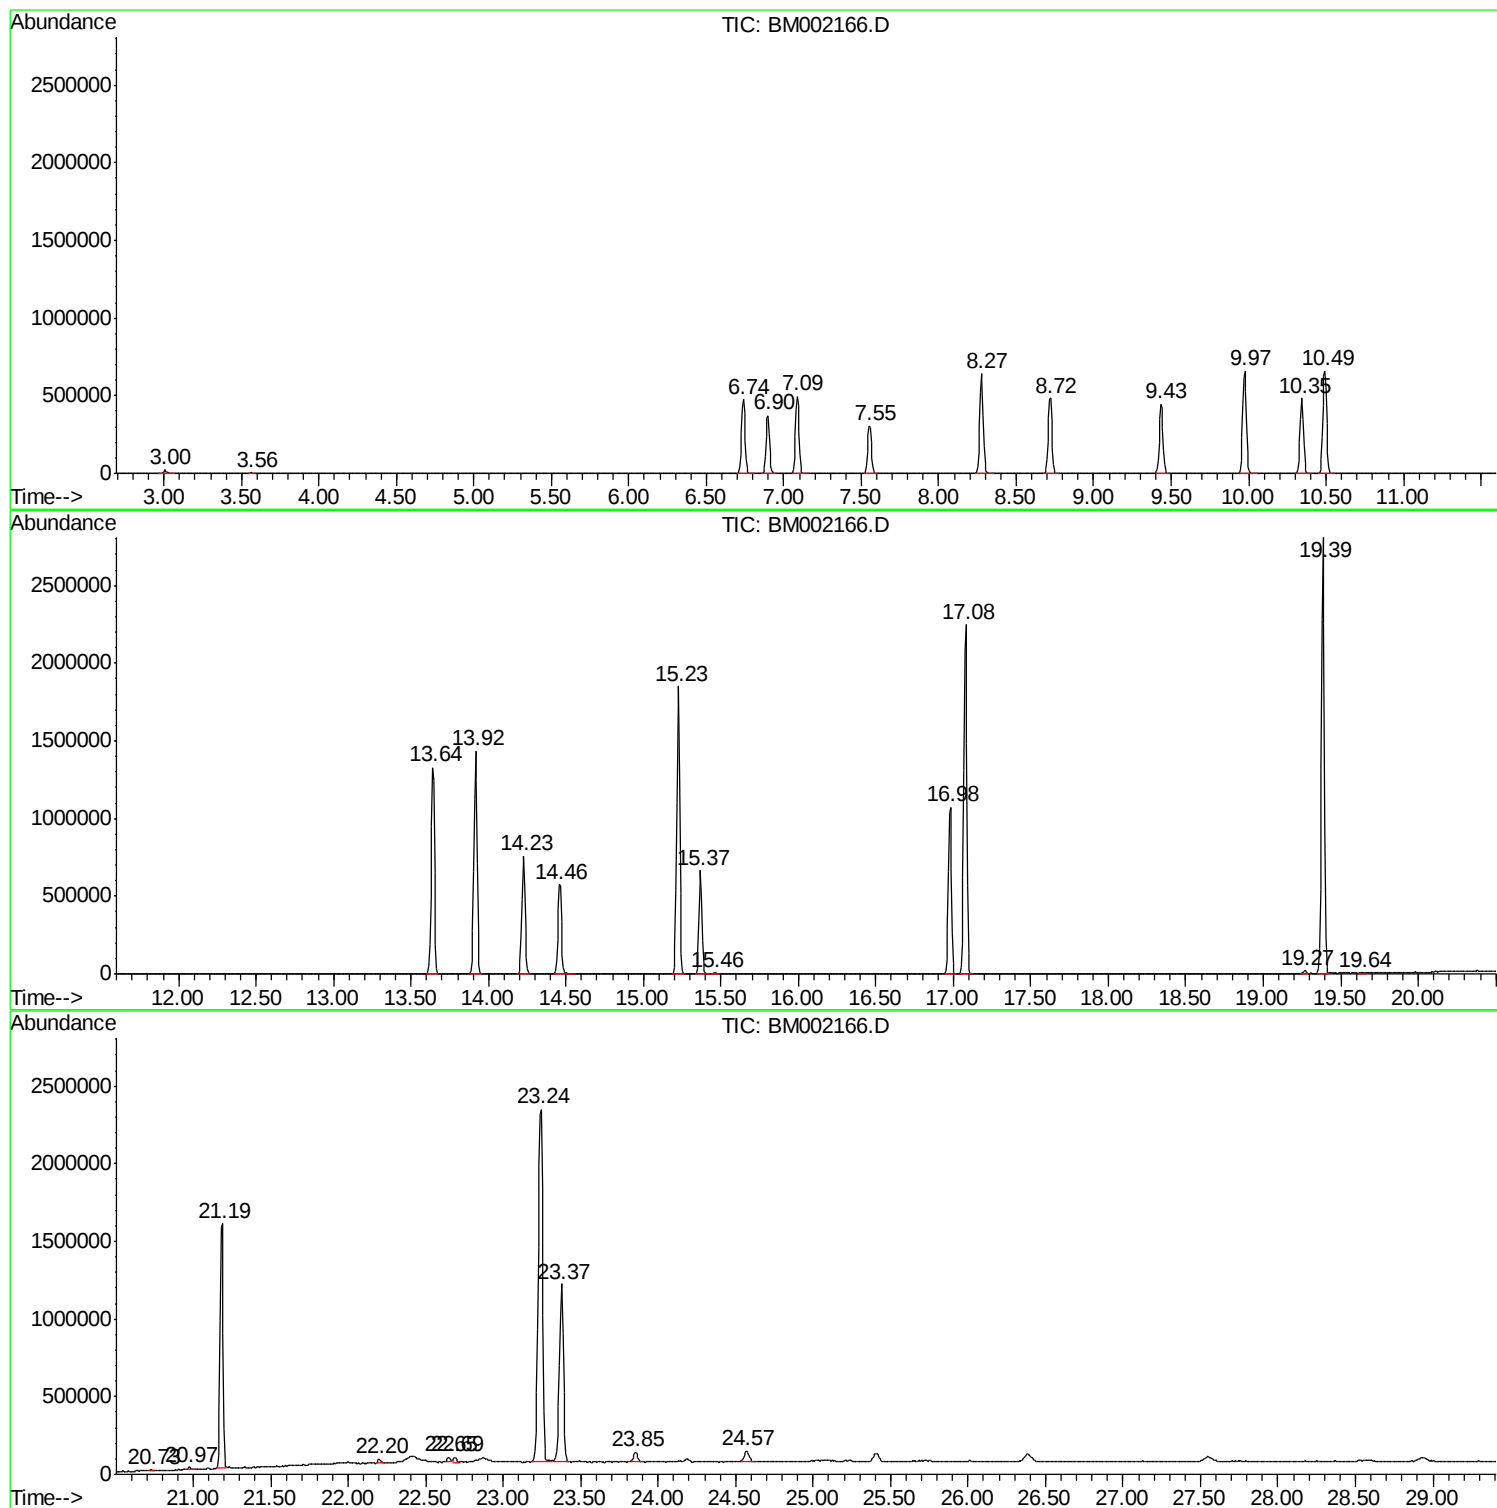

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002166.D
Acq On : 02 Aug 2015 12:28
Operator : TP
Sample : PB84595BL
Misc : SBLK95
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK95

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002166.D
Acq On : 02 Aug 2015 12:28
Operator : TP
Sample : PB84595BL
Misc : SBLK95
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK95

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc