

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
 Data File : BM002170.D
 Acq On : 02 Aug 2015 15:48
 Operator : TP
 Sample : G3095-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01Q8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.746	8	10	14	rVB2	3083	3680	0.17%	0.023%
2	3.011	51	55	60	rVB	4653	5075	0.24%	0.032%
3	3.293	98	103	110	rBV	3773	5468	0.25%	0.035%
4	3.358	110	114	120	rVB	17851	22466	1.05%	0.143%
5	6.069	572	575	582	rBV	5952	7994	0.37%	0.051%
6	6.734	683	688	698	rBB	119923	186864	8.71%	1.187%
7	6.852	704	708	711	rBV	11278	17122	0.80%	0.109%
8	6.893	711	715	722	rVB	91997	136741	6.37%	0.868%
9	7.087	742	748	756	rBB	126996	195954	9.13%	1.244%
10	7.552	821	827	836	rBB	362303	563929	26.29%	3.581%
11	8.275	944	950	960	rBB	162686	259503	12.10%	1.648%
12	8.387	965	969	971	rBB	1705	2291	0.11%	0.015%
13	8.716	1019	1025	1032	rBB	100480	158261	7.38%	1.005%
14	9.434	1141	1147	1154	rBB	75929	116026	5.41%	0.737%
15	9.969	1233	1238	1248	rBB	166956	275450	12.84%	1.749%
16	10.122	1260	1264	1269	rBB	5362	7671	0.36%	0.049%
17	10.340	1294	1301	1309	rBV	517421	864531	40.30%	5.490%
18	10.487	1319	1326	1335	rBV	146165	242093	11.29%	1.537%
19	12.016	1581	1586	1590	rBB2	2376	3828	0.18%	0.024%
20	12.245	1621	1625	1628	rBB3	2668	3427	0.16%	0.022%
21	12.557	1673	1678	1683	rBV2	6654	10778	0.50%	0.068%
22	12.739	1705	1709	1712	rBB	2387	2532	0.12%	0.016%
23	12.816	1717	1722	1726	rBB3	12541	18300	0.85%	0.116%
24	13.386	1818	1819	1825	rVB2	2240	2618	0.12%	0.017%
25	13.539	1840	1845	1848	rBB	3325	5019	0.23%	0.032%
26	13.592	1851	1854	1855	rBV	3187	2633	0.12%	0.017%
27	13.634	1856	1861	1866	rVV	323120	446375	20.81%	2.835%
28	13.681	1866	1869	1875	rVB	96820	127803	5.96%	0.812%
29	13.916	1902	1909	1917	rVB	342195	504487	23.52%	3.204%
30	14.228	1955	1962	1969	rBV2	812716	1269563	59.18%	8.062%
31	14.286	1969	1972	1976	rVB	6398	7776	0.36%	0.049%
32	14.457	1993	2001	2010	rBV	73927	118940	5.54%	0.755%
33	14.622	2023	2029	2033	rBV	7018	11157	0.52%	0.071%
34	14.657	2033	2035	2038	rVB	4531	3475	0.16%	0.022%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
 Data File : BM002170.D
 Acq On : 02 Aug 2015 15:48
 Operator : TP
 Sample : G3095-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01Q8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Title : SVOA CALIBRATION

35	14.698	2038	2042	2046	rBV	4120	4782	0.22%	0.030%
36	14.845	2063	2067	2071	rBB	3183	4737	0.22%	0.030%
37	14.898	2072	2076	2079	rBB	3600	3871	0.18%	0.025%
38	15.022	2089	2097	2099	rBV3	4331	7699	0.36%	0.049%
39	15.051	2099	2102	2110	rVB	22528	29907	1.39%	0.190%
40	15.222	2125	2131	2137	rBV	466751	639599	29.81%	4.062%
41	15.280	2137	2141	2144	rVB	7731	10428	0.49%	0.066%
42	15.363	2151	2155	2160	rVV	55151	75289	3.51%	0.478%
43	15.398	2160	2161	2165	rVB	5340	4893	0.23%	0.031%
44	15.439	2165	2168	2169	rBV2	2934	2851	0.13%	0.018%
45	15.480	2170	2175	2180	rVB4	6166	10615	0.49%	0.067%
46	15.575	2188	2191	2193	rBV2	1576	2359	0.11%	0.015%
47	15.722	2213	2216	2219	rBV3	2441	3359	0.16%	0.021%
48	15.786	2222	2227	2230	rVV4	2910	4901	0.23%	0.031%
49	15.957	2250	2256	2265	rVB3	8364	18431	0.86%	0.117%
50	16.039	2267	2270	2274	rBV3	2610	4173	0.19%	0.026%
51	16.116	2281	2283	2288	rVB2	5783	7766	0.36%	0.049%
52	16.169	2290	2292	2297	rBV3	1894	3025	0.14%	0.019%
53	16.333	2315	2320	2325	rBV3	6993	10759	0.50%	0.068%
54	16.380	2325	2328	2329	rBV	2906	2990	0.14%	0.019%
55	16.439	2334	2338	2340	rVB4	2671	3506	0.16%	0.022%
56	16.474	2340	2344	2348	rVB6	2327	3854	0.18%	0.024%
57	16.527	2348	2353	2355	rBV5	3720	6981	0.33%	0.044%
58	16.551	2355	2357	2361	rVB4	2623	3378	0.16%	0.021%
59	16.633	2367	2371	2374	rVB3	3107	4338	0.20%	0.028%
60	16.733	2384	2388	2390	rBV2	6344	7325	0.34%	0.047%
61	16.786	2394	2397	2404	rVB4	9681	15873	0.74%	0.101%
62	16.974	2422	2429	2434	rBV2	1162288	1640530	76.47%	10.417%
63	17.016	2434	2436	2440	rVV	63085	71189	3.32%	0.452%
64	17.074	2440	2446	2455	rVV	518505	730499	34.05%	4.639%
65	17.174	2457	2463	2466	rBV6	3814	7307	0.34%	0.046%
66	17.210	2466	2469	2472	rBV3	1963	3197	0.15%	0.020%
67	17.251	2474	2476	2483	rVB2	3922	6508	0.30%	0.041%
68	17.327	2486	2489	2490	rBV3	3124	3393	0.16%	0.022%
69	17.386	2495	2499	2505	rVB2	10423	20075	0.94%	0.127%
70	17.439	2505	2508	2509	rBV3	3736	3846	0.18%	0.024%
71	17.469	2509	2513	2517	rVB5	8193	11213	0.52%	0.071%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
 Data File : BM002170.D
 Acq On : 02 Aug 2015 15:48
 Operator : TP
 Sample : G3095-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01Q8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Title : SVOA CALIBRATION

72	17.557	2525	2528	2534	rVB5	7292	10891	0.51%	0.069%
73	17.639	2540	2542	2545	rVB4	3878	3673	0.17%	0.023%
74	17.692	2549	2551	2553	rBV3	2756	2539	0.12%	0.016%
75	17.751	2555	2561	2562	rBV4	3988	6827	0.32%	0.043%
76	17.874	2578	2582	2585	rBV3	34938	43519	2.03%	0.276%
77	17.945	2590	2594	2598	rBV	18409	22846	1.06%	0.145%
78	17.986	2598	2601	2605	rBV6	7539	9583	0.45%	0.061%
79	18.045	2607	2611	2616	rVB4	17387	21416	1.00%	0.136%
80	18.163	2628	2631	2633	rBV3	5920	7716	0.36%	0.049%
81	18.398	2669	2671	2674	rVB3	7076	7601	0.35%	0.048%
82	18.551	2695	2697	2698	rBV2	7078	4918	0.23%	0.031%
83	19.045	2776	2781	2785	rBV	81037	114590	5.34%	0.728%
84	19.098	2786	2790	2794	rVB	64169	80850	3.77%	0.513%
85	19.380	2833	2838	2851	rBV2	678937	1027873	47.91%	6.527%
86	20.898	3093	3096	3103	rVB3	92387	144022	6.71%	0.915%
87	21.180	3139	3144	3149	rBV	1709180	2145244	100.00%	13.622%
88	21.674	3226	3228	3233	rVB	78330	88701	4.13%	0.563%
89	21.821	3250	3253	3257	rVB2	120940	146376	6.82%	0.929%
90	23.233	3487	3493	3498	rBV	451374	815570	38.02%	5.179%
91	23.374	3510	3517	3531	rVB	1062974	2037803	94.99%	12.940%


Sum of corrected areas: 15747834

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002170.D
Acq On : 02 Aug 2015 15:48
Operator : TP
Sample : G3095-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01Q8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

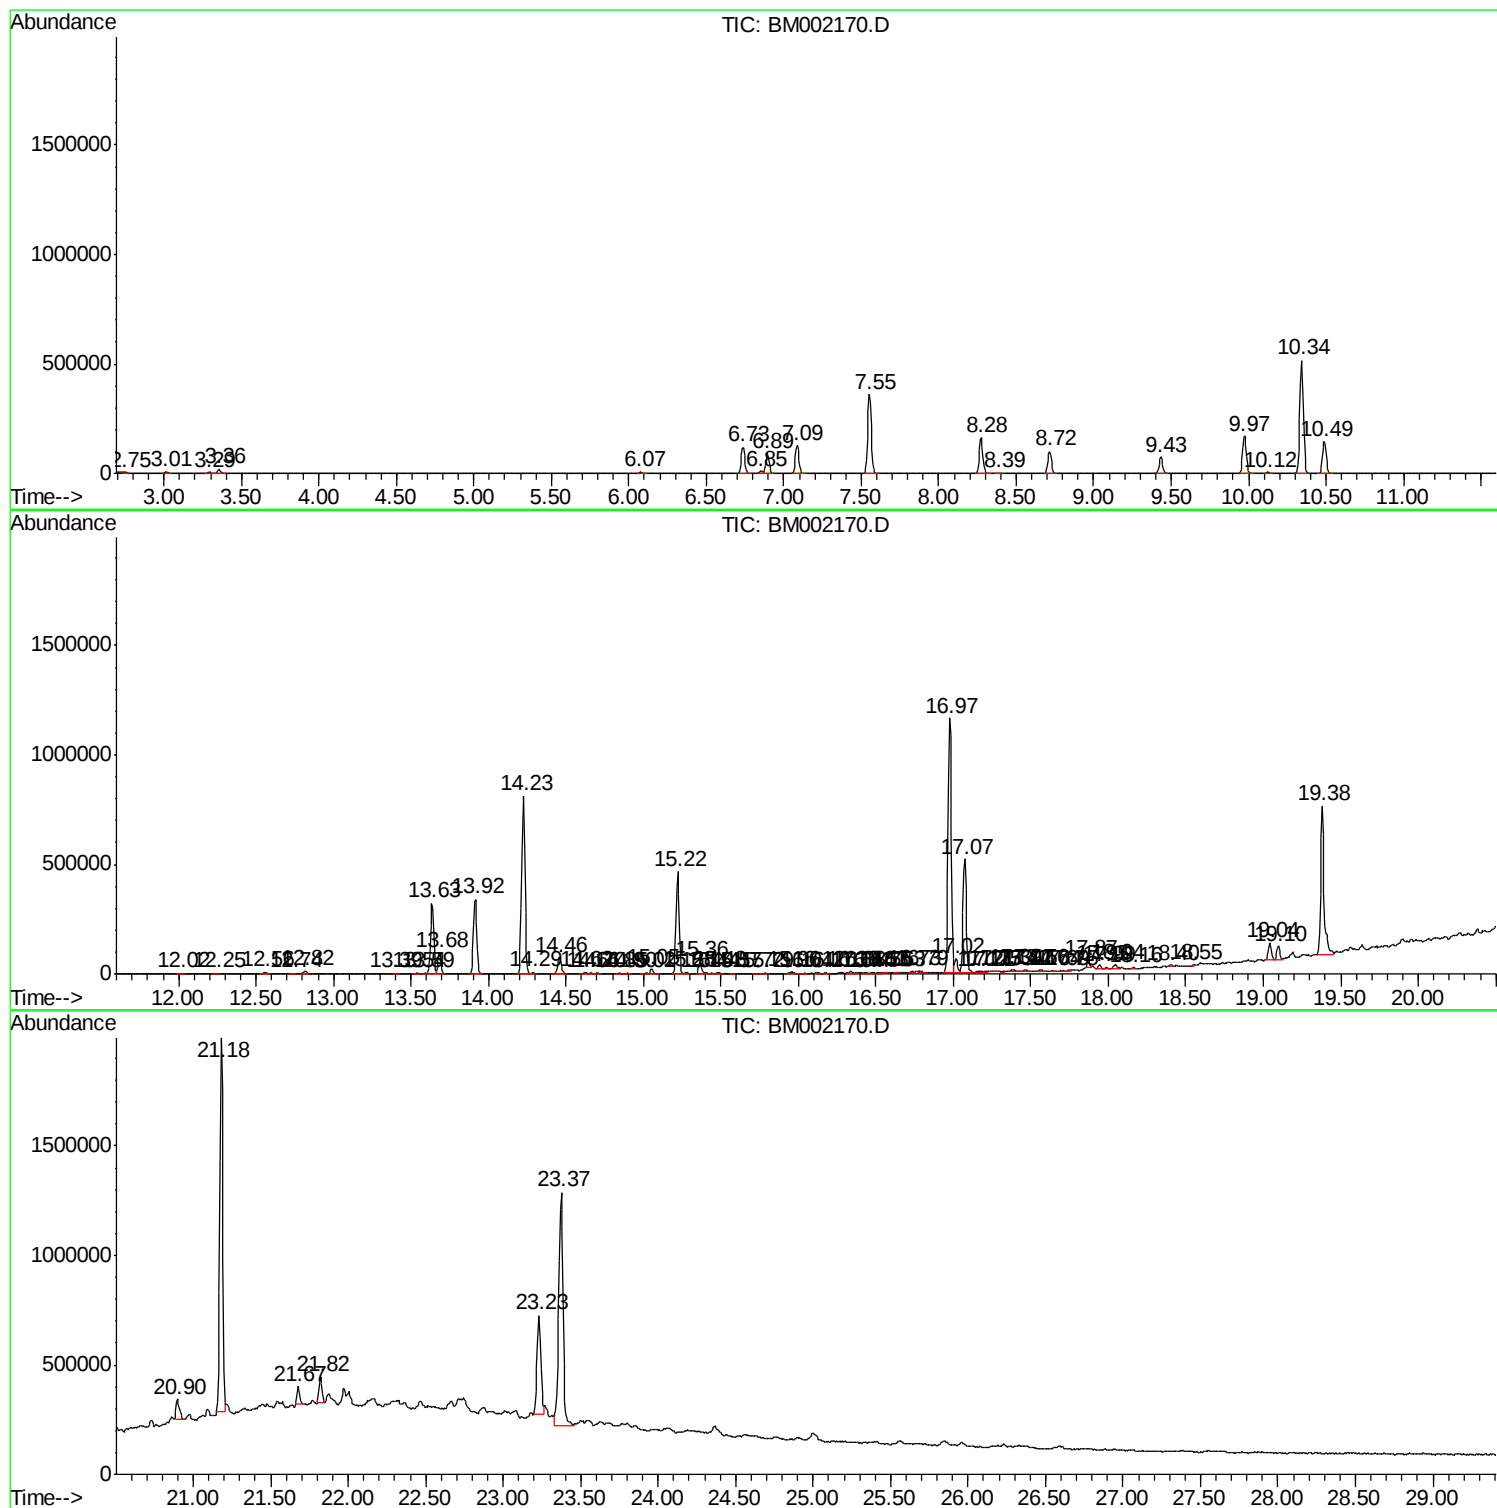

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002170.D
Acq On : 02 Aug 2015 15:48
Operator : TP
Sample : G3095-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01Q8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080215\
Data File : BM002170.D
Acq On : 02 Aug 2015 15:48
Operator : TP
Sample : G3095-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01Q8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
