


Data Path : Z:\HPCHEM1\BNA_M\Data\BM080215\
 Data File : BM002163.D
 Acq On : 02 Aug 2015 10:25
 Operator : TP
 Sample : DFTPP87
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP87

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Title : SVOA CALIBRATION
 Last Update : Mon Aug 03 02:05:53 2015

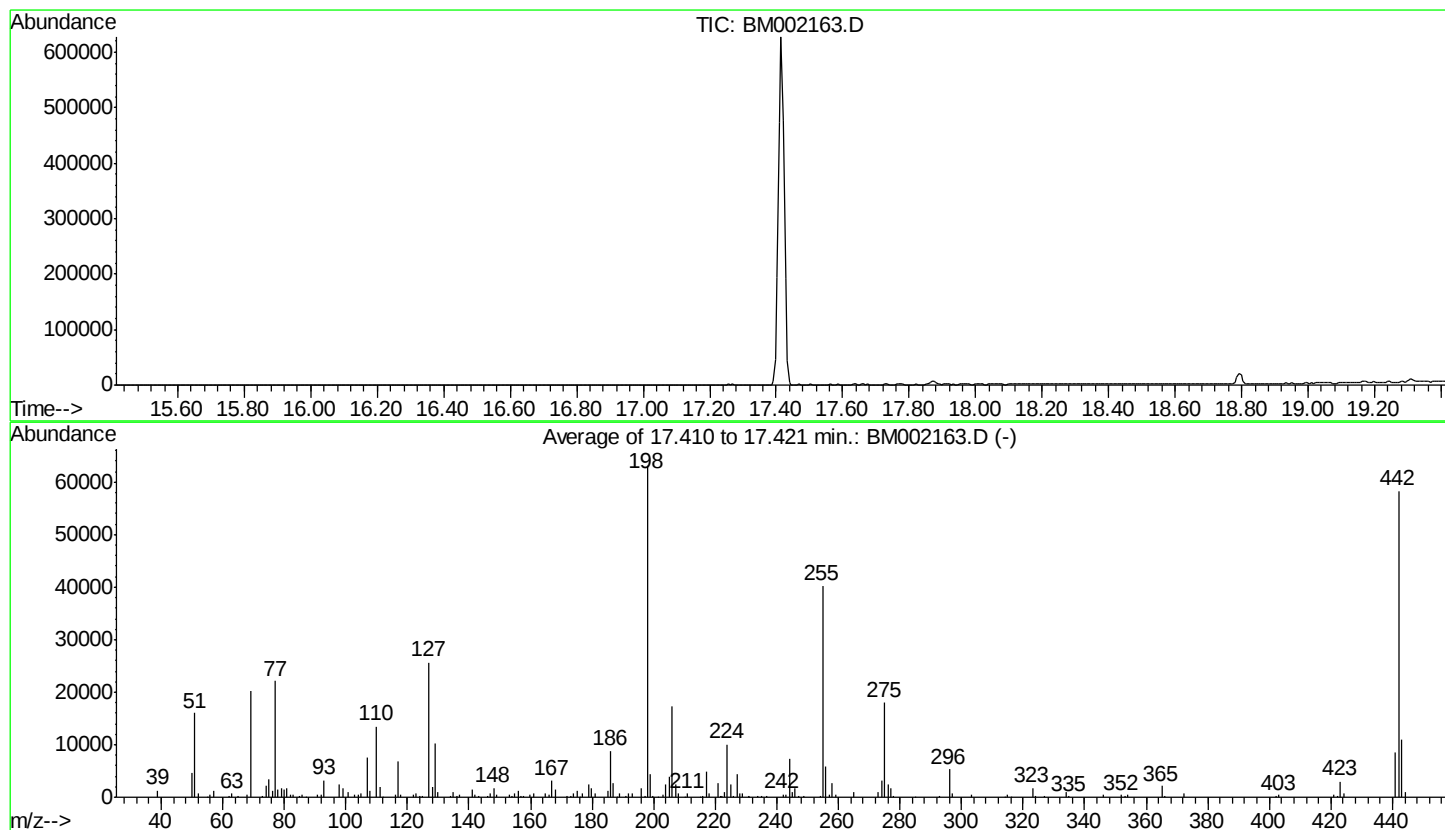

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	16009	PASS
68	69	0.00	2	2.0	399	PASS
69	198	0.00	100	32.2	20343	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.6	25605	PASS
197	198	0.00	2	0.2	142	PASS
198	198	100	100	100.0	63130	PASS
199	198	5	9	6.8	4282	PASS
275	198	10	60	28.5	17968	PASS
365	198	1	100	3.4	2168	PASS
441	443	0.01	100	78.7	8626	PASS
442	198	50	100	92.3	58282	PASS
443	442	15	24	18.8	10960	PASS

m/z	Abundance
39.00	1455.0
44.00	645.0
50.00	4873.0
51.10	16332.0
52.00	843.0
56.00	758.0
57.00	1436.0
62.00	332.0
63.00	710.0
65.10	412.0
68.10	345.0
69.00	20984.0
72.90	330.0
74.00	2231.0
75.00	3751.0
76.00	1124.0
77.10	22712.0
78.00	1614.0
79.00	1780.0
80.00	1431.0
80.90	1927.0
81.90	458.0
83.00	512.0
85.00	362.0
85.90	614.0
87.00	303.0
91.00	513.0
91.90	486.0
93.00	3243.0
98.00	2254.0
99.00	1714.0
100.90	949.0
102.90	404.0
104.00	671.0
105.00	589.0
107.00	7862.0
107.90	1341.0
110.00	13364.0
111.00	1943.0
116.10	405.0
117.00	6935.0
118.00	455.0
121.90	503.0
123.00	827.0
124.00	332.0
124.90	451.0
127.00	24856.0
128.00	1960.0
129.00	10165.0
130.00	882.0
133.90	323.0
135.00	811.0
137.10	382.0
140.90	1383.0
142.00	356.0
143.00	335.0
146.00	362.0
146.90	641.0
148.00	1851.0
149.00	323.0
152.90	398.0
153.90	329.0
154.90	820.0
156.00	1167.0
157.00	361.0
160.00	436.0
161.00	566.0
164.90	673.0
166.00	484.0
167.00	2737.0
168.00	1530.0
174.00	701.0
175.00	1144.0
176.00	337.0
177.00	638.0
178.90	2162.0
180.00	1563.0
181.00	745.0
184.90	1124.0
186.00	8276.0
187.00	2268.0
188.90	562.0
191.90	684.0
193.00	717.0
196.00	1638.0
197.10	426.0
197.90	57264.0
199.00	4365.0
202.90	496.0
203.90	2318.0
205.00	3577.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

206.00	15504.0
207.00	2611.0
208.00	784.0
210.90	591.0
216.00	307.0
217.00	4257.0
217.90	457.0
221.00	2248.0
221.80	540.0
223.00	929.0
224.00	9034.0
225.00	2266.0
227.00	3830.0
228.00	607.0
229.00	650.0
230.80	376.0
236.90	347.0
242.00	526.0
243.10	461.0
244.10	6480.0
245.00	990.0
246.00	1487.0
246.90	309.0
254.00	306.0
255.00	35384.0
256.00	5140.0
256.90	325.0
258.00	2112.0
259.00	317.0
265.10	798.0
273.00	1019.0
274.00	2589.0
275.00	14920.0
276.00	1983.0
277.00	1484.0
296.00	4735.0
296.90	583.0
303.10	435.0
315.00	418.0
323.00	1472.0
334.00	959.0
345.90	322.0
352.00	424.0
353.00	353.0
354.00	473.0
365.00	1593.0
366.00	307.0
372.10	421.0
402.10	325.0
403.10	345.0
420.90	368.0
423.00	2247.0
424.00	539.0
441.00	6286.0
442.10	41632.0
443.10	7951.0
444.00	705.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

m/z	Abundance
39.00	1577.0
44.00	735.0
50.00	5267.0
51.00	18784.0
52.00	938.0
55.00	342.0
55.90	548.0
57.00	1360.0
62.00	354.0
63.00	777.0
65.00	531.0
68.00	499.0
69.00	24416.0
73.00	342.0
74.00	2681.0
75.00	3959.0
76.10	1468.0
77.10	26192.0
78.10	1799.0
79.00	2245.0
80.00	1626.0
81.00	2149.0
82.00	628.0
83.00	441.0
85.10	422.0
85.90	704.0
91.00	545.0
92.00	535.0
93.00	3553.0
98.00	2891.0
99.00	2043.0
101.00	1067.0
103.00	411.0
104.10	632.0
104.90	815.0
107.00	9363.0
108.00	1593.0
110.00	16101.0
111.00	2492.0
111.90	311.0
116.10	410.0
117.00	8267.0
117.90	594.0
121.90	571.0
123.00	1019.0
124.00	488.0
125.00	388.0
127.00	30768.0
128.00	2359.0
129.00	12200.0
130.00	1018.0
134.00	386.0
135.00	1226.0
136.00	583.0
137.00	615.0
141.00	1780.0
141.90	770.0
143.00	522.0
146.00	337.0
147.00	1130.0
148.00	2159.0
149.00	440.0
152.90	435.0
153.90	433.0
155.00	903.0
156.00	1469.0
156.90	313.0
157.80	401.0
159.90	459.0
161.00	770.0
164.90	915.0
166.00	529.0
166.90	3637.0
167.90	1836.0
171.90	387.0
173.00	344.0
174.00	582.0
175.00	1387.0
176.90	774.0
179.00	2513.0
180.00	1830.0
180.90	906.0
184.90	1180.0
186.00	10403.0
187.00	2936.0
188.00	384.0
188.90	807.0
191.10	344.0
192.00	836.0
193.00	1035.0
196.00	2005.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

198.00	74976.0
198.90	5136.0
199.90	362.0
201.50	349.0
203.00	542.0
204.00	2674.0
205.10	4869.0
206.00	20680.0
207.10	3084.0
208.00	793.0
210.00	355.0
210.90	868.0
214.90	340.0
215.90	472.0
217.00	5650.0
217.90	964.0
221.10	2846.0
222.10	699.0
223.00	1118.0
224.00	11891.0
225.00	3024.0
226.00	409.0
227.00	5468.0
227.90	842.0
229.00	1095.0
231.00	445.0
234.00	331.0
234.90	398.0
236.90	400.0
242.00	631.0
243.00	634.0
244.00	8926.0
245.00	1195.0
246.00	1923.0
247.00	418.0
248.90	372.0
254.10	374.0
255.00	48440.0
256.00	6852.0
256.90	619.0
258.00	2924.0
258.90	499.0
264.90	1189.0
273.00	1197.0
274.00	3917.0
275.00	21232.0
276.00	2850.0
277.00	1919.0
278.00	413.0
285.00	300.0
293.10	357.0
296.00	5965.0
297.00	857.0
303.00	668.0
314.00	325.0
314.90	576.0
316.00	381.0
323.00	2084.0
324.00	339.0
327.00	308.0
334.00	1216.0
334.90	427.0
345.90	482.0
352.00	567.0
353.00	321.0
354.10	592.0
365.00	2592.0
366.00	330.0
372.10	915.0
402.00	316.0
403.00	665.0
421.00	482.0
422.00	502.0
423.10	3572.0
424.10	762.0
441.10	9938.0
442.10	67816.0
443.10	12962.0
444.00	1029.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

m/z	Abundance
39.00	895.0
44.00	785.0
50.10	3569.0
51.10	12913.0
52.00	602.0
56.00	388.0
56.90	1043.0
63.00	549.0
68.00	354.0
69.00	15631.0
74.00	1941.0
75.00	2563.0
76.00	965.0
77.10	17352.0
78.00	1132.0
78.90	1391.0
80.00	1074.0
81.00	1418.0
82.00	338.0
83.00	343.0
84.90	318.0
86.00	431.0
90.90	431.0
91.90	431.0
93.00	2732.0
98.00	1974.0
99.00	1535.0
101.00	882.0
103.00	355.0
103.90	500.0
104.90	508.0
107.00	5590.0
107.90	765.0
110.00	10827.0
111.00	1693.0
116.10	433.0
117.00	5300.0
118.00	497.0
121.90	466.0
122.90	653.0
127.00	21192.0
128.00	1594.0
129.00	8685.0
130.00	759.0
135.00	711.0
137.10	380.0
141.00	1392.0
142.10	356.0
146.00	303.0
147.00	650.0
147.90	1375.0
148.90	368.0
153.00	327.0
154.00	302.0
154.90	690.0
155.90	1073.0
159.90	426.0
160.90	668.0
164.90	506.0
166.00	450.0
167.00	3023.0
168.00	1095.0
171.90	301.0
172.90	304.0
174.00	691.0
175.00	1171.0
177.00	624.0
179.00	2320.0
179.90	1398.0
181.10	661.0
185.00	1073.0
186.00	7681.0
187.00	2552.0
189.00	594.0
190.90	344.0
192.00	903.0
192.90	727.0
196.00	1776.0
197.90	57152.0
199.00	3346.0
199.90	320.0
203.00	405.0
204.00	2313.0
205.00	3426.0
206.00	15557.0
207.00	2617.0
208.00	597.0
211.00	619.0
217.00	4629.0
218.00	463.0
221.00	2720.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

221.70	580.0
223.00	728.0
224.00	9096.0
225.00	2187.0
227.00	3910.0
227.90	441.0
229.00	775.0
233.90	310.0
242.00	508.0
243.00	466.0
244.00	6471.0
245.00	1004.0
246.00	1434.0
248.90	316.0
254.20	344.0
255.00	37184.0
256.00	5756.0
257.00	397.0
258.00	2736.0
258.90	424.0
264.90	829.0
273.10	899.0
274.00	2814.0
275.00	17752.0
276.00	2436.0
277.00	1485.0
292.90	436.0
296.00	5167.0
297.10	741.0
303.00	509.0
315.00	570.0
323.00	1649.0
324.00	366.0
326.90	330.0
334.00	1048.0
345.90	428.0
352.00	447.0
353.00	365.0
354.00	621.0
365.00	2320.0
365.90	353.0
372.10	920.0
401.90	369.0
403.00	384.0
421.00	478.0
421.90	353.0
423.00	3241.0
424.10	680.0
441.00	9655.0
442.10	65400.0
443.00	11969.0
444.00	1075.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87

m/z	Abundance
44.00	743.0
206.90	398.0

Instrument :
BNA_M
ClientSampleId :
DFTPP87