

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080216\
 Data File : BM006841.D
 Acq On : 02 Aug 2016 20:17
 Operator : UM/SJ
 Sample : H4095-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJF8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.845	718	724	736	rBV	162409	336348	19.50%	2.572%
2	6.951	736	742	756	rVB	128561	214885	12.46%	1.644%
3	7.151	771	776	789	rBV	196178	344050	19.95%	2.631%
4	7.586	844	850	860	rBV	160949	280959	16.29%	2.149%
5	8.363	977	982	999	rBV	188817	386246	22.40%	2.954%
6	8.763	1044	1050	1070	rVB	185508	333082	19.31%	2.548%
7	9.480	1166	1172	1186	rBV	158645	304378	17.65%	2.328%
8	10.039	1262	1267	1284	rBV	171889	388625	22.53%	2.972%
9	10.369	1317	1323	1337	rBV	209730	372710	21.61%	2.851%
10	10.551	1348	1354	1372	rBV	127343	328783	19.06%	2.515%
11	13.686	1881	1887	1891	rBV	429058	600927	34.85%	4.596%
12	13.733	1891	1895	1907	rVB	240556	399975	23.19%	3.059%
13	13.939	1924	1930	1945	rBV	436166	697281	40.43%	5.333%
14	14.204	1970	1975	1977	rBV2	17087	25382	1.47%	0.194%
15	14.251	1977	1983	1995	rVB2	320223	537644	31.18%	4.112%
16	14.580	2034	2039	2059	rBV2	99378	290617	16.85%	2.223%
17	15.251	2147	2153	2162	rBV	580230	906306	52.55%	6.932%
18	15.409	2175	2180	2190	rBV	184342	305543	17.72%	2.337%
19	15.956	2267	2273	2280	rBV3	12429	24849	1.44%	0.190%
20	16.021	2280	2284	2295	rVB	21478	47854	2.77%	0.366%
21	17.003	2445	2451	2459	rBV2	462193	679100	39.38%	5.194%
22	17.103	2462	2468	2481	rVB	641863	1003969	58.22%	7.679%
23	17.921	2602	2607	2613	rBV7	24433	45098	2.62%	0.345%
24	19.409	2855	2860	2870	rBV	847873	1300207	75.39%	9.944%
25	21.215	3162	3167	3174	rBV	766151	1195441	69.32%	9.143%
26	23.274	3513	3517	3526	rVB	949981	1724554	100.00%	13.190%


Sum of corrected areas: 13074813

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080216\
Data File : BM006841.D
Acq On : 02 Aug 2016 20:17
Operator : UM/SJ
Sample : H4095-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF8

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

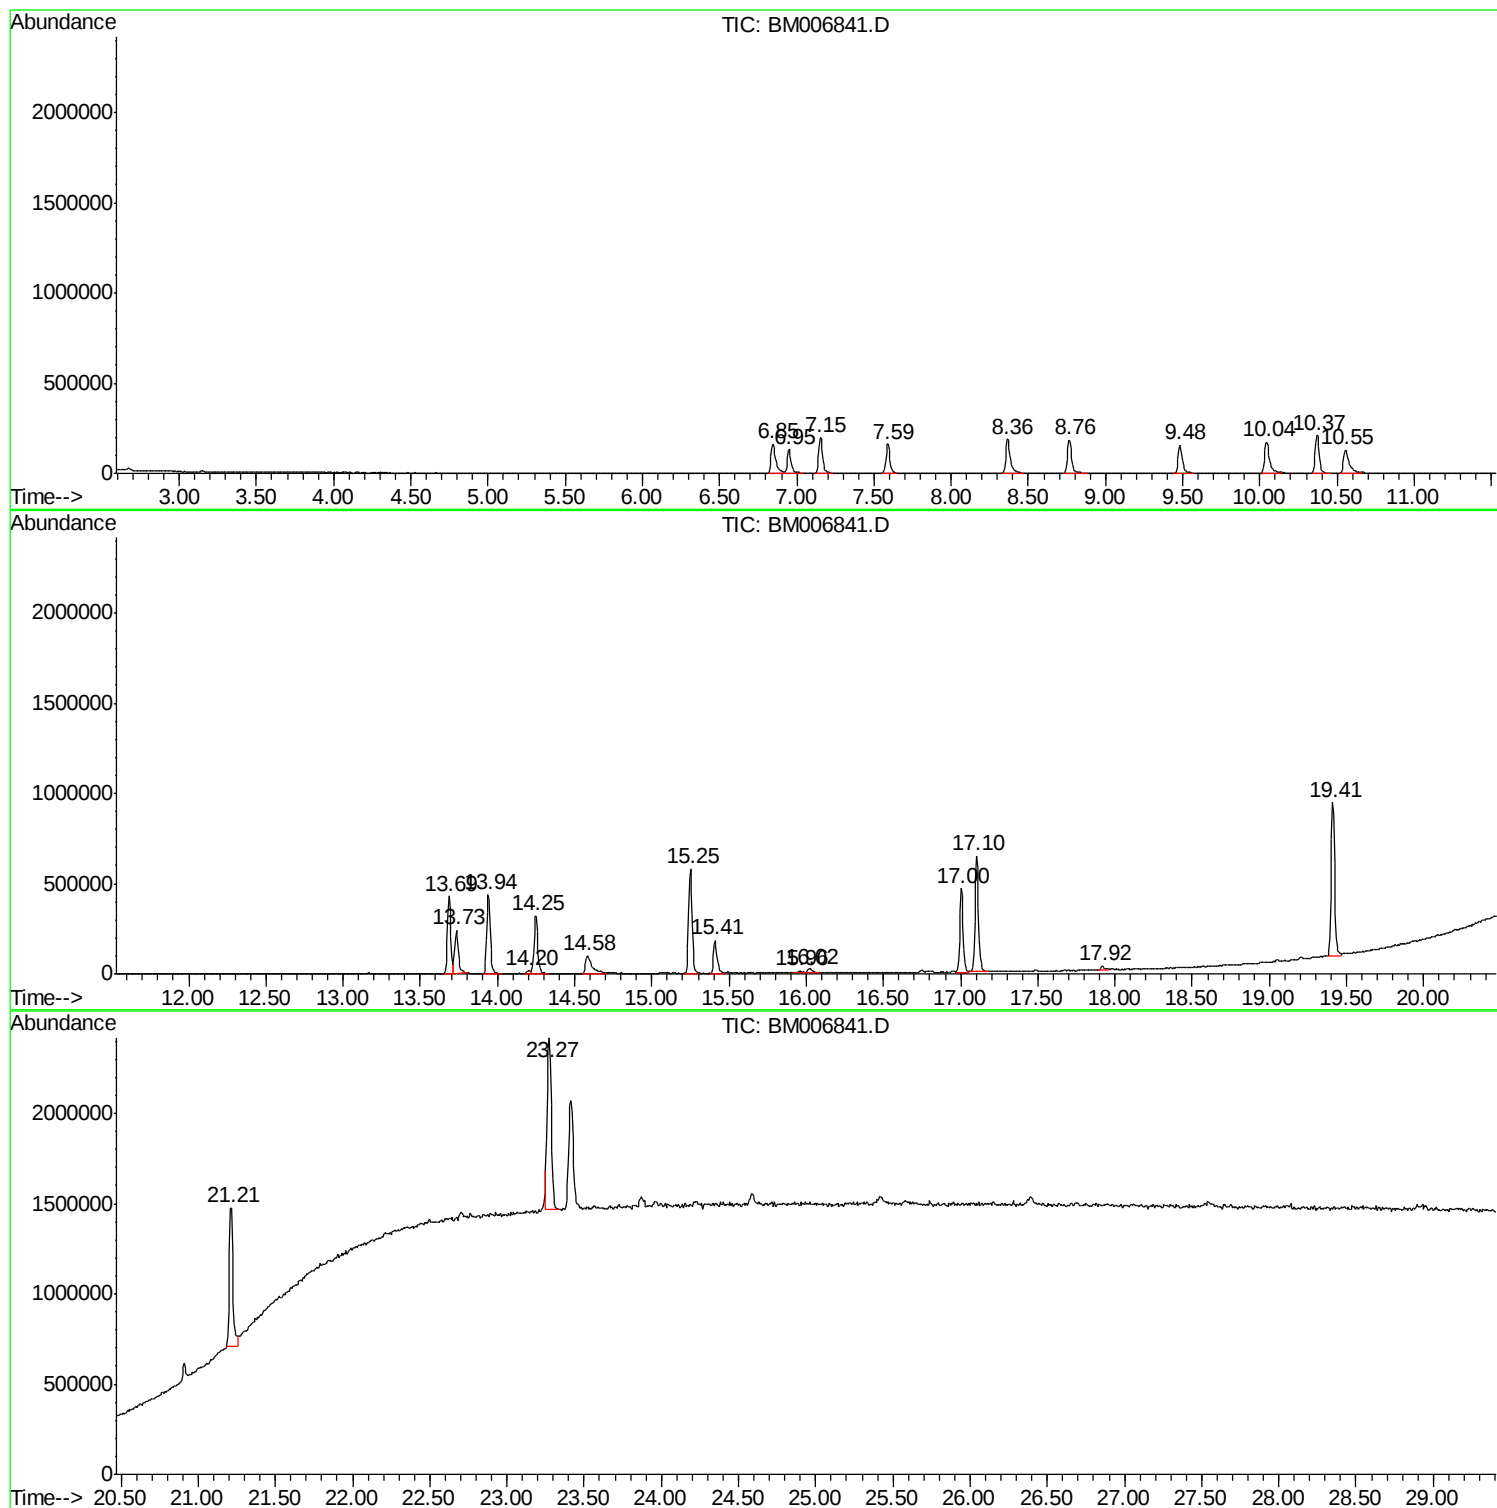

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080216\
Data File : BM006841.D
Acq On : 02 Aug 2016 20:17
Operator : UM/SJ
Sample : H4095-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080216\
Data File : BM006841.D
Acq On : 02 Aug 2016 20:17
Operator : UM/SJ
Sample : H4095-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJF8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc