

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080216\
 Data File : BM006843.D
 Acq On : 02 Aug 2016 21:30
 Operator : UM/SJ
 Sample : H4095-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.839	718	723	737	rBV2	85280	191393	15.41%	2.024%
2	6.945	737	741	752	rVB	74224	123991	9.99%	1.311%
3	7.151	770	776	788	rBV	119438	196185	15.80%	2.075%
4	7.586	844	850	861	rBV	206120	337794	27.20%	3.572%
5	8.363	977	982	996	rBV2	103811	218718	17.61%	2.313%
6	8.763	1043	1050	1063	rBV	103056	194334	15.65%	2.055%
7	9.480	1166	1172	1185	rBV2	85153	168377	13.56%	1.781%
8	10.045	1262	1268	1285	rBV	93450	219933	17.71%	2.326%
9	10.369	1316	1323	1339	rBV	254446	443092	35.68%	4.686%
10	10.557	1349	1355	1375	rBV2	75110	192360	15.49%	2.034%
11	13.680	1881	1886	1891	rBV	240863	372376	29.99%	3.938%
12	13.733	1891	1895	1906	rVB	127821	220237	17.74%	2.329%
13	13.939	1924	1930	1946	rBV	249239	402063	32.38%	4.252%
14	14.245	1976	1982	1993	rVB2	383216	598670	48.21%	6.331%
15	14.592	2035	2041	2057	rBV2	39120	135792	10.94%	1.436%
16	15.245	2147	2152	2161	rBV	336912	544192	43.83%	5.755%
17	15.410	2175	2180	2190	rBV	76149	129263	10.41%	1.367%
18	15.980	2269	2277	2280	rBV5	10879	27483	2.21%	0.291%
19	17.004	2445	2451	2462	rBV	528972	783802	63.12%	8.289%
20	17.104	2462	2468	2484	rVB	390368	628545	50.62%	6.647%
21	17.909	2601	2605	2613	rBV7	14788	32975	2.66%	0.349%
22	19.409	2855	2860	2869	rBV2	541162	827385	66.63%	8.749%
23	21.209	3162	3166	3175	rBV	846313	1241704	100.00%	13.131%
24	23.415	3537	3541	3550	rVB	670029	1225721	98.71%	12.962%


Sum of corrected areas: 9456385

Data Path : Z:\HPCHEM1\BNA M\DATA\BM080216\
Data File : BM006843.D
Acq On : 02 Aug 2016 21:30
Operator : UM/SJ
Sample : H4095-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJG0

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

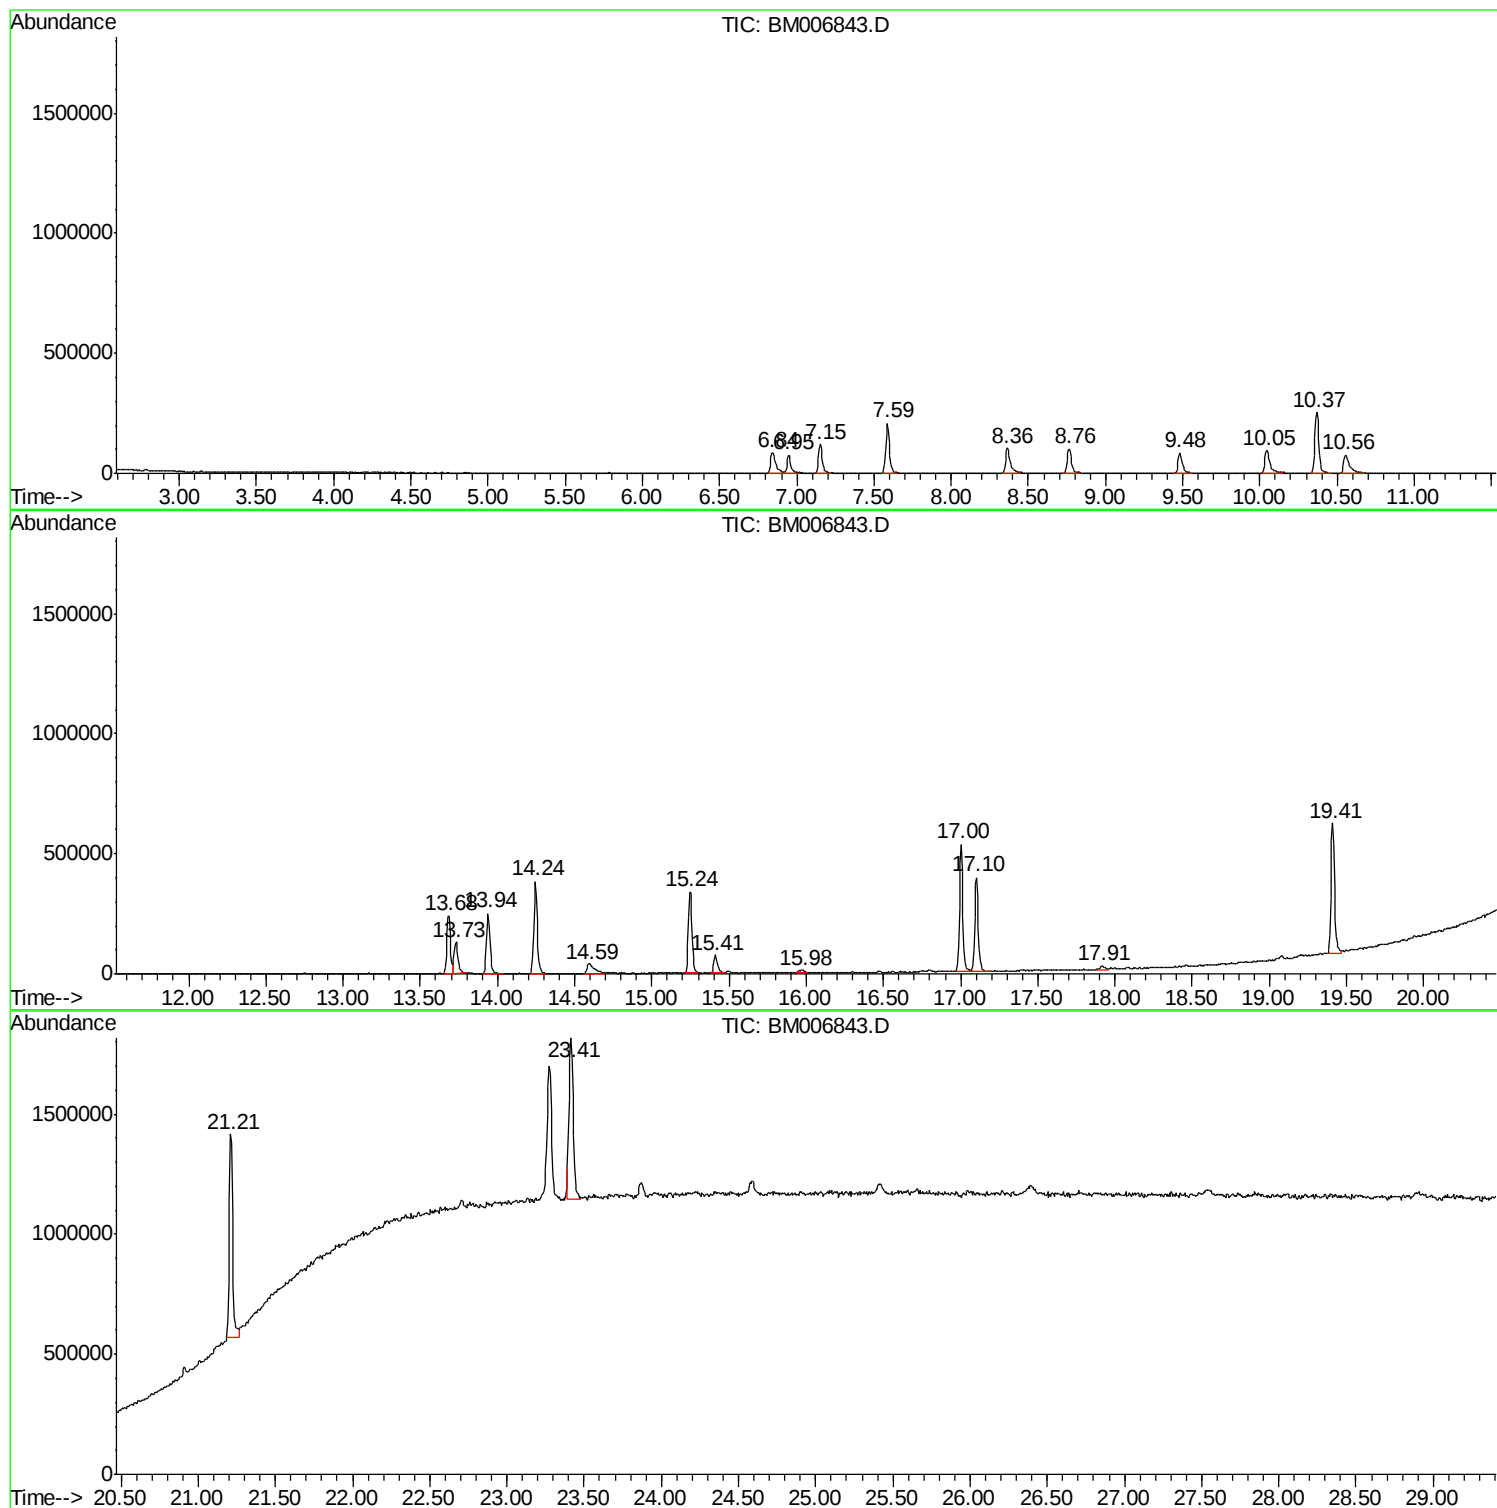

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080216\
Data File : BM006843.D
Acq On : 02 Aug 2016 21:30
Operator : UM/SJ
Sample : H4095-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJG0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080216\
Data File : BM006843.D
Acq On : 02 Aug 2016 21:30
Operator : UM/SJ
Sample : H4095-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJG0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc