


Data Path : Z:\HPCHEM1\BNA M\DATA\BM080217\
 Data File : BM011090.D
 Acq On : 02 Aug 2017 10:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

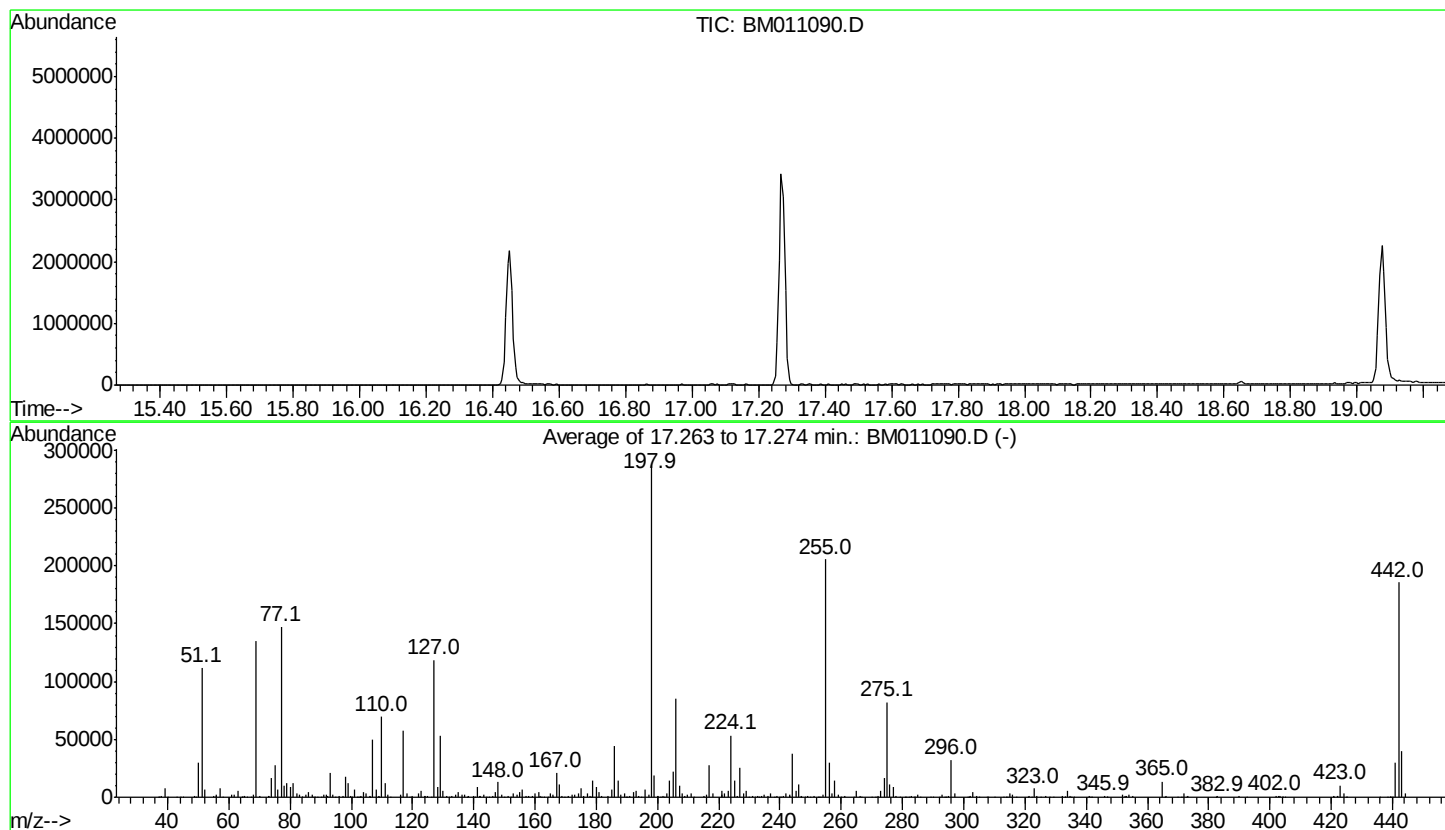

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	112013	PASS
68	69	0.00	2	1.6	2214	PASS
69	198	0.00	100	47.1	135074	PASS
70	69	0.00	2	0.5	701	PASS
127	198	10	80	41.4	118717	PASS
197	198	0.00	2	0.8	2392	PASS
198	198	100	100	100.0	286677	PASS
199	198	5	9	6.6	18883	PASS
275	198	10	60	28.6	82008	PASS
365	198	1	100	4.6	13315	PASS
441	443	0.01	100	75.5	29762	PASS
442	198	50	100	64.8	185794	PASS
443	442	15	24	21.2	39408	PASS