


Data Path : Z:\HPCHEM1\BNA M\DATA\BM080217\
 Data File : BM011093.D
 Acq On : 02 Aug 2017 13:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

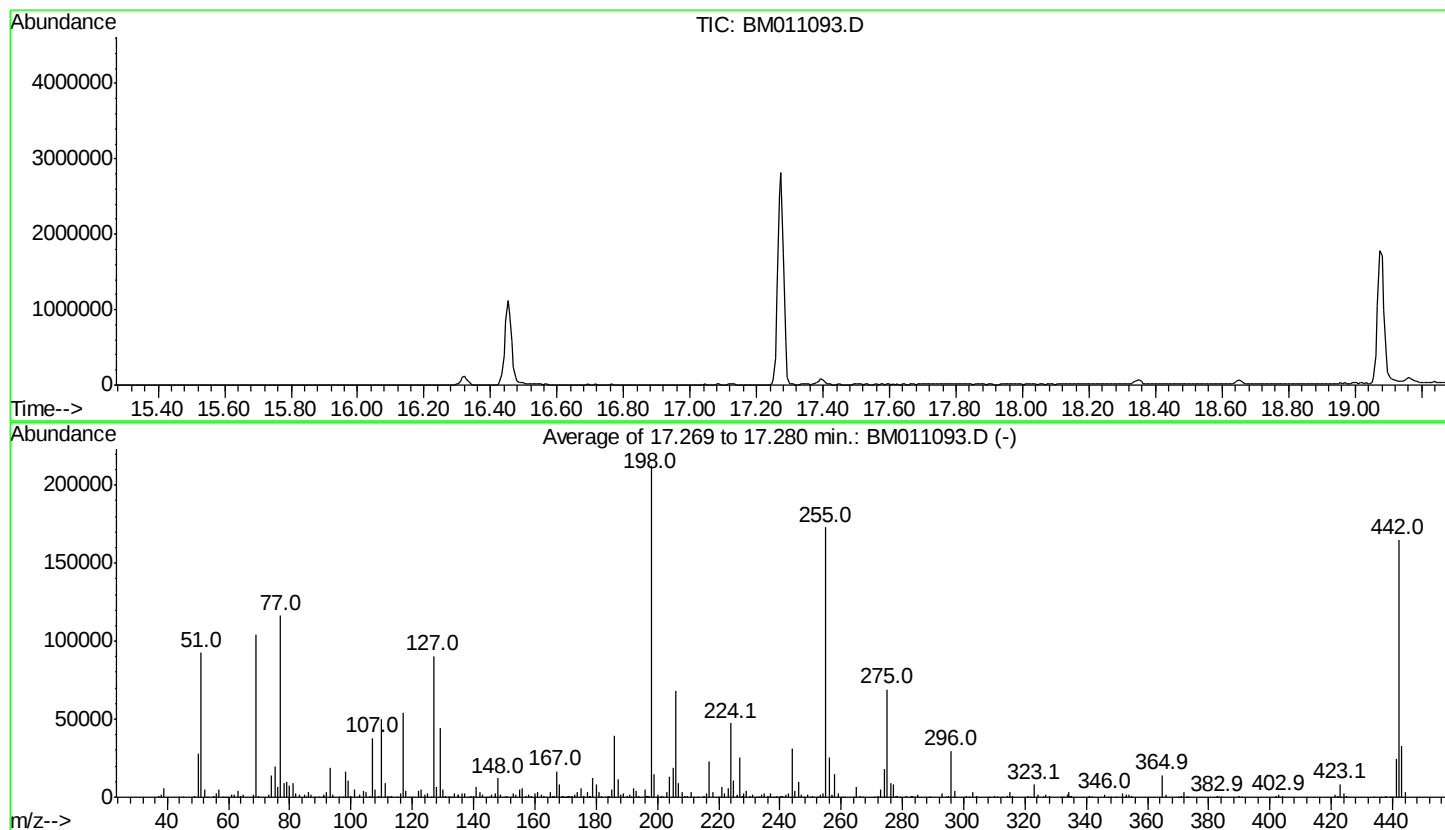

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	92629	PASS
68	69	0.00	2	1.7	1827	PASS
69	198	0.00	100	49.2	104469	PASS
70	69	0.00	2	0.5	523	PASS
127	198	10	80	42.5	90274	PASS
197	198	0.00	2	0.3	711	PASS
198	198	100	100	100.0	212437	PASS
199	198	5	9	7.0	14913	PASS
275	198	10	60	32.5	69125	PASS
365	198	1	100	6.7	14156	PASS
441	443	0.01	100	74.1	24274	PASS
442	198	50	100	77.7	165120	PASS
443	442	15	24	19.8	32776	PASS