


Data Path : Z:\HPCHEM1\BNA M\DATA\BM080217\
 Data File : BM011106.D
 Acq On : 03 Aug 2017 02:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

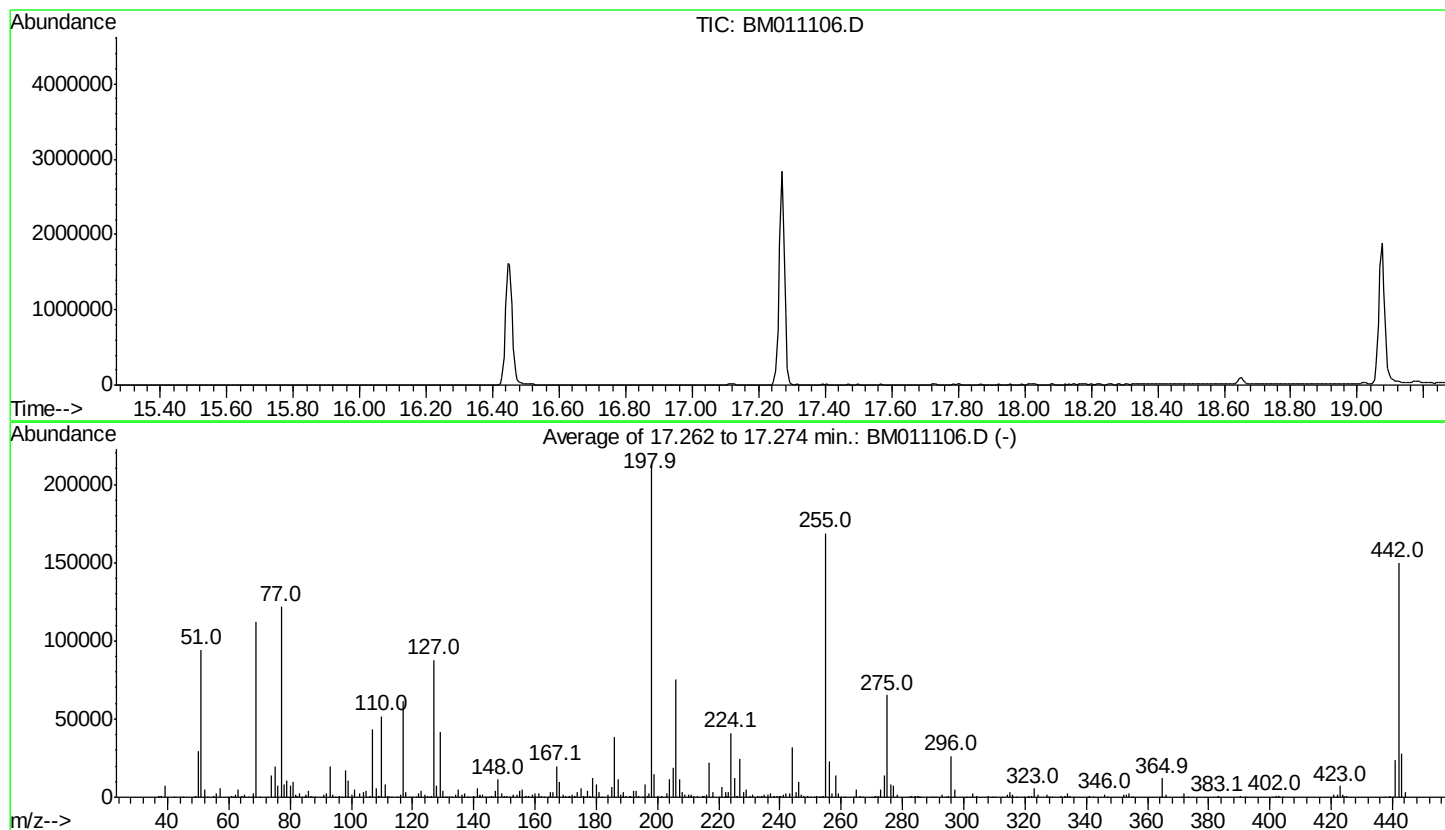

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	94296	PASS
68	69	0.00	2	1.9	2178	PASS
69	198	0.00	100	53.1	112512	PASS
70	69	0.00	2	0.2	206	PASS
127	198	10	80	41.5	87890	PASS
197	198	0.00	2	1.1	2371	PASS
198	198	100	100	100.0	211925	PASS
199	198	5	9	6.9	14518	PASS
275	198	10	60	30.7	65154	PASS
365	198	1	100	5.6	11959	PASS
441	443	0.01	100	83.5	23356	PASS
442	198	50	100	70.7	149925	PASS
443	442	15	24	18.7	27976	PASS