
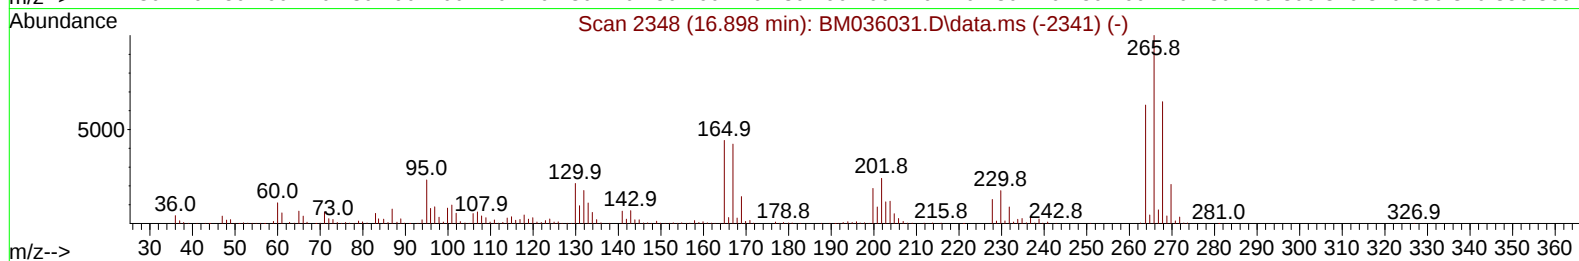
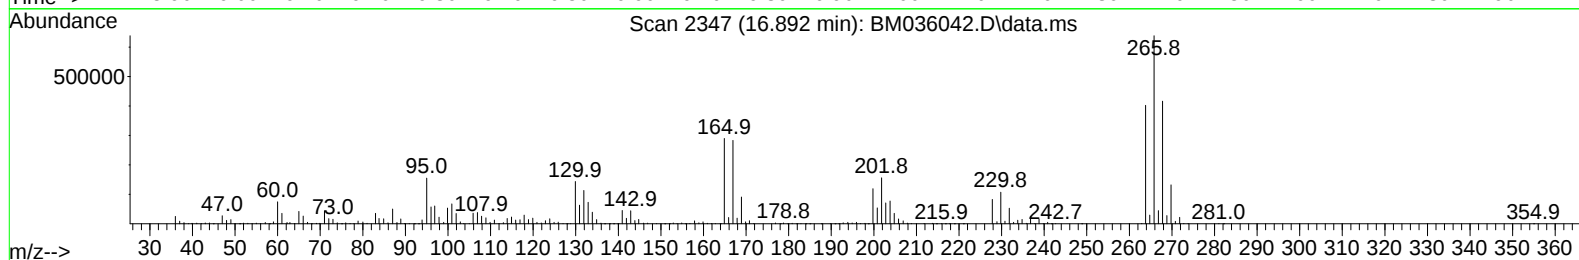


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080222\
Data File : BM036042.D
Acq On : 02 Aug 2022 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 06:07:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 17:50:14 2022
Response via : Initial Calibration

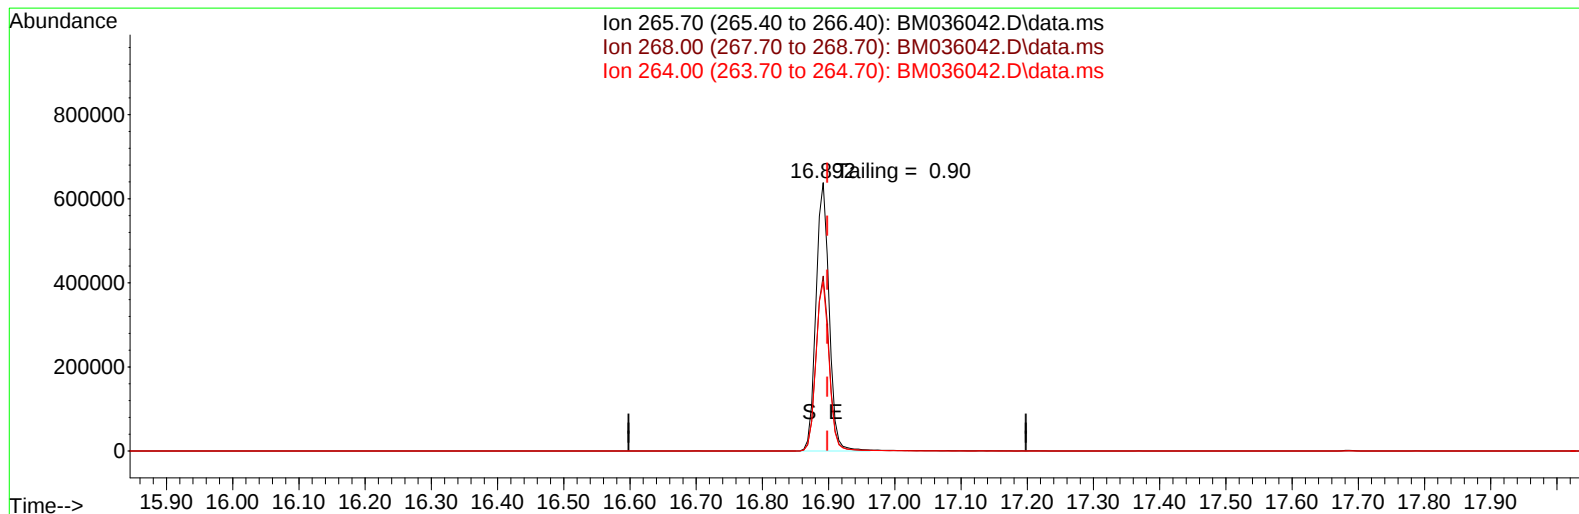

TIC: BM036042.D\data.ms

(70) Pentachlorophenol (C)




16.892min (-0.006) 915019.58 ng

response 885656

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	65.18
264.00	63.30	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080222\
 Data File : BM036042.D
 Acq On : 02 Aug 2022 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 06:07:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 17:50:14 2022
 Response via : Initial Calibration

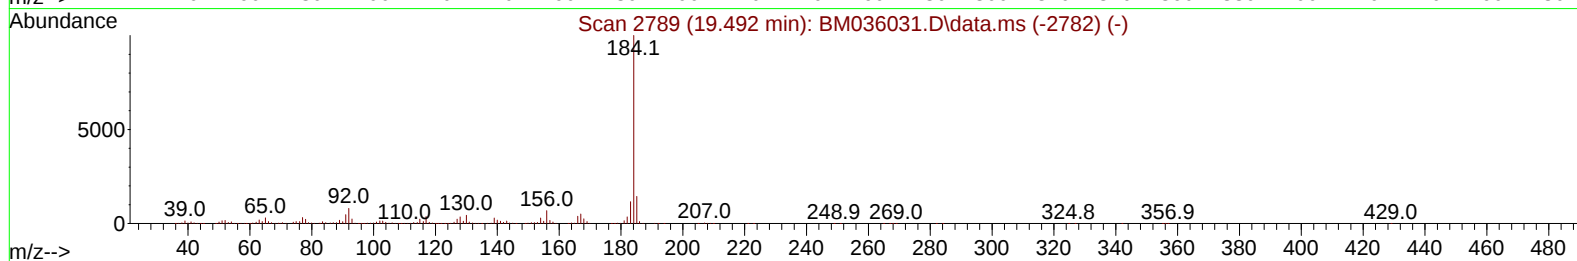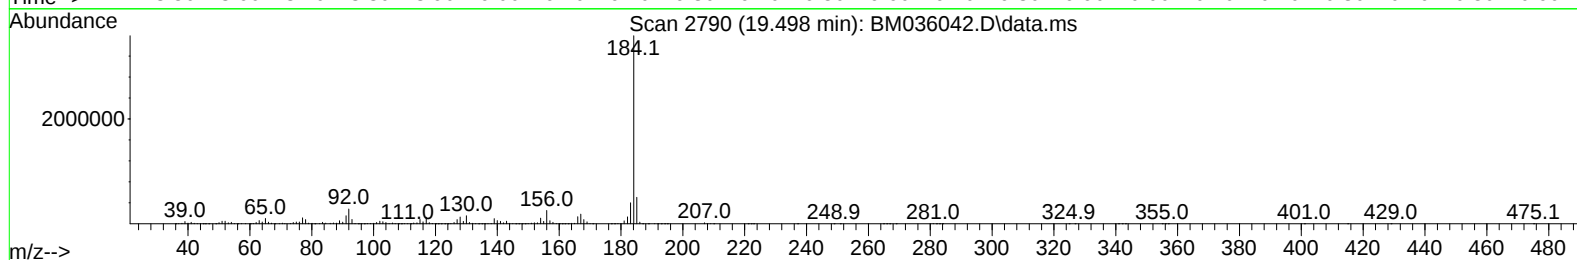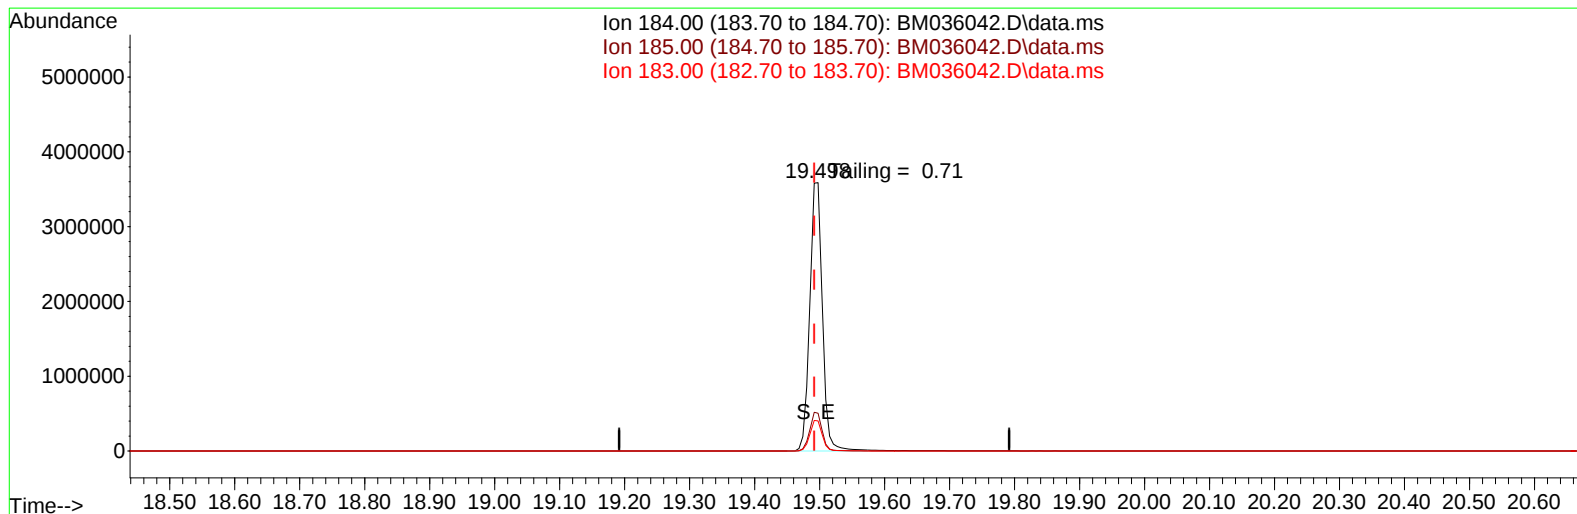

TIC: BM036042.D\data.ms

(77) Benzidine**19.498min (+ 0.006) 57117.96 ng****response 4891191**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.06
183.00	11.90	11.20
0.00	0.00	0.00