
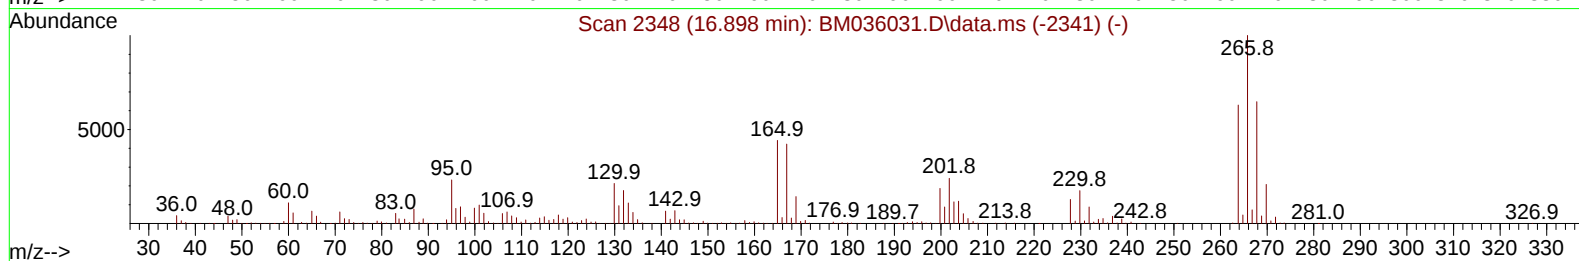
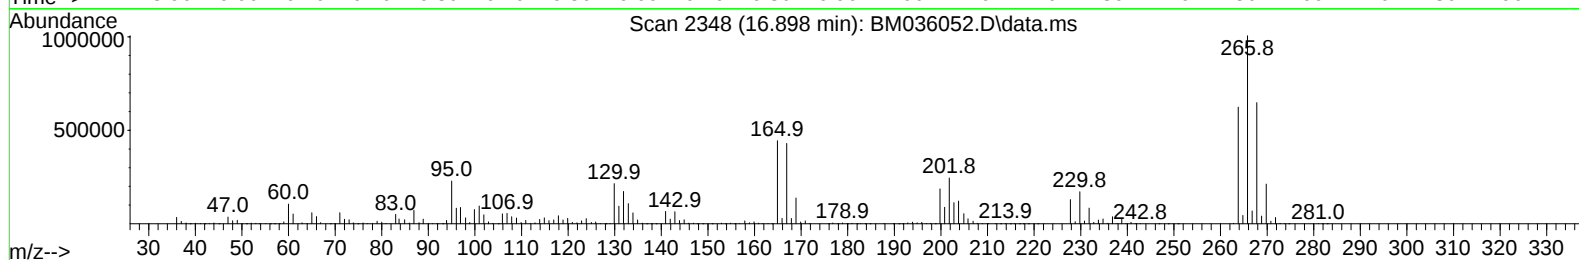


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080222\
Data File : BM036052.D
Acq On : 02 Aug 2022 15:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 06:08:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 17:50:14 2022
Response via : Initial Calibration

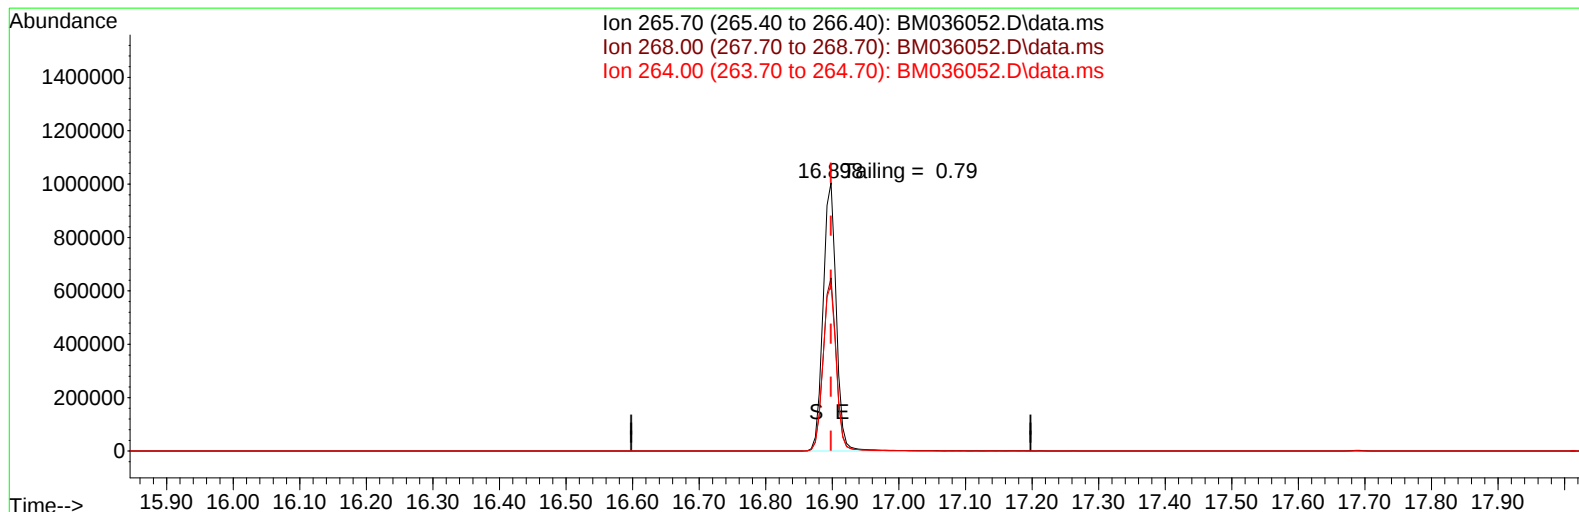

TIC: BM036052.D\data.ms

(70) Pentachlorophenol (C)




16.898min (+ 0.000) 312430.48 ng

response 1379720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.48
264.00	63.30	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080222\
Data File : BM036052.D
Acq On : 02 Aug 2022 15:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 06:08:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 17:50:14 2022
Response via : Initial Calibration

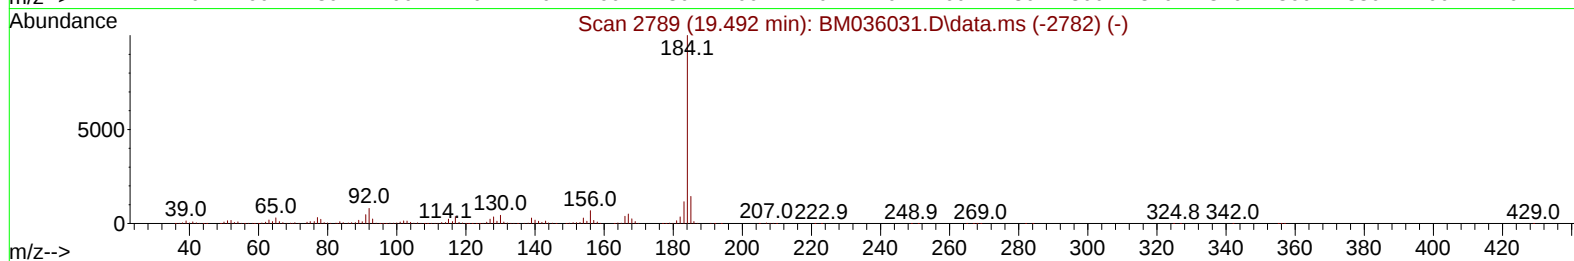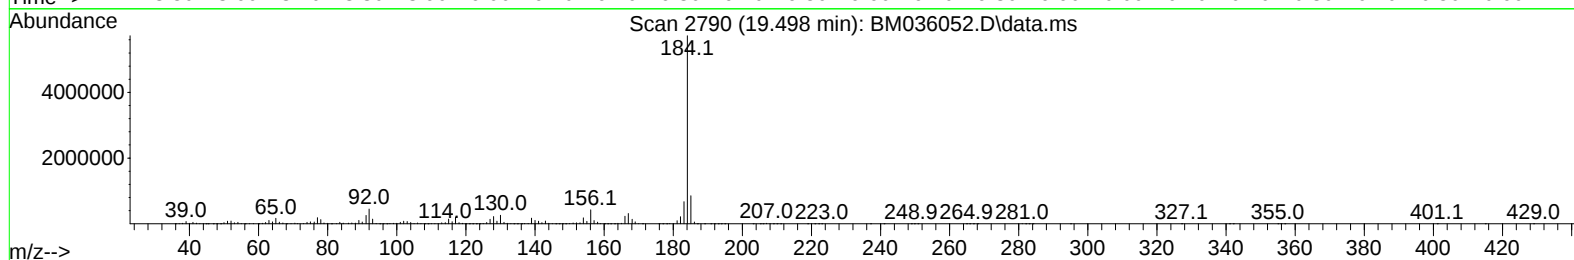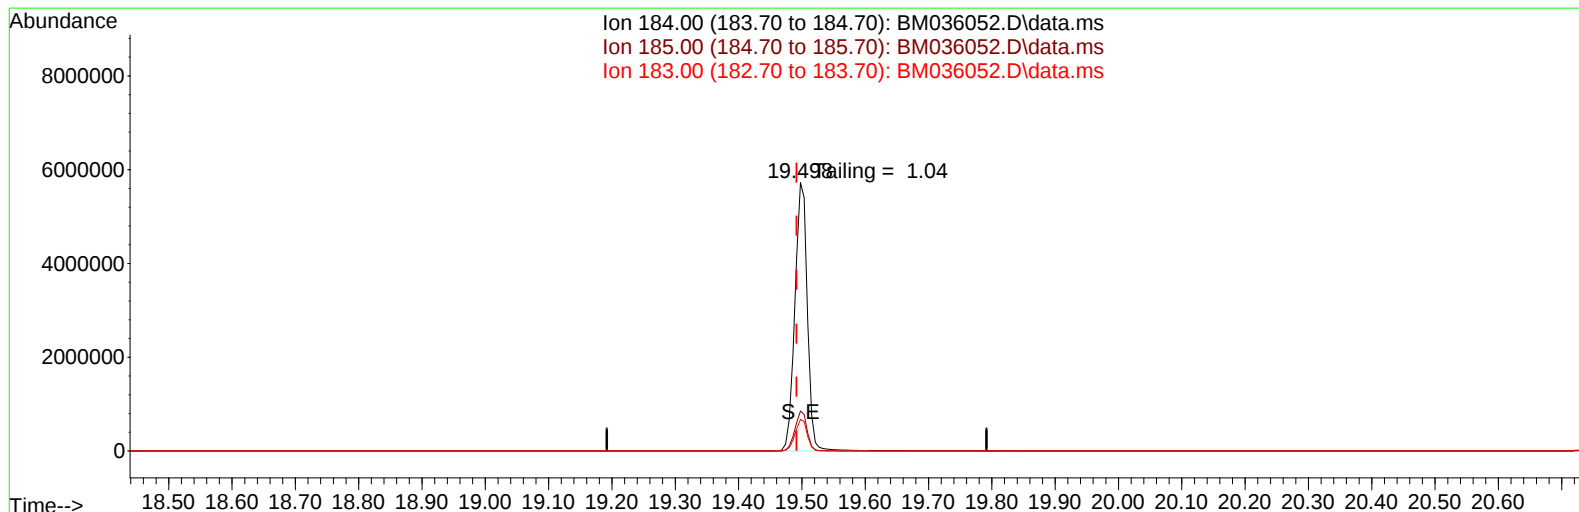

TIC: BM036052.D\data.ms

(77) Benzidine**19.498min (+ 0.006) 489339.50 ng****response 7889047**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.91
183.00	11.90	11.76
0.00	0.00	0.00