
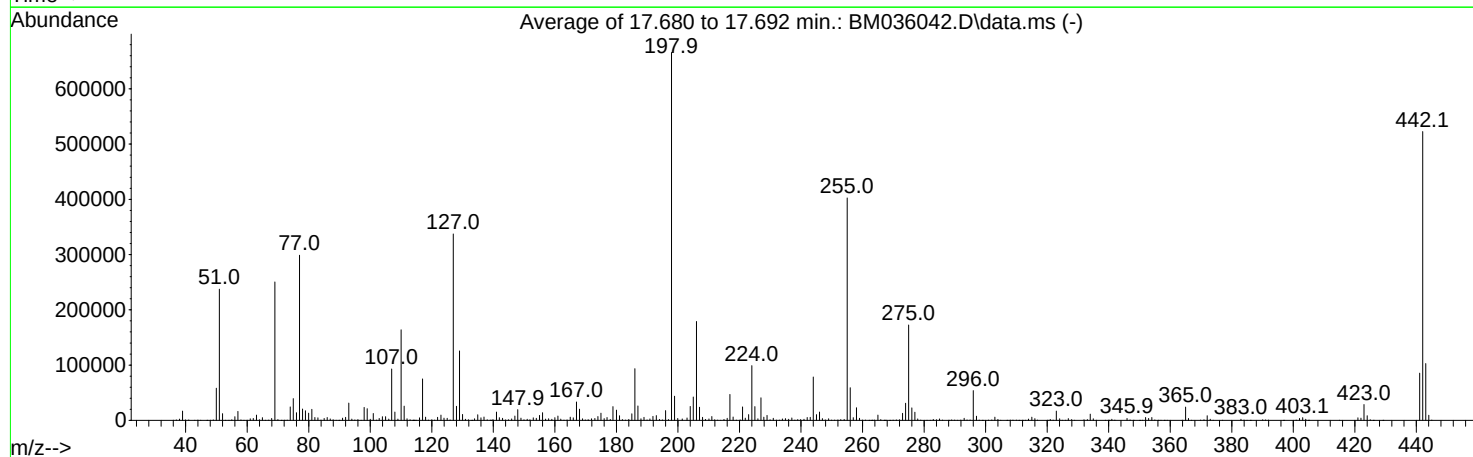


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080222\
 Data File : BM036042.D
 Acq On : 02 Aug 2022 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 17:50:14 2022

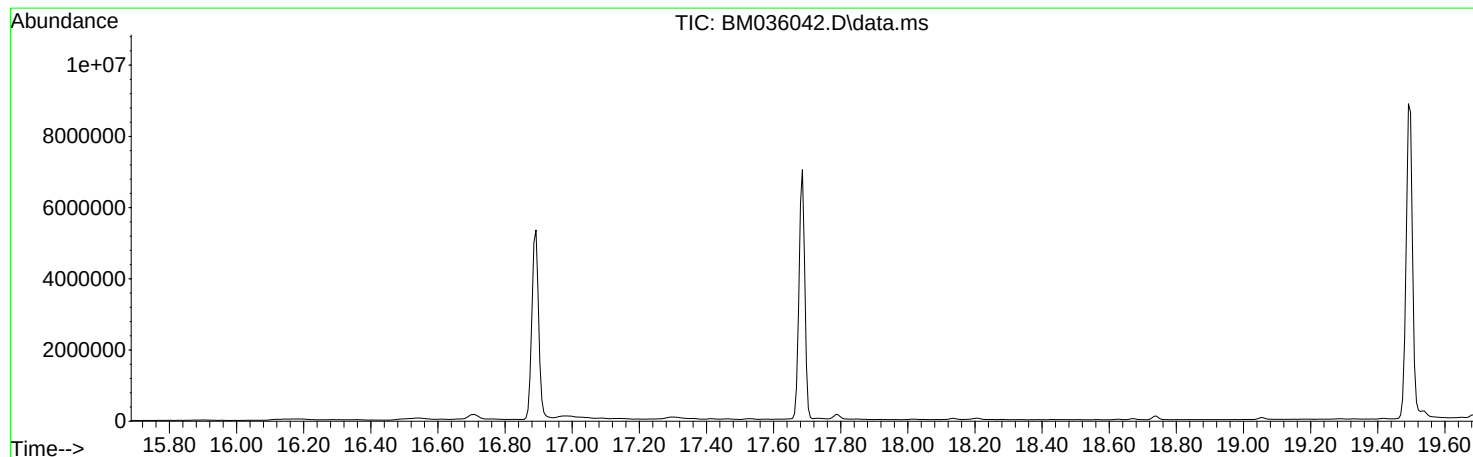




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	237340	PASS
68	69	0.00	2	1.4	3450	PASS
69	198	0.00	100	37.6	250428	PASS
70	69	0.00	2	0.6	1386	PASS
127	198	10	80	50.7	337494	PASS
197	198	0.00	2	0.2	1526	PASS
198	198	100	100	100.0	665728	PASS
199	198	5	9	6.6	43856	PASS
275	198	10	60	25.9	172672	PASS
365	198	1	100	3.6	24077	PASS
441	198	0.01	100	12.8	85531	PASS
442	442	50	100	100.0	522731	PASS
443	442	15	24	19.6	102688	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080222\
 Data File : BM036042.D
 Acq On : 02 Aug 2022 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 03 06:07:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 17:50:14 2022
 Response via : Initial Calibration

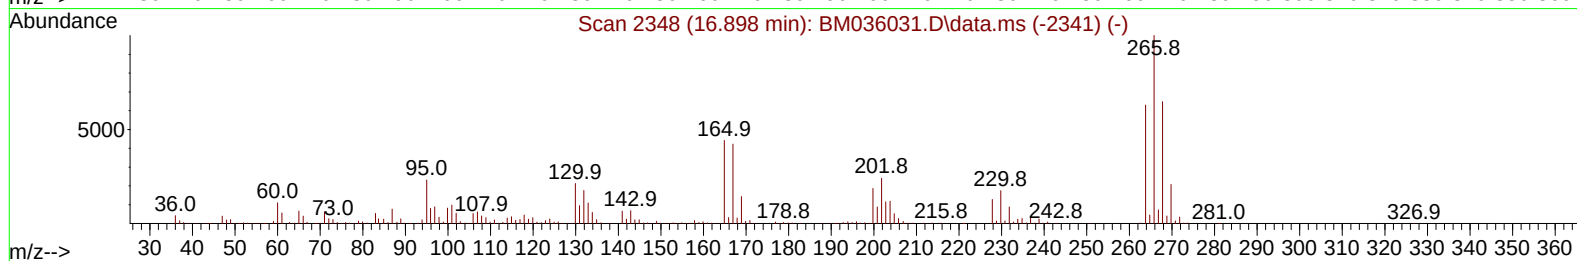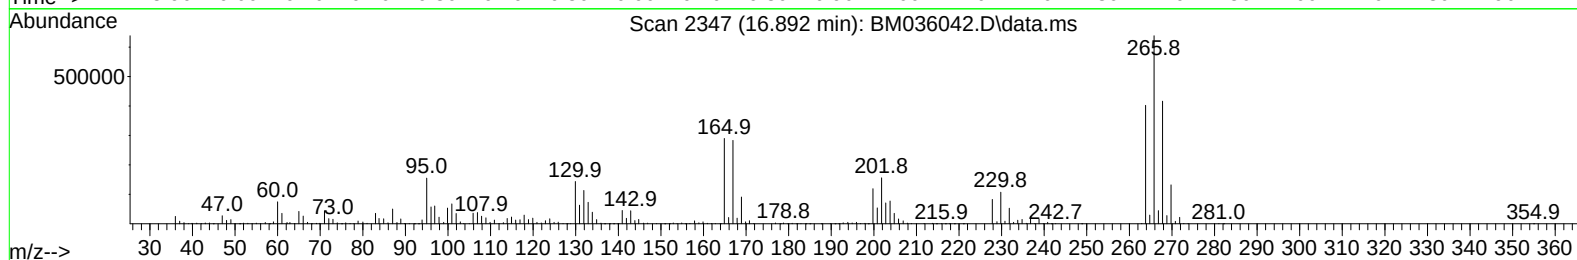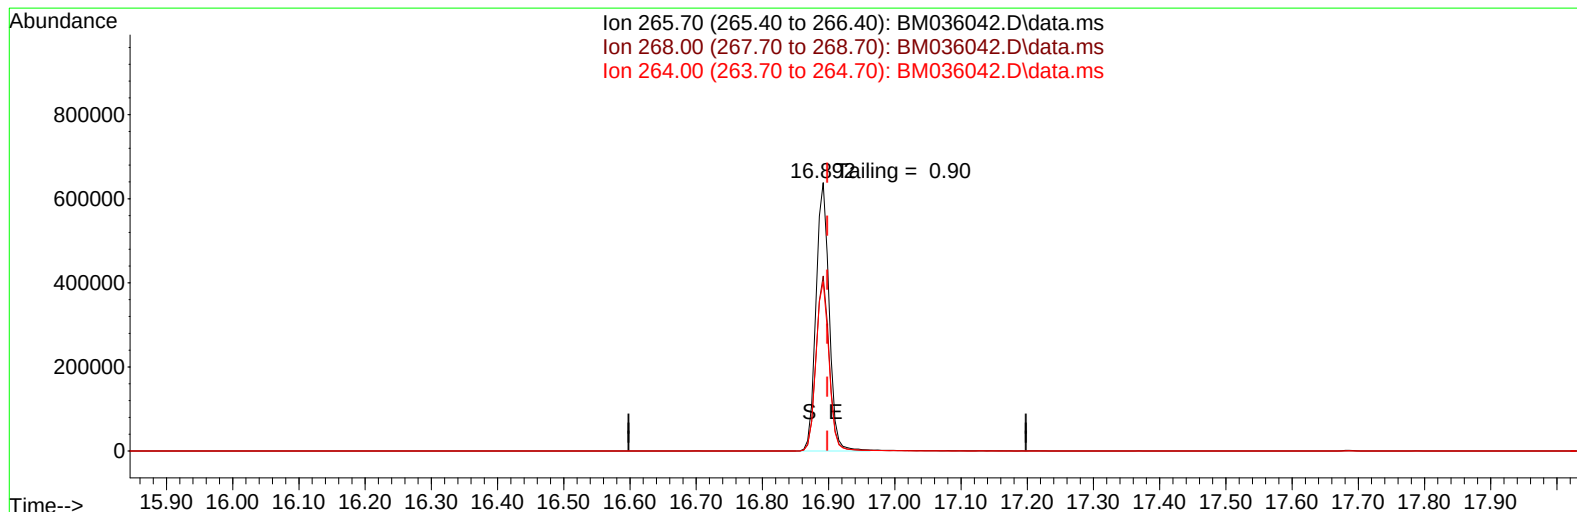

TIC: BM036042.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.006) 915019.58 ng




response 885656

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	65.18
264.00	63.30	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080222\
Data File : BM036042.D
Acq On : 02 Aug 2022 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 03 06:07:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 17:50:14 2022
Response via : Initial Calibration

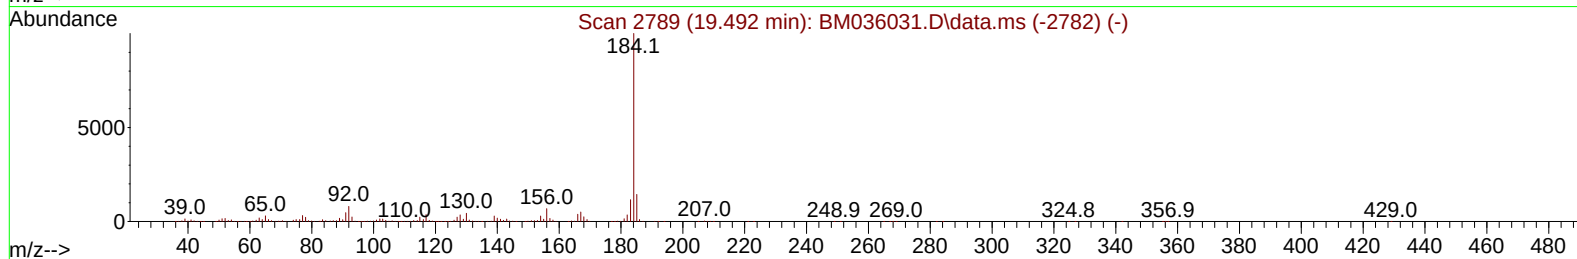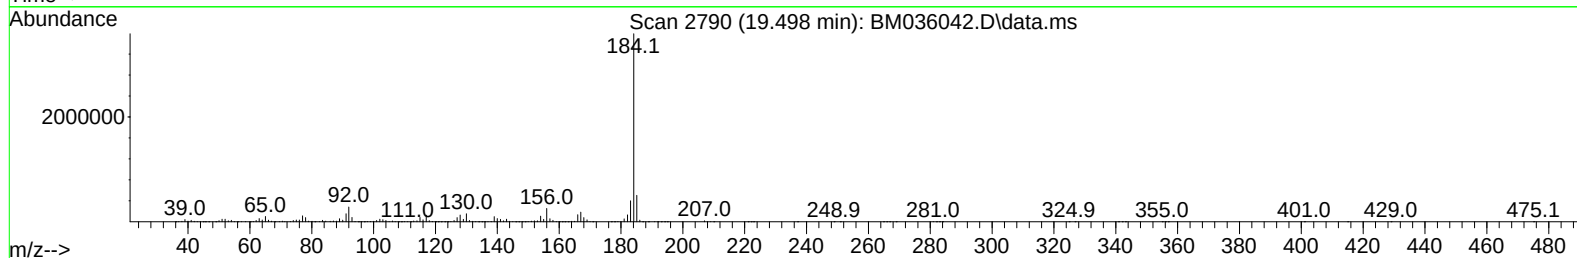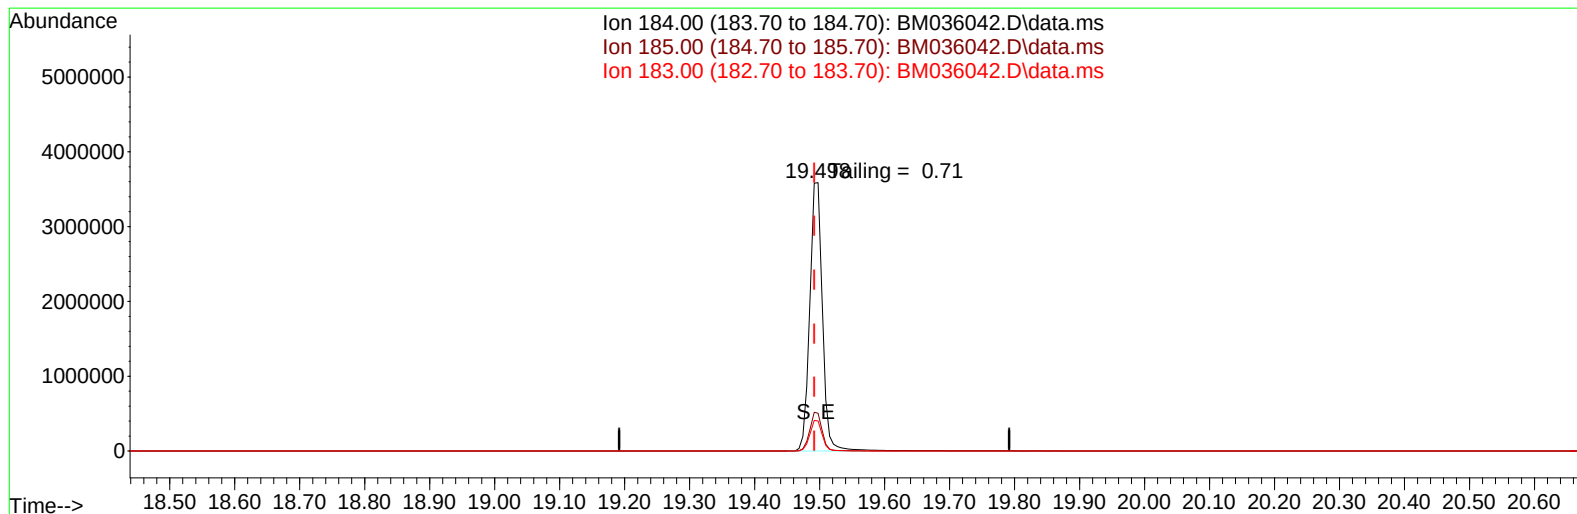

TIC: BM036042.D\data.ms

(77) Benzidine

19.498min (+ 0.006) 57117.96 ng

response 4891191

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.06
183.00	11.90	11.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2022	BNA_M	<u>BM036042.D</u>
Compound Name	Response	Retention Time
DDT	2307332	20.727
DDD	17264	20.286
DDE	1948	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19212	2326544	0.83

Instrument :
BNA_M
ClientSampleId :
DFTPP