
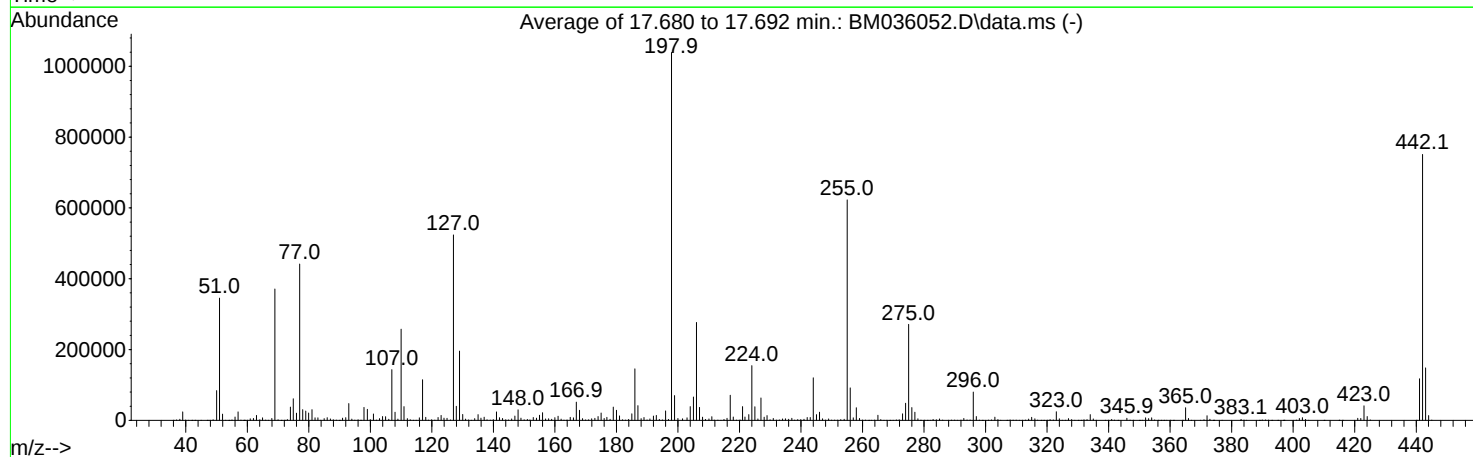


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080222\
 Data File : BM036052.D
 Acq On : 02 Aug 2022 15:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 17:50:14 2022

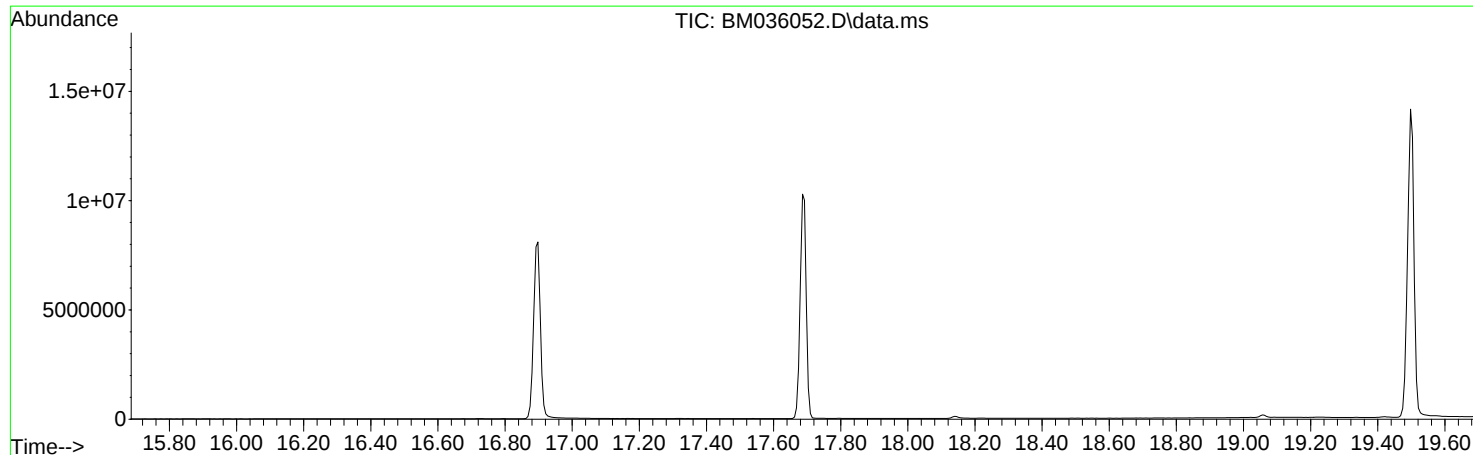




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	345174	PASS
68	69	0.00	2	1.4	5251	PASS
69	198	0.00	100	35.7	370899	PASS
70	69	0.00	2	0.5	1888	PASS
127	198	10	80	50.4	523712	PASS
197	198	0.00	2	0.3	2963	PASS
198	198	100	100	100.0	1039061	PASS
199	198	5	9	6.8	70299	PASS
275	198	10	60	26.1	271211	PASS
365	198	1	100	3.4	35624	PASS
441	198	0.01	100	11.3	117752	PASS
442	442	50	100	100.0	751211	PASS
443	442	15	24	19.7	148133	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080222\
 Data File : BM036052.D
 Acq On : 02 Aug 2022 15:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 03 06:08:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 17:50:14 2022
 Response via : Initial Calibration

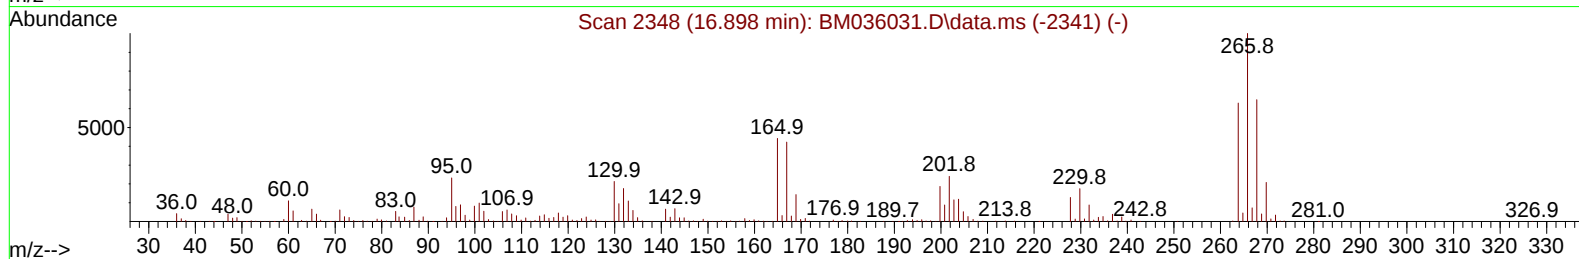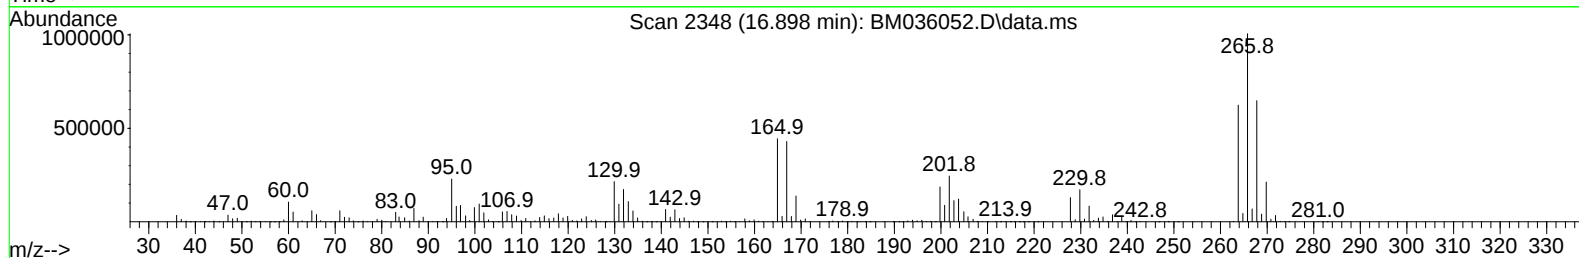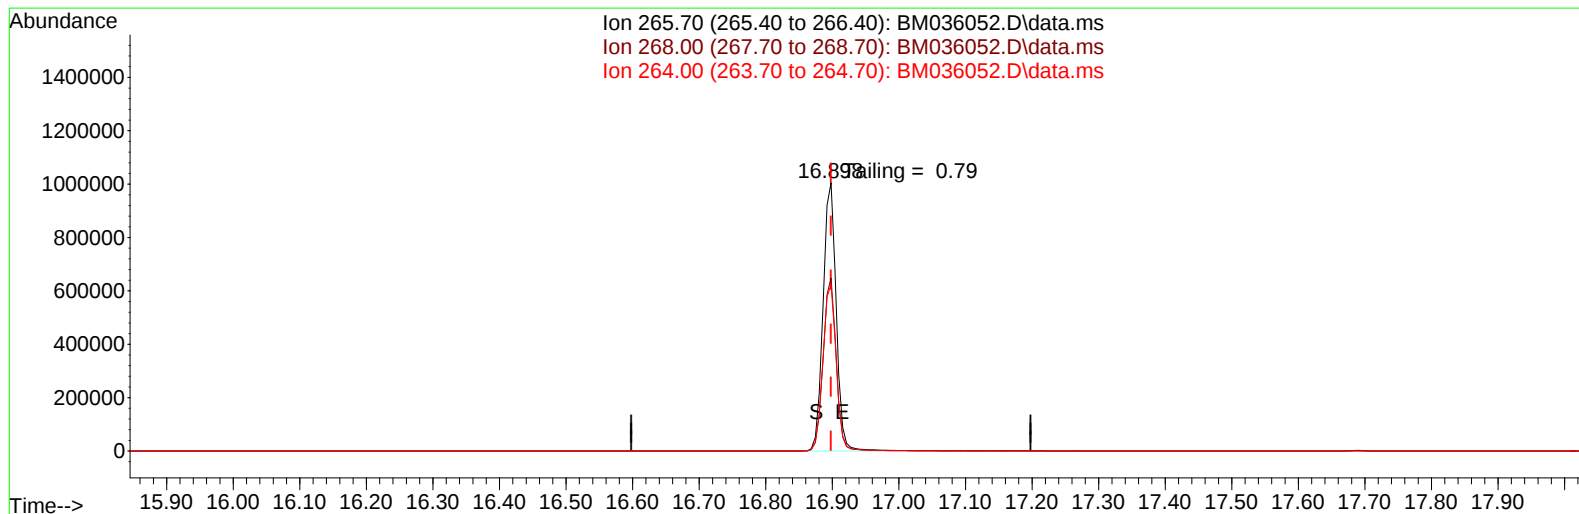

TIC: BM036052.D\data.ms

(70) Pentachlorophenol (C)

16.898min (+ 0.000) 312430.48 ng

response 1379720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.48
264.00	63.30	62.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2022	BNA_M	<u>BM036052.D</u>
Compound Name	Response	Retention Time
DDT	3784917	20.727
DDD	29840	20.286
DDE	2140	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31980	3816897	0.84

Instrument :
BNA_M
ClientSampleId :
DFTPP