

m/z	Abundance
41.00	326.0
43.00	439.0
44.00	402.0
46.90	686.0
49.00	2841.0
51.00	837.0
83.90	2629.0
85.90	1769.0
87.90	315.0

Instrument :
BNA_M
ClientSampleId :
DFTPP88

m/z	Abundance
39.00	1021.0
41.00	340.0
43.00	484.0
44.00	414.0
47.00	663.0
49.00	2654.0
50.00	3215.0
51.00	12325.0
52.00	715.0
55.00	330.0
56.00	488.0
57.00	1046.0
63.00	532.0
65.00	322.0
69.00	13286.0
74.00	1274.0
75.00	1989.0
76.10	806.0
77.00	14347.0
78.00	1037.0
79.00	1205.0
79.90	787.0
81.00	1254.0
83.00	418.0
83.90	2715.0
85.10	425.0
86.00	2022.0
87.90	325.0
91.00	311.0
92.00	384.0
93.00	1842.0
98.00	1398.0
99.00	1199.0
100.90	517.0
104.00	456.0
105.00	500.0
107.00	4630.0
108.10	701.0
110.00	8152.0
111.00	1442.0
117.00	4692.0
117.90	319.0
122.10	339.0
123.00	650.0
127.00	15509.0
128.00	1219.0
129.00	6468.0
129.90	621.0
134.90	674.0
137.10	300.0
140.90	838.0
146.90	569.0
148.00	956.0
152.90	305.0
155.00	450.0
155.90	738.0
159.90	304.0
161.10	401.0
165.00	477.0
166.00	356.0
167.00	1554.0
168.00	932.0
173.90	353.0
175.00	696.0
176.90	318.0
178.90	1372.0
180.00	932.0
181.00	460.0
185.00	663.0
186.00	5193.0
186.90	1562.0
189.00	315.0
192.00	498.0
193.00	589.0
196.00	1023.0
197.90	34776.0
198.90	2907.0
203.00	371.0
204.00	1338.0
205.00	2195.0
206.00	10147.0
207.00	1327.0
208.00	356.0
211.00	379.0
216.90	2687.0
221.00	1530.0
221.70	681.0
222.90	511.0
224.00	4958.0
225.00	1484.0
227.00	2542.0

Instrument :
BNA_M
ClientSampleId :
DFTPP88

227.90	360.0
228.90	485.0
244.00	3618.0
245.00	486.0
246.00	860.0
255.00	20320.0
256.00	3228.0
258.00	1379.0
264.90	486.0
273.00	536.0
274.00	1651.0
275.00	8433.0
276.00	1119.0
276.90	835.0
296.00	2848.0
296.90	352.0
303.00	351.0
314.80	327.0
323.00	717.0
334.00	466.0
352.00	317.0
354.10	315.0
365.00	1107.0
371.90	384.0
423.00	1076.0
441.10	3158.0
442.00	21376.0
443.10	4315.0
443.90	481.0

Instrument :
BNA_M
ClientSampleId :
DFTPP88

m/z	Abundance
39.00	1369.0
41.00	347.0
43.10	415.0
44.00	545.0
47.00	706.0
47.90	318.0
49.00	3069.0
50.00	4568.0
51.10	16664.0
52.00	880.0
55.00	415.0
56.00	529.0
57.00	1282.0
61.00	338.0
62.90	877.0
65.10	378.0
68.10	462.0
69.00	20568.0
73.00	306.0
74.00	2009.0
75.00	3226.0
76.10	1067.0
77.10	20944.0
78.10	1444.0
79.00	1862.0
80.00	1398.0
81.00	1834.0
82.00	572.0
83.00	534.0
84.00	2726.0
85.00	485.0
85.90	2411.0
87.00	381.0
87.90	401.0
91.00	555.0
92.00	424.0
93.00	3046.0
98.00	2482.0
99.00	1471.0
101.00	803.0
102.90	508.0
103.90	588.0
105.00	608.0
107.00	7405.0
108.00	1121.0
108.90	350.0
110.00	12517.0
111.00	2078.0
116.00	533.0
117.00	6512.0
117.90	450.0
121.90	593.0
123.00	761.0
124.00	328.0
124.90	442.0
127.00	25072.0
128.00	1977.0
129.00	10497.0
130.00	891.0
135.00	810.0
136.00	369.0
136.90	454.0
141.00	1489.0
141.90	510.0
142.80	376.0
146.90	675.0
147.90	1889.0
149.00	380.0
153.00	519.0
155.00	891.0
156.00	1198.0
159.90	546.0
161.00	672.0
165.00	591.0
166.00	471.0
167.00	2644.0
168.00	1375.0
169.00	303.0
172.90	359.0
173.90	569.0
175.00	1241.0
176.10	316.0
177.00	589.0
179.00	2002.0
180.00	1350.0
180.90	727.0
185.00	1189.0
186.00	8249.0
186.90	2284.0
189.00	640.0
190.90	345.0

Instrument :
BNA_M
ClientSampleId :
DFTPP88

192.00	829.0
193.00	718.0
196.00	1693.0
196.90	480.0
197.90	57400.0
198.90	4109.0
202.90	319.0
204.00	2230.0
205.00	3637.0
206.00	15574.0
207.00	2678.0
208.00	578.0
211.00	601.0
216.10	312.0
217.00	4726.0
217.90	603.0
221.00	2121.0
223.00	881.0
224.00	9177.0
225.00	2295.0
226.10	374.0
227.00	3903.0
228.00	693.0
228.90	923.0
231.00	526.0
242.00	374.0
243.00	422.0
244.00	7180.0
245.00	791.0
246.00	1426.0
255.00	36400.0
256.00	5494.0
257.00	428.0
257.90	1991.0
265.00	1073.0
273.00	1153.0
274.00	2864.0
275.00	15442.0
276.00	2027.0
277.00	1795.0
278.00	386.0
293.00	330.0
296.00	4813.0
296.90	665.0
303.10	465.0
315.00	752.0
323.00	1361.0
327.00	322.0
334.00	836.0
345.90	418.0
352.00	523.0
353.00	341.0
354.00	392.0
365.00	1818.0
366.00	387.0
372.00	632.0
402.00	330.0
420.90	360.0
423.00	2380.0
424.10	594.0
441.00	6984.0
442.10	47272.0
443.10	9104.0
444.00	828.0

Instrument :
BNA_M
ClientSampleId :
DFTPP88

m/z	Abundance
39.00	1239.0
41.10	373.0
43.00	437.0
43.90	432.0
47.00	603.0
48.00	330.0
49.00	2925.0
50.00	4180.0
51.10	15162.0
52.00	591.0
55.00	367.0
55.90	529.0
57.00	1044.0
63.00	668.0
65.00	440.0
67.90	388.0
69.00	17024.0
73.00	390.0
74.00	2084.0
75.00	2760.0
76.00	863.0
77.10	18496.0
78.00	1166.0
79.00	1439.0
79.90	1174.0
81.00	1808.0
82.00	484.0
83.00	558.0
84.00	2506.0
85.00	512.0
86.00	2103.0
87.90	302.0
91.00	413.0
91.90	446.0
93.00	2754.0
98.00	2095.0
99.00	1471.0
101.00	753.0
104.00	659.0
105.00	566.0
107.00	6494.0
108.00	1141.0
110.00	11709.0
111.00	1838.0
116.00	378.0
117.00	6130.0
118.00	388.0
121.90	493.0
122.90	900.0
127.00	22264.0
128.00	1805.0
129.00	9560.0
130.00	862.0
135.00	737.0
136.00	377.0
137.10	527.0
141.00	1267.0
142.00	560.0
146.00	310.0
147.00	778.0
147.90	1495.0
148.90	421.0
152.90	508.0
153.90	370.0
155.10	774.0
156.00	1173.0
159.80	477.0
161.00	598.0
164.90	556.0
165.80	437.0
167.00	3212.0
168.00	1203.0
168.90	329.0
172.90	356.0
174.00	650.0
175.00	1249.0
176.90	533.0
179.00	2277.0
180.00	1344.0
181.00	672.0
185.00	1138.0
186.00	7835.0
187.00	2375.0
188.90	505.0
190.90	300.0
191.90	674.0
193.00	916.0
196.00	1756.0
197.10	415.0
197.90	57104.0
199.00	3662.0

Instrument :
BNA_M
ClientSampleId :
DFTPP88

201.40	353.0
203.00	572.0
204.00	1930.0
205.00	3839.0
206.00	15439.0
207.00	2392.0
207.90	658.0
210.10	322.0
210.90	651.0
214.90	309.0
217.00	4475.0
217.90	580.0
221.00	2350.0
223.00	821.0
224.00	8786.0
225.00	2170.0
226.90	4079.0
228.00	580.0
229.00	806.0
231.00	406.0
233.90	384.0
235.00	378.0
237.00	420.0
241.90	531.0
242.90	506.0
244.00	6893.0
245.00	718.0
245.90	1606.0
246.90	328.0
255.00	38680.0
256.00	5401.0
257.00	447.0
258.00	2433.0
259.00	481.0
265.00	861.0
273.00	1039.0
274.00	2944.0
275.00	17216.0
276.00	2206.0
277.00	1453.0
292.90	366.0
296.00	5257.0
297.00	627.0
303.00	653.0
314.00	317.0
314.90	636.0
316.00	316.0
323.00	1634.0
326.90	465.0
334.00	842.0
345.90	306.0
352.00	468.0
352.90	307.0
354.00	560.0
365.00	2369.0
366.00	303.0
372.00	941.0
402.00	366.0
402.90	445.0
421.00	358.0
422.00	550.0
423.00	2804.0
424.00	580.0
441.00	8423.0
442.10	61440.0
443.00	10991.0
444.10	953.0

Instrument :

BNA_M

ClientSampleId :


DFTPP88

Data Path : Z:\HPCHEM1\BNA_M\Data\BM080315\
 Data File : BM002192.D
 Acq On : 03 Aug 2015 10:52
 Operator : TP
 Sample : DFTPP88
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP88

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072715.M
 Title : SVOA CALIBRATION
 Last Update : Tue Aug 04 02:31:26 2015

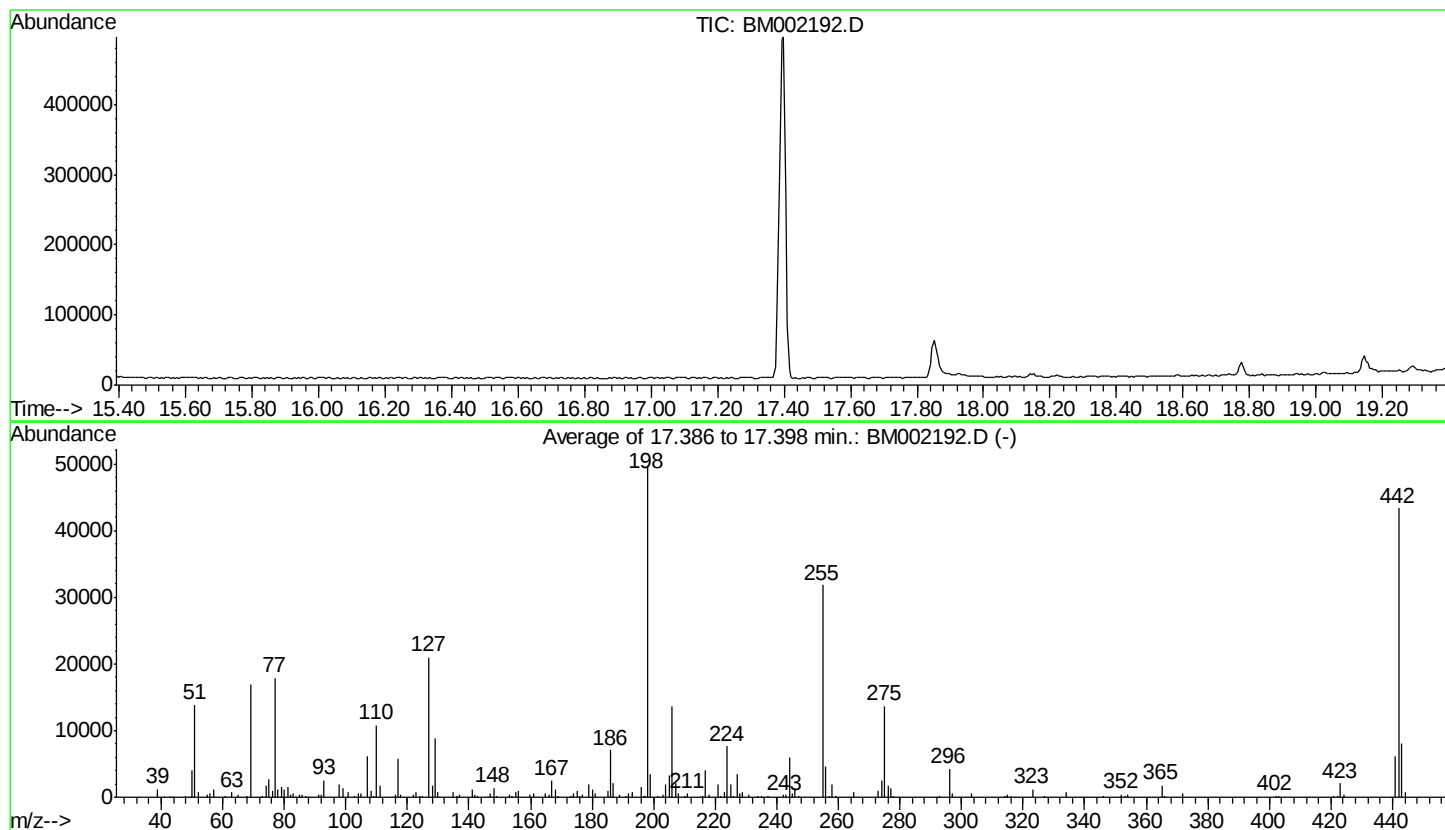

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	13880	PASS
68	69	0.00	2	1.7	283	PASS
69	198	0.00	100	34.1	16959	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.1	20948	PASS
197	198	0.00	2	0.3	160	PASS
198	198	100	100	100.0	49760	PASS
199	198	5	9	7.2	3559	PASS
275	198	10	60	27.5	13697	PASS
365	198	1	100	3.5	1764	PASS
441	443	0.01	100	76.1	6188	PASS
442	198	50	100	87.1	43362	PASS
443	442	15	24	18.8	8136	PASS