

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080316\
 Data File : BM006853.D
 Acq On : 03 Aug 2016 21:28
 Operator : UM/SJ
 Sample : SSTD02036
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD02049

Quant Time: Aug 04 04:56:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 04 04:55:08 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	142586	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	559683	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	388806	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	965330	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	1043674	20.00	ng/ul	0.00
83) Perylene-d12	23.38	264	907240	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.11	96	21353	6.08	ng/uL	0.00
5) Phenol-d5	6.80	99	199784	16.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	144379	19.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	168201	17.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	159006	16.91	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	78732	18.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	91874	19.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	194390	22.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	186654	21.08	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	640046	20.61	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	780014	20.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	126435	22.81	ng/ul	0.00
57) Fluorene-d10	15.23	176	590830	21.66	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.39	200	120539	22.03	ng/ul	0.00
70) Anthracene-d10	17.08	188	948251	20.92	ng/ul	0.00
76) Pyrene-d10	19.39	212	1083917	21.97	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	883857	21.30	ng/ul	0.00

Target Compounds

					Qvalue
2) 1,4-Dioxane	3.15	88	21846	6.10	ng/uL 100
4) Benzaldehyde	6.75	77	148908	19.03	ng/ul 100
6) Phenol	6.83	94	213741	16.86	ng/ul 100
8) Bis(2-Chloroethyl)ether	7.01	93	160080	16.77	ng/ul 100
10) 2-Chlorophenol	7.15	128	169509	17.49	ng/ul 100
11) 2-Methylphenol	8.06	108	161630	17.05	ng/ul 100
12) 2,2'-oxybis(1-Chloropropan	8.11	45	357037	23.65	ng/ul 100
14) Acetophenone	8.40	105	287600	19.20	ng/ul 100
15) N-Nitroso-di-n-propylamine	8.39	70	153786	18.87	ng/ul 100
16) 4-Methylphenol	8.39	108	172906	17.17	ng/ul 100
17) Hexachloroethane	8.62	117	84613	19.90	ng/ul 100
20) Nitrobenzene	8.78	77	245825	21.85	ng/ul 100
21) Isophorone	9.30	82	388904	19.02	ng/ul 100
23) 2-Nitrophenol	9.49	139	95822	19.01	ng/ul 100
24) 2,4-Dimethylphenol	9.57	107	240972	21.74	ng/ul 100
25) Bis(2-Chloroethoxy)methane	9.78	93	215494	17.50	ng/ul 100
27) 2,4-Dichlorophenol	10.03	162	194671	22.41	ng/ul 100
28) Naphthalene	10.39	128	563808	20.19	ng/ul 100
30) 4-Chloroaniline	10.54	127	197369	21.51	ng/ul 100
31) Hexachlorobutadiene	10.66	225	171254	28.57	ng/ul 100
32) Caprolactam	11.40	113	24146	8.94	ng/ul 100
33) 4-Chloro-3-methylphenol	11.70	107	195604	19.92	ng/ul 100
34) 2-Methylnaphthalene	12.02	142	456080	21.83	ng/ul 100


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM080316\
 Data File : BM006853.D
 Acq On : 03 Aug 2016 21:28
 Operator : UM/SJ
 Sample : SSTD02036
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD02049

Quant Time: Aug 04 04:56:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 04 04:55:08 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 1,2,4,5-Tetrachlorobenzene	12.39	216	308223	23.64	ng/ul	100
37) Hexachlorocyclopentadiene	12.36	237	146003	24.83	ng/ul	100
38) 2,4,6-Trichlorophenol	12.67	196	191220	22.37	ng/ul	100
39) 2,4,5-Trichlorophenol	12.76	196	197210	22.25	ng/ul	100
40) 1,1'-Biphenyl	13.04	154	630672	20.06	ng/ul	100
41) 2-Chloronaphthalene	13.09	162	495774	20.27	ng/ul	100
42) 2-Nitroaniline	13.34	65	186296	21.48	ng/ul	100
44) Dimethylphthalate	13.70	163	651833	20.90	ng/ul	100
45) 2,6-Dinitrotoluene	13.83	165	122417	19.31	ng/ul	100
47) Acenaphthylene	13.94	152	791999	19.71	ng/ul	100
48) 3-Nitroaniline	14.19	138	105211	18.60	ng/ul	100
49) Acenaphthene	14.29	153	516571	20.07	ng/ul	100
50) 2,4-Dinitrophenol	14.40	184	68941	20.61	ng/ul	100
52) 4-Nitrophenol	14.54	109	176508	31.35	ng/ul	100
53) Dibenzofuran	14.63	168	787976	21.19	ng/ul	100
54) 2,4-Dinitrotoluene	14.63	165	193933	21.30	ng/ul	100
55) 2,3,4,6-Tetrachlorophenol	14.88	232	192487	25.00	ng/ul	100
56) Diethylphthalate	15.07	149	666935	20.34	ng/ul	100
58) Fluorene	15.28	166	674243	22.24	ng/ul	100
59) 4-Chlorophenyl-phenylether	15.27	204	368734	24.35	ng/ul	100
60) 4-Nitroaniline	15.36	138	87650	13.17	ng/ul	100
63) 4,6-Dinitro-2-methylphenol	15.40	198	127024	21.83	ng/ul	100
64) N-Nitrosodiphenylamine	15.50	169	567158	19.78	ng/ul	100
65) 4-Bromophenyl-phenylether	16.17	248	240216	22.68	ng/ul	100
66) Hexachlorobenzene	16.29	284	268644	23.13	ng/ul	100
67) Atrazine	16.47	200	233367	22.31	ng/ul	100
68) Pentachlorophenol	16.66	266	133424	24.76	ng/ul	100
69) Phenanthrene	17.02	178	1076897	20.56	ng/ul	100
71) Anthracene	17.12	178	1131793	20.87	ng/ul	100
72) Carbazole	17.41	167	903492	19.54	ng/ul	100
73) Di-n-butylphthalate	17.95	149	1015358	16.68	ng/ul	100
74) Fluoranthene	19.05	202	1368882	22.77	ng/ul	100
77) Pyrene	19.42	202	1398178	21.60	ng/ul	100
78) Butylbenzylphthalate	20.32	149	477864	16.98	ng/ul	100
79) 3,3'-Dichlorobenzidine	21.11	252	400713	22.39	ng/ul	100
80) Benzo(a)anthracene	21.17	228	1284136	20.59	ng/ul	100
81) Bis(2-ethylhexyl)phthalate	21.10	149	654782	16.32	ng/ul	100
82) Chrysene	21.23	228	1139141	20.17	ng/ul	100
84) Di-n-octyl phthalate	21.96	149	1001240	18.11	ng/ul	100
85) Benzo(b)fluoranthene	22.73	252	1120714	20.93	ng/ul	100
86) Benzo(k)fluoranthene	22.77	252	1134116	22.45	ng/ul	100
88) Benzo(a)pyrene	23.29	252	1083240	21.08	ng/ul	100
89) Indeno(1,2,3-cd)pyrene	25.57	276	1301790	21.49	ng/ul	100
90) Dibenzo(a,h)anthracene	25.57	278	1119128	22.11	ng/ul	100
91) Benzo(g,h,i)perylene	26.24	276	1066298	20.57	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 6.10 ng/uL

RT: 3.15 min Scan# 95

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28

Instrument :

BNA_M

ClientSampleId :

SSTD02049





Tgt Ion: 88 Resp: 21846

Ion Ratio Lower Upper

88 100

43 86.5 69.2 103.8

58 106.5 85.2 127.8

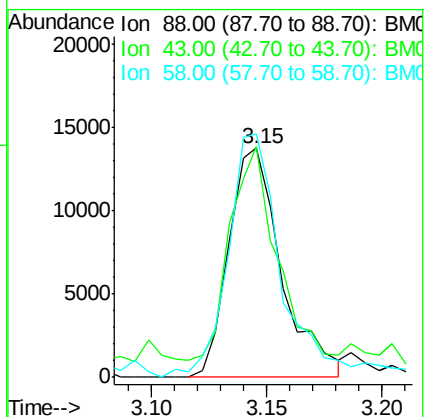

#4

Benzaldehyde

Concen: 19.03 ng/uL

RT: 6.75 min Scan# 707

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28




Tgt Ion: 77 Resp: 148908


Ion Ratio Lower Upper

77 100

105 84.6 67.7 101.5

106 75.9 60.7 91.1

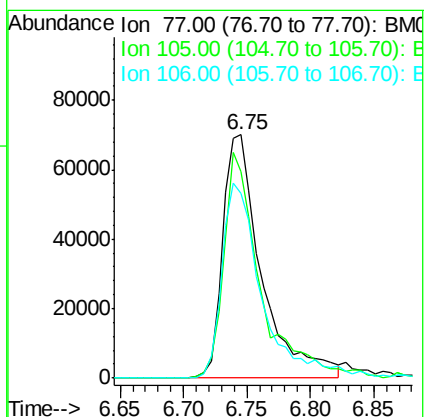



#6

Phenol

Concen: 16.86 ng/ul

RT: 6.83 min Scan# 721

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28

Instrument :

BNA_M

ClientSampleId :

SSTD02049


Tgt Ion: 94 Resp: 213741

Ion Ratio Lower Upper

94 100

65 49.1 39.3 58.9




66 75.9 60.7 91.1



Abundance Ion 94.00 (93.70 to 94.70): BM006853.D (-713) (-)

Ion 65.00 (64.70 to 65.70): BM006853.D (-713) (-)

Ion 66.00 (65.70 to 66.70): BM006853.D (-713) (-)

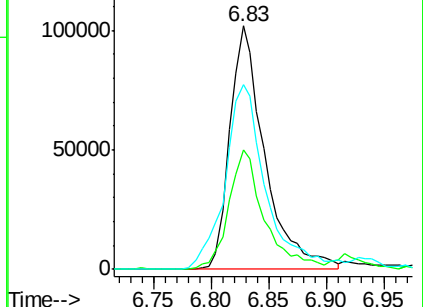

#8

Bis(2-Chloroethyl)ether

Concen: 16.77 ng/ul

RT: 7.01 min Scan# 752

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28


Tgt Ion: 93 Resp: 160080

Ion Ratio Lower Upper

93 100

63 96.1 76.9 115.3



95 35.2 28.2 42.2




Abundance Ion 93.00 (92.70 to 93.70): BM006853.D (-745) (-)

Ion 63.00 (62.70 to 63.70): BM006853.D (-745) (-)

Ion 95.00 (94.70 to 95.70): BM006853.D (-745) (-)

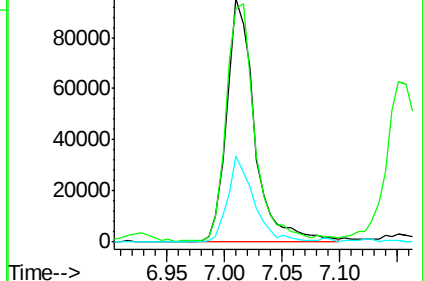

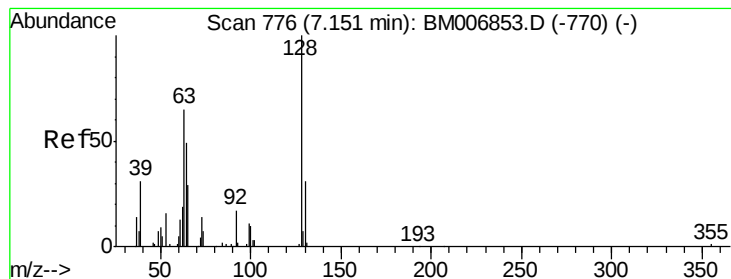

#10

2-Chlorophenol

Concen: 17.49 ng/ul

RT: 7.15 min Scan# 776

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28

Instrument :

BNA_M

ClientSampleId :

SSTD02049


Tgt Ion:128 Resp: 169509

Ion Ratio Lower Upper

128 100

64 66.3 53.0 79.6




130 31.5 25.2 37.8



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 130.00 (129.70 to 130.70): E

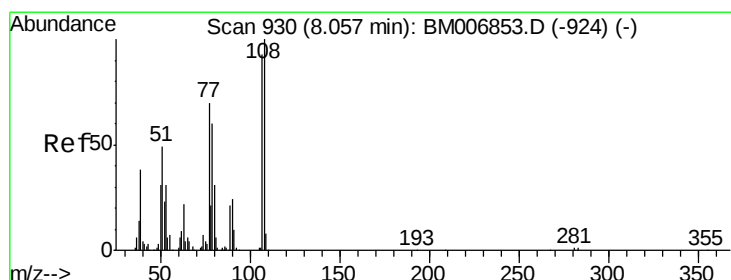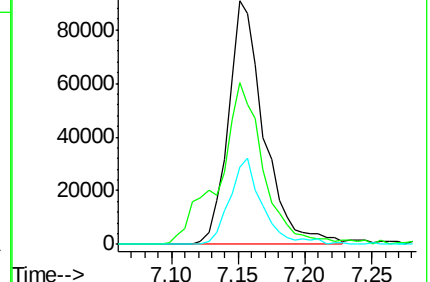

#11

2-Methylphenol

Concen: 17.05 ng/ul

RT: 8.06 min Scan# 930

Delta R.T. 0.00 min

Lab File: BM006853.D


Acq: 03 Aug 2016 21:28

Tgt Ion:108 Resp: 161630

Ion Ratio Lower Upper



108 100


107 93.4 74.7 112.1



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

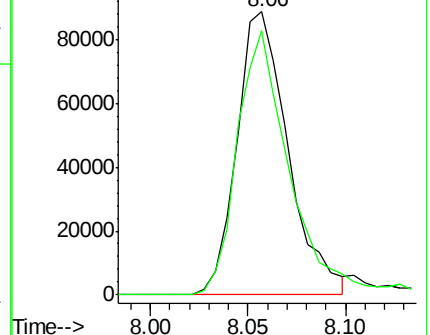

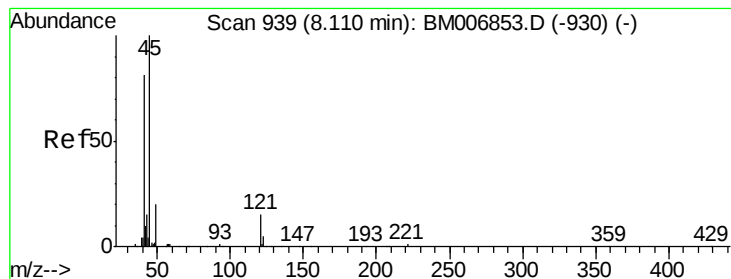

#12

2,2'-oxybis(1-chloropropane)

Concen: 23.65 ng/ul

RT: 8.11 min Scan# 939

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28

Instrument :

BNA_M

ClientSampleId :

SSTD02049





Tgt Ion: 45 Resp: 357037

Ion Ratio Lower Upper

45 100

77 13.8 11.0 16.6

79 9.9 7.9 11.9

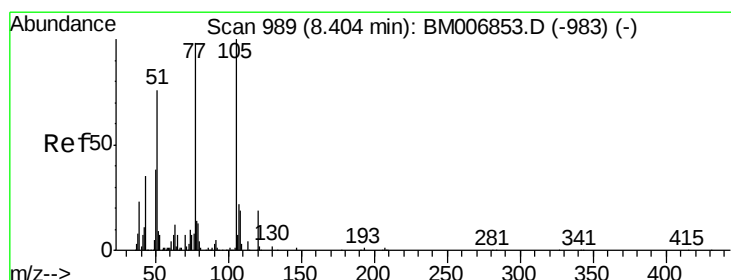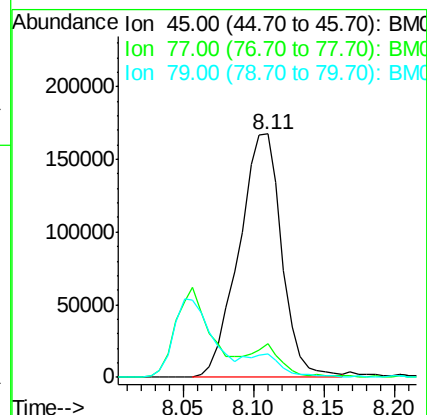

#14

Acetophenone

Concen: 19.20 ng/ul

RT: 8.40 min Scan# 989

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28




Tgt Ion: 105 Resp: 287600


Ion Ratio Lower Upper

105 100

77 107.8 86.2 129.4

51 82.3 65.8 98.8

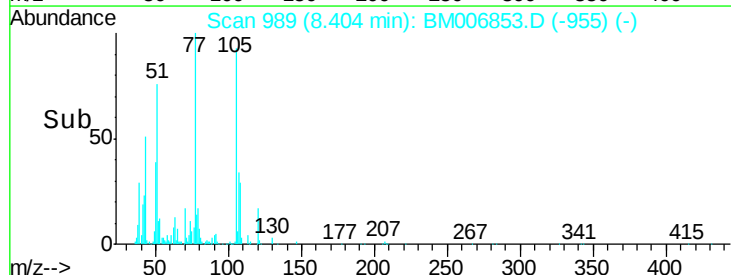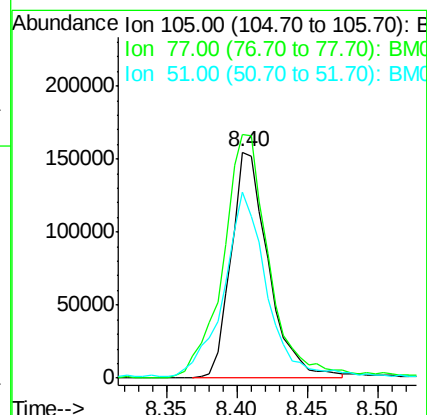







#15
N-Nitroso-di-n-propylamine
Concen: 18.87 ng/ul
RT: 8.39 min Scan# 986
Delta R.T. 0.00 min
Lab File: BM006853.D
Acq: 03 Aug 2016 21:28

Instrument :
BNA_M
ClientSampleId :
SSTD02049

Tgt Ion: 70 Resp: 153786
Ion Ratio Lower Upper
70 100
42 106.6 85.3 127.9
101 12.2 9.8 14.6
130 20.1 16.1 24.1




Abundance Ion 70.00 (69.70 to 70.70): BM0
Ion 42.00 (41.70 to 42.70): BM0
Ion 101.00 (100.70 to 101.70): E
Ion 130.00 (129.70 to 130.70): E


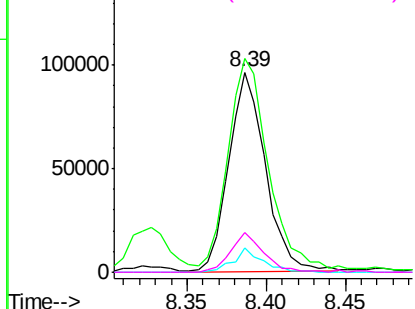



#16
4-Methylphenol
Concen: 17.17 ng/ul
RT: 8.39 min Scan# 987
Delta R.T. 0.00 min
Lab File: BM006853.D
Acq: 03 Aug 2016 21:28

Tgt Ion: 108 Resp: 172906
Ion Ratio Lower Upper
108 100
107 101.5 81.2 121.8



Abundance Ion 108.00 (107.70 to 108.70): E
Ion 107.00 (106.70 to 107.70): E

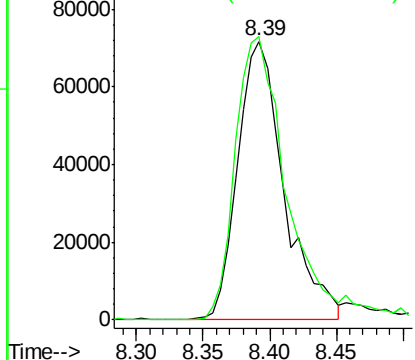


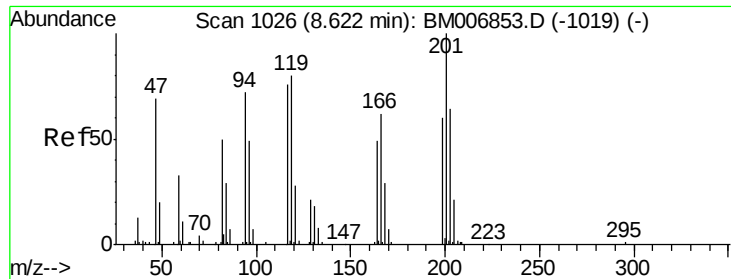




#17
Hexachloroethane
Concen: 19.90 ng/ul
RT: 8.62 min Scan# 1026
Delta R.T. 0.00 min
Lab File: BM006853.D
Acq: 03 Aug 2016 21:28

Instrument :
BNA_M
ClientSampleId :
SSTD02049

Tgt Ion:117 Resp: 84613
Ion Ratio Lower Upper
117 100
201 132.2 105.8 158.6
199 79.9 63.9 95.9




Abundance Ion 117.00 (116.70 to 117.70): E
Ion 201.00 (200.70 to 201.70): E
Ion 199.00 (198.70 to 199.70): E


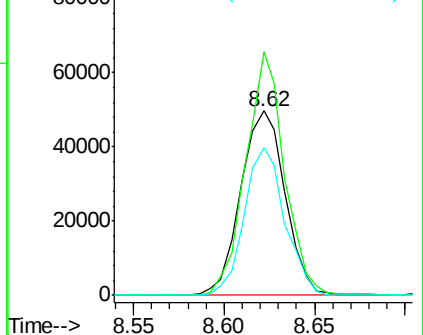



#20
Nitrobenzene
Concen: 21.85 ng/ul
RT: 8.78 min Scan# 1053
Delta R.T. 0.00 min
Lab File: BM006853.D
Acq: 03 Aug 2016 21:28

Tgt Ion: 77 Resp: 245825
Ion Ratio Lower Upper
77 100
123 33.4 26.7 40.1
65 21.4 17.1 25.7



Abundance Ion 77.00 (76.70 to 77.70): BM
Ion 123.00 (122.70 to 123.70): E
Ion 65.00 (64.70 to 65.70): BM

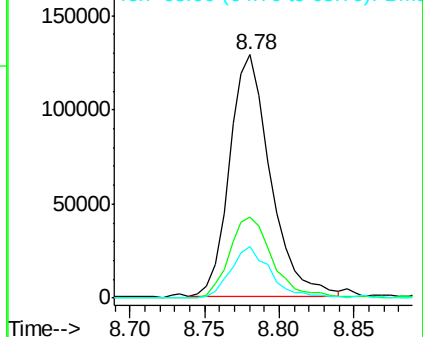

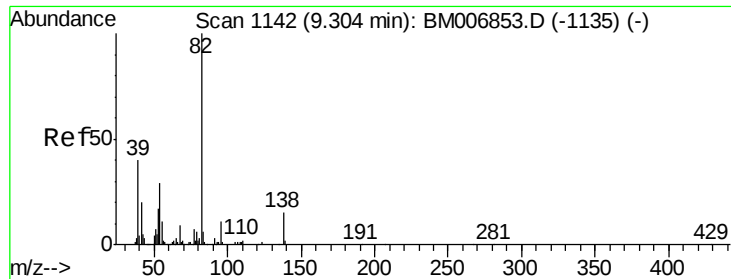

#21

Isophorone

Concen: 19.02 ng/ul

RT: 9.30 min Scan# 1142

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28

Instrument :

BNA_M

ClientSampleId :

SSTD02049





Tgt Ion: 82 Resp: 388904

Ion Ratio Lower Upper

82 100

95 10.8 8.6 13.0

138 15.4 12.3 18.5

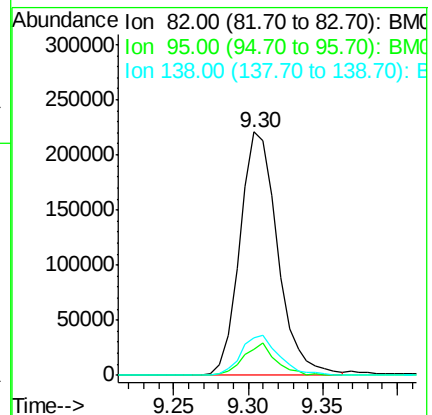

#23

2-Nitrophenol

Concen: 19.01 ng/ul

RT: 9.49 min Scan# 1173

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28




Tgt Ion: 139 Resp: 95822


Ion Ratio Lower Upper

139 100

65 81.7 65.4 98.0

109 58.9 47.1 70.7


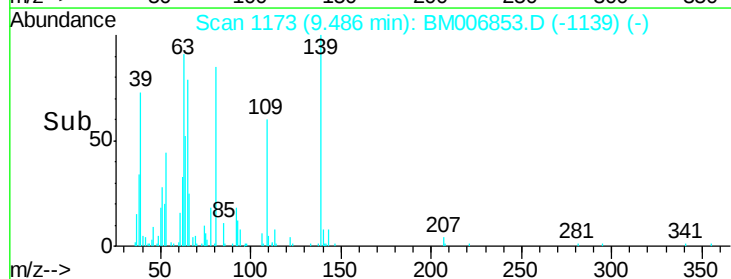
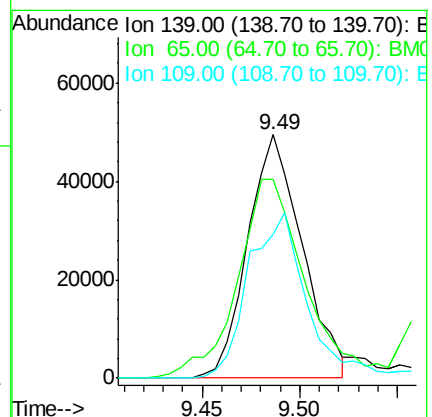





#24
 2,4-Dimethylphenol
 Concen: 21.74 ng/ul
 RT: 9.57 min Scan# 1187
 Delta R.T. 0.00 min
 Lab File: BM006853.D
 Acq: 03 Aug 2016 21:28




Instrument :
 BNA_M
 ClientSampleId :
 SST02049


Tgt Ion: 107 Resp: 240972
 Ion Ratio Lower Upper
 107 100
 121 43.2 34.6 51.8
 122 67.6 54.1 81.1

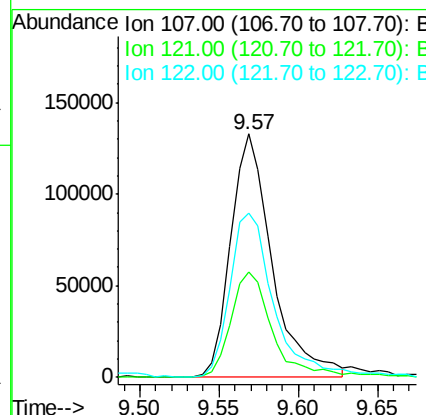

#25
 Bis(2-Chloroethoxy)methane
 Concen: 17.50 ng/ul
 RT: 9.78 min Scan# 1223
 Delta R.T. 0.00 min
 Lab File: BM006853.D
 Acq: 03 Aug 2016 21:28

Tgt Ion: 93 Resp: 215494
 Ion Ratio Lower Upper
 93 100
 95 33.0 26.4 39.6
 123 10.9 8.7 13.1



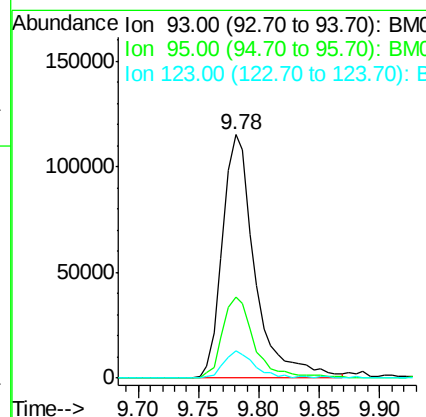





#27
 2,4-Dichlorophenol
 Concen: 22.41 ng/ul
 RT: 10.03 min Scan# 1266
 Delta R.T. 0.00 min
 Lab File: BM006853.D
 Acq: 03 Aug 2016 21:28




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02049


Tgt Ion	Ratio	Lower	Upper
162	100		
164	75.5	60.4	90.6
98	33.2	26.6	39.8

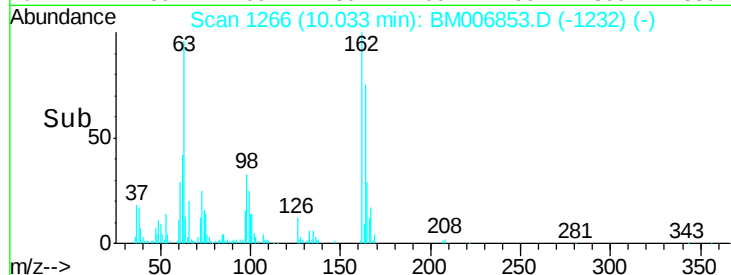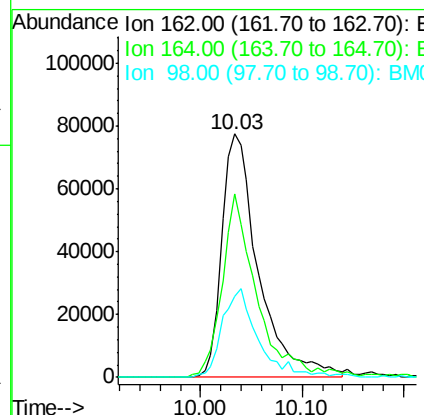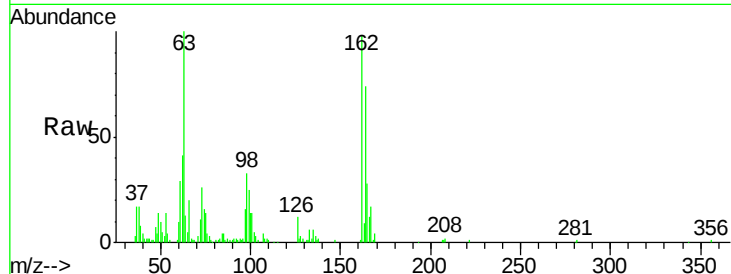

#28
 Naphthalene
 Concen: 20.19 ng/ul
 RT: 10.39 min Scan# 1327
 Delta R.T. 0.00 min
 Lab File: BM006853.D
 Acq: 03 Aug 2016 21:28

Tgt Ion	Ratio	Lower	Upper
128	100		
129	11.1	8.9	13.3
127	14.6	11.7	17.5



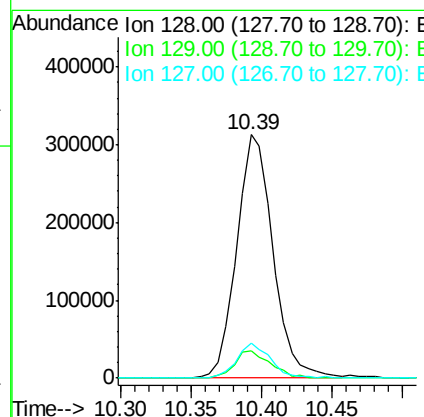



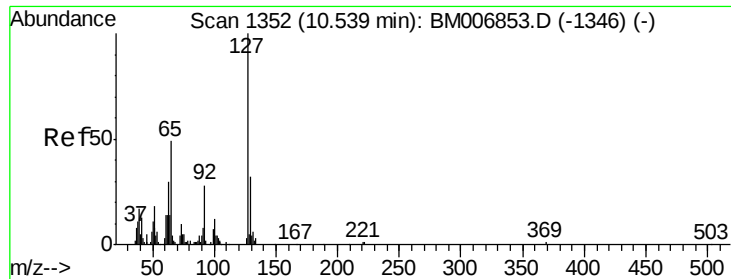

#30
4-Chloroaniline
Concen: 21.51 ng/ul
RT: 10.54 min Scan# 1352
Delta R.T. 0.00 min
Lab File: BM006853.D
Acq: 03 Aug 2016 21:28




Instrument :
BNA_M
ClientSampleId :
SSTD02049


Tgt Ion:127 Resp: 197369
Ion Ratio Lower Upper
127 100
129 31.5 25.2 37.8

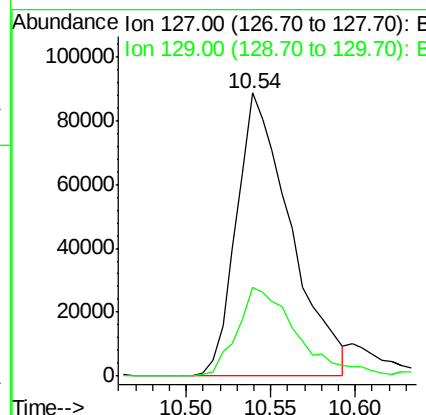

#31
Hexachlorobutadiene
Concen: 28.57 ng/ul
RT: 10.66 min Scan# 1373
Delta R.T. 0.00 min
Lab File: BM006853.D
Acq: 03 Aug 2016 21:28

Tgt Ion:225 Resp: 171254
Ion Ratio Lower Upper
225 100
223 60.1 48.1 72.1
227 61.9 49.5 74.3

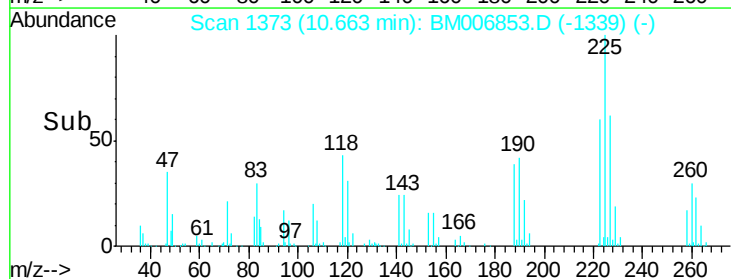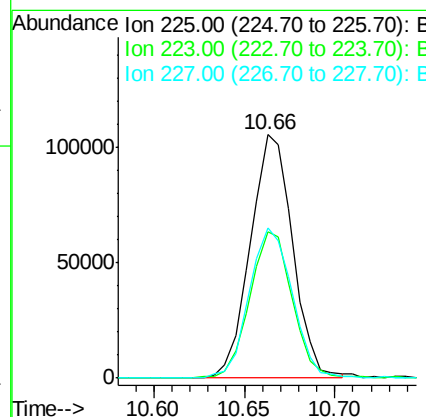

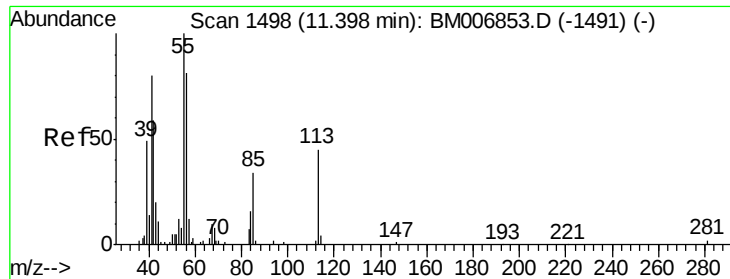

#32

Caprolactam

Concen: 8.94 ng/ul

RT: 11.40 min Scan# 1498

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28

Instrument :

BNA_M

ClientSampleId :

SSTD02049


Tgt Ion:113 Resp: 24146

Ion Ratio Lower Upper

113 100

55 223.9 179.1 268.7




56 180.8 144.6 217.0

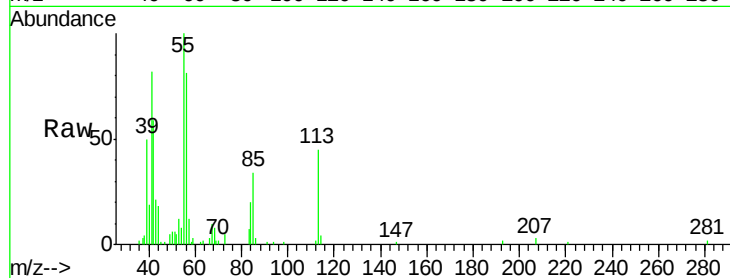

Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BM

Ion 56.00 (55.70 to 56.70): BM

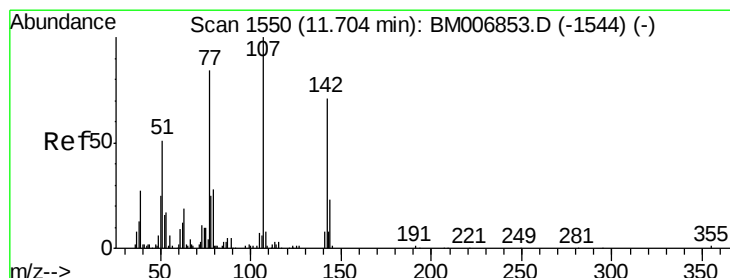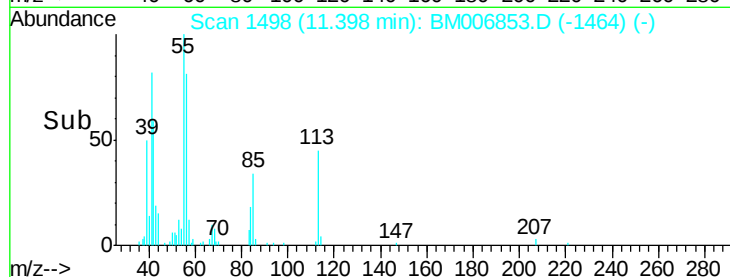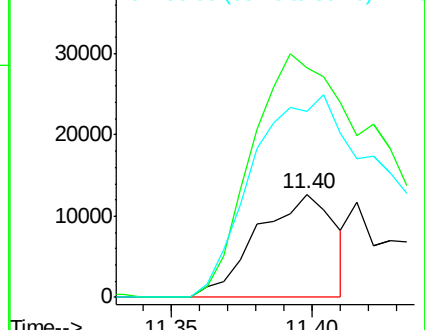

#33

4-Chloro-3-methylphenol

Concen: 19.92 ng/ul

RT: 11.70 min Scan# 1550

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28


Tgt Ion:107 Resp: 195604

Ion Ratio Lower Upper

107 100

144 22.9 18.3 27.5



142 71.4 57.1 85.7

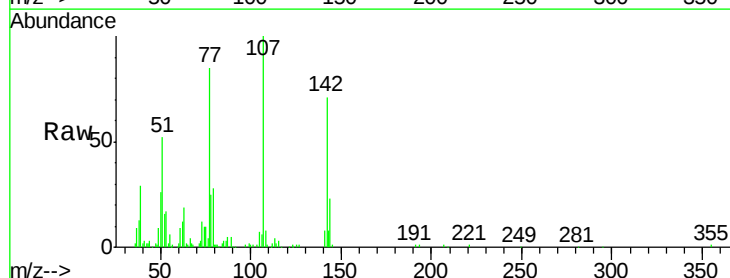


Abundance Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E



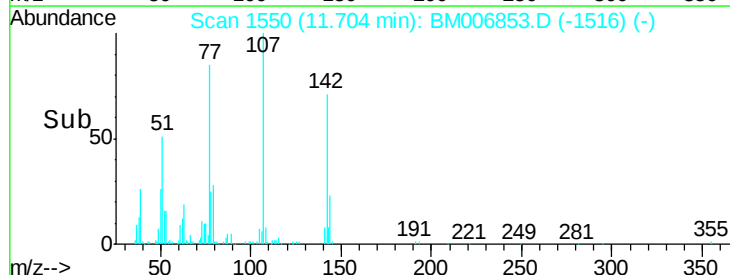
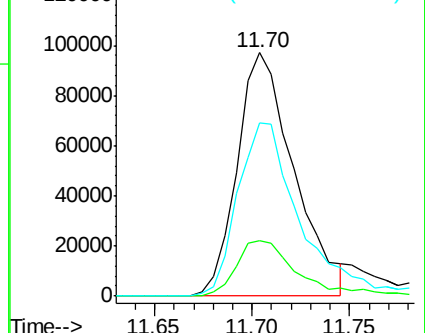




#34
 2-Methylnaphthalene
 Concen: 21.83 ng/ul
 RT: 12.02 min Scan# 1604
 Delta R.T. 0.00 min
 Lab File: BM006853.D
 Acq: 03 Aug 2016 21:28




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02049


Tgt Ion:142 Resp: 456080
 Ion Ratio Lower Upper
 142 100
 141 89.1 71.3 106.9

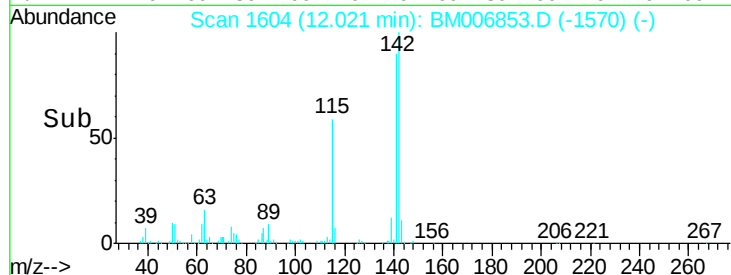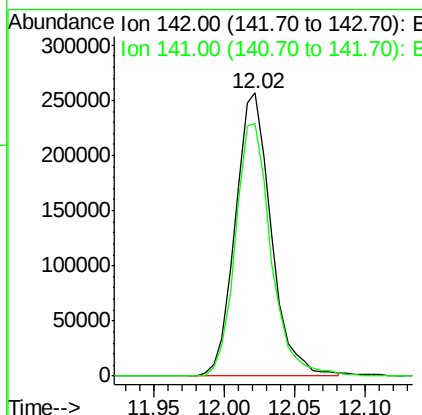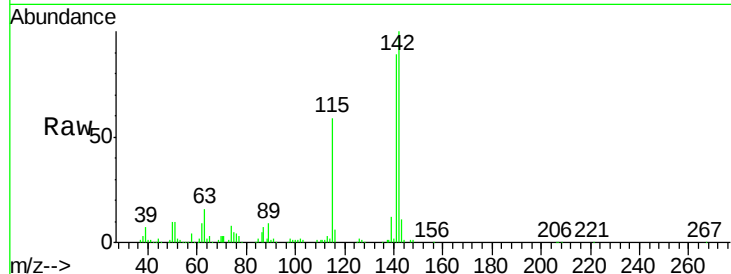

#36
 1,2,4,5-Tetrachlorobenzene
 Concen: 23.64 ng/ul
 RT: 12.39 min Scan# 1667
 Delta R.T. 0.00 min
 Lab File: BM006853.D
 Acq: 03 Aug 2016 21:28

Tgt Ion:216 Resp: 308223
 Ion Ratio Lower Upper
 216 100
 214 70.6 56.5 84.7
 179 20.4 16.3 24.5
 108 21.9 17.5 26.3

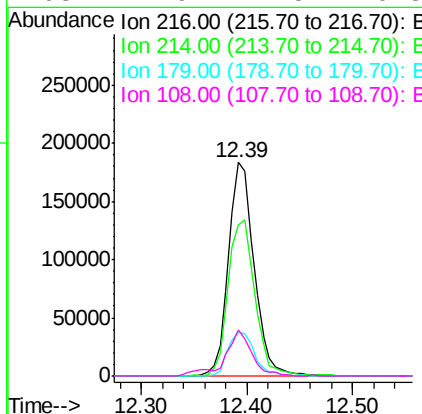

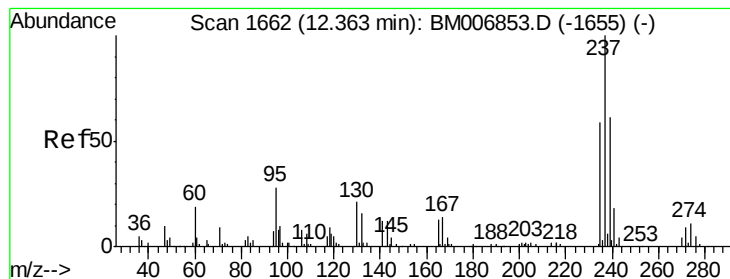

#37

Hexachlorocyclopentadiene

Concen: 24.83 ng/ul

RT: 12.36 min Scan# 1662

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28

Instrument :

BNA_M

ClientSampleId :

SSTD02049


Tgt Ion:237 Resp: 146003

Ion Ratio Lower Upper

237 100

235 58.9 47.1 70.7




272 9.1 7.3 10.9

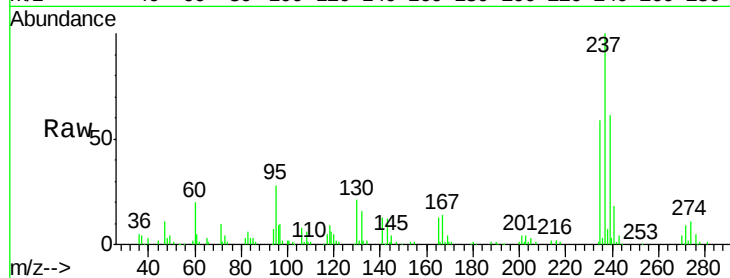

Abundance Ion 237.00 (236.70 to 237.70): E

Ion 235.00 (234.70 to 235.70): E

Ion 272.00 (271.70 to 272.70): E

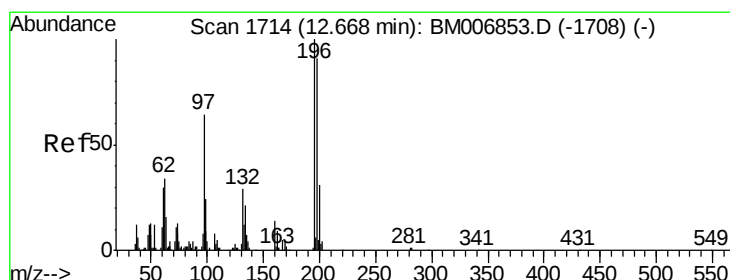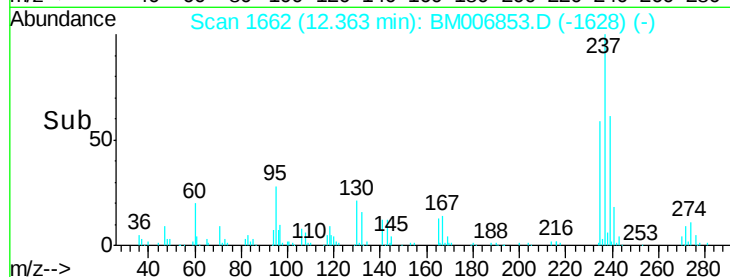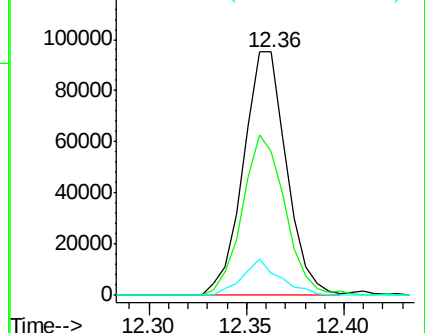

#38

2,4,6-Trichlorophenol

Concen: 22.37 ng/ul

RT: 12.67 min Scan# 1714

Delta R.T. 0.00 min

Lab File: BM006853.D

Acq: 03 Aug 2016 21:28


Tgt Ion:196 Resp: 191220

Ion Ratio Lower Upper

196 100

198 91.5 73.2 109.8

200 31.4 25.1 37.7

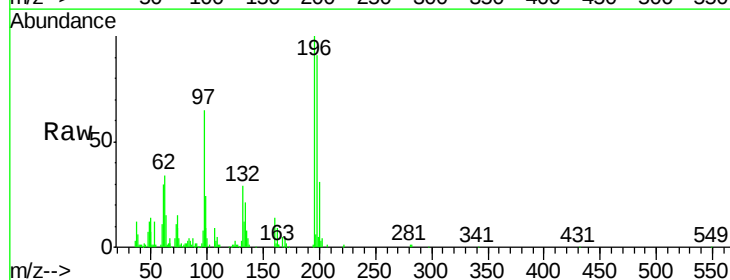

Abundance Ion 196.00 (195.70 to 196.70): E

Ion 198.00 (197.70 to 198.70): E

Ion 200.00 (199.70 to 200.70): E

