


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080320\
Data File : BM026990.D
Acq On : 03 Aug 2020 22:16
Operator : JU/CG
Sample : L3424-18DL 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 04 04:57:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
Quant Title : SVOA CALIBRATION
Qlast Update : Mon Aug 03 10:21:18 2020
Response via : Initial Calibration

Instrument :
BNA_M
Client Sample Id :
C0S93DL

Manual Integrations
APPROVED

mohammad
8/5/2020 10:26:26 AM

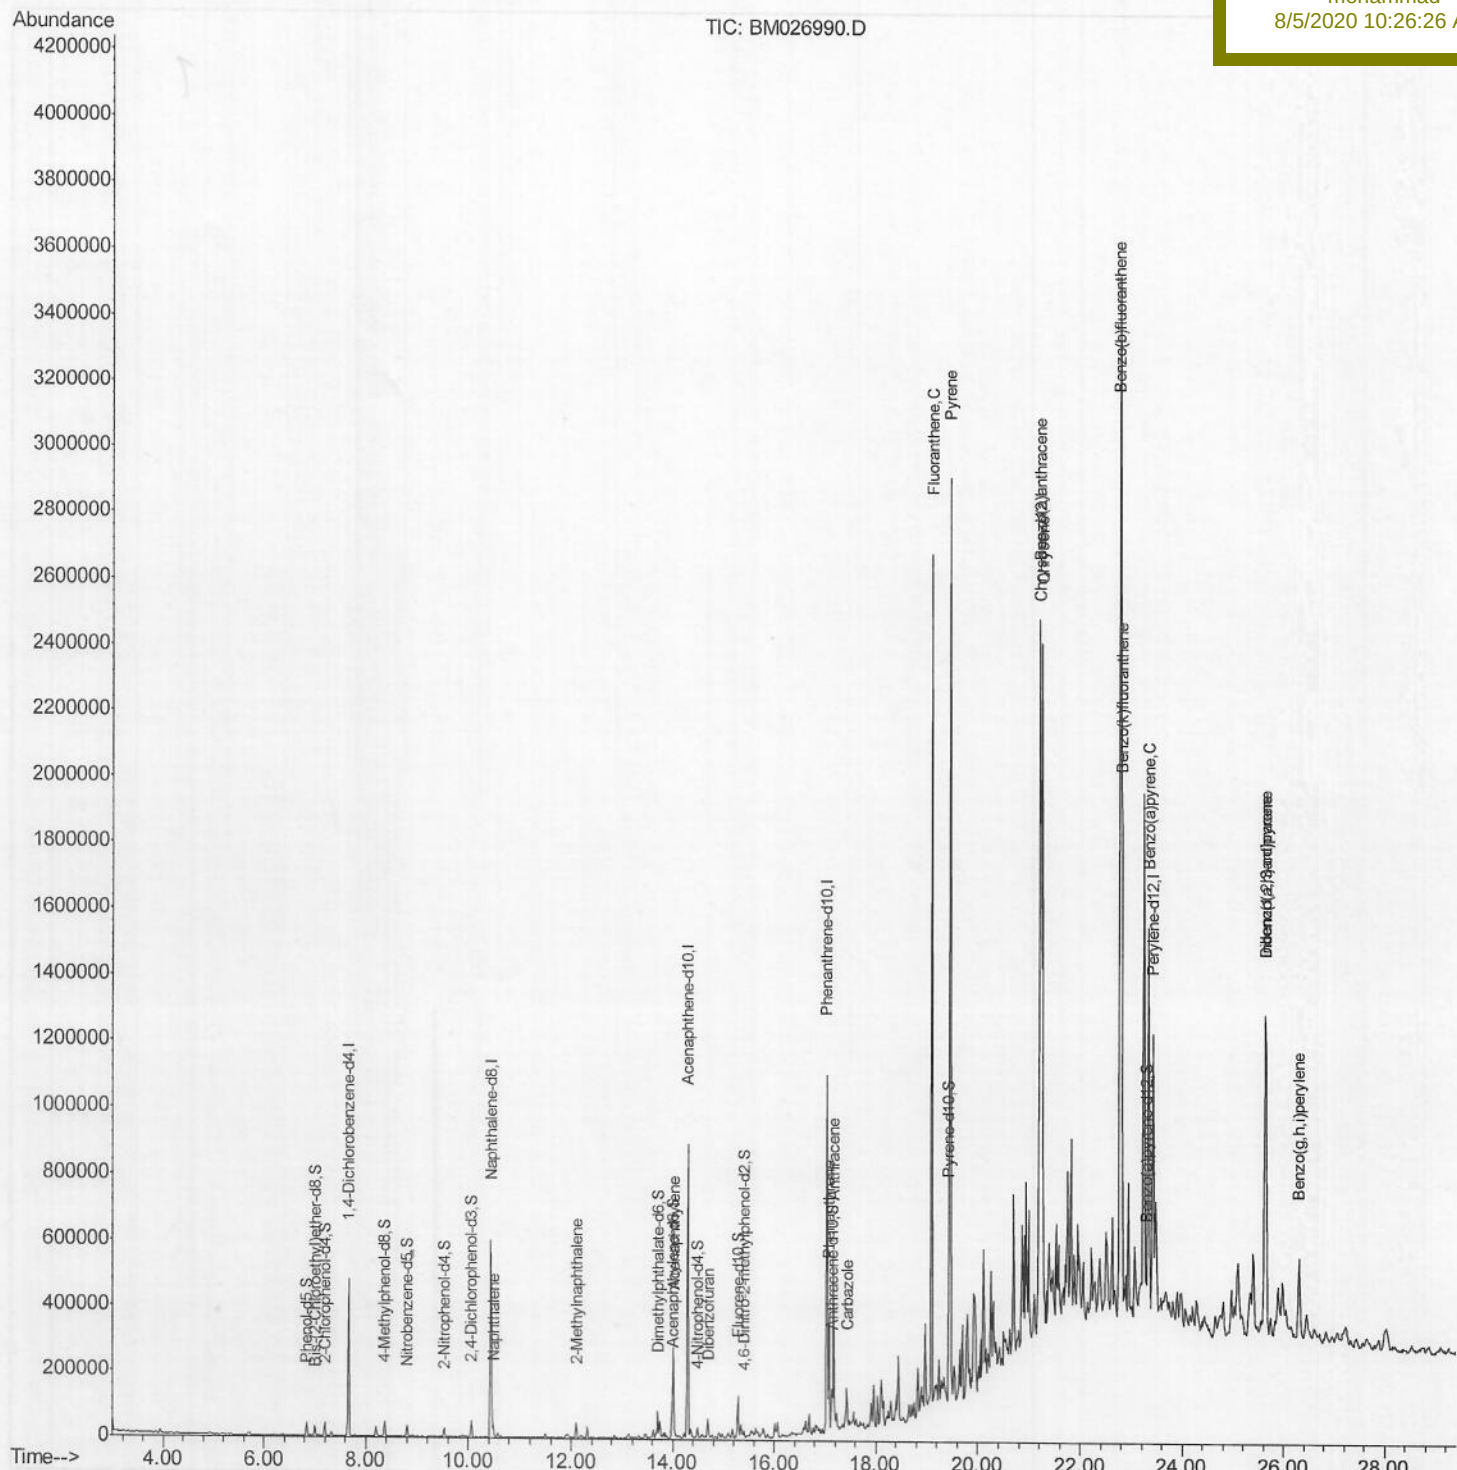

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080320\

Data File : BM026990.D

Acq On : 03 Aug 2020 22:16

Operator : JU/CG

Sample : L3424-18DL 10X

Misc :

ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 04 02:38:36 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Aug 03 10:21:18 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


C0S93DL

Manual Integrations

APPROVED

mohammad

8/5/2020 10:26:26 AM

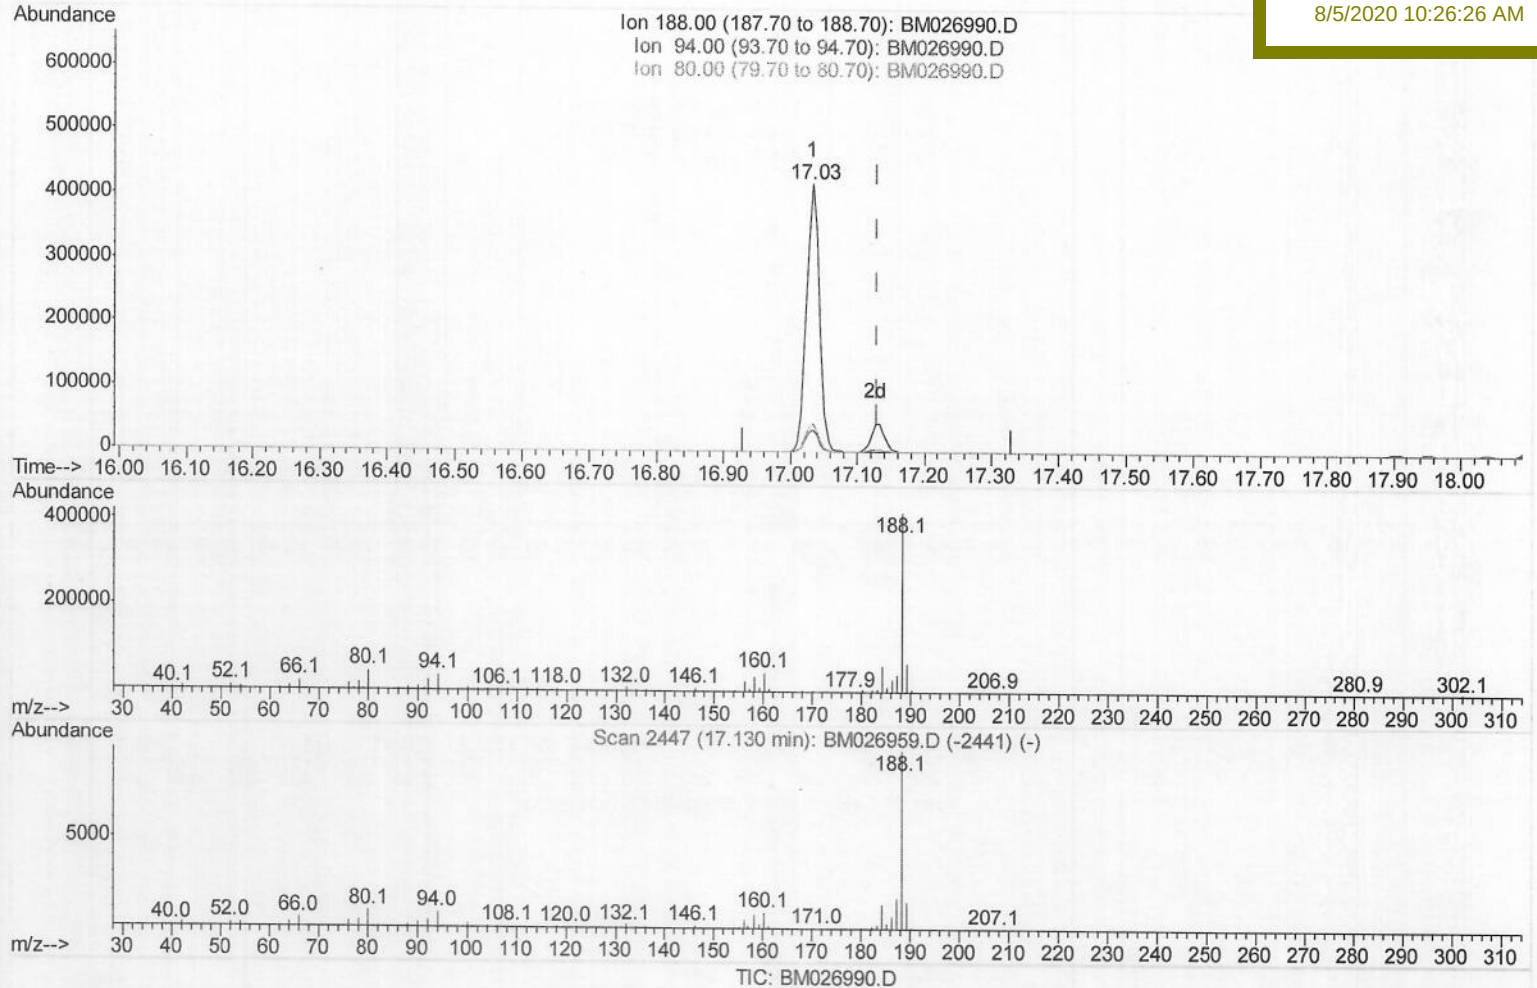

(71) Anthracene-d10 (S)

17.033min (-0.097) 20.01ng/ul

response 565740

Ion	Exp%	Act%
188.00	100	100
94.00	9.40	8.27
80.00	9.90	10.34
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080320\
 Data File : BM026990.D
 Acq On : 03 Aug 2020 22:16
 Operator : JU/CG
 Sample : L3424-18DL 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 04 02:38:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 03 10:21:18 2020
 Response via : Initial Calibration

Instrument :

BNA_M

Client Sampled :




C0S93DL

Manual Integrations

APPROVED

mohammad

8/5/2020 10:26:26 AM

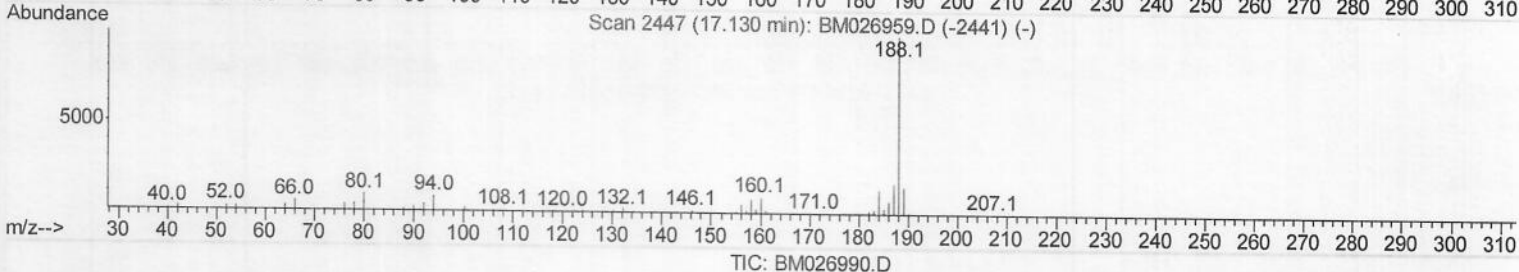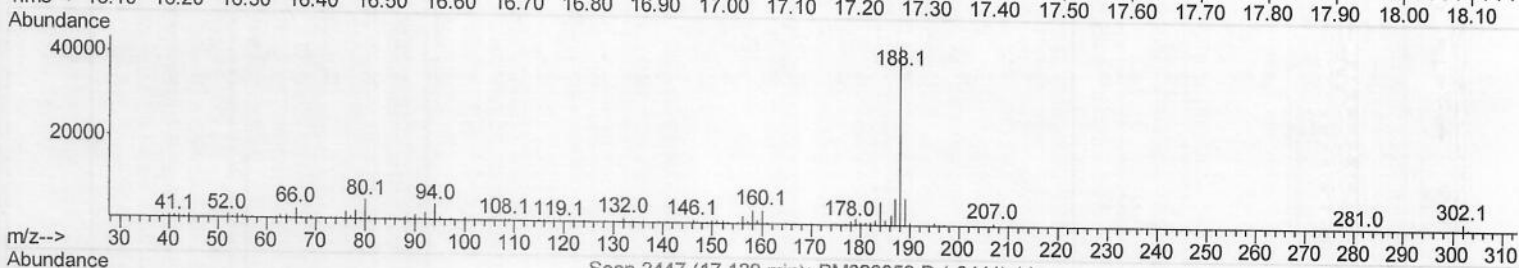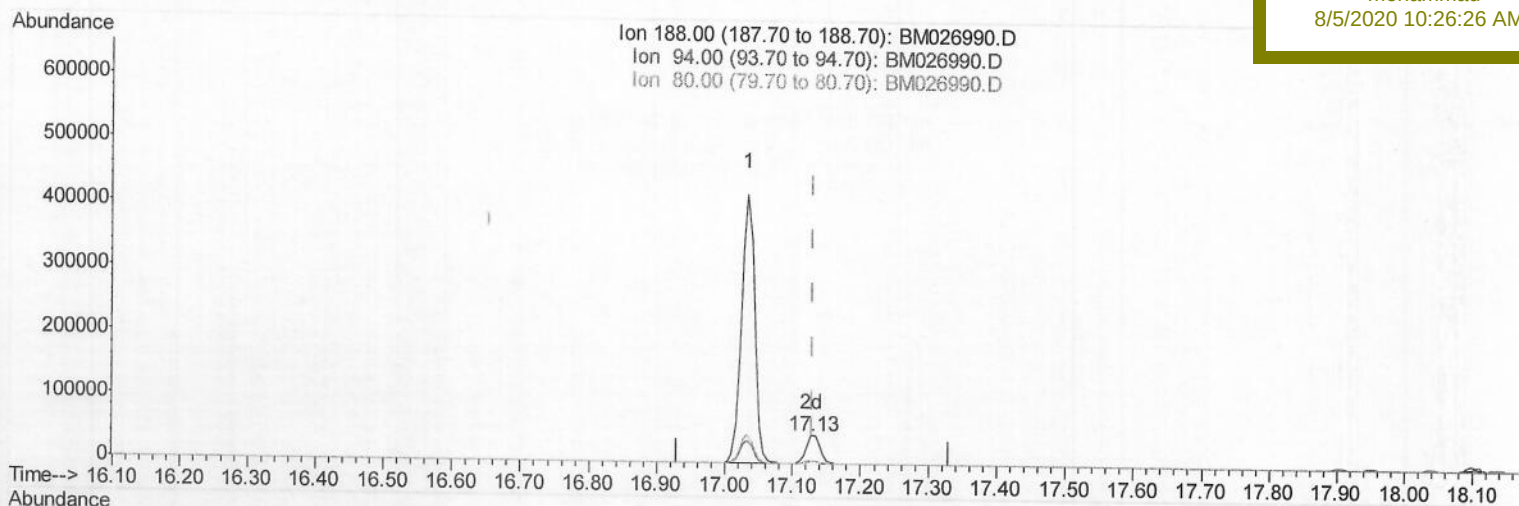

(71) Anthracene-d10 (S)

17.127min (-0.003) 2.19ng/ul m -> 08/05/2020 JU

response 62030

Ion	Exp%	Act%
188.00	100	100
94.00	9.40	8.94
80.00	9.90	11.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080320\

Data File : BM026990.D

Acq On : 03 Aug 2020 22:16

Operator : JU/CG

Sample : L3424-18DL 10X

Misc :

ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 04 02:38:36 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Aug 03 10:21:18 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


C0S93DL

Manual Integrations

APPROVED

mohammad

8/5/2020 10:26:26 AM

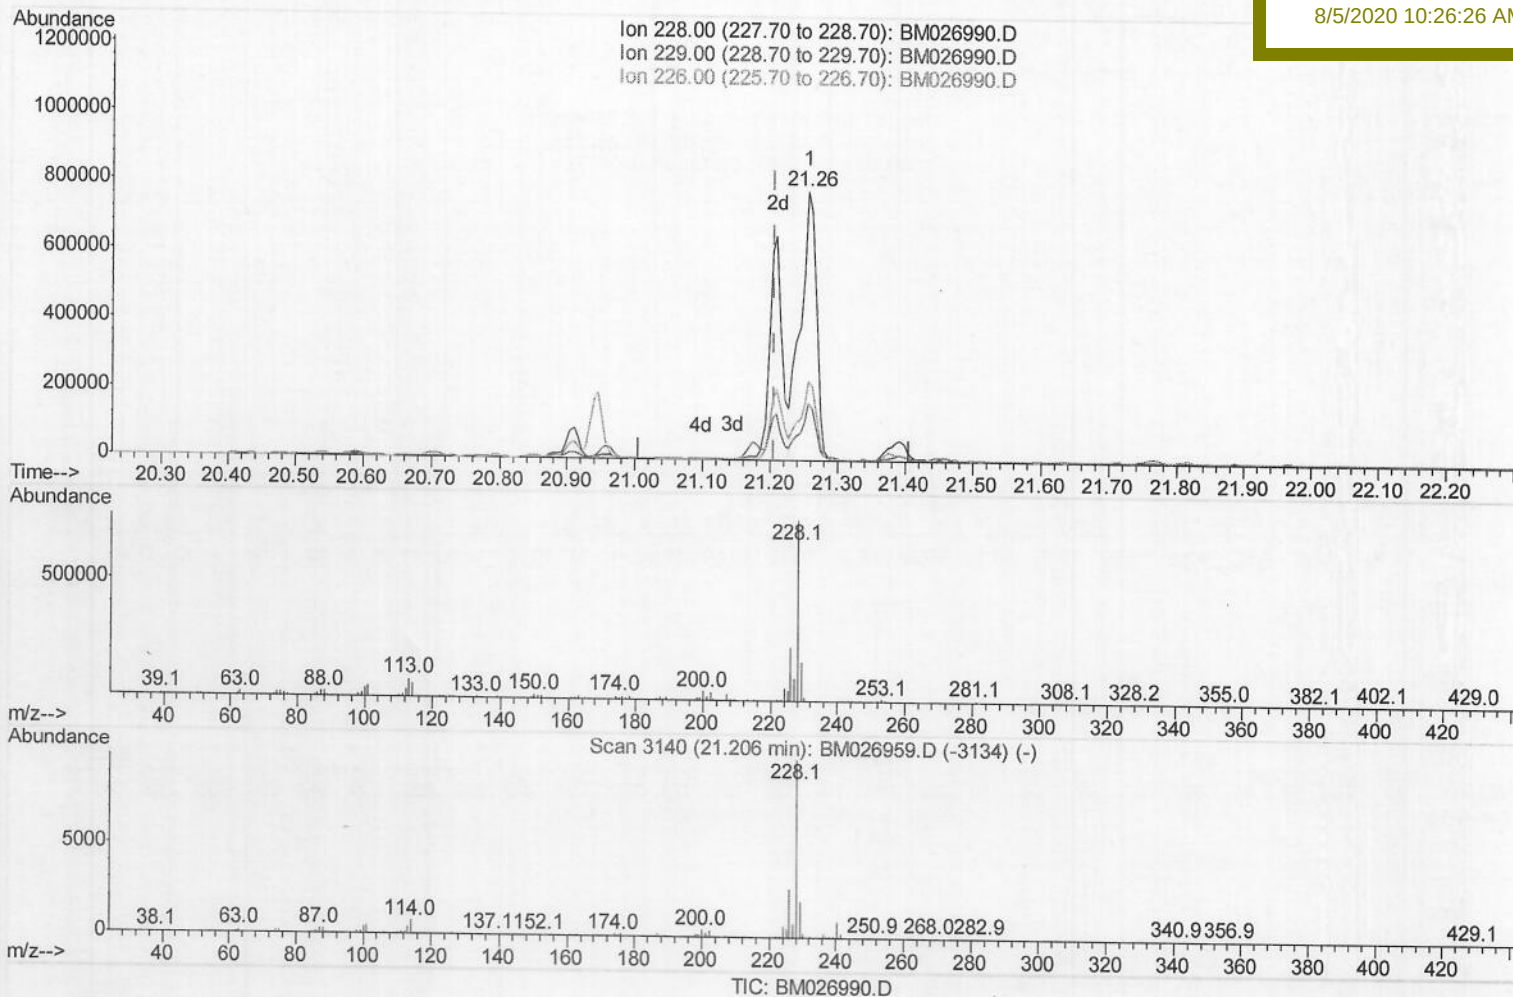

(83) Benzo(a)anthracene

21.256min (+0.050) 33.48ng/ul

response 1271108

Ion	Exp%	Act%
228.00	100	100
229.00	19.30	21.26
226.00	26.10	29.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080320\
 Data File : BM026990.D
 Acq On : 03 Aug 2020 22:16
 Operator : JU/CG
 Sample : L3424-18DL 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 04 02:38:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 03 10:21:18 2020
 Response via : Initial Calibration

Instrument :



BNA_M

Client Sampled :

C0S93DL

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:26:26 AM

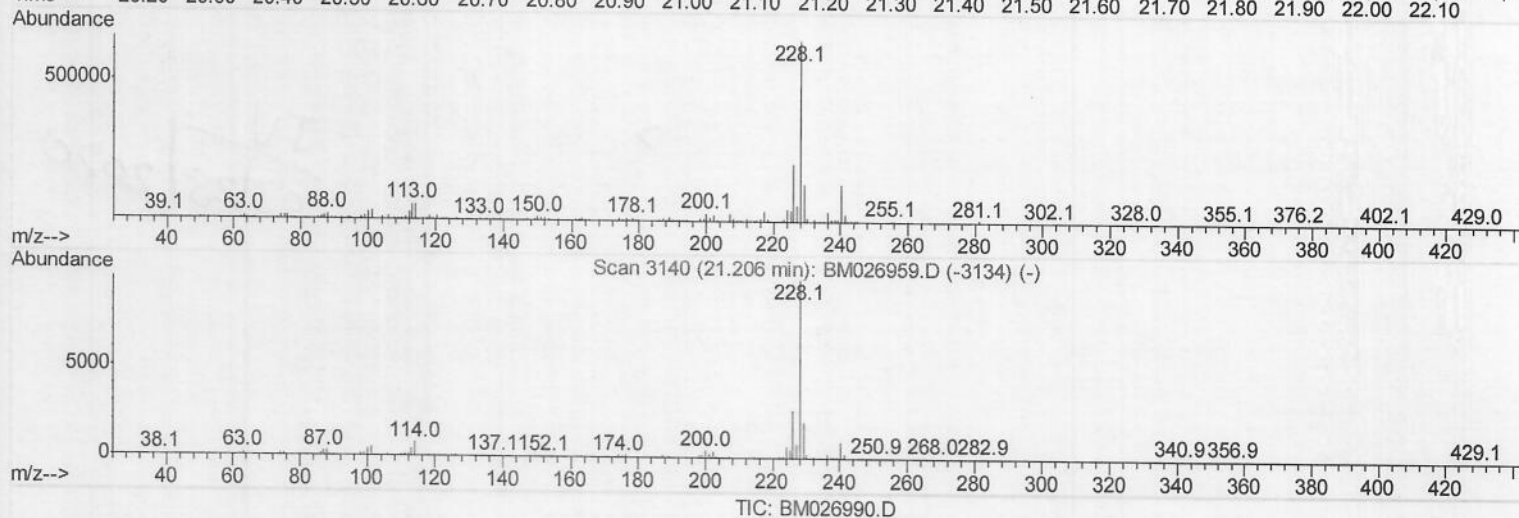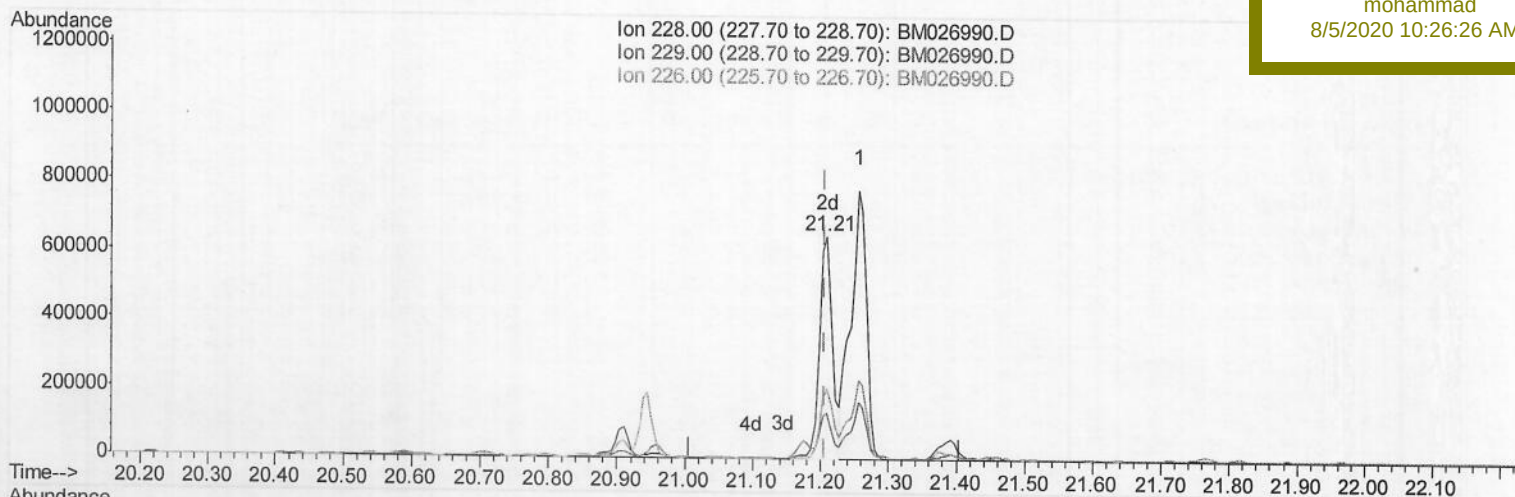

(83) Benzo(a)anthracene

21.209min (+0.003) 23.03ng/ul m -> 08/05/2020 JU

response 874492

Ion	Exp%	Act%
228.00	100	100
229.00	19.30	20.72
226.00	26.10	31.54#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080320\
 Data File : BM026990.D
 Acq On : 03 Aug 2020 22:16
 Operator : JU/CG
 Sample : L3424-18DL 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 04 04:57:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 03 10:21:18 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C0S93DL

Manual Integrations
 APPROVED

mohammad
 8/5/2020 10:26:26 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	113771	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	452929	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	271972	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	565740	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	550880	20.00	ng/ul	0.00
86) Perylene-d12	23.43	264	560846	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	840	0.34	ng/uL	0.00
5) Phenol-d5	6.84	99	19796	1.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	13907	2.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	15055	2.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	14894	1.94	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	7289	2.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	6714	2.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	14898	1.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	6488	0.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	46145	2.16	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	56700	2.09	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	5134	1.42	ng/ul	0.00
58) Fluorene-d10	15.29	176	38635	2.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	3261	1.29	ng/ul	0.00
71) Anthracene-d10	17.13	188	62030m ->	2.19	ng/ul	0.00
79) Pyrene-d10	19.43	212	64100	2.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.29	264	64511	2.04	ng/ul	0.00

Target Compounds

					Ovalue
28) Naphthalene	10.48	128	35939	1.420	ng/ul# 95
34) 2-Methylnaphthalene	12.10	142	18191	1.017	ng/ul 99
48) Acenaphthylene	14.01	152	203507	7.381	ng/ul 99
54) Dibenzofuran	14.69	168	27979	1.063	ng/ul 92
70) Phenanthrene	17.07	178	185973	5.415	ng/ul 99
72) Anthracene	17.17	178	336451	9.532	ng/ul 97
75) Carbazole	17.43	167	66193	2.121	ng/ul 96
77) Fluoranthene	19.10	202	1428853	35.239	ng/ul 99
80) Pyrene	19.46	202	1602422	39.981	ng/ul 98
83) Benzo(a)anthracene	21.21	228	874492m ->	23.031	ng/ul 98
85) Chrysene	21.26	228	1271108	34.329	ng/ul 98
88) Benzo(b)fluoranthene	22.78	252	2482838	61.884	ng/ul 99
89) Benzo(k)fluoranthene	22.82	252	697564	18.119	ng/ul 97
91) Benzo(a)pyrene	23.33	252	800861	22.121	ng/ul 98
92) Indeno(1,2,3-cd)pyrene	25.64	276	829493	18.469	ng/ul 95
93) Dibenzo(a,h)anthracene	25.64	278	222299	5.852	ng/ul# 86
94) Benzo(a,h,i)perylene	26.30	276	266748	7.183	ng/ul 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed