

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM080322\  
 Data File : BM036091.D  
 Acq On : 03 Aug 2022 23:09  
 Operator : CG/JU  
 Sample : N3930-03  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RVE-96

Quant Time: Aug 04 01:32:35 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM080122.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 01 17:50:14 2022  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-----------------------------|--------|------|----------|---------|-------|----------|
| -----                       |        |      |          |         |       |          |
| Internal Standards          |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.863  | 152  | 185231   | 20.000  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.669 | 136  | 886477   | 20.000  | ng    | 0.00     |
| 39) Acenaphthene-d10        | 14.504 | 164  | 584740   | 20.000  | ng    | 0.00     |
| 64) Phenanthrene-d10        | 17.245 | 188  | 1305105  | 20.000  | ng    | 0.00     |
| 76) Chrysene-d12            | 21.421 | 240  | 1561289  | 20.000  | ng    | 0.00     |
| 86) Perylene-d12            | 23.786 | 264  | 1658492  | 20.000  | ng    | 0.00     |
| System Monitoring Compounds |        |      |          |         |       |          |
| 5) 2-Fluorophenol           | 5.428  | 112  | 1429959  | 125.159 | ng    | 0.00     |
| 7) Phenol-d6                | 7.034  | 99   | 1964425  | 135.127 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 9.028  | 82   | 1162496  | 73.406  | ng    | -0.01    |
| 42) 2,4,6-Tribromophenol    | 15.992 | 330  | 936653   | 136.543 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 13.133 | 172  | 2839853  | 71.707  | ng    | 0.00     |
| 79) Terphenyl-d14           | 19.868 | 244  | 5455582  | 68.923  | ng    | 0.00     |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM080322\  
Data File : BM036091.D  
Acq On : 03 Aug 2022 23:09  
Operator : CG/JU  
Sample : N3930-03  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
RVE-96

Quant Time: Aug 04 01:32:35 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM080122.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 01 17:50:14 2022  
Response via : Initial Calibration




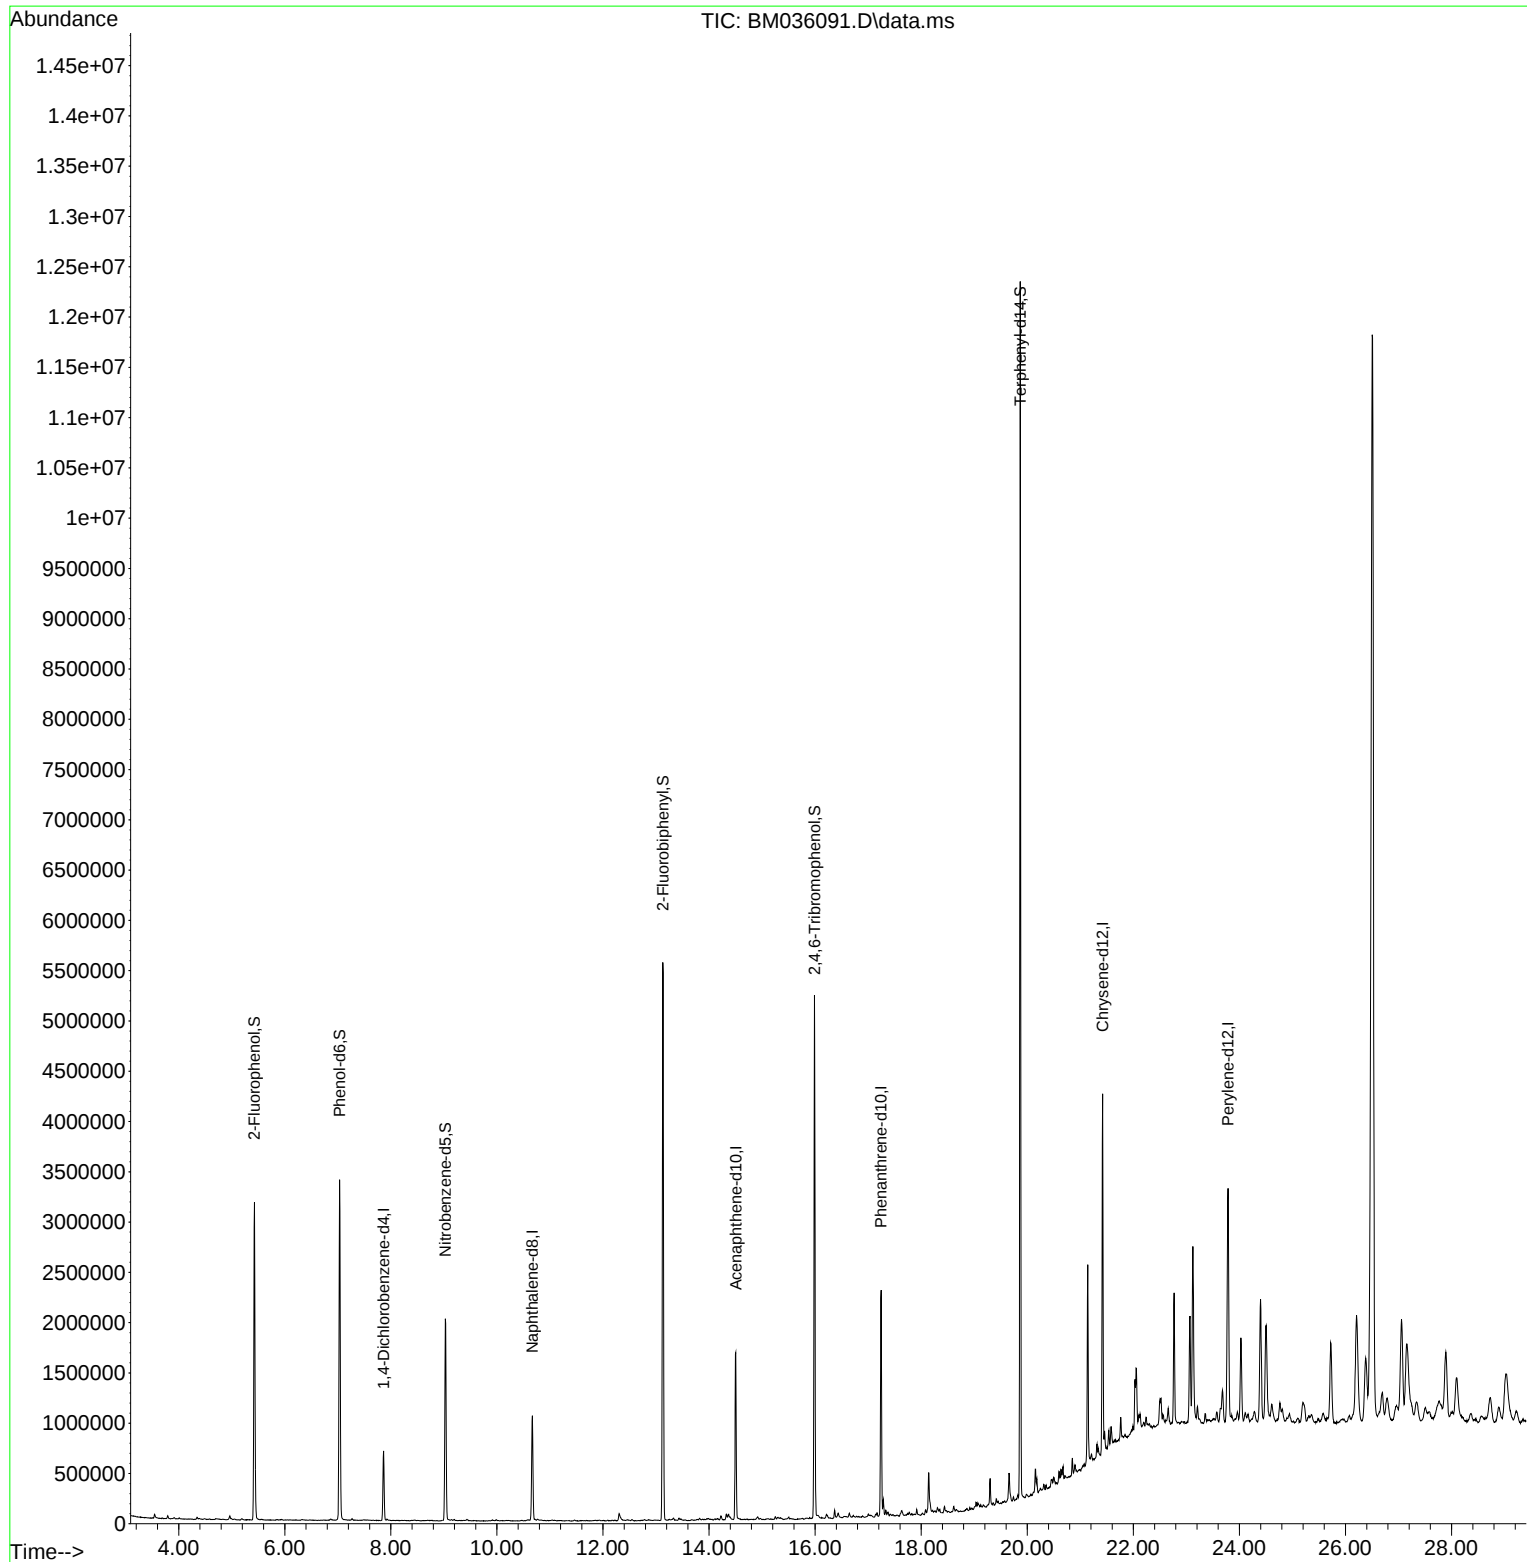


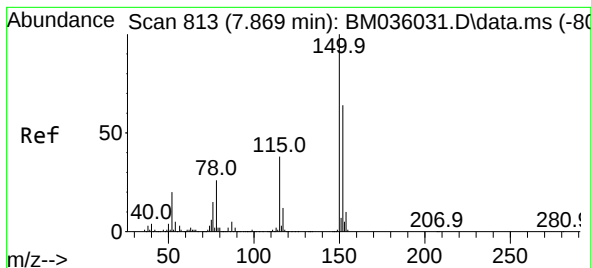

#1  
1,4-Dichlorobenzene-d4  
Concen: 20.000 ng  
RT: 7.863 min Scan# 813  
Delta R.T. -0.006 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09




Instrument :  
BNA\_M  
ClientSampleId :  
RVE-96


Tgt Ion:152 Resp: 185231  
Ion Ratio Lower Upper  
152 100  
150 156.4 124.9 187.3  
115 57.9 47.9 71.9

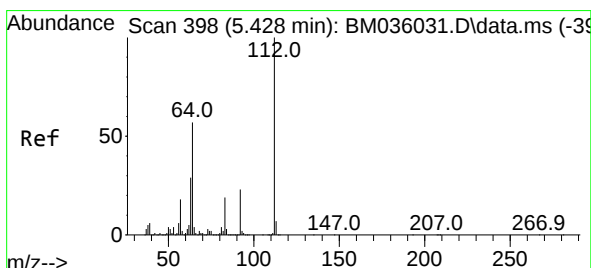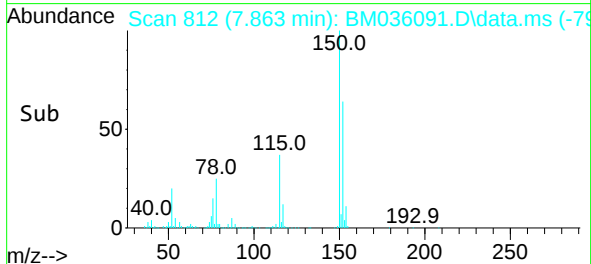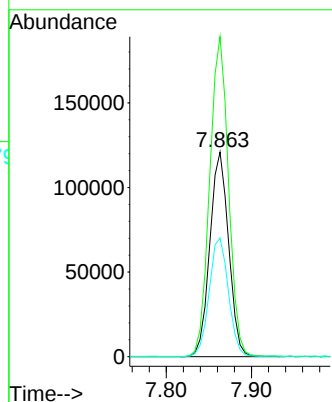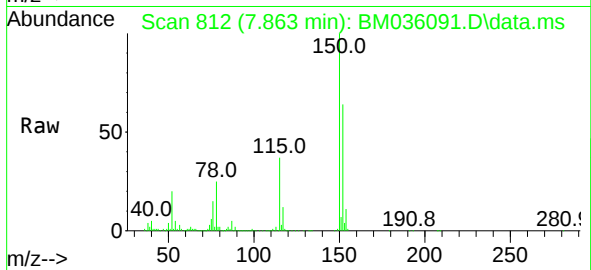

#5  
2-Fluorophenol  
Concen: 125.159 ng  
RT: 5.428 min Scan# 398  
Delta R.T. -0.000 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09

Tgt Ion:112 Resp: 1429959  
Ion Ratio Lower Upper  
112 100  
64 54.2 47.8 71.6  
63 28.3 26.6 40.0

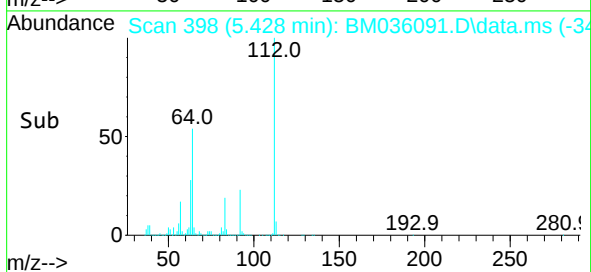
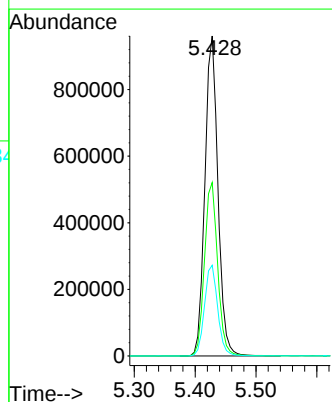
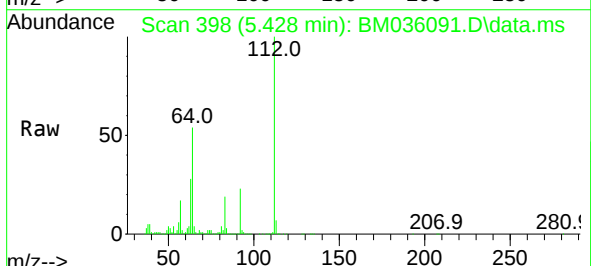


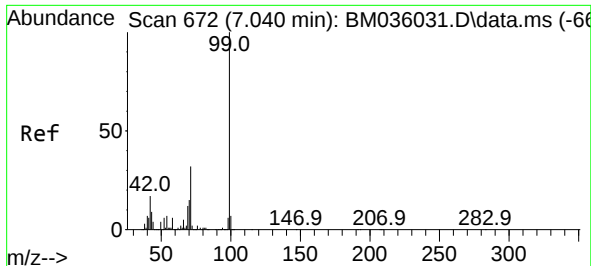

#7  
Phenol-d6  
Concen: 135.127 ng  
RT: 7.034 min Scan# 61  
Delta R.T. -0.006 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09




Instrument :  
BNA\_M  
ClientSampleId :  
RVE-96


Tgt Ion: 99 Resp: 1964425  
Ion Ratio Lower Upper  
99 100  
42 17.1 18.8 28.2#  
71 31.8 30.2 45.2

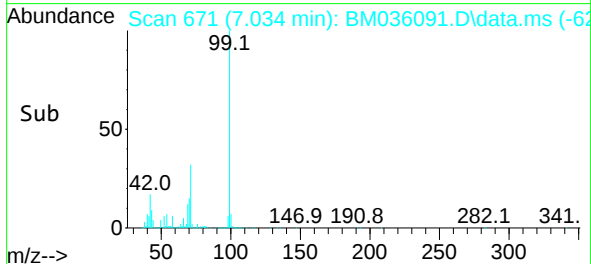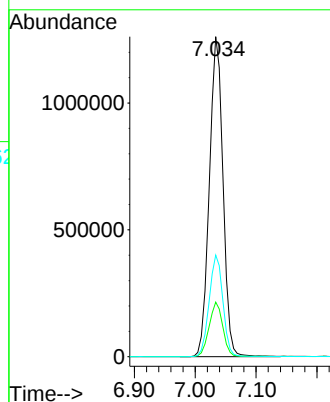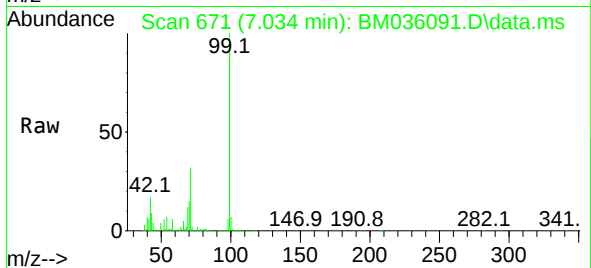

#21  
Naphthalene-d8  
Concen: 20.000 ng  
RT: 10.669 min Scan# 1289  
Delta R.T. -0.006 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09

Tgt Ion: 136 Resp: 886477  
Ion Ratio Lower Upper  
136 100  
137 11.3 8.9 13.3  
54 7.2 7.0 10.4  
68 5.7 4.3 6.5


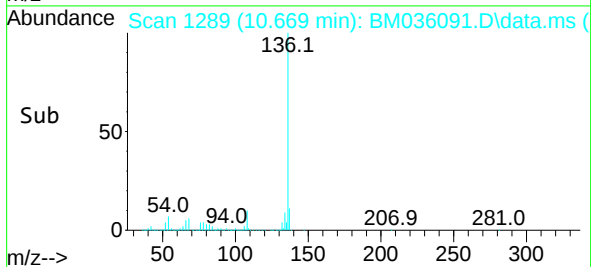
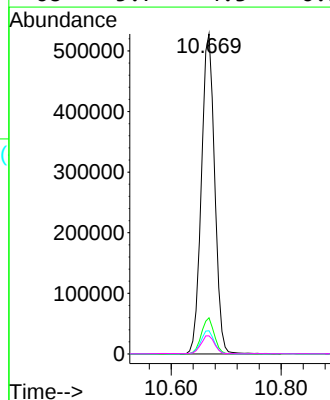
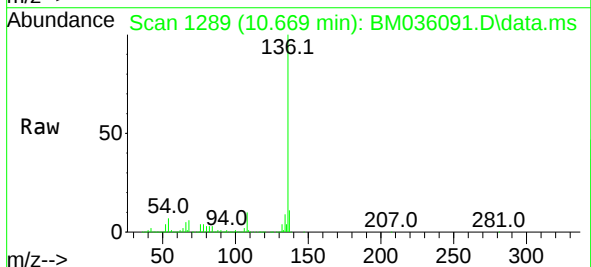


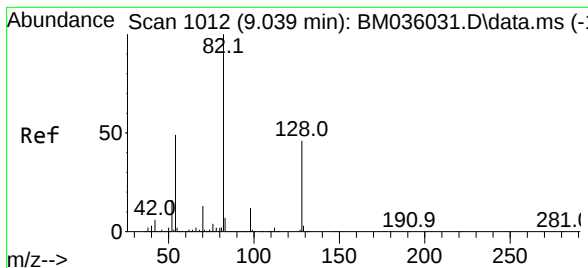

#23  
Nitrobenzene-d5  
Concen: 73.406 ng  
RT: 9.028 min Scan# 1012  
Delta R.T. -0.012 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09




Instrument :  
BNA\_M  
ClientSampleId :  
RVE-96

Tgt Ion: 82 Resp: 1162496  
Ion Ratio Lower Upper  
82 100  
128 45.8 33.7 50.5  
54 48.4 43.2 64.8

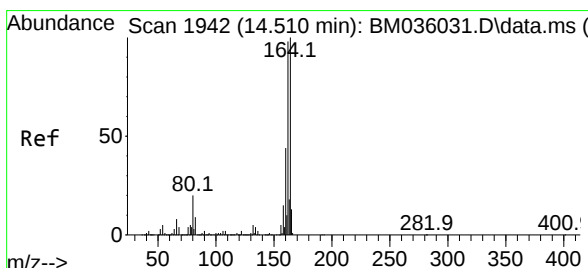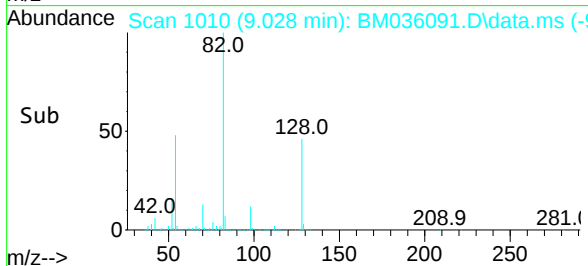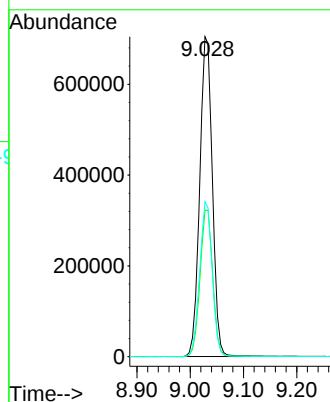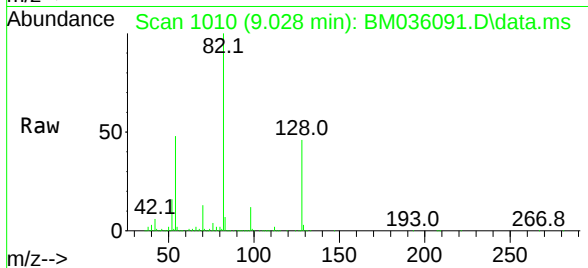

#39  
Acenaphthene-d10  
Concen: 20.000 ng  
RT: 14.504 min Scan# 1941  
Delta R.T. -0.006 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09

Tgt Ion:164 Resp: 584740  
Ion Ratio Lower Upper  
164 100  
162 99.9 83.0 124.6  
160 44.5 37.0 55.4


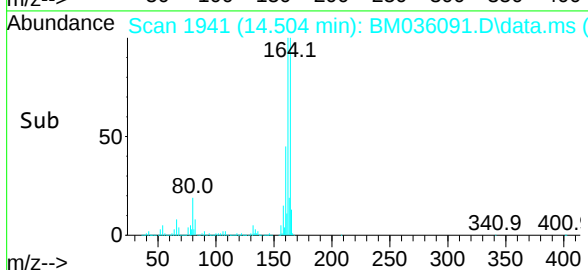
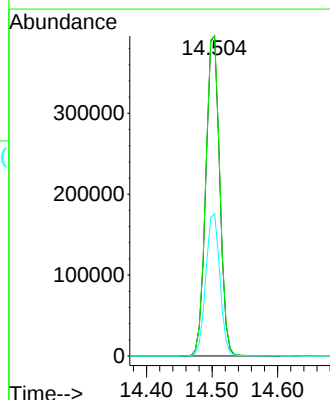
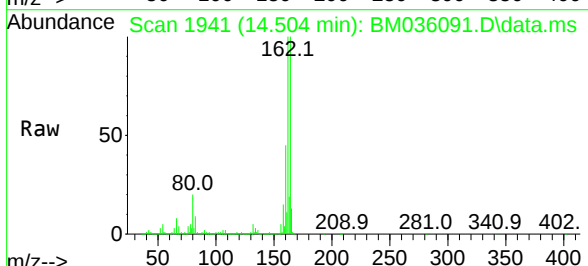




#42  
2,4,6-Tribromophenol  
Concen: 136.543 ng  
RT: 15.992 min Scan# 2195  
Delta R.T. -0.006 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09




Instrument :  
BNA\_M  
ClientSampleId :  
RVE-96


Tgt Ion:330 Resp: 936653  
Ion Ratio Lower Upper  
330 100  
332 96.7 77.0 115.4  
141 36.8 35.3 52.9

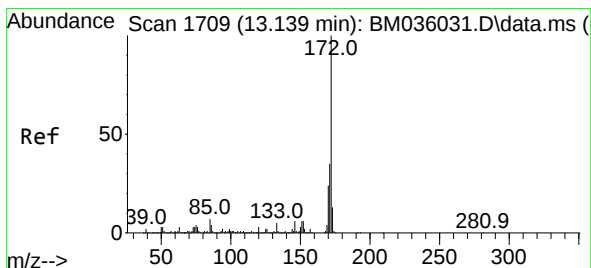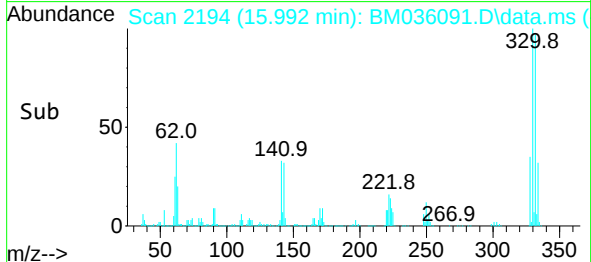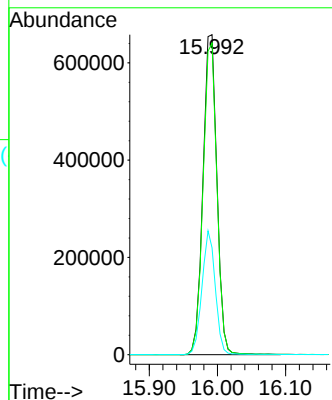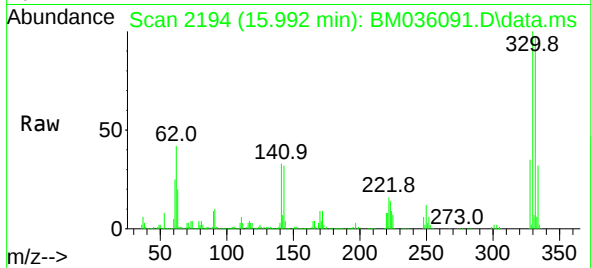

#45  
2-Fluorobiphenyl  
Concen: 71.707 ng  
RT: 13.133 min Scan# 1708  
Delta R.T. -0.006 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09

Tgt Ion:172 Resp: 2839853  
Ion Ratio Lower Upper  
172 100  
171 34.7 28.5 42.7  
170 23.8 18.7 28.1


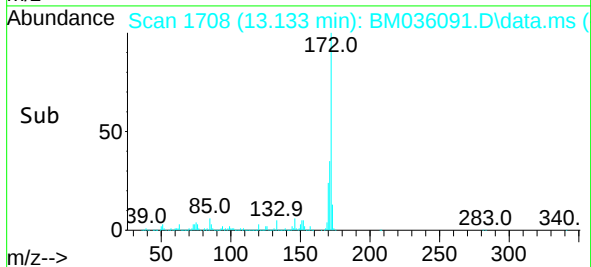
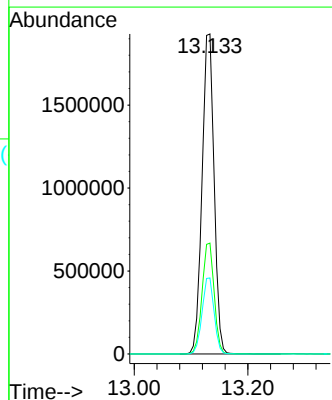
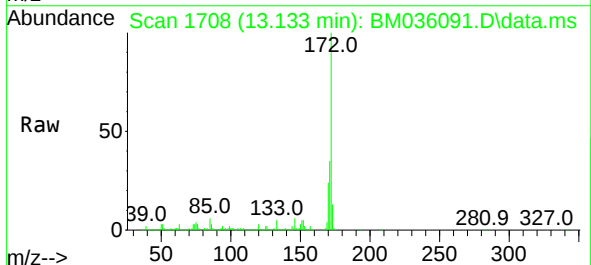


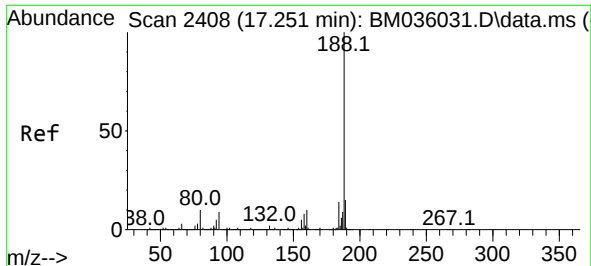

#64  
Phenanthrene-d10  
Concen: 20.000 ng  
RT: 17.245 min Scan# 2408  
Delta R.T. -0.006 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09




Instrument :  
BNA\_M  
ClientSampleId :  
RVE-96


Tgt Ion:188 Resp: 1305105  
Ion Ratio Lower Upper  
188 100  
94 9.3 7.0 10.4  
80 9.8 7.6 11.4

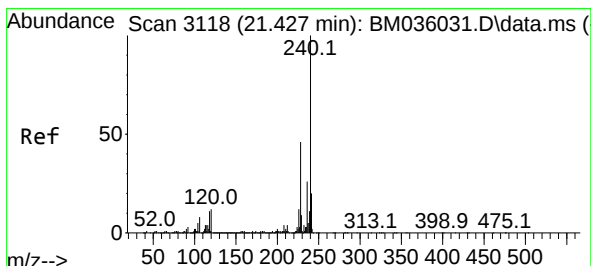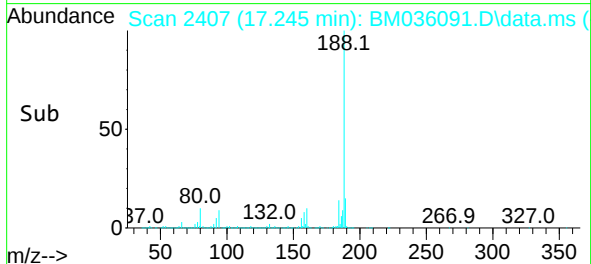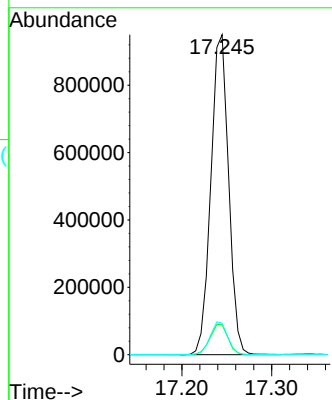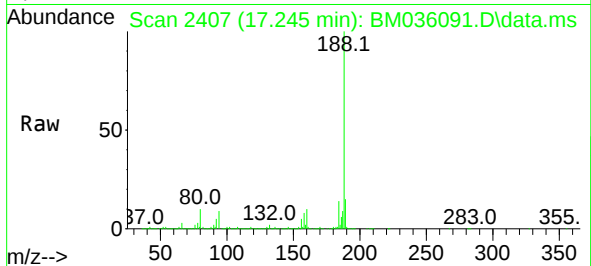

#76  
Chrysene-d12  
Concen: 20.000 ng  
RT: 21.421 min Scan# 3117  
Delta R.T. -0.006 min  
Lab File: BM036091.D  
Acq: 03 Aug 2022 23:09

Tgt Ion:240 Resp: 1561289  
Ion Ratio Lower Upper  
240 100  
120 11.4 9.4 14.0  
236 26.2 20.6 30.8


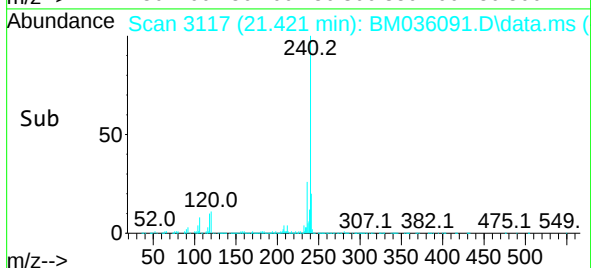
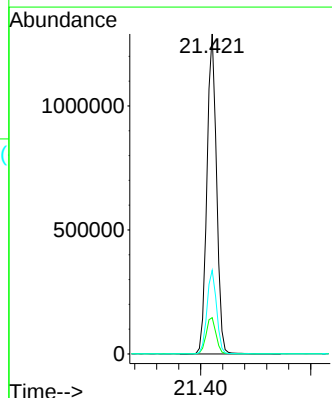
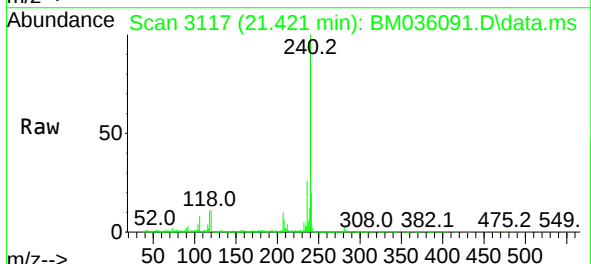


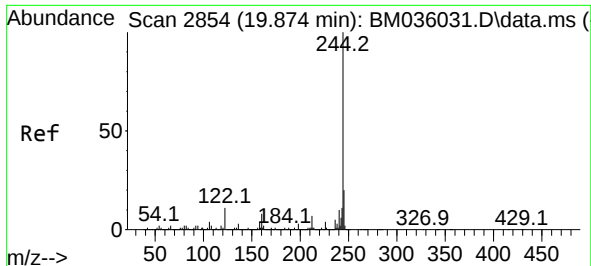

#79  
 Terphenyl-d14  
 Concen: 68.923 ng  
 RT: 19.868 min Scan# 21  
 Delta R.T. -0.006 min  
 Lab File: BM036091.D  
 Acq: 03 Aug 2022 23:09

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RVE-96

Tgt Ion:244 Resp: 5455582  
 Ion Ratio Lower Upper  
 244 100  
 212 7.2 6.2 9.4  
 122 11.2 8.3 12.5

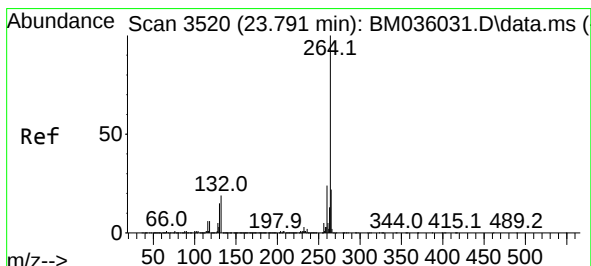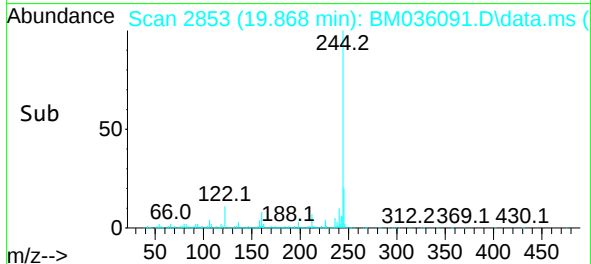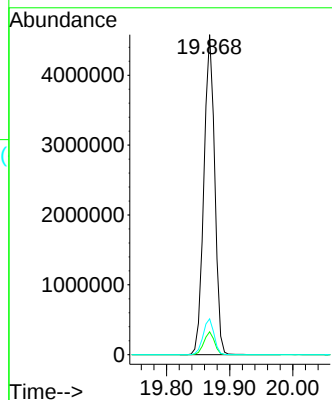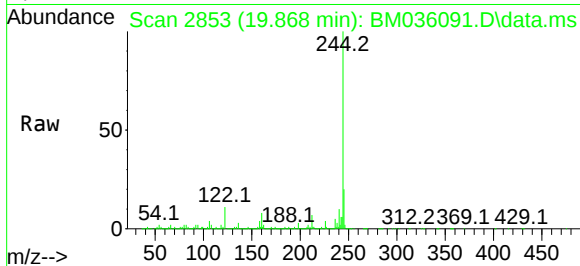

#86  
 Perylene-d12  
 Concen: 20.000 ng  
 RT: 23.786 min Scan# 3519  
 Delta R.T. -0.006 min  
 Lab File: BM036091.D  
 Acq: 03 Aug 2022 23:09

Tgt Ion:264 Resp: 1658492  
 Ion Ratio Lower Upper  
 264 100  
 260 24.0 18.9 28.3  
 265 22.3 17.5 26.3

