

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
 Data File : BM036080.D
 Acq On : 03 Aug 2022 16:24
 Operator : CG/JU
 Sample : N3947-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 NSB06-14-15

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	391	398	414	rBV	3200751	4793956	32.20%	7.320%
2	7.034	659	671	683	rBV	3412070	5358421	35.99%	8.182%
3	7.863	805	812	820	rBV	709411	1090258	7.32%	1.665%
4	9.034	1002	1011	1019	rBV	2021926	3266636	21.94%	4.988%
5	10.669	1281	1289	1298	rBV	1030932	1708830	11.48%	2.609%
6	13.133	1700	1708	1722	rBV	5703497	8254663	55.44%	12.604%
7	14.504	1934	1941	1947	rBV	1811715	2585608	17.37%	3.948%
8	15.986	2187	2193	2212	rBV	5472344	7957869	53.45%	12.151%
9	17.245	2400	2407	2416	rBV	2392055	3361859	22.58%	5.133%
10	17.921	2517	2522	2526	rBV	135713	172511	1.16%	0.263%
11	18.145	2554	2560	2570	rBV	646595	1014584	6.81%	1.549%
12	19.421	2773	2777	2784	rBV	236375	338313	2.27%	0.517%
13	19.868	2848	2853	2859	rBV	11916648	14889757	100.00%	22.735%
14	21.145	3065	3070	3078	rBV	1117515	1615732	10.85%	2.467%
15	21.427	3113	3118	3124	rBV	3576764	4256893	28.59%	6.500%
16	23.791	3514	3520	3531	rVB2	2407212	4825813	32.41%	7.369%




Sum of corrected areas: 65491703

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
Data File : BM036080.D
Acq On : 03 Aug 2022 16:24
Operator : CG/JU
Sample : N3947-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
NSB06-14-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

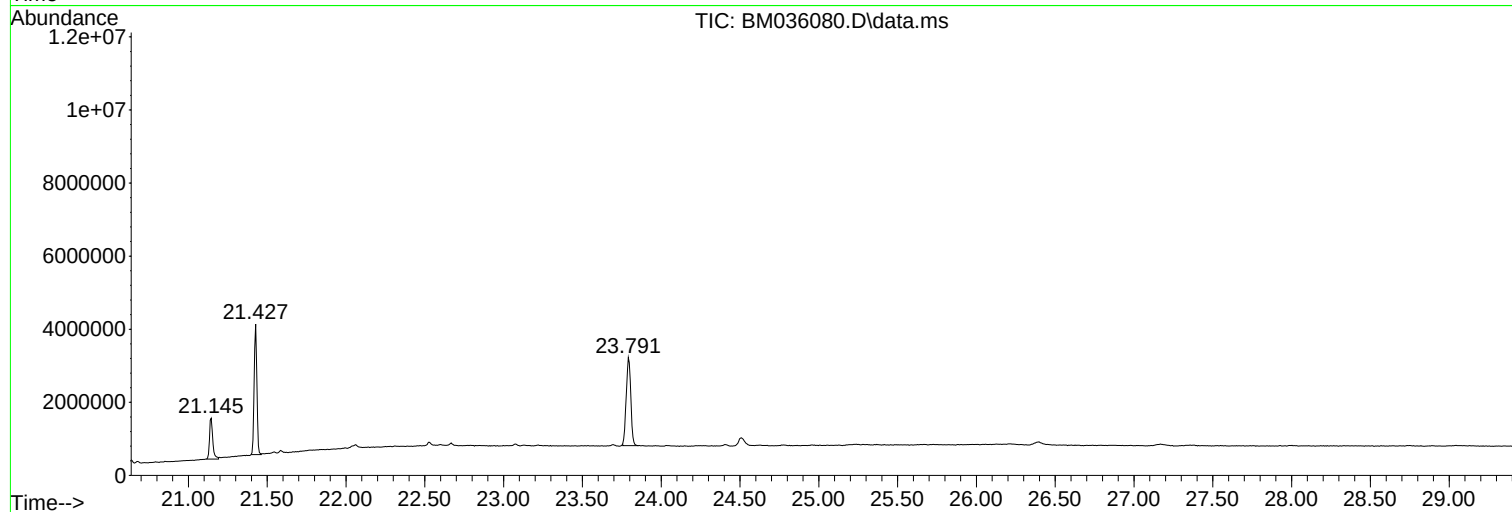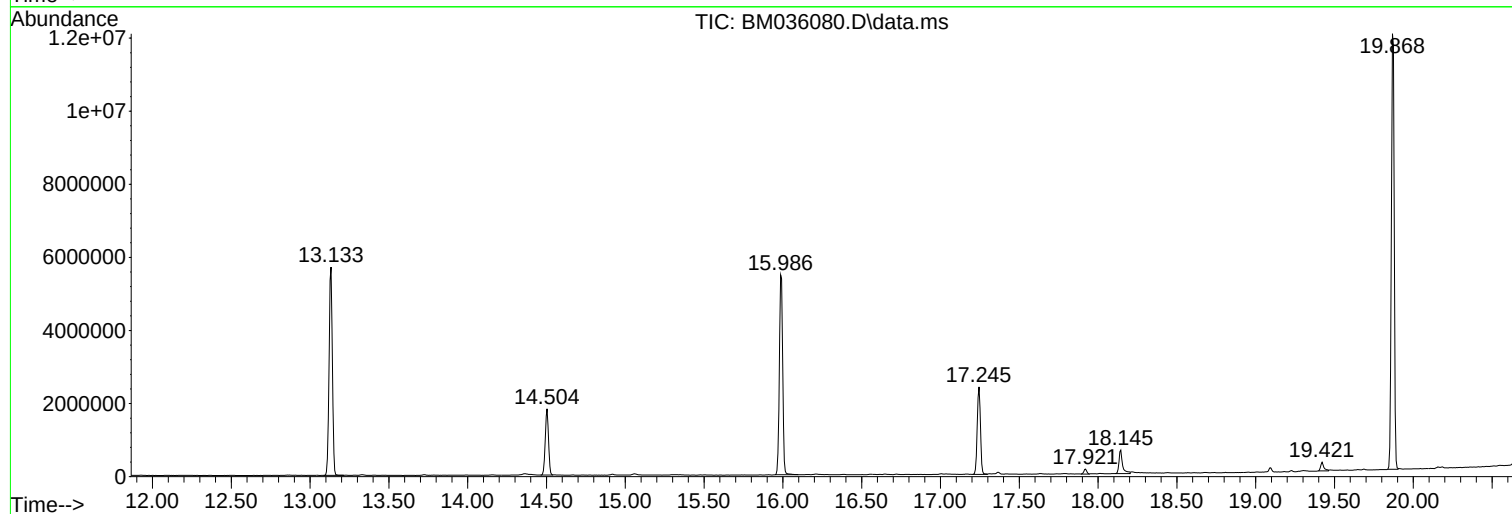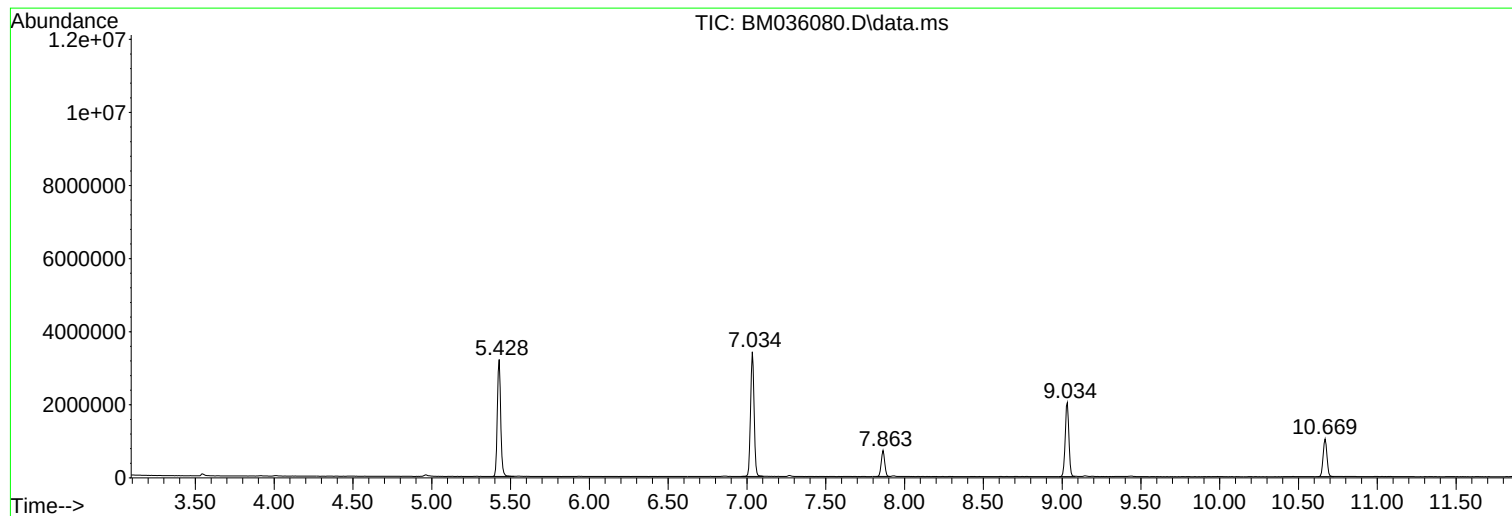

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
Data File : BM036080.D
Acq On : 03 Aug 2022 16:24
Operator : CG/JU
Sample : N3947-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
NSB06-14-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
Data File : BM036080.D
Acq On : 03 Aug 2022 16:24
Operator : CG/JU
Sample : N3947-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
NSB06-14-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------