

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
 Data File : BM036091.D
 Acq On : 03 Aug 2022 23:09
 Operator : CG/JU
 Sample : N3930-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RVE-96

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	391	398	411	rBV	3157774	4711141	13.43%	3.908%
2	7.034	659	671	685	rBV	3386552	5370240	15.31%	4.455%
3	7.863	804	812	820	rBV	692260	1079490	3.08%	0.896%
4	9.028	1002	1010	1021	rBV	2007664	3335454	9.51%	2.767%
5	10.669	1281	1289	1295	rBV	1038545	1737176	4.95%	1.441%
6	13.127	1700	1707	1719	rBV	5548584	8147900	23.22%	6.759%
7	14.504	1933	1941	1947	rBV	1658973	2506575	7.14%	2.079%
8	15.986	2184	2193	2201	rBV	5203358	7291974	20.78%	6.049%
9	17.245	2401	2407	2411	rBV	2242280	3097585	8.83%	2.570%
10	18.139	2552	2559	2569	rBV2	396616	711527	2.03%	0.590%
11	19.656	2813	2817	2827	rVB	279826	471688	1.34%	0.391%
12	19.868	2847	2853	2858	rBV	12090340	14349926	40.90%	11.904%
13	21.139	3064	3069	3077	rBV2	1949637	2490884	7.10%	2.066%
14	21.421	3111	3117	3121	rBV	3590171	4638732	13.22%	3.848%
15	22.033	3217	3221	3222	rBV2	503843	614202	1.75%	0.510%
16	22.768	3341	3346	3356	rVB	1294916	1859273	5.30%	1.542%
17	23.068	3392	3397	3401	rBV	999587	1609958	4.59%	1.336%
18	23.121	3401	3406	3417	rVB	1707557	3256519	9.28%	2.702%
19	23.786	3512	3519	3527	rVB2	2271920	4450410	12.68%	3.692%
20	24.027	3556	3560	3568	rVB	828490	1490191	4.25%	1.236%
21	24.397	3617	3623	3632	rVB	1185302	2484647	7.08%	2.061%
22	24.503	3635	3641	3652	rVB2	904842	2218927	6.32%	1.841%
23	25.721	3844	3848	3858	rVB2	796268	1909475	5.44%	1.584%
24	26.209	3925	3931	3948	rVB3	1050186	3396704	9.68%	2.818%
25	26.503	3969	3981	3998	rVB	10758483	35084169	100.00%	29.105%
26	27.056	4069	4075	4083	rVB4	847763	2227957	6.35%	1.848%




Sum of corrected areas: 120542724

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
Data File : BM036091.D
Acq On : 03 Aug 2022 23:09
Operator : CG/JU
Sample : N3930-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RVE-96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

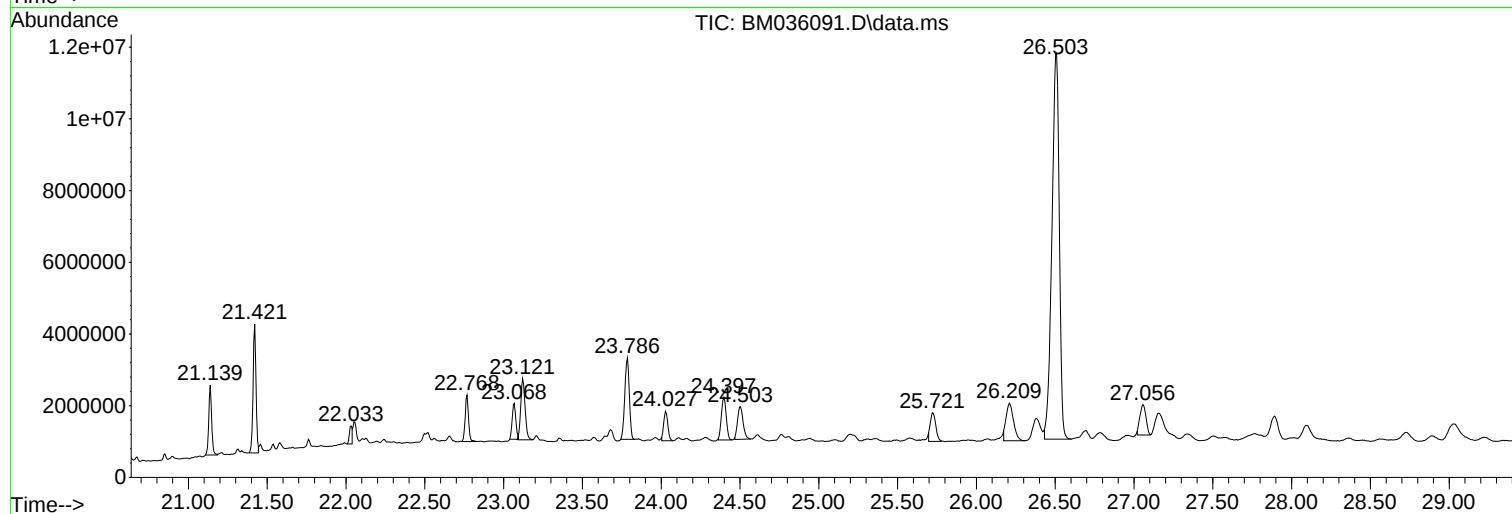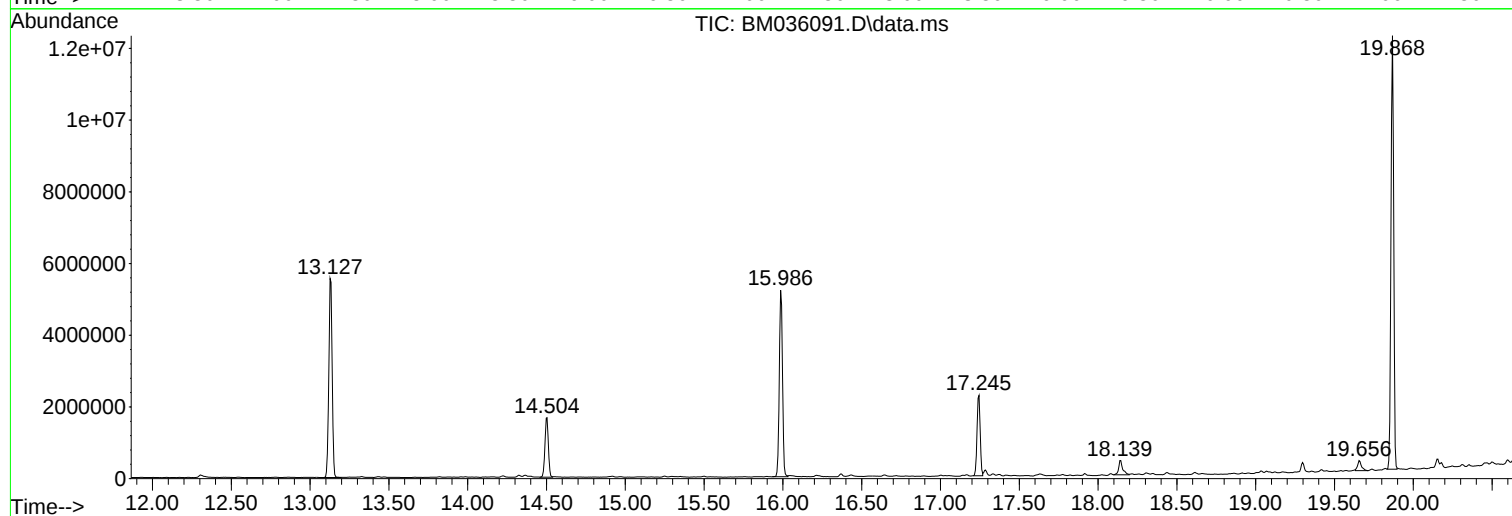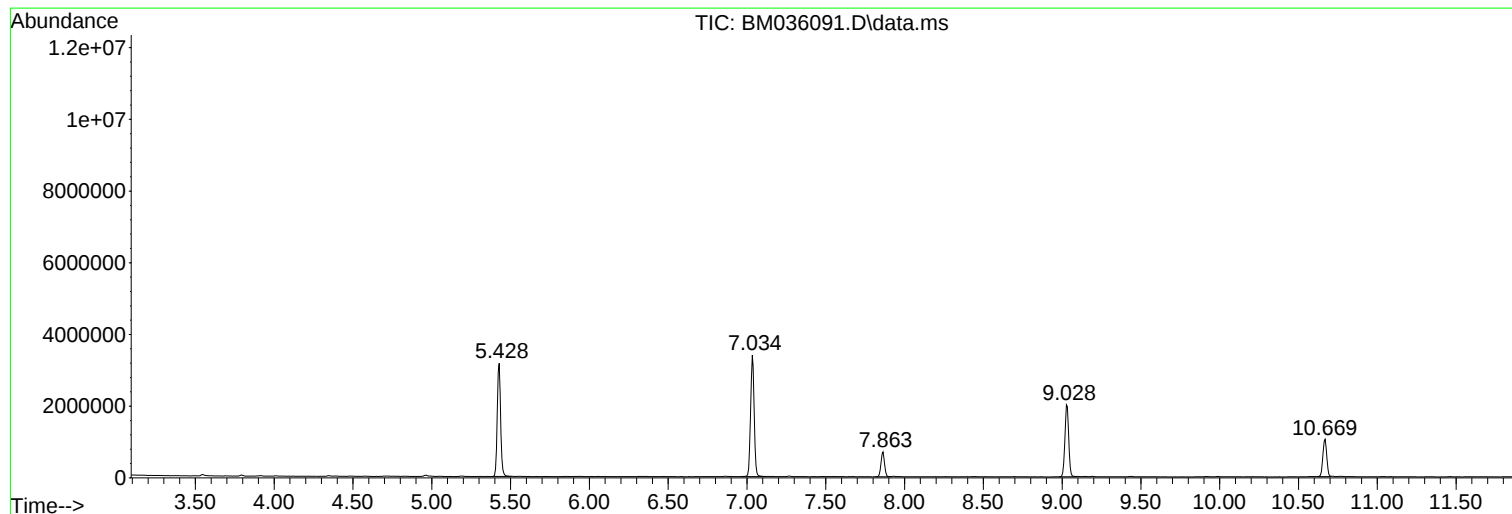

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
Data File : BM036091.D
Acq On : 03 Aug 2022 23:09
Operator : CG/JU
Sample : N3930-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RVE-96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
Data File : BM036091.D
Acq On : 03 Aug 2022 23:09
Operator : CG/JU
Sample : N3930-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RVE-96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc