


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
 Data File : BM036072.D
 Acq On : 03 Aug 2022 11:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 17:50:14 2022

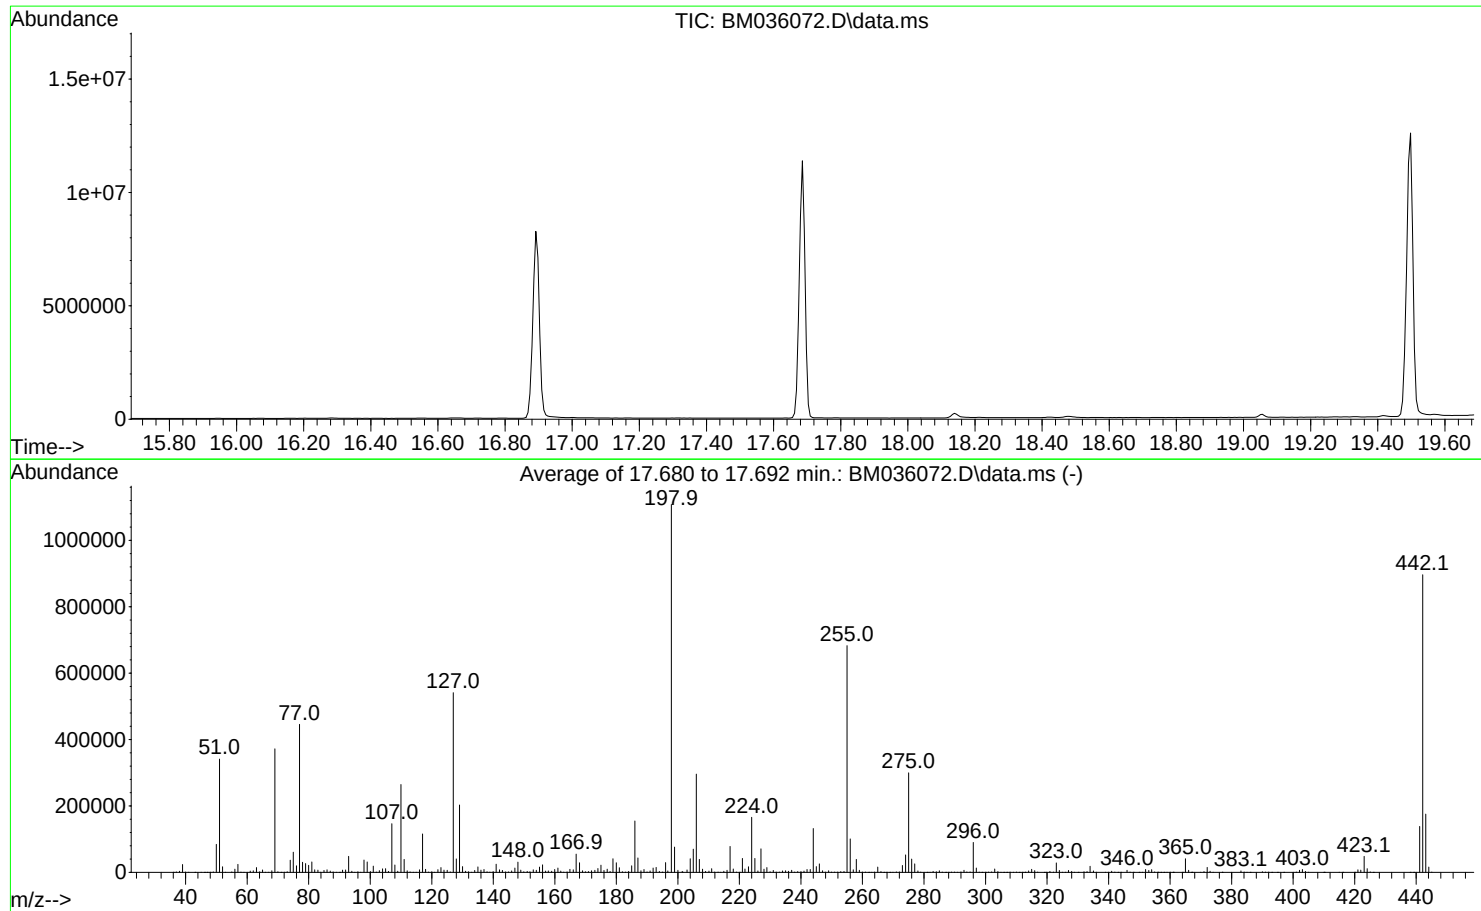




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	341446	PASS
68	69	0.00	2	1.3	4985	PASS
69	198	0.00	100	33.6	372186	PASS
70	69	0.00	2	0.5	1954	PASS
127	198	10	80	48.9	541355	PASS
197	198	0.00	2	0.4	4305	PASS
198	198	100	100	100.0	1107989	PASS
199	198	5	9	6.9	76237	PASS
275	198	10	60	27.1	299968	PASS
365	198	1	100	3.7	41149	PASS
441	198	0.01	100	12.5	138285	PASS
442	442	50	100	100.0	896448	PASS
443	442	15	24	19.6	175531	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
Data File : BM036072.D
Acq On : 03 Aug 2022 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 04 04:30:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 17:50:14 2022
Response via : Initial Calibration

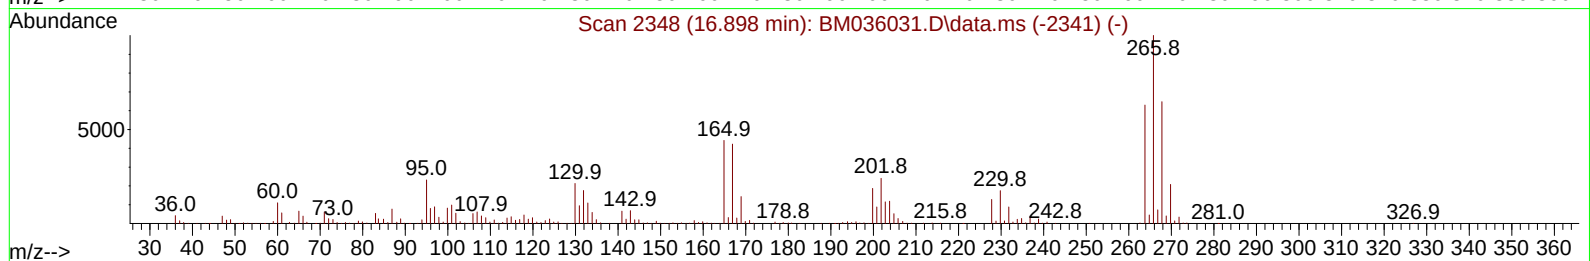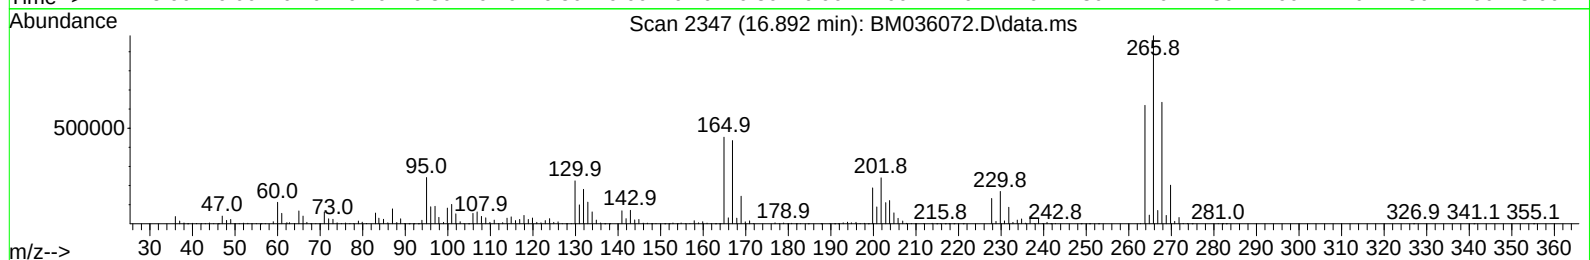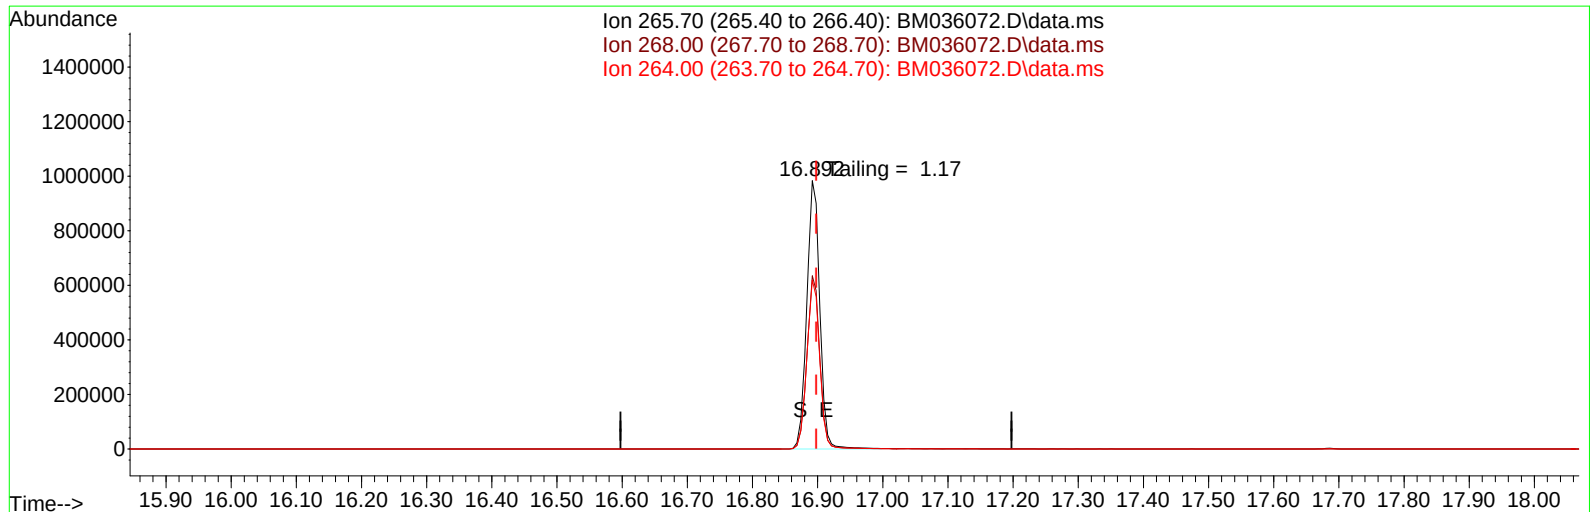

TIC: BM036072.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.006) 286309.78 ng




response 1366365

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.58
264.00	63.30	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080322\
Data File : BM036072.D
Acq On : 03 Aug 2022 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 04 04:30:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 17:50:14 2022
Response via : Initial Calibration

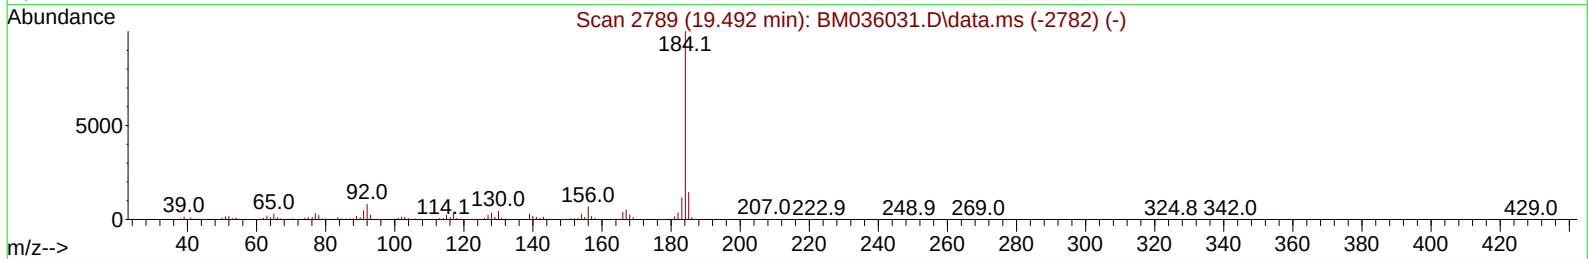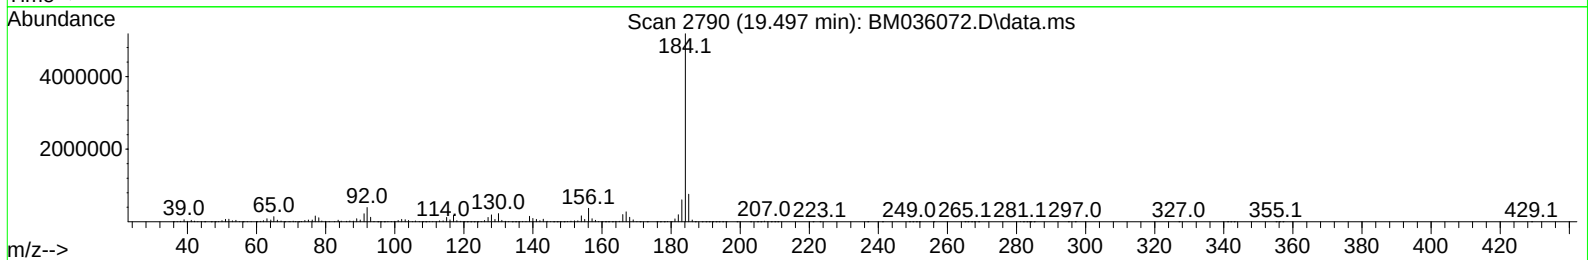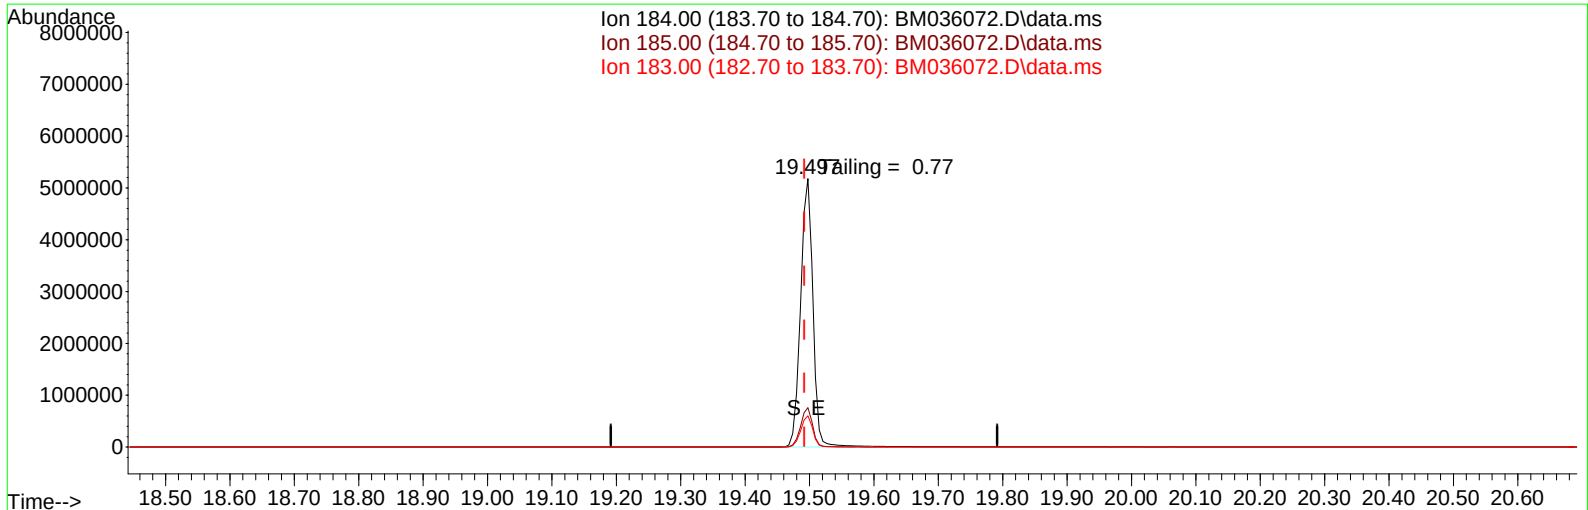

TIC: BM036072.D\data.ms

(77) Benzidine

19.497min (+ 0.006) 245875.57 ng

response 6906515

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.66
183.00	11.90	11.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2022	BNA_M	<u>BM036072.D</u>
Compound Name	Response	Retention Time
DDT	3942565	20.727
DDD	24678	20.333
DDE	1184	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25862	3968427	0.65

Instrument :
BNA_M
ClientSampleId :
DFTPP