




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046980.D
 Acq On : 04 Aug 2024 01:30
 Operator : MA/JU
 Sample : P3276-21
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J8

Manual IntegrationsAPPROVED

Quant Time: Aug 05 00:59:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 03 02:51:11 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
 Supervised By :mohammad ahmed 08/05/2024

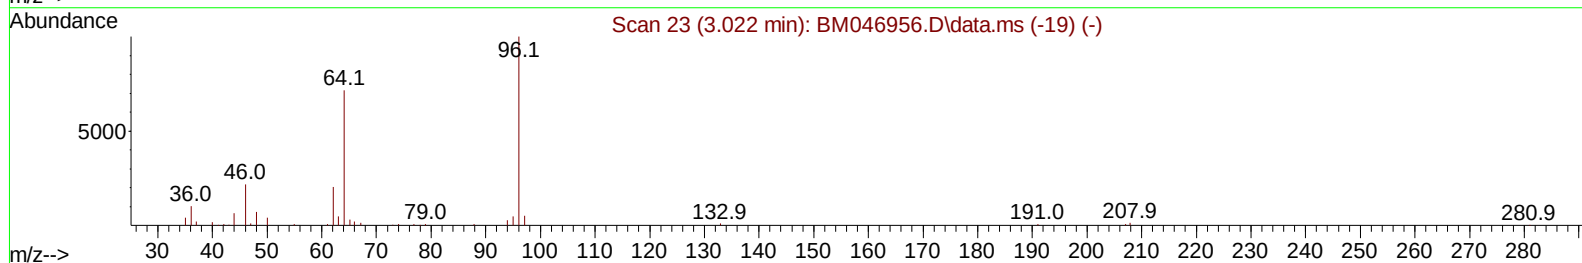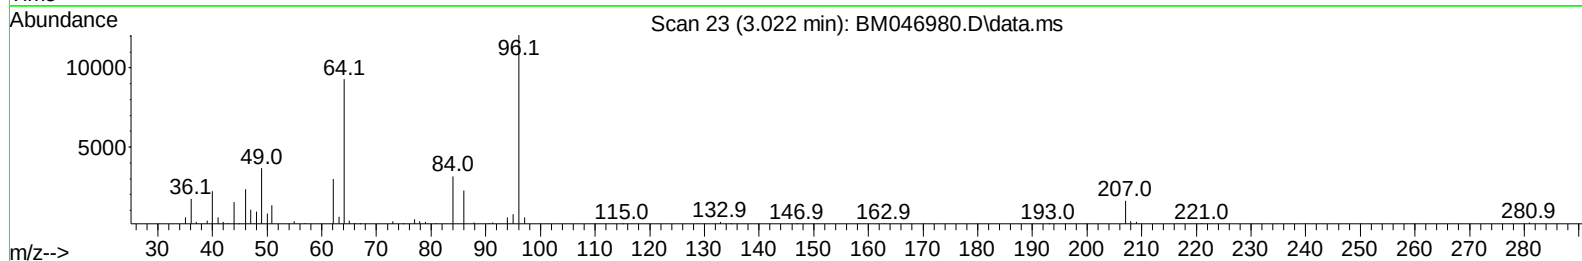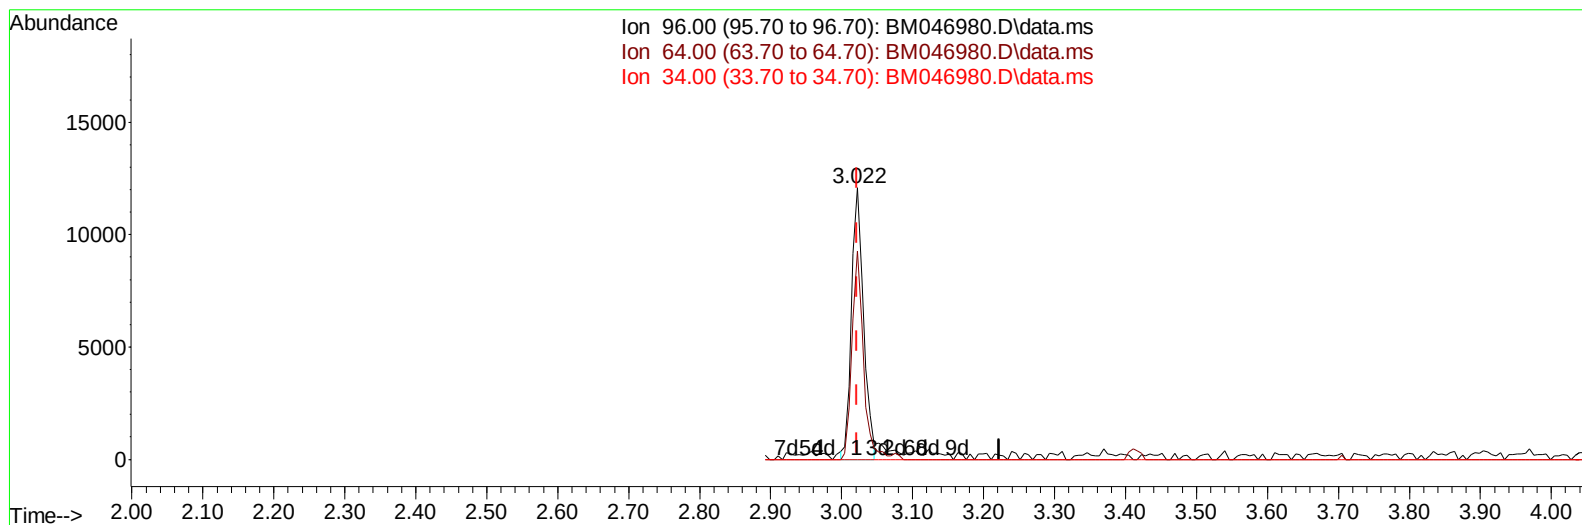

TIC: BM046980.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.022min (+ 0.000) 3.04 ng/uL

response 14028

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	81.60	76.77
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046980.D
Acq On : 04 Aug 2024 01:30
Operator : MA/JU
Sample : P3276-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J8

Manual IntegrationsAPPROVED

Quant Time: Aug 05 00:59:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 03 02:51:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
Supervised By :mohammad ahmed 08/05/2024

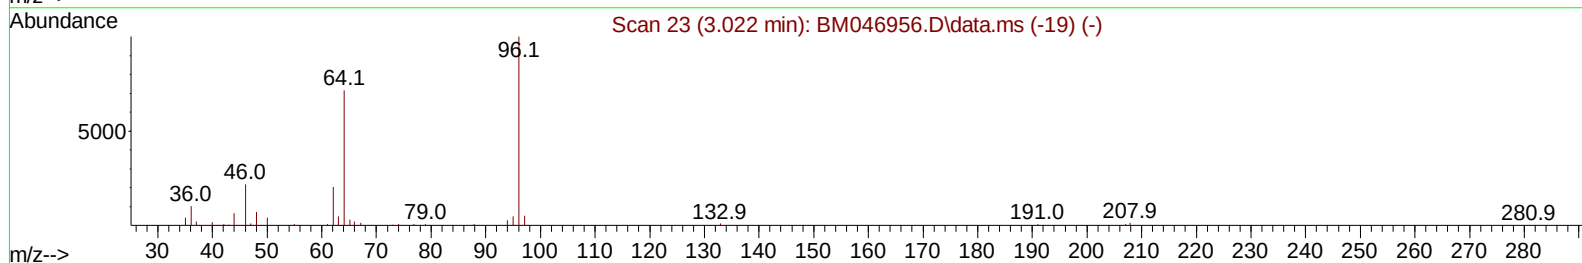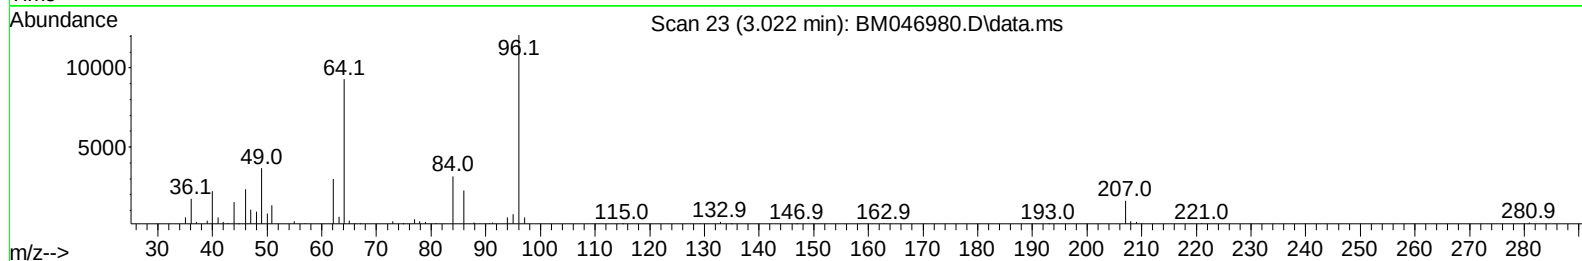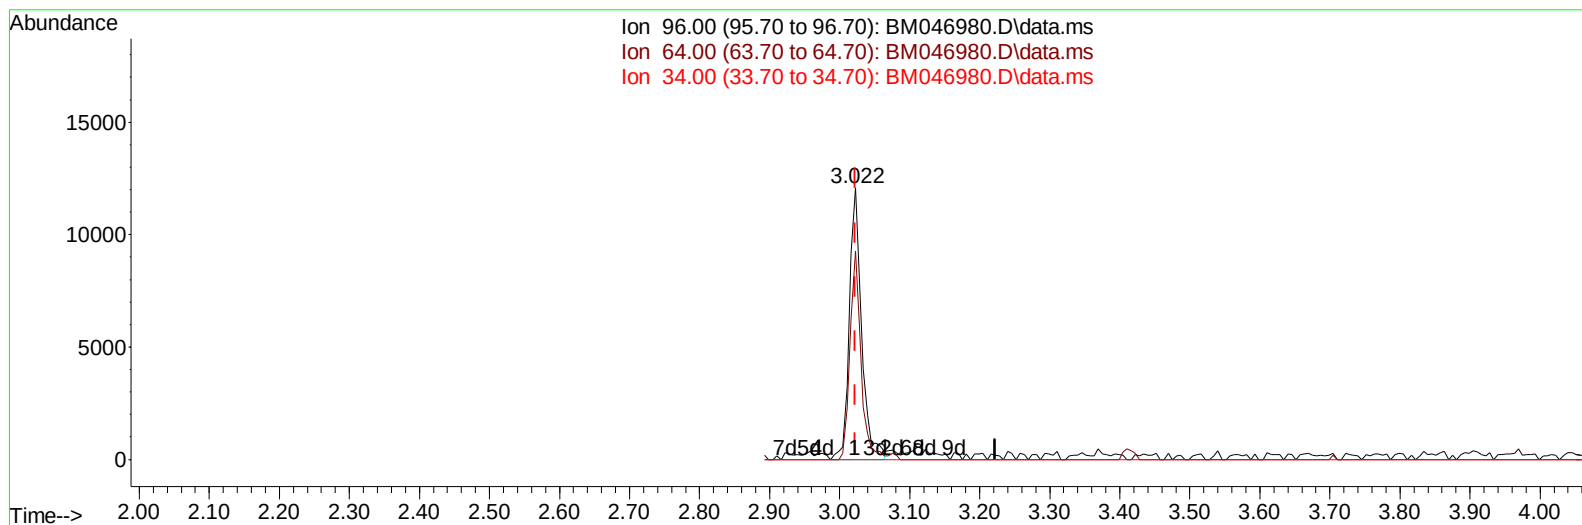

TIC: BM046980.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.022min (+ 0.000) 3.22 ng/uL m

response 14838

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	81.60	76.77
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046980.D
 Acq On : 04 Aug 2024 01:30
 Operator : MA/JU
 Sample : P3276-21
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/05/2024
 Supervised By :mohammad ahmed 08/05/2024

Quant Time: Aug 05 01:42:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 03 02:51:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.398	152	182809	20.000	ng/ul	0.00
20) Naphthalene-d8	10.157	136	686526	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.057	164	428718	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.815	188	890395	20.000	ng/ul	0.00
79) Chrysene-d12	21.045	240	909714	20.000	ng/ul	-0.01
88) Perylene-d12	23.762	264	1204746	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.022	96	14838m	3.216	ng/uL	0.00
4) Pyridine-d5	3.410	84	200999	15.969	ng/ul	0.00
7) Phenol-d5	6.598	99	260630	18.768	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.751	67	168696	18.462	ng/ul	0.00
11) 2-Chlorophenol-d4	6.940	132	208567	17.730	ng/ul	0.00
15) 4-Methylphenol-d8	8.116	113	203940	18.538	ng/ul	0.00
21) Nitrobenzene-d5	8.545	128	96680	17.550	ng/ul	0.00
24) 2-Nitrophenol-d4	9.257	143	107323	17.839	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.792	165	199066	17.234	ng/ul	0.00
31) 4-Chloroaniline-d4	10.304	131	270978	17.851	ng/ul	0.00
46) Dimethylphthalate-d6	13.480	166	618408	18.865	ng/ul	0.00
49) Acenaphthylene-d8	13.739	160	685929	18.746	ng/ul	0.00
54) 4-Nitrophenol-d4	14.292	143	99034	15.625	ng/ul	0.00
60) Fluorene-d10	15.057	176	518929	18.506	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.198	200	79206	14.080	ng/ul	0.00
73) Anthracene-d10	16.910	188	817745	19.373	ng/ul	0.00
81) Pyrene-d10	19.227	212	949415	18.231	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.580	264	1229360	19.379	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046980.D
Acq On : 04 Aug 2024 01:30
Operator : MA/JU
Sample : P3276-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J8

Manual IntegrationsAPPROVED

Quant Time: Aug 05 01:42:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 03 02:51:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
Supervised By :mohammad ahmed 08/05/2024

