

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046957.D
 Acq On : 03 Aug 2024 09:27
 Operator : MA/JU
 Sample : PB162235BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	19	23	31	rVB	43556	56518	1.96%	0.169%
2	3.410	85	89	108	rBV	497071	710102	24.60%	2.122%
3	3.710	137	140	145	rVB	14962	17360	0.60%	0.052%
4	3.928	175	177	180	rBV4	3096	3507	0.12%	0.010%
5	4.163	215	217	222	rBV4	2920	3961	0.14%	0.012%
6	6.057	535	539	541	rBV4	2313	3053	0.11%	0.009%
7	6.604	626	632	642	rBV	576745	867850	30.07%	2.593%
8	6.757	652	658	666	rBV	458023	685671	23.76%	2.049%
9	6.945	682	690	701	rBV	558293	881115	30.53%	2.633%
10	7.398	761	767	776	rBV	641737	970709	33.63%	2.900%
11	8.122	883	890	903	rBV	643823	1019635	35.33%	3.047%
12	8.545	954	962	975	rBV	543043	859754	29.79%	2.569%
13	8.939	1023	1029	1033	rVB6	1784	4314	0.15%	0.013%
14	9.257	1075	1083	1094	rBV	452106	719815	24.94%	2.151%
15	9.792	1167	1174	1188	rBV	645358	1052637	36.47%	3.145%
16	10.157	1229	1236	1245	rVB	771660	1262438	43.74%	3.772%
17	10.304	1255	1261	1275	rBV	607999	1045617	36.23%	3.124%
18	11.198	1411	1413	1418	rBV4	1761	3128	0.11%	0.009%
19	11.763	1503	1509	1515	rBV3	8751	13424	0.47%	0.040%
20	13.486	1796	1802	1813	rBV	1149116	1590697	55.11%	4.753%
21	13.745	1839	1846	1854	rBV	1197400	1742977	60.39%	5.208%
22	14.057	1892	1899	1910	rBV	1152332	1649304	57.14%	4.928%
23	14.292	1933	1939	1952	rBV	523523	822720	28.50%	2.458%
24	15.063	2061	2070	2085	rBV	1525388	2138020	74.07%	6.388%
25	15.198	2087	2093	2104	rVV	595451	778893	26.99%	2.327%
26	15.304	2108	2111	2114	rVB5	5615	6994	0.24%	0.021%
27	15.851	2200	2204	2208	rBV4	3772	5193	0.18%	0.016%
28	16.821	2362	2369	2375	rBV	1404105	1991520	69.00%	5.951%
29	16.915	2379	2385	2396	rBV2	1704593	2377988	82.39%	7.105%
30	17.762	2524	2529	2535	rBV8	7327	16518	0.57%	0.049%
31	18.715	2688	2691	2692	rBV2	4274	4815	0.17%	0.014%
32	18.786	2700	2703	2709	rVB5	21110	29711	1.03%	0.089%
33	18.862	2712	2716	2719	rBV2	20660	27908	0.97%	0.083%
34	19.233	2772	2779	2785	rBV	2037575	2722919	94.34%	8.136%
35	21.056	3083	3089	3095	rBV	1584686	2182628	75.62%	6.522%
36	23.586	3511	3519	3530	rVB2	1286166	2886296	100.00%	8.624%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046957.D
Acq On : 03 Aug 2024 09:27
Operator : MA/JU
Sample : PB162235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Title : SVOA CALIBRATION

37	23.768	3543	3550	3559	rBV	1018703	2311272	80.08%	6.906%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 33466981

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046957.D
Acq On : 03 Aug 2024 09:27
Operator : MA/JU
Sample : PB162235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

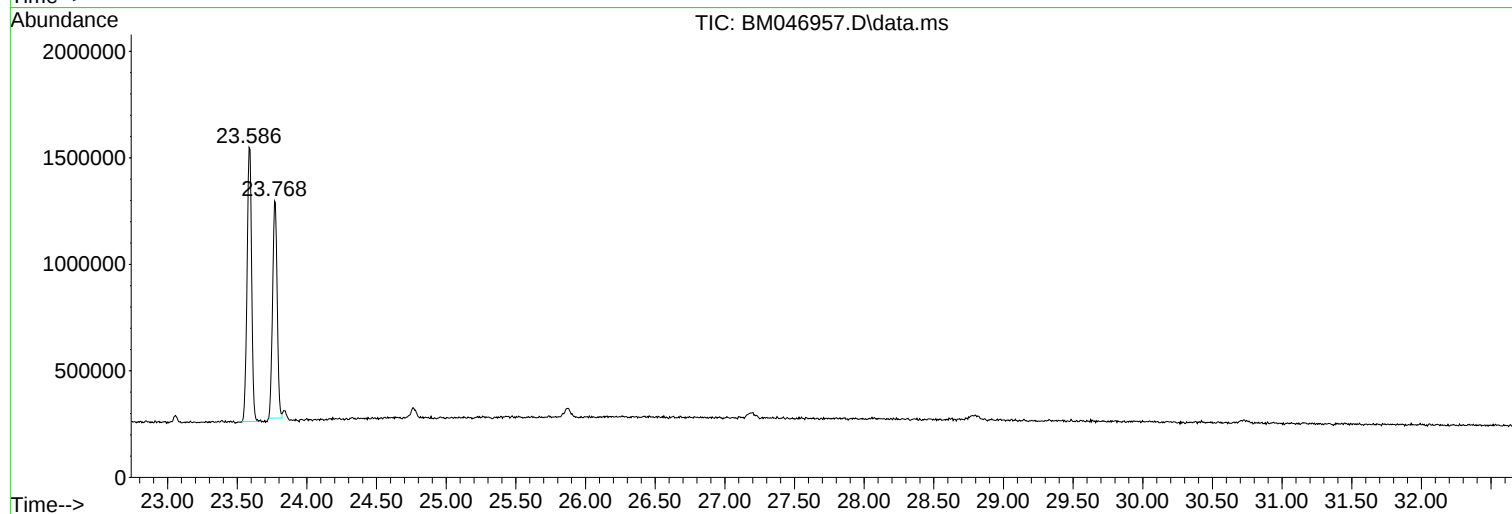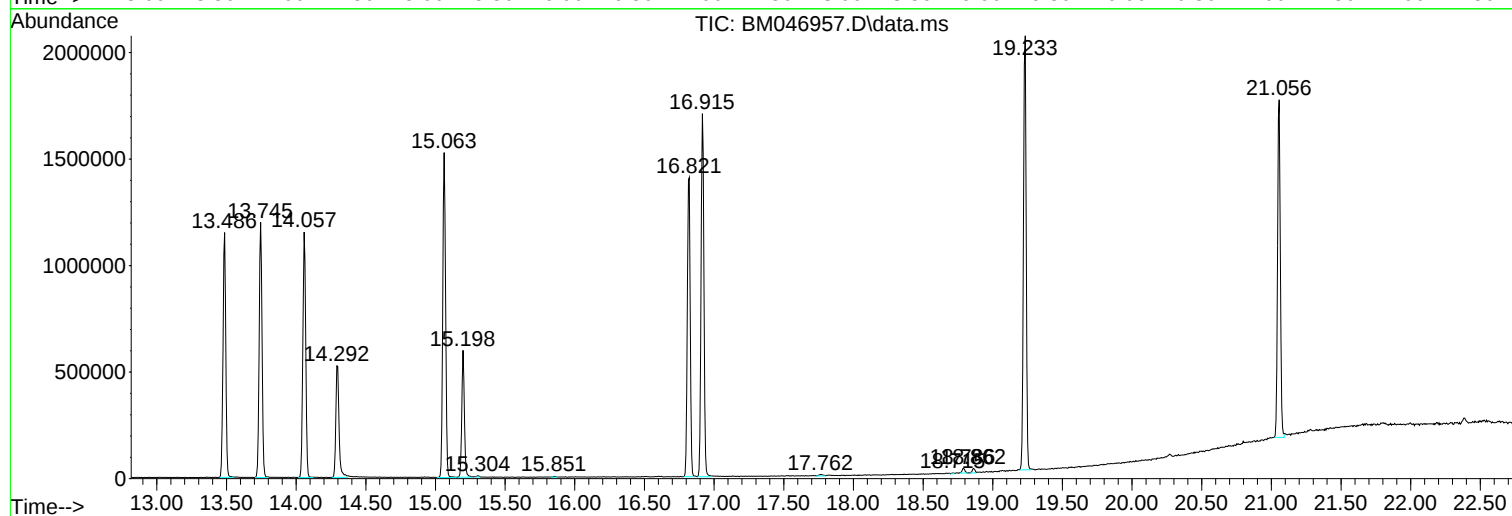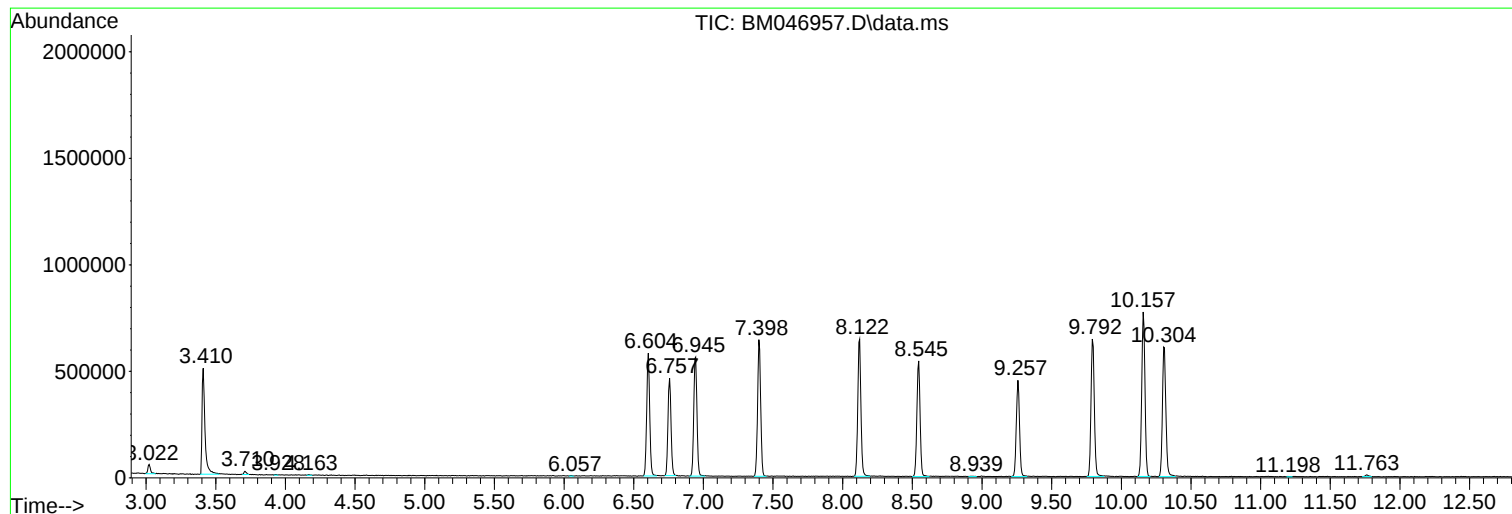

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046957.D
Acq On : 03 Aug 2024 09:27
Operator : MA/JU
Sample : PB162235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046957.D
Acq On : 03 Aug 2024 09:27
Operator : MA/JU
Sample : PB162235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------