

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046958.D
 Acq On : 03 Aug 2024 10:08
 Operator : MA/JU
 Sample : P3276-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1ZS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	19	23	30	rVB3	14711	19390	1.18%	0.122%
2	3.193	50	52	54	rBV3	1699	1767	0.11%	0.011%
3	3.287	65	68	76	rBV	24780	37400	2.27%	0.235%
4	3.416	87	90	100	rBV	158476	229561	13.94%	1.445%
5	3.687	134	136	137	rBV2	1929	1822	0.11%	0.011%
6	3.710	137	140	144	rVV4	7215	10242	0.62%	0.064%
7	3.763	147	149	151	rBV3	2507	1838	0.11%	0.012%
8	3.822	157	159	163	rVB5	2048	1819	0.11%	0.011%
9	3.957	180	182	187	rVB3	2124	2063	0.13%	0.013%
10	4.169	216	218	221	rVB3	2126	2433	0.15%	0.015%
11	4.593	287	290	295	rVB6	2178	3283	0.20%	0.021%
12	4.887	338	340	344	rVB4	2123	2751	0.17%	0.017%
13	5.010	360	361	364	rBV3	1937	1911	0.12%	0.012%
14	5.204	392	394	396	rBV3	1643	1739	0.11%	0.011%
15	5.457	435	437	440	rBV4	1964	2197	0.13%	0.014%
16	6.075	540	542	547	rVV6	1301	1856	0.11%	0.012%
17	6.140	551	553	558	rVB6	2344	3266	0.20%	0.021%
18	6.181	558	560	565	rBV4	1821	2283	0.14%	0.014%
19	6.369	588	592	593	rVB4	2042	1968	0.12%	0.012%
20	6.604	626	632	642	rVB	215019	325335	19.76%	2.048%
21	6.757	651	658	665	rBV	169503	251705	15.29%	1.585%
22	6.810	665	667	671	rVB4	1937	2226	0.14%	0.014%
23	6.945	683	690	697	rBV	208803	330860	20.10%	2.083%
24	7.051	704	708	709	rBV3	1400	1753	0.11%	0.011%
25	7.398	760	767	776	rVV	430763	651501	39.58%	4.102%
26	7.710	816	820	823	rBV6	1491	2250	0.14%	0.014%
27	7.881	848	849	852	rVB2	1865	1783	0.11%	0.011%
28	7.934	852	858	861	rBV6	1715	4037	0.25%	0.025%
29	8.116	881	889	899	rBV	245246	385324	23.41%	2.426%
30	8.545	955	962	970	rVB	198104	315492	19.16%	1.986%
31	9.134	1058	1062	1070	rVB4	9740	16332	0.99%	0.103%
32	9.257	1077	1083	1092	rBV	161172	254874	15.48%	1.605%
33	9.322	1092	1094	1097	rVB4	1677	1676	0.10%	0.011%
34	9.457	1113	1117	1121	rBV4	1482	2346	0.14%	0.015%
35	9.792	1168	1174	1182	rBV	230697	387104	23.52%	2.437%
36	10.157	1229	1236	1244	rBV	510898	836140	50.79%	5.265%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046958.D
 Acq On : 03 Aug 2024 10:08
 Operator : MA/JU
 Sample : P3276-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1ZS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	10.304	1254	1261	1272	rBV	218792	388328	23.59%	2.445%
38	10.410	1278	1279	1283	rVB2	2229	1770	0.11%	0.011%
39	10.639	1314	1318	1321	rBV6	1060	1801	0.11%	0.011%
40	10.739	1330	1335	1340	rBV3	2409	4406	0.27%	0.028%

41	10.922	1359	1366	1375	rBV2	16589	36809	2.24%	0.232%
42	11.763	1503	1509	1513	rBV6	3384	6074	0.37%	0.038%
43	12.392	1613	1616	1620	rBV3	1145	1812	0.11%	0.011%
44	12.845	1688	1693	1695	rBV4	1351	2337	0.14%	0.015%
45	13.210	1751	1755	1758	rBV5	1605	2359	0.14%	0.015%

46	13.480	1795	1801	1812	rBV	406670	571876	34.74%	3.601%
47	13.557	1812	1814	1816	rVB3	2296	1700	0.10%	0.011%
48	13.745	1836	1846	1855	rBV	443189	651335	39.57%	4.101%
49	13.839	1858	1862	1865	rVB4	1368	1990	0.12%	0.013%
50	14.057	1893	1899	1906	rVB	747826	1058261	64.29%	6.663%

51	14.198	1918	1923	1924	rBV3	1392	2031	0.12%	0.013%
52	14.298	1934	1940	1950	rBV	173197	291215	17.69%	1.834%
53	14.427	1960	1962	1965	rVB3	1786	1935	0.12%	0.012%
54	14.510	1973	1976	1978	rVB3	1754	1839	0.11%	0.012%
55	14.692	2005	2007	2010	rVB3	1981	1923	0.12%	0.012%

56	14.892	2038	2041	2043	rBV4	1826	1952	0.12%	0.012%
57	14.957	2047	2052	2056	rVB5	2669	3452	0.21%	0.022%
58	15.063	2062	2070	2080	rBV	581274	803114	48.79%	5.057%
59	15.198	2087	2093	2101	rBV	171848	225187	13.68%	1.418%
60	15.263	2101	2104	2107	rVV4	1825	2653	0.16%	0.017%

61	15.304	2107	2111	2114	rVB4	2106	2248	0.14%	0.014%
62	15.410	2125	2129	2131	rVB4	1409	2059	0.13%	0.013%
63	15.463	2133	2138	2141	rBV6	2199	4185	0.25%	0.026%
64	15.586	2155	2159	2162	rBV4	1158	1929	0.12%	0.012%
65	15.663	2170	2172	2174	rVB3	1805	1671	0.10%	0.011%

66	15.768	2187	2190	2193	rBV4	1541	2125	0.13%	0.013%
67	15.821	2196	2199	2204	rBV5	2084	4143	0.25%	0.026%
68	16.186	2258	2261	2265	rVB5	1317	1884	0.11%	0.012%
69	16.268	2272	2275	2278	rBV3	2290	2556	0.16%	0.016%
70	16.327	2283	2285	2294	rVB6	1668	4074	0.25%	0.026%

71	16.615	2330	2334	2340	rVV6	2473	4888	0.30%	0.031%
72	16.815	2362	2368	2374	rBV	901523	1270384	77.17%	7.999%
73	16.915	2378	2385	2397	rBV	640363	873509	53.06%	5.500%
74	17.039	2403	2406	2409	rBV4	4174	3862	0.23%	0.024%
75	17.133	2419	2422	2425	rBV4	2346	3045	0.18%	0.019%

76	17.274	2445	2446	2449	rBV3	2234	2188	0.13%	0.014%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046958.D
 Acq On : 03 Aug 2024 10:08
 Operator : MA/JU
 Sample : P3276-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1ZS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

77	17.533	2488	2490	2494	rVV5	2474	2502	0.15%	0.016%
78	17.633	2506	2507	2511	rVB4	3209	2415	0.15%	0.015%
79	17.662	2511	2512	2514	rBV2	2254	1920	0.12%	0.012%
80	17.715	2518	2521	2523	rBV4	2354	3047	0.19%	0.019%
81	17.757	2523	2528	2536	rBV2	54139	86304	5.24%	0.543%
82	17.821	2538	2539	2541	rVB2	2956	1805	0.11%	0.011%
83	17.857	2544	2545	2548	rBV2	2353	2807	0.17%	0.018%
84	17.962	2561	2563	2565	rBV3	2615	2001	0.12%	0.013%
85	17.998	2567	2569	2572	rBV4	1606	1944	0.12%	0.012%
86	18.162	2595	2597	2598	rBV2	2745	2040	0.12%	0.013%
87	18.262	2612	2614	2616	rBV3	2170	2295	0.14%	0.014%
88	18.574	2665	2667	2669	rBV3	3831	4214	0.26%	0.027%
89	18.786	2701	2703	2708	rVB5	6571	7825	0.48%	0.049%
90	18.862	2712	2716	2719	rBV3	7484	11963	0.73%	0.075%
91	18.909	2722	2724	2726	rBV2	5599	3958	0.24%	0.025%
92	19.056	2745	2749	2755	rBV6	18830	34038	2.07%	0.214%
93	19.227	2772	2778	2786	rBV	765533	1026823	62.38%	6.465%
94	20.797	3041	3045	3051	rBV4	71807	97925	5.95%	0.617%
95	21.050	3083	3088	3096	rBV	1093331	1465173	89.00%	9.225%
96	23.580	3511	3518	3527	rBV	517286	1123669	68.26%	7.075%
97	23.768	3543	3550	3558	rBV	741552	1646190	100.00%	10.365%




Sum of corrected areas: 15882094

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046958.D
Acq On : 03 Aug 2024 10:08
Operator : MA/JU
Sample : P3276-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1ZS4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

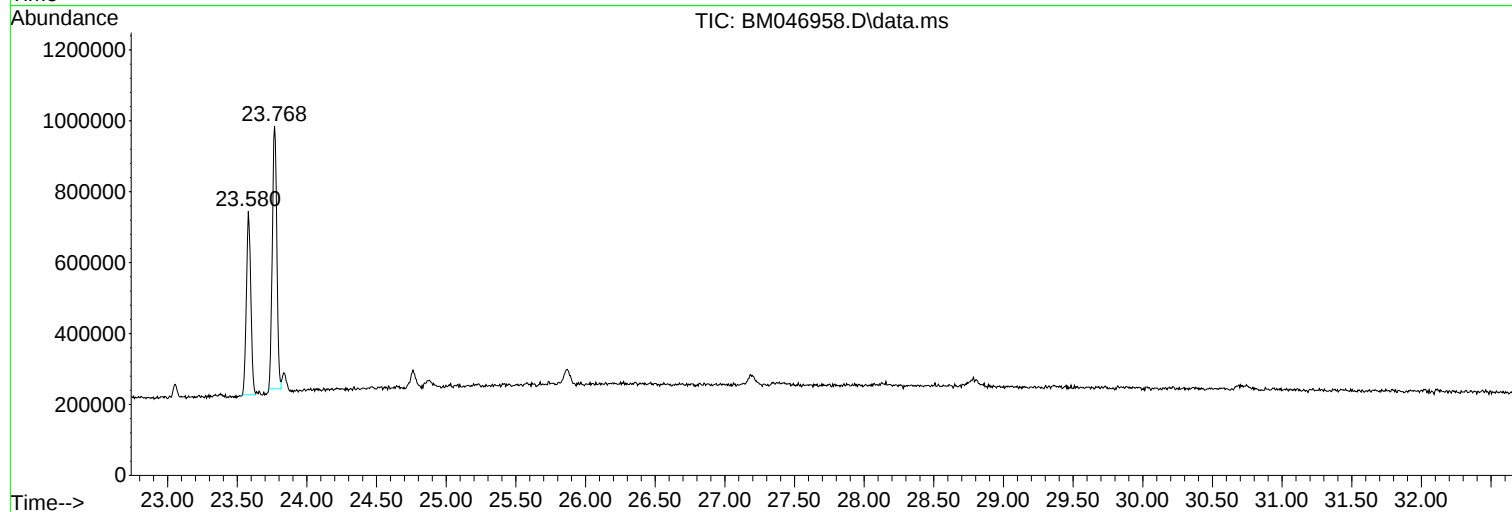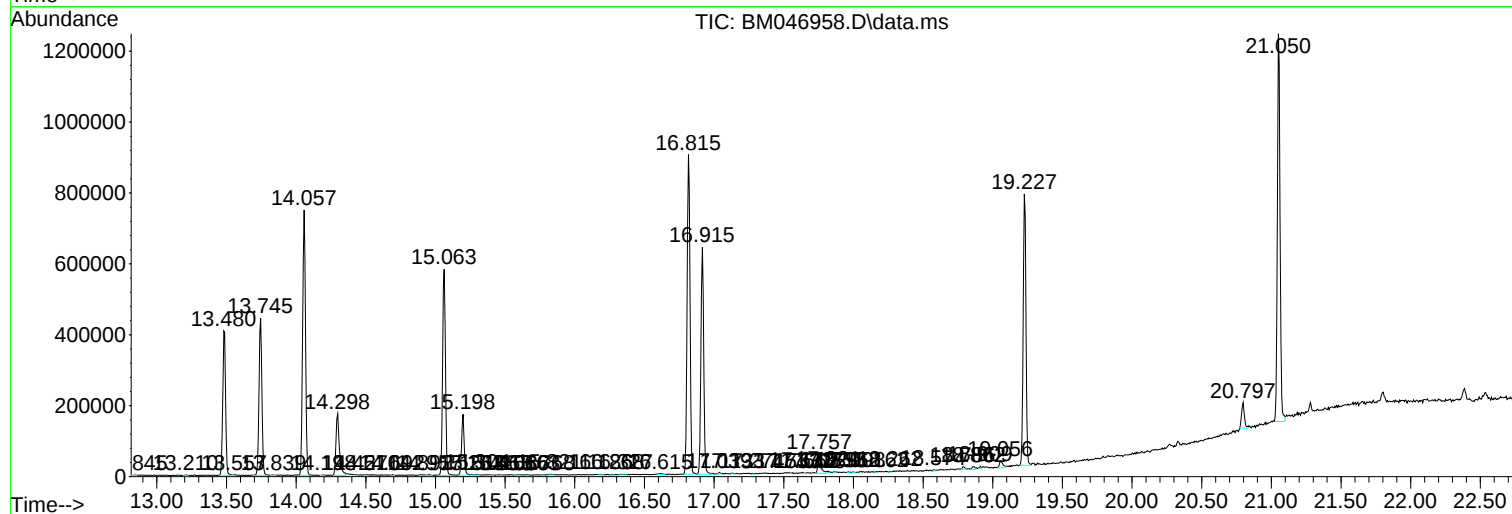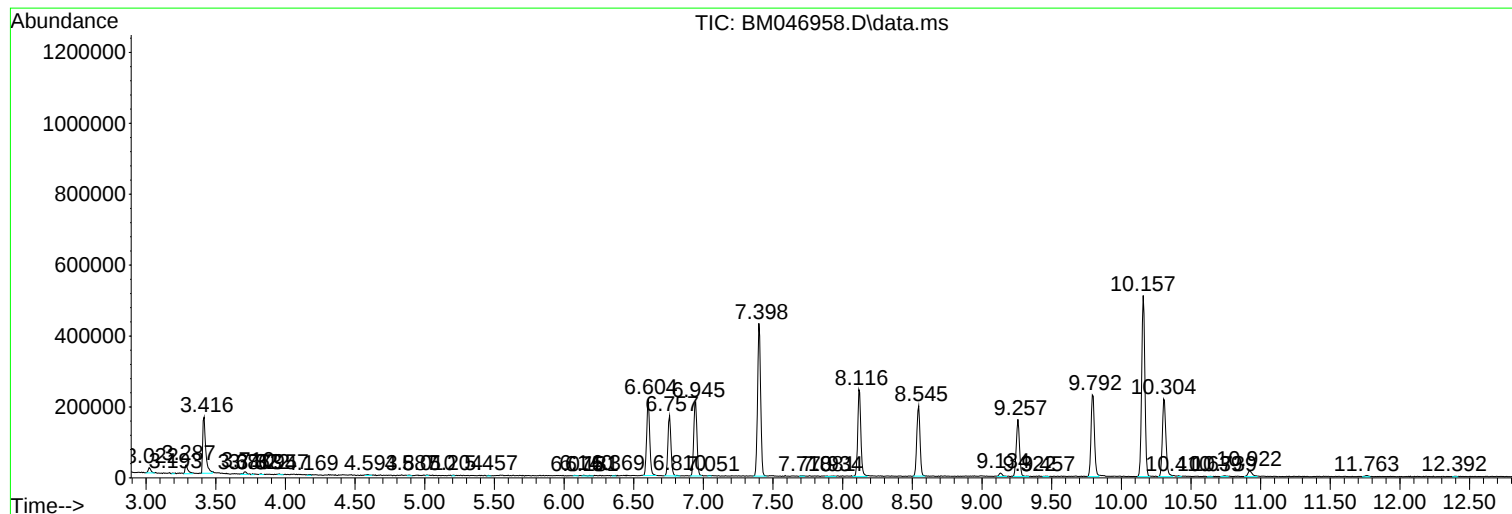

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046958.D
Acq On : 03 Aug 2024 10:08
Operator : MA/JU
Sample : P3276-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1ZS4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046958.D
Acq On : 03 Aug 2024 10:08
Operator : MA/JU
Sample : P3276-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1ZS4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------