

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046970.D
 Acq On : 03 Aug 2024 18:49
 Operator : MA/JU
 Sample : PB162235BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	19	23	28	rBV	65794	74381	1.76%	0.154%
2	3.410	85	89	108	rBV	743542	1046445	24.82%	2.174%
3	3.710	136	140	147	rVB2	20427	27371	0.65%	0.057%
4	3.922	174	176	179	rBV4	4103	4531	0.11%	0.009%
5	5.181	389	390	396	rBV6	3240	5206	0.12%	0.011%
6	6.604	625	632	644	rBV	842008	1304621	30.94%	2.710%
7	6.757	651	658	670	rVB	709580	1052410	24.96%	2.186%
8	6.939	681	689	701	rBV	871603	1332677	31.61%	2.768%
9	7.398	760	767	774	rBV	768098	1153940	27.37%	2.397%
10	7.857	842	845	848	rBV5	3476	4448	0.11%	0.009%
11	8.116	882	889	900	rBV	1002173	1568176	37.19%	3.257%
12	8.545	955	962	971	rVV	801658	1298046	30.78%	2.696%
13	8.992	1035	1038	1041	rBV4	3374	5008	0.12%	0.010%
14	9.257	1075	1083	1092	rBV	690644	1102772	26.15%	2.291%
15	9.792	1166	1174	1186	rBV	1032983	1656400	39.28%	3.441%
16	10.157	1229	1236	1243	rBV	978934	1572692	37.30%	3.267%
17	10.304	1254	1261	1274	rBV	970289	1622908	38.49%	3.371%
18	10.598	1309	1311	1315	rVB4	4288	4747	0.11%	0.010%
19	11.757	1501	1508	1515	rVB2	17441	31037	0.74%	0.064%
20	13.480	1795	1801	1811	rBV	1677683	2413593	57.24%	5.013%
21	13.745	1839	1846	1856	rVV	1848227	2731791	64.79%	5.674%
22	14.057	1892	1899	1908	rBV	1470727	2104682	49.92%	4.372%
23	14.115	1908	1909	1912	rVB3	4685	4621	0.11%	0.010%
24	14.180	1917	1920	1922	rBV3	4406	4954	0.12%	0.010%
25	14.292	1933	1939	1950	rBV	866842	1287408	30.53%	2.674%
26	15.062	2063	2070	2081	rBV	2369717	3320352	78.75%	6.897%
27	15.198	2087	2093	2102	rBV	890950	1192115	28.27%	2.476%
28	15.298	2107	2110	2116	rVB4	11688	19292	0.46%	0.040%
29	15.851	2197	2204	2207	rBV9	4953	7858	0.19%	0.016%
30	16.815	2362	2368	2375	rBV	1866143	2507830	59.48%	5.209%
31	16.915	2379	2385	2398	rVV	2757167	3661982	86.85%	7.606%
32	17.133	2419	2422	2426	rVB6	5277	7420	0.18%	0.015%
33	17.509	2484	2486	2492	rVB7	4873	6851	0.16%	0.014%
34	17.756	2523	2528	2536	rBV9	12501	19649	0.47%	0.041%
35	17.956	2556	2562	2564	rBV6	3533	6248	0.15%	0.013%
36	18.056	2577	2579	2583	rBV5	4235	4428	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046970.D
Acq On : 03 Aug 2024 18:49
Operator : MA/JU
Sample : PB162235BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Title : SVOA CALIBRATION

37	18.315	2622	2623	2627	rBV3	4371	5648	0.13%	0.012%
38	18.786	2699	2703	2710	rVB4	32265	48111	1.14%	0.100%
39	18.856	2712	2715	2720	rBV	31917	45310	1.07%	0.094%
40	19.227	2771	2778	2790	rBV	3187627	4160260	98.67%	8.641%
41	21.050	3083	3088	3096	rBV	2014438	2594776	61.54%	5.390%
42	23.044	3424	3427	3434	rVB	121676	208627	4.95%	0.433%
43	23.580	3510	3518	3531	rVB2	1923631	4216509	100.00%	8.758%
44	23.762	3542	3549	3556	rBV	1166869	2695467	63.93%	5.599%




Sum of corrected areas: 48143598

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046970.D
Acq On : 03 Aug 2024 18:49
Operator : MA/JU
Sample : PB162235BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

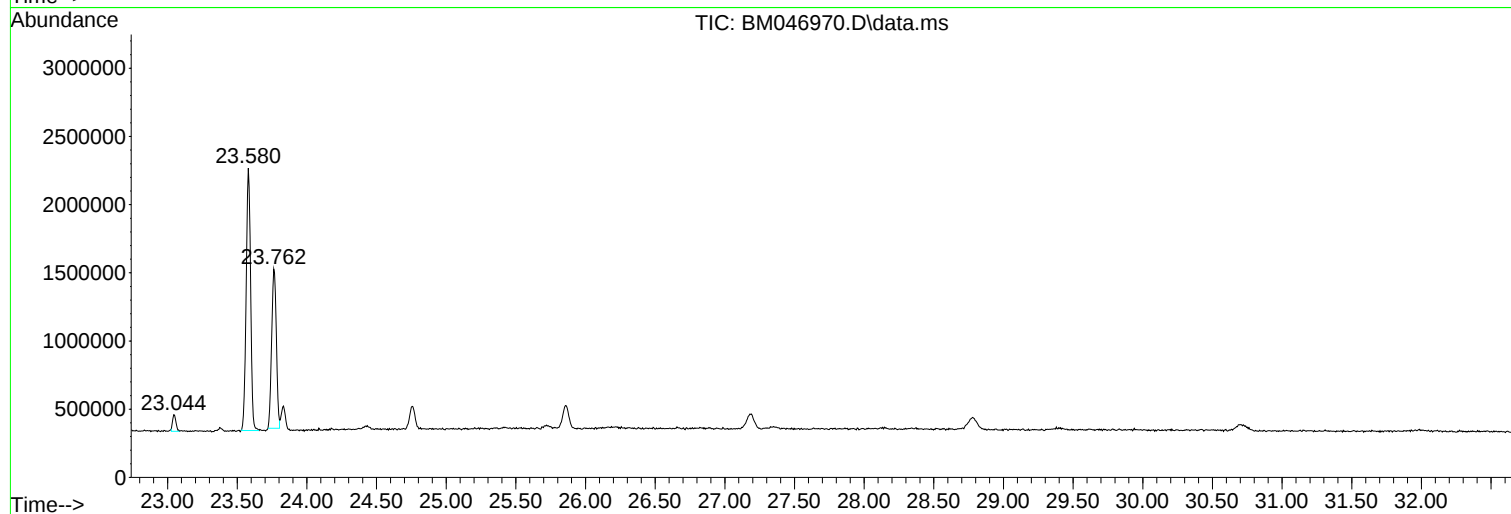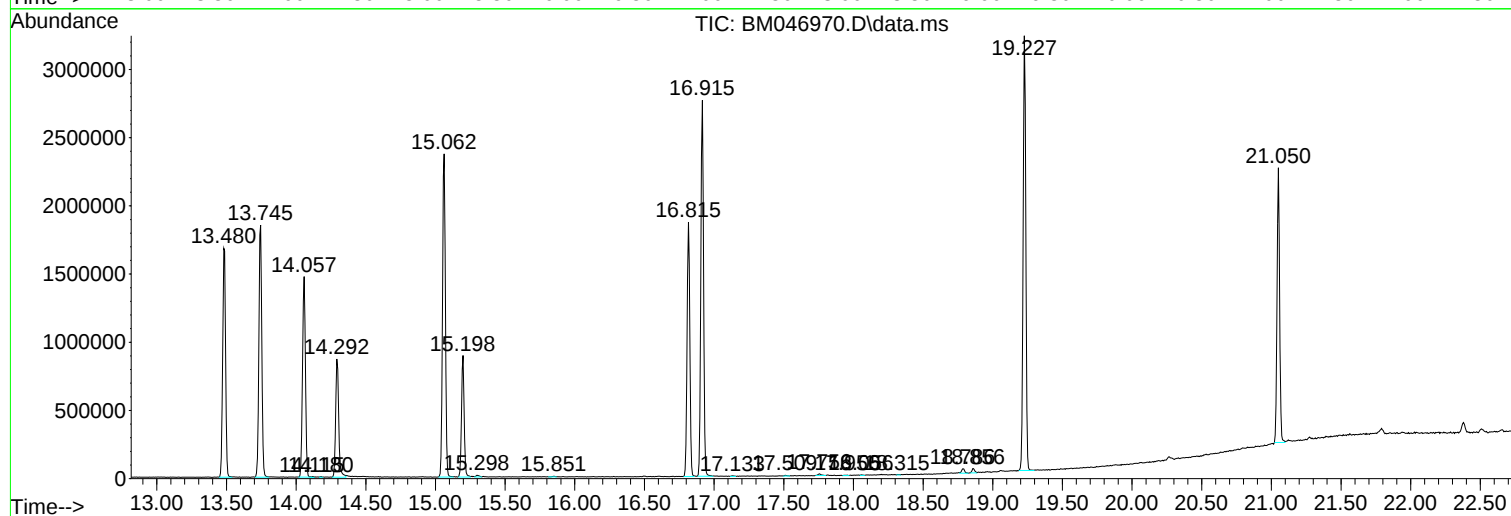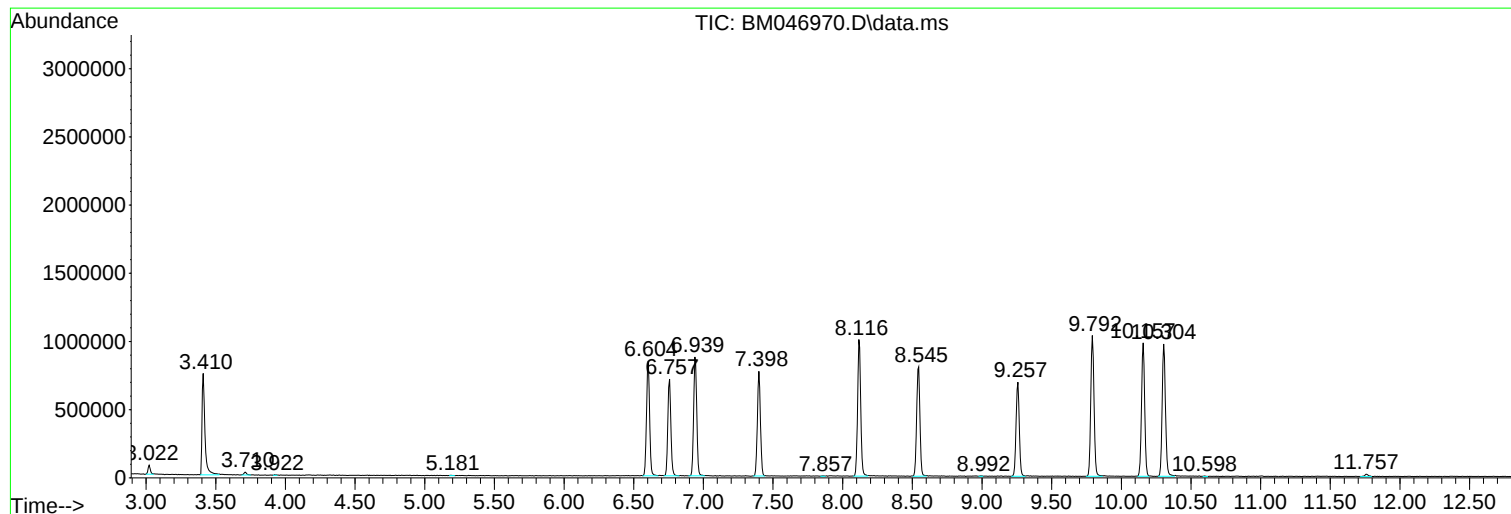

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046970.D
Acq On : 03 Aug 2024 18:49
Operator : MA/JU
Sample : PB162235BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046970.D
Acq On : 03 Aug 2024 18:49
Operator : MA/JU
Sample : PB162235BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------