

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046972.D
 Acq On : 03 Aug 2024 20:09
 Operator : MA/JU
 Sample : P3276-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	19	23	30	rVB	25474	35765	1.27%	0.138%
2	3.422	87	91	92	rBV4	6113	7583	0.27%	0.029%
3	3.511	102	106	110	rVB	21597	26505	0.94%	0.102%
4	3.675	130	134	137	rBV6	6465	8834	0.31%	0.034%
5	3.711	137	140	146	rVB4	12925	19187	0.68%	0.074%
6	4.063	198	200	205	rVB6	6220	9064	0.32%	0.035%
7	4.240	226	230	234	rVV6	4542	6220	0.22%	0.024%
8	4.428	260	262	265	rVB4	2980	2892	0.10%	0.011%
9	4.469	265	269	273	rBV5	7295	10849	0.38%	0.042%
10	4.587	284	289	294	rBV	23516	32465	1.15%	0.125%
11	5.040	364	366	370	rVB4	3247	3795	0.13%	0.015%
12	5.169	385	388	392	rBV6	4051	5544	0.20%	0.021%
13	5.440	429	434	435	rBV5	2531	3198	0.11%	0.012%
14	5.546	449	452	457	rVB4	6022	9027	0.32%	0.035%
15	5.699	474	478	483	rVB8	5902	9162	0.32%	0.035%
16	5.999	527	529	533	rVB5	2919	3507	0.12%	0.014%
17	6.128	548	551	557	rVB7	2589	5208	0.18%	0.020%
18	6.222	562	567	568	rBV4	2919	3167	0.11%	0.012%
19	6.293	573	579	583	rBV10	3309	7135	0.25%	0.028%
20	6.604	623	632	641	rBV	314221	508749	18.04%	1.963%
21	6.757	652	658	665	rBV	304364	475517	16.86%	1.834%
22	6.940	682	689	700	rBV	311102	482343	17.11%	1.861%
23	7.046	703	707	709	rVB5	5090	5824	0.21%	0.022%
24	7.234	735	739	742	rBV5	2562	3357	0.12%	0.013%
25	7.299	745	750	751	rBV5	2967	3013	0.11%	0.012%
26	7.399	760	767	775	rBV	716388	1077295	38.21%	4.156%
27	7.487	777	782	786	rVB6	4140	7460	0.26%	0.029%
28	8.116	883	889	900	rBV	366837	574987	20.39%	2.218%
29	8.216	902	906	912	rVB2	21024	36238	1.29%	0.140%
30	8.540	955	961	972	rVB	357541	580087	20.57%	2.238%
31	8.993	1034	1038	1043	rVB5	6271	10877	0.39%	0.042%
32	9.128	1056	1061	1066	rBV3	18920	30181	1.07%	0.116%
33	9.257	1076	1083	1093	rBV	182346	305704	10.84%	1.179%
34	9.322	1093	1094	1101	rVB6	3281	3561	0.13%	0.014%
35	9.440	1110	1114	1115	rBV4	4087	4233	0.15%	0.016%
36	9.463	1115	1118	1125	rVV7	4525	8734	0.31%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046972.D
 Acq On : 03 Aug 2024 20:09
 Operator : MA/JU
 Sample : P3276-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	9.528	1125	1129	1135	rVB7	4402	8050	0.29%	0.031%
38	9.616	1142	1144	1148	rVB4	3147	3078	0.11%	0.012%
39	9.793	1167	1174	1189	rBV	312756	505416	17.93%	1.950%
40	10.157	1229	1236	1249	rBV	884730	1464854	51.95%	5.651%
41	10.304	1251	1261	1275	rBV	359127	632691	22.44%	2.441%
42	10.728	1331	1333	1336	rBV4	3156	3133	0.11%	0.012%
43	10.916	1360	1365	1374	rBV2	30445	62053	2.20%	0.239%
44	10.987	1374	1377	1382	rVV6	5401	9399	0.33%	0.036%
45	11.757	1504	1508	1513	rVB4	7343	11345	0.40%	0.044%
46	11.834	1519	1521	1526	rBV5	2682	3500	0.12%	0.014%
47	12.404	1615	1618	1623	rVB5	3246	4869	0.17%	0.019%
48	12.669	1657	1663	1666	rVB6	3677	6437	0.23%	0.025%
49	12.898	1697	1702	1705	rBV6	5307	8317	0.29%	0.032%
50	13.386	1782	1785	1791	rBV6	3566	4729	0.17%	0.018%
51	13.481	1795	1801	1808	rBV	770794	1028281	36.47%	3.967%
52	13.575	1814	1817	1820	rVB4	2488	3238	0.11%	0.012%
53	13.739	1839	1845	1854	rBV	822880	1238763	43.93%	4.779%
54	13.992	1883	1888	1892	rBV6	3737	6490	0.23%	0.025%
55	14.057	1892	1899	1907	rVV	1274539	1889706	67.02%	7.290%
56	14.310	1934	1942	1949	rBV3	31898	69242	2.46%	0.267%
57	14.451	1962	1966	1967	rBV3	5632	6499	0.23%	0.025%
58	14.469	1967	1969	1971	rVV3	3773	3328	0.12%	0.013%
59	14.510	1973	1976	1980	rVB6	4932	7336	0.26%	0.028%
60	14.898	2035	2042	2048	rBV7	6593	15616	0.55%	0.060%
61	14.951	2048	2051	2054	rVV5	5195	5032	0.18%	0.019%
62	15.063	2063	2070	2083	rBV	1067972	1536115	54.48%	5.926%
63	15.204	2088	2094	2097	rBV7	6367	8245	0.29%	0.032%
64	15.257	2100	2103	2107	rVB5	3777	4334	0.15%	0.017%
65	15.304	2107	2111	2116	rBV5	4912	7187	0.25%	0.028%
66	15.451	2134	2136	2143	rVB6	3243	4353	0.15%	0.017%
67	15.522	2145	2148	2152	rVB4	2963	4750	0.17%	0.018%
68	15.822	2196	2199	2202	rBV4	7458	10400	0.37%	0.040%
69	16.180	2257	2260	2261	rBV2	2750	2930	0.10%	0.011%
70	16.222	2265	2267	2270	rBV4	3727	4734	0.17%	0.018%
71	16.269	2272	2275	2276	rBV3	3286	3656	0.13%	0.014%
72	16.380	2290	2294	2296	rBV2	12247	12590	0.45%	0.049%
73	16.563	2323	2325	2329	rBV4	4770	7293	0.26%	0.028%
74	16.610	2329	2333	2336	rVV6	8844	12499	0.44%	0.048%
75	16.763	2355	2359	2360	rBV4	3685	3470	0.12%	0.013%
76	16.816	2362	2368	2373	rVV	1592123	2229601	79.07%	8.601%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046972.D
 Acq On : 03 Aug 2024 20:09
 Operator : MA/JU
 Sample : P3276-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

77	16.857	2373	2375	2379	rVV2	24606	28579	1.01%	0.110%
78	16.916	2379	2385	2394	rVV	1162038	1635453	58.00%	6.309%
79	17.033	2403	2405	2409	rVB4	5216	6052	0.21%	0.023%
80	17.127	2419	2421	2423	rBV3	4260	4965	0.18%	0.019%
81	17.427	2469	2472	2474	rVB4	3523	3478	0.12%	0.013%
82	17.527	2483	2489	2494	rBV7	7103	15493	0.55%	0.060%
83	17.698	2514	2518	2520	rBV5	4766	7114	0.25%	0.027%
84	17.751	2523	2527	2535	rVV	115986	172083	6.10%	0.664%
85	17.816	2535	2538	2543	rVB	25029	34849	1.24%	0.134%
86	18.304	2619	2621	2627	rBV6	5722	8514	0.30%	0.033%
87	18.692	2685	2687	2689	rBV3	6141	6313	0.22%	0.024%
88	18.857	2712	2715	2717	rBV2	16611	20344	0.72%	0.078%
89	18.892	2717	2721	2725	rVB	61678	86520	3.07%	0.334%
90	19.051	2745	2748	2756	rBV3	46334	69807	2.48%	0.269%
91	19.227	2772	2778	2787	rBV	1247698	1723924	61.14%	6.650%
92	20.792	3040	3044	3049	rBV2	176838	261225	9.26%	1.008%
93	21.051	3082	3088	3093	rBV	1846708	2517819	89.30%	9.713%
94	23.580	3512	3518	3526	rVB	624382	1320317	46.83%	5.093%
95	23.762	3542	3549	3557	rBV	1300907	2819609	100.00%	10.877%




Sum of corrected areas: 25923284

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046972.D
Acq On : 03 Aug 2024 20:09
Operator : MA/JU
Sample : P3276-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

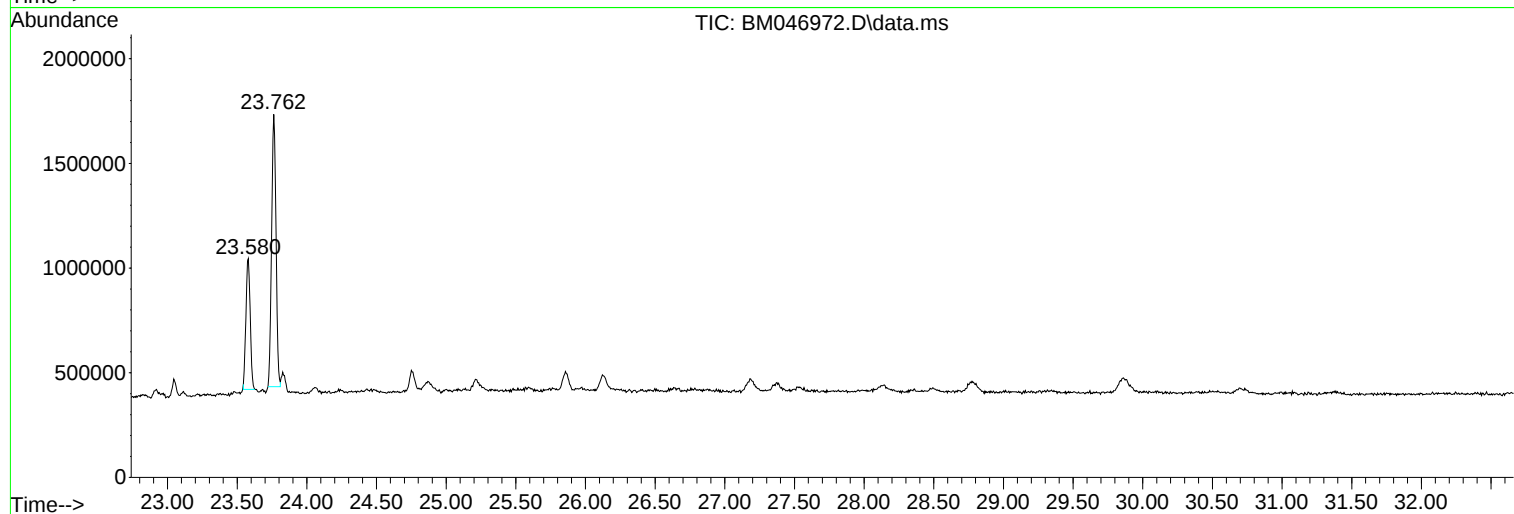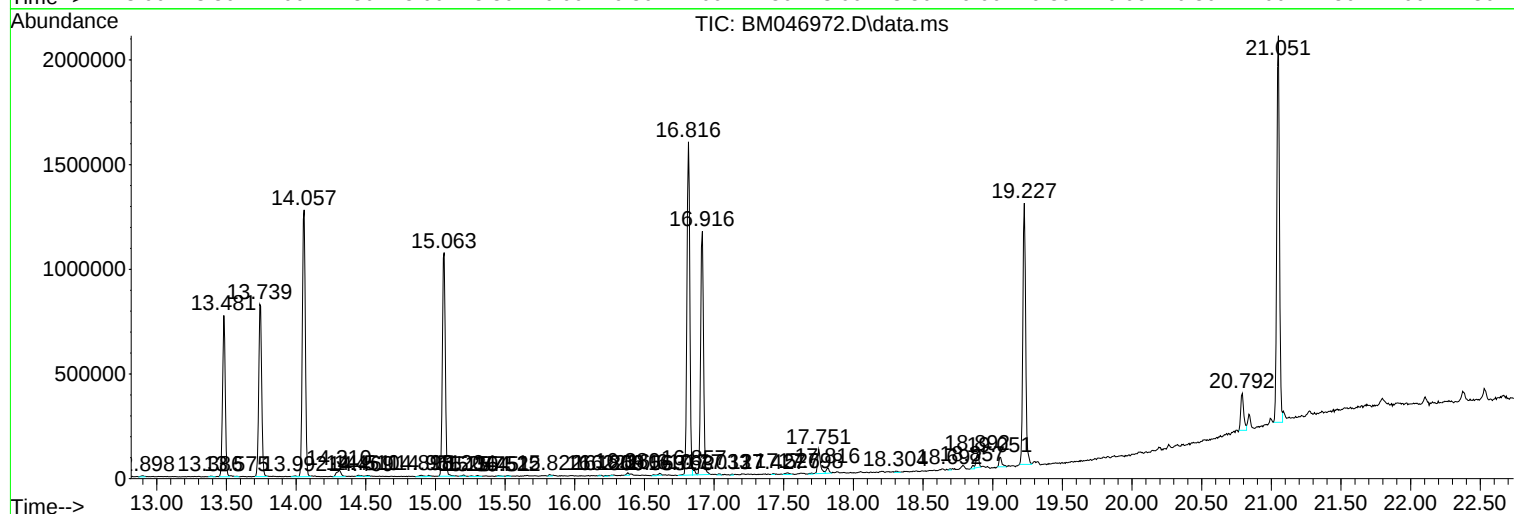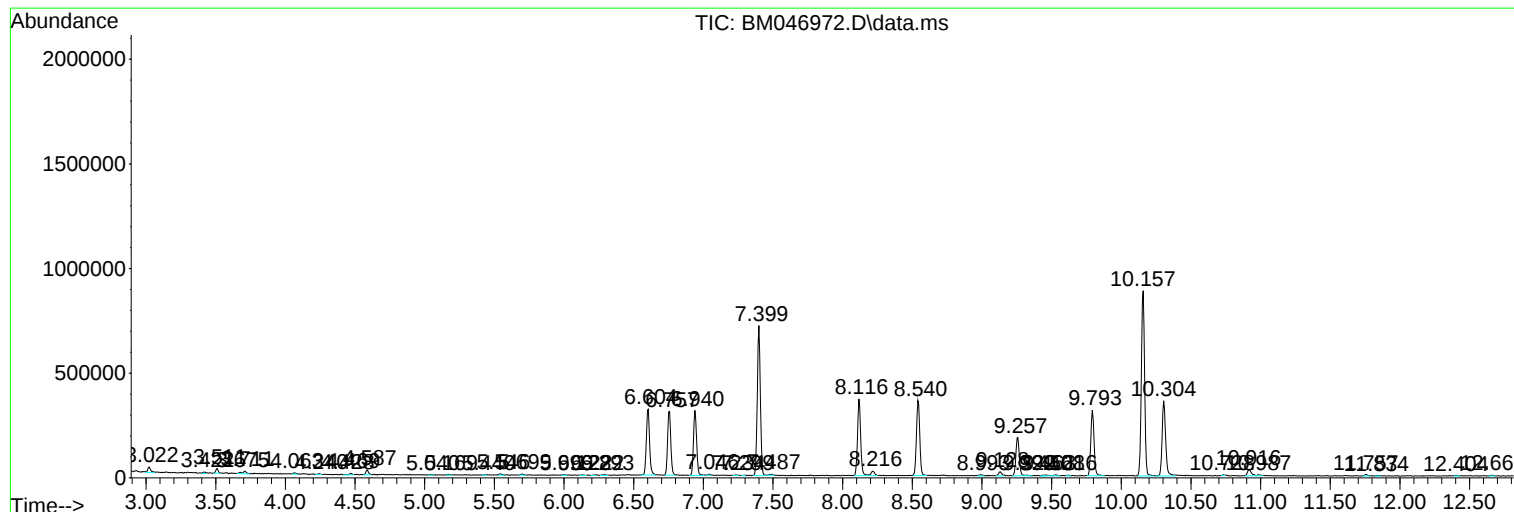

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046972.D
Acq On : 03 Aug 2024 20:09
Operator : MA/JU
Sample : P3276-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.792	2.08 ng/ul	261225	Chrysene-d12	21.051

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
2			9-Eicosene, (E)-	280	C20H40	074685-29-3	93
3			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	91
4			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	91
5			n-Nonadecanol-1	284	C19H40O	001454-84-8	90

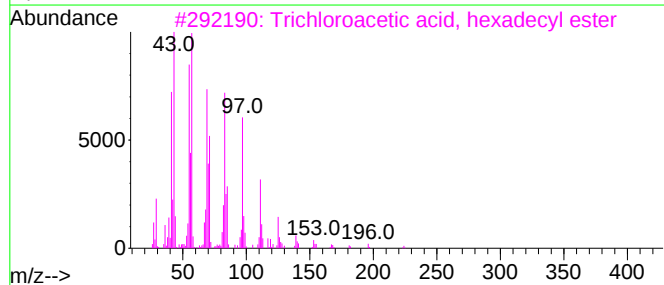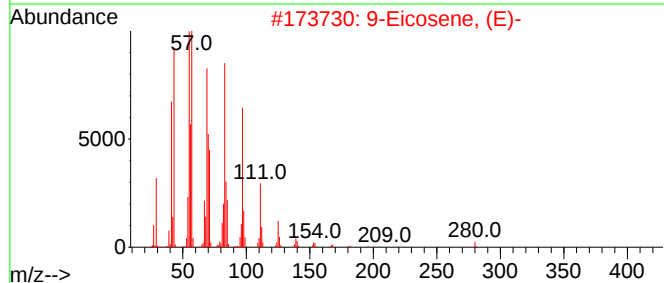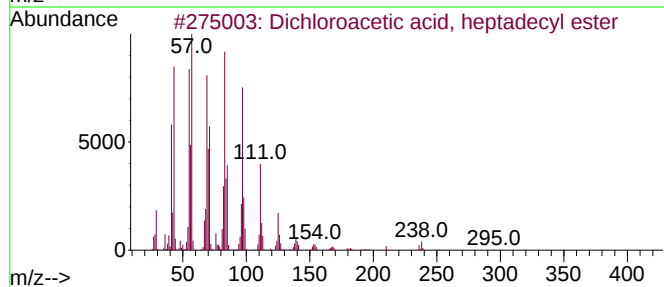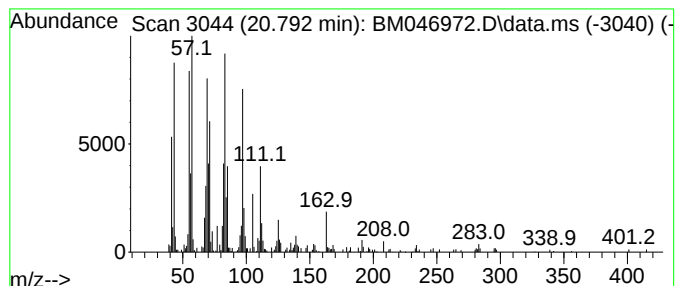

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046972.D
Acq On : 03 Aug 2024 20:09
Operator : MA/JU
Sample : P3276-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	20.792	2.1	ng/u1	261225	5	21.051	2517820	20.0