

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046976.D
 Acq On : 03 Aug 2024 22:49
 Operator : MA/JU
 Sample : P3276-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.946	6	10	13	rBV3	11249	15396	0.54%	0.043%
2	2.987	13	17	32	rVV	1660858	2258584	79.09%	6.247%
3	3.293	66	69	76	rVB2	8755	13100	0.46%	0.036%
4	3.410	86	89	107	rBV	326431	477702	16.73%	1.321%
5	3.675	132	134	136	rBV3	3310	3628	0.13%	0.010%
6	3.710	137	140	144	rVB3	12775	16276	0.57%	0.045%
7	4.210	220	225	234	rVB	138249	194202	6.80%	0.537%
8	4.275	234	236	241	rBV6	2753	3464	0.12%	0.010%
9	4.893	339	341	346	rVB6	2630	2992	0.10%	0.008%
10	4.957	349	352	355	rBV4	2791	3182	0.11%	0.009%
11	5.010	357	361	363	rBV5	2618	3722	0.13%	0.010%
12	5.381	422	424	426	rBV2	3163	3857	0.14%	0.011%
13	5.540	448	451	453	rBV4	3251	2918	0.10%	0.008%
14	5.993	527	528	531	rBV3	3323	3652	0.13%	0.010%
15	6.193	561	562	565	rBV3	2946	3143	0.11%	0.009%
16	6.469	604	609	611	rBV6	3256	4898	0.17%	0.014%
17	6.598	624	631	643	rBV	424036	689528	24.15%	1.907%
18	6.751	651	657	665	rBV	352470	544710	19.07%	1.507%
19	6.940	681	689	696	rBV	459608	697498	24.42%	1.929%
20	7.040	703	706	711	rBV7	2346	4153	0.15%	0.011%
21	7.398	758	767	776	rBV	776364	1186373	41.54%	3.281%
22	8.116	882	889	902	rBV	552147	863717	30.24%	2.389%
23	8.539	954	961	968	rBV	427138	685966	24.02%	1.897%
24	8.722	989	992	994	rVV3	4888	5298	0.19%	0.015%
25	8.757	997	998	1002	rVB4	3273	3622	0.13%	0.010%
26	8.987	1034	1037	1045	rVB8	4990	10233	0.36%	0.028%
27	9.128	1056	1061	1066	rBV3	16415	27414	0.96%	0.076%
28	9.257	1076	1083	1090	rBV	347589	566983	19.85%	1.568%
29	9.334	1094	1096	1101	rVB6	4471	5309	0.19%	0.015%
30	9.528	1127	1129	1131	rBV3	3231	3263	0.11%	0.009%
31	9.675	1151	1154	1160	rVB5	6216	8425	0.30%	0.023%
32	9.792	1166	1174	1185	rBV	552606	901396	31.56%	2.493%
33	10.157	1227	1236	1243	rBV	980879	1631652	57.14%	4.513%
34	10.304	1254	1261	1275	rBV	513730	871780	30.53%	2.411%
35	10.739	1330	1335	1340	rBV8	4480	7845	0.27%	0.022%
36	10.875	1353	1358	1359	rBV4	2359	2905	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046976.D
 Acq On : 03 Aug 2024 22:49
 Operator : MA/JU
 Sample : P3276-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	10.916	1359	1365	1374	rBV2	28336	60832	2.13%	0.168%
38	11.216	1413	1416	1421	rVB5	2554	3919	0.14%	0.011%
39	11.757	1501	1508	1515	rBV3	9550	16099	0.56%	0.045%
40	11.904	1530	1533	1535	rBV3	2806	3153	0.11%	0.009%
41	12.392	1613	1616	1619	rBV4	2791	3058	0.11%	0.008%
42	12.604	1648	1652	1654	rBV5	2233	2963	0.10%	0.008%
43	12.863	1689	1696	1699	rBV7	4459	8794	0.31%	0.024%
44	12.904	1699	1703	1707	rVV3	4063	5951	0.21%	0.016%
45	12.969	1709	1714	1715	rBV4	1871	3081	0.11%	0.009%
46	13.063	1725	1730	1732	rBV4	4669	7802	0.27%	0.022%
47	13.357	1778	1780	1783	rVB2	3727	3625	0.13%	0.010%
48	13.392	1783	1786	1787	rBV3	3286	2915	0.10%	0.008%
49	13.480	1795	1801	1813	rBV	990666	1370361	47.99%	3.790%
50	13.574	1815	1817	1819	rVB3	3637	3207	0.11%	0.009%
51	13.745	1839	1846	1856	rBV	1086146	1616724	56.61%	4.472%
52	13.880	1865	1869	1872	rVB6	2826	4214	0.15%	0.012%
53	13.992	1885	1888	1891	rVB4	4562	4614	0.16%	0.013%
54	14.057	1892	1899	1907	rVV	1472912	2138158	74.87%	5.914%
55	14.233	1925	1929	1932	rVB6	2290	3255	0.11%	0.009%
56	14.292	1932	1939	1956	rBV	357317	653205	22.87%	1.807%
57	14.439	1963	1964	1968	rVB4	2324	2887	0.10%	0.008%
58	14.521	1975	1978	1982	rVB6	3305	3574	0.13%	0.010%
59	14.692	2004	2007	2010	rBV3	2967	3611	0.13%	0.010%
60	14.892	2037	2041	2047	rVB7	6031	10071	0.35%	0.028%
61	14.951	2047	2051	2056	rBV8	5496	8805	0.31%	0.024%
62	15.057	2062	2069	2077	rBV	1391912	2008660	70.34%	5.556%
63	15.198	2086	2093	2099	rBV	317343	441430	15.46%	1.221%
64	15.310	2107	2112	2113	rVB5	5693	7713	0.27%	0.021%
65	15.463	2134	2138	2142	rVB6	4989	5797	0.20%	0.016%
66	15.521	2144	2148	2150	rVV4	3395	4042	0.14%	0.011%
67	15.657	2169	2171	2175	rVB5	3135	4414	0.15%	0.012%
68	15.815	2195	2198	2201	rBV5	5415	7245	0.25%	0.020%
69	15.845	2201	2203	2208	rVB7	2961	3993	0.14%	0.011%
70	15.980	2224	2226	2230	rVB4	3179	3535	0.12%	0.010%
71	16.274	2270	2276	2282	rVB10	4821	10129	0.35%	0.028%
72	16.321	2282	2284	2286	rBV3	2766	2897	0.10%	0.008%
73	16.410	2294	2299	2303	rBV7	5006	7414	0.26%	0.021%
74	16.445	2303	2305	2309	rVB5	2851	3524	0.12%	0.010%
75	16.615	2330	2334	2338	rVB5	4851	7400	0.26%	0.020%
76	16.815	2360	2368	2378	rVV	1829733	2522173	88.32%	6.976%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046976.D
 Acq On : 03 Aug 2024 22:49
 Operator : MA/JU
 Sample : P3276-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20J3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

77	16.915	2378	2385	2395	rVV	1585132	2204502	77.20%	6.097%
78	17.033	2402	2405	2409	rVB5	10618	13847	0.48%	0.038%
79	17.074	2411	2412	2416	rVV4	2620	2944	0.10%	0.008%
80	17.127	2419	2421	2427	rVB7	5097	10102	0.35%	0.028%
81	17.239	2437	2440	2443	rBV4	4648	6917	0.24%	0.019%
82	17.345	2456	2458	2459	rBV2	4768	3944	0.14%	0.011%
83	17.398	2466	2467	2470	rVB3	3566	2928	0.10%	0.008%
84	17.427	2470	2472	2476	rBV5	4024	4856	0.17%	0.013%
85	17.509	2482	2486	2488	rBV4	6547	8991	0.31%	0.025%
86	17.621	2503	2505	2511	rBV6	5892	11304	0.40%	0.031%
87	17.751	2523	2527	2535	rBV	95214	145644	5.10%	0.403%
88	18.033	2573	2575	2576	rBV2	3880	3294	0.12%	0.009%
89	18.262	2612	2614	2616	rBV3	5802	2994	0.10%	0.008%
90	18.786	2700	2703	2706	rVB2	21898	23425	0.82%	0.065%
91	18.856	2712	2715	2720	rBV3	20841	32191	1.13%	0.089%
92	18.904	2720	2723	2725	rBV4	14373	15436	0.54%	0.043%
93	19.056	2745	2749	2755	rBV3	33499	51734	1.81%	0.143%
94	19.227	2772	2778	2785	rBV	1920520	2500266	87.55%	6.915%
95	19.321	2791	2794	2800	rVB3	46608	53247	1.86%	0.147%
96	20.792	3040	3044	3050	rBV3	150850	235879	8.26%	0.652%
97	21.045	3082	3087	3096	rBV2	1970550	2658637	93.10%	7.353%
98	23.574	3510	3517	3528	rVB	1167070	2592890	90.80%	7.171%
99	23.762	3541	3549	3557	rBV	1278457	2855737	100.00%	7.898%




Sum of corrected areas: 36155739

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046976.D
Acq On : 03 Aug 2024 22:49
Operator : MA/JU
Sample : P3276-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

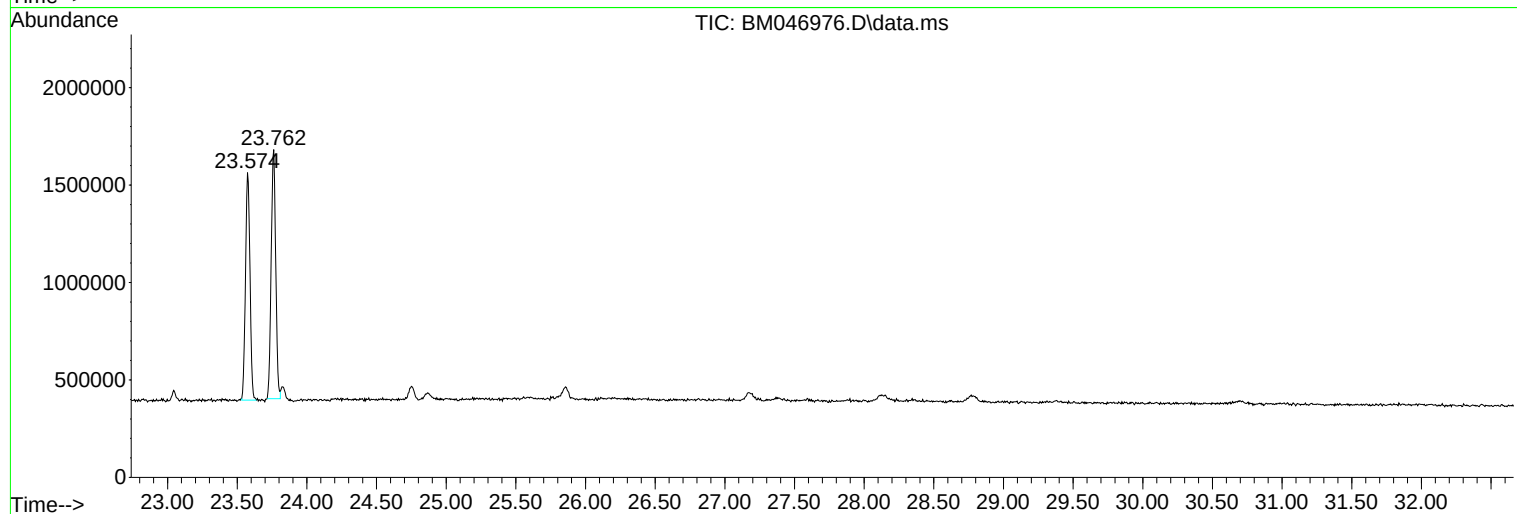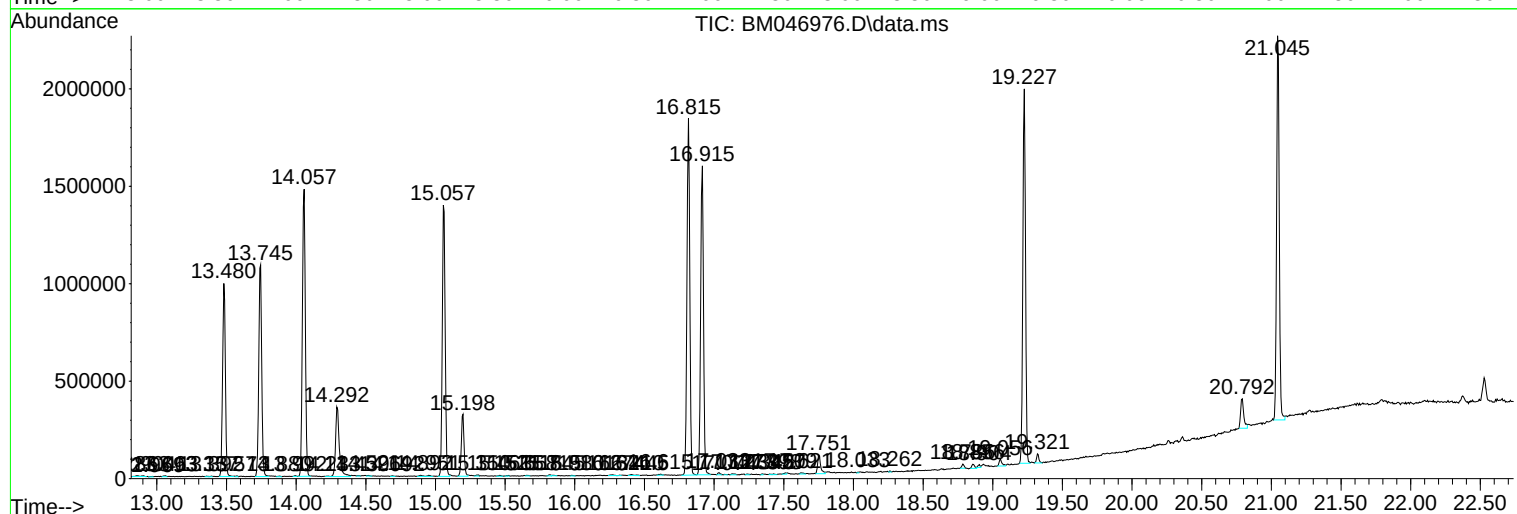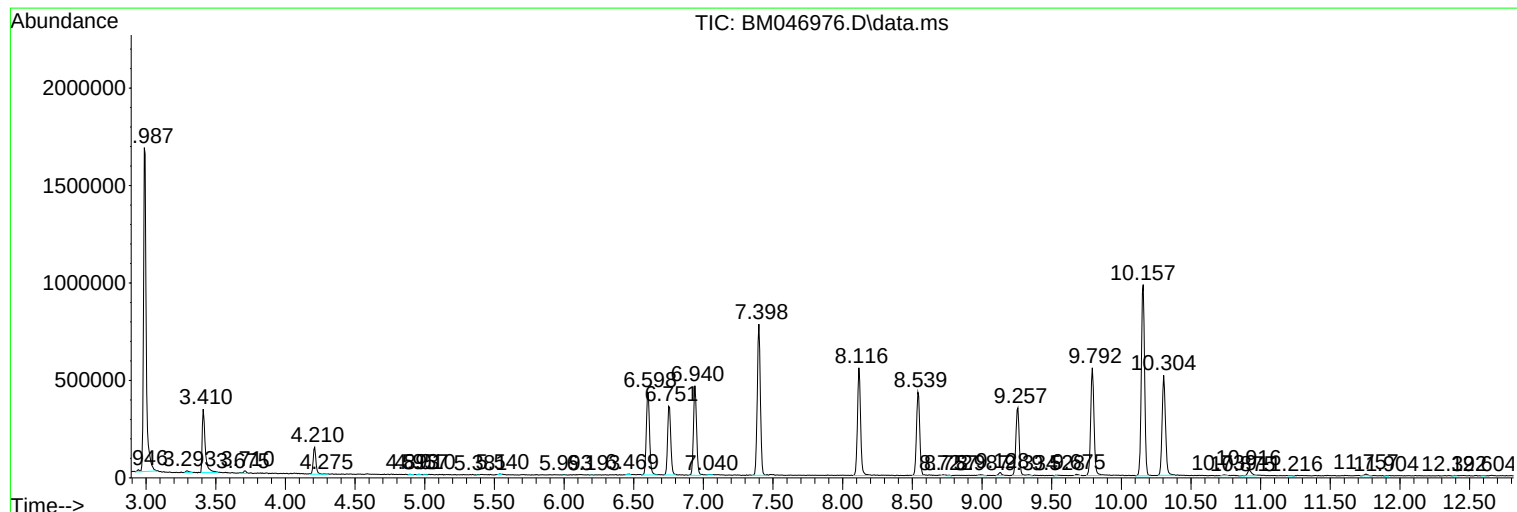

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046976.D
Acq On : 03 Aug 2024 22:49
Operator : MA/JU
Sample : P3276-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046976.D
Acq On : 03 Aug 2024 22:49
Operator : MA/JU
Sample : P3276-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20J3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc