

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046977.D
 Acq On : 03 Aug 2024 23:29
 Operator : MA/JU
 Sample : P3276-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20H7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.946	7	10	13	rBV4	8306	9704	0.35%	0.034%
2	2.987	13	17	39	rVB	671009	961322	35.10%	3.414%
3	3.287	65	68	75	rBV	31814	45985	1.68%	0.163%
4	3.410	86	89	107	rVB	243401	352639	12.88%	1.252%
5	3.710	135	140	145	rBV2	12215	15479	0.57%	0.055%
6	4.287	236	238	242	rVV5	2290	3223	0.12%	0.011%
7	4.322	242	244	246	rVB3	2900	2773	0.10%	0.010%
8	5.022	360	363	365	rBV4	2576	3173	0.12%	0.011%
9	5.116	375	379	381	rBV5	2902	3262	0.12%	0.012%
10	5.540	448	451	458	rVB7	6008	11854	0.43%	0.042%
11	6.081	540	543	545	rBV4	2604	3194	0.12%	0.011%
12	6.357	586	590	592	rBV4	2340	3289	0.12%	0.012%
13	6.463	604	608	610	rBV5	4911	6769	0.25%	0.024%
14	6.604	625	632	643	rVB	328010	519970	18.99%	1.847%
15	6.757	652	658	668	rVV	264989	414574	15.14%	1.472%
16	6.940	683	689	697	rBV	336513	515085	18.81%	1.829%
17	7.046	703	707	709	rBV5	4385	5740	0.21%	0.020%
18	7.240	738	740	745	rVB5	2442	4366	0.16%	0.016%
19	7.398	760	767	777	rBV	727492	1094421	39.96%	3.887%
20	7.493	777	783	785	rBV5	4586	8287	0.30%	0.029%
21	7.540	790	791	796	rVB4	3096	2825	0.10%	0.010%
22	7.575	796	797	801	rBV4	2250	2750	0.10%	0.010%
23	8.028	871	874	879	rBV6	2433	3492	0.13%	0.012%
24	8.116	883	889	904	rBV	396368	630012	23.00%	2.237%
25	8.540	954	961	970	rBV	315193	508110	18.55%	1.805%
26	8.722	989	992	997	rVV7	2702	4512	0.16%	0.016%
27	8.998	1035	1039	1043	rVB6	3665	5988	0.22%	0.021%
28	9.075	1049	1052	1053	rBV3	2659	2863	0.10%	0.010%
29	9.128	1056	1061	1066	rVB2	23658	35778	1.31%	0.127%
30	9.257	1075	1083	1090	rBV	250989	412282	15.05%	1.464%
31	9.434	1110	1113	1117	rBV4	2589	2927	0.11%	0.010%
32	9.534	1127	1130	1132	rBV4	4331	6129	0.22%	0.022%
33	9.792	1166	1174	1185	rBV	406076	663395	24.22%	2.356%
34	9.886	1187	1190	1193	rVV5	1609	2776	0.10%	0.010%
35	10.157	1226	1236	1243	rBV	901425	1503056	54.88%	5.338%
36	10.304	1250	1261	1271	rBV	383003	645478	23.57%	2.292%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046977.D
 Acq On : 03 Aug 2024 23:29
 Operator : MA/JU
 Sample : P3276-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20H7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	10.469	1287	1289	1293	rVB5	2658	2993	0.11%	0.011%
38	10.581	1305	1308	1312	rVB6	2517	3459	0.13%	0.012%
39	10.739	1331	1335	1337	rBV5	5362	7270	0.27%	0.026%
40	10.916	1358	1365	1374	rBV2	32235	68884	2.52%	0.245%
41	10.998	1376	1379	1386	rVB9	3410	5872	0.21%	0.021%
42	11.116	1394	1399	1402	rVB5	2591	4308	0.16%	0.015%
43	11.263	1421	1424	1430	rBV6	2067	4723	0.17%	0.017%
44	11.757	1502	1508	1513	rBV5	7104	13330	0.49%	0.047%
45	11.963	1540	1543	1548	rVB5	1896	2909	0.11%	0.010%
46	12.169	1576	1578	1582	rVB4	1834	2912	0.11%	0.010%
47	12.380	1611	1614	1616	rVV3	2884	3304	0.12%	0.012%
48	12.604	1648	1652	1654	rVB5	2640	3196	0.12%	0.011%
49	12.786	1677	1683	1686	rBV6	2081	4366	0.16%	0.016%
50	12.898	1697	1702	1707	rBV6	6311	9574	0.35%	0.034%
51	13.480	1795	1801	1809	rBV	675184	946974	34.58%	3.363%
52	13.575	1811	1817	1820	rVB8	4552	8005	0.29%	0.028%
53	13.604	1820	1822	1825	rBV4	3076	3157	0.12%	0.011%
54	13.739	1839	1845	1853	rBV2	759477	1137004	41.52%	4.038%
55	13.822	1858	1859	1864	rVB5	2448	3241	0.12%	0.012%
56	13.992	1884	1888	1891	rBV4	6621	7836	0.29%	0.028%
57	14.057	1892	1899	1906	rBV	1329315	1952666	71.30%	6.935%
58	14.292	1930	1939	1955	rBV	304439	557478	20.36%	1.980%
59	14.504	1971	1975	1977	rBV3	4273	6650	0.24%	0.024%
60	14.892	2035	2041	2043	rBV4	5873	6585	0.24%	0.023%
61	14.951	2048	2051	2054	rVV4	7755	7895	0.29%	0.028%
62	15.057	2063	2069	2076	rBV	947411	1384825	50.57%	4.918%
63	15.192	2087	2092	2100	rBV	249206	356727	13.03%	1.267%
64	15.251	2100	2102	2106	rVV5	4362	6593	0.24%	0.023%
65	15.298	2106	2110	2115	rVB7	4779	7432	0.27%	0.026%
66	15.369	2115	2122	2124	rBV7	4247	7501	0.27%	0.027%
67	15.463	2136	2138	2141	rVB4	3244	3314	0.12%	0.012%
68	15.527	2148	2149	2152	rVB3	4567	2758	0.10%	0.010%
69	15.645	2166	2169	2172	rBV5	2483	3709	0.14%	0.013%
70	15.710	2178	2180	2184	rVB5	3168	2922	0.11%	0.010%
71	15.757	2184	2188	2192	rVV6	1866	3273	0.12%	0.012%
72	15.821	2195	2199	2201	rVV3	9961	13483	0.49%	0.048%
73	15.845	2201	2203	2211	rVB7	9173	13736	0.50%	0.049%
74	15.992	2224	2228	2231	rVB5	3099	4144	0.15%	0.015%
75	16.104	2244	2247	2250	rBV5	2530	3011	0.11%	0.011%
76	16.168	2255	2258	2260	rBV3	2244	2752	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
 Data File : BM046977.D
 Acq On : 03 Aug 2024 23:29
 Operator : MA/JU
 Sample : P3276-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E20H7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

77	16.404	2294	2298	2301	rVB5	4423	5170	0.19%	0.018%
78	16.615	2327	2334	2339	rBV8	8573	15349	0.56%	0.055%
79	16.668	2341	2343	2347	rVB4	4714	4828	0.18%	0.017%
80	16.815	2360	2368	2375	rBV	1716791	2309779	84.34%	8.203%
81	16.915	2378	2385	2395	rBV2	1031217	1496753	54.65%	5.316%
82	17.033	2402	2405	2410	rVB6	11298	15153	0.55%	0.054%
83	17.210	2430	2435	2436	rBV4	4787	7115	0.26%	0.025%
84	17.351	2456	2459	2467	rVB9	4871	9332	0.34%	0.033%
85	17.527	2488	2489	2493	rVB4	7000	5560	0.20%	0.020%
86	17.627	2504	2506	2509	rBV3	3085	3312	0.12%	0.012%
87	17.751	2523	2527	2535	rBV	94588	135330	4.94%	0.481%
88	18.045	2575	2577	2580	rVB4	4692	3979	0.15%	0.014%
89	18.098	2582	2586	2587	rBV4	4731	6368	0.23%	0.023%
90	18.157	2595	2596	2598	rBV2	3783	3506	0.13%	0.012%
91	18.786	2699	2703	2707	rBV5	15051	21131	0.77%	0.075%
92	18.857	2713	2715	2719	rVB3	12856	16714	0.61%	0.059%
93	19.051	2745	2748	2754	rBV6	29848	49025	1.79%	0.174%
94	19.227	2771	2778	2785	rBV	1286637	1756067	64.12%	6.237%
95	19.321	2792	2794	2799	rVB3	25929	26146	0.95%	0.093%
96	20.792	3040	3044	3051	rBV2	137660	208142	7.60%	0.739%
97	21.050	3083	3088	3095	rBV	1848483	2465587	90.03%	8.756%
98	23.574	3511	3517	3533	rVB	843853	1846084	67.41%	6.556%
99	23.762	3542	3549	3557	rBV	1263508	2738626	100.00%	9.726%




Sum of corrected areas: 28157309

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046977.D
Acq On : 03 Aug 2024 23:29
Operator : MA/JU
Sample : P3276-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20H7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

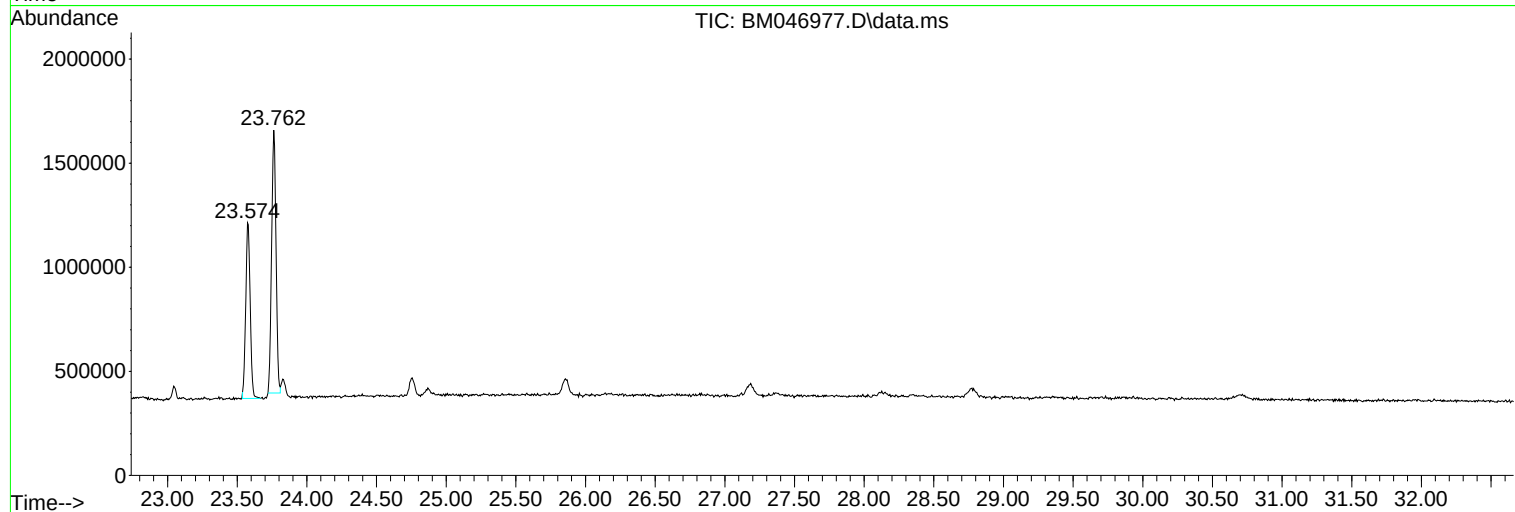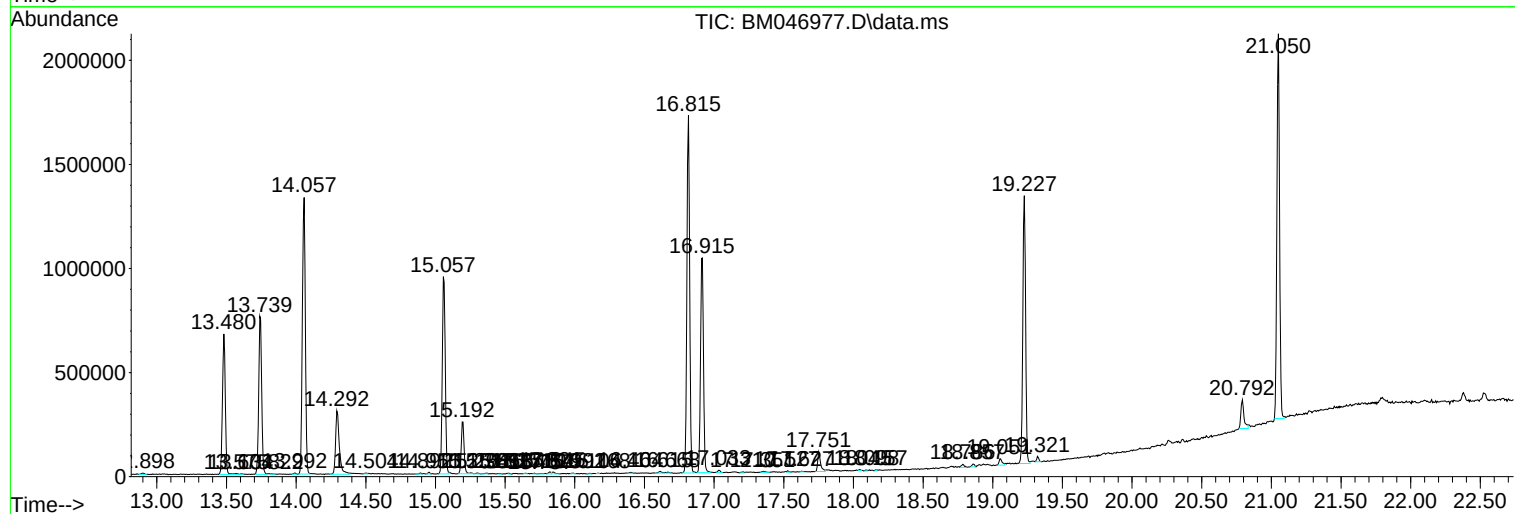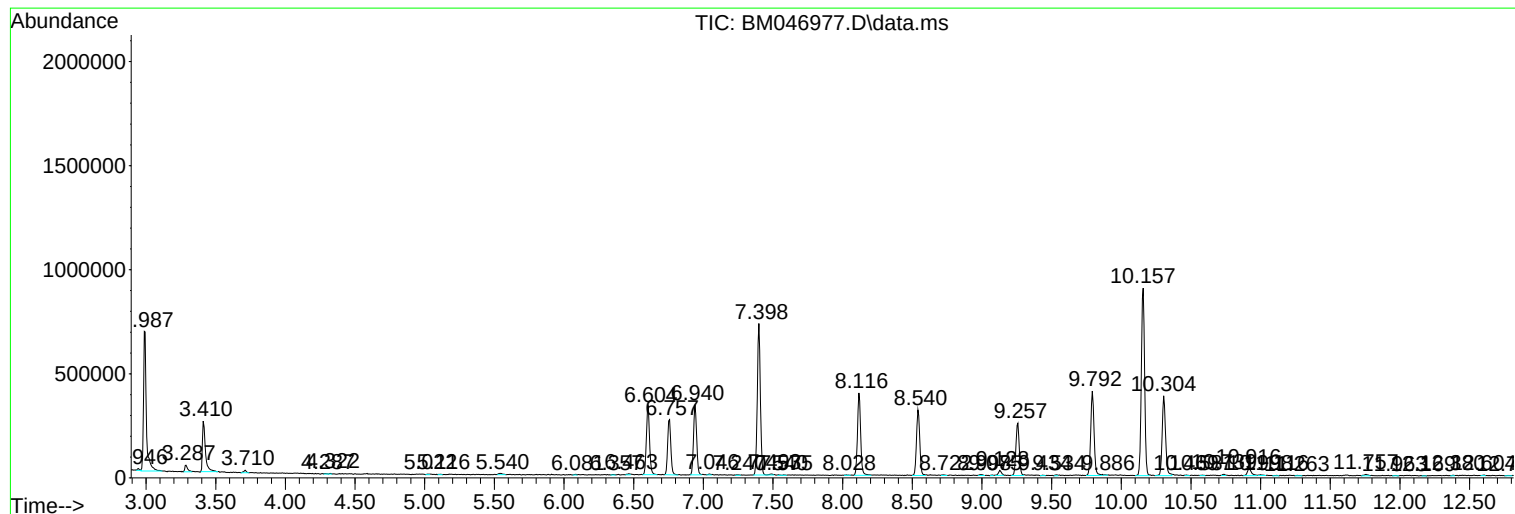

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046977.D
Acq On : 03 Aug 2024 23:29
Operator : MA/JU
Sample : P3276-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20H7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080324\
Data File : BM046977.D
Acq On : 03 Aug 2024 23:29
Operator : MA/JU
Sample : P3276-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E20H7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc